

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048114.D
 Acq On : 18 Apr 2022 12:35
 Operator : SY/MD
 Sample : N2387-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048114.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	100	rVB	166702	197031	15.84%	1.971%
2	1.916	171	179	198	rVB	129823	178606	14.36%	1.786%
3	2.571	371	383	403	rBV	276793	458935	36.89%	4.590%
4	2.735	432	434	436	rBV3	356	217	0.02%	0.002%
5	2.787	445	450	451	rBV3	790	673	0.05%	0.007%
6	2.829	461	463	467	rVB3	407	287	0.02%	0.003%
7	3.041	526	529	531	rVV	412	301	0.02%	0.003%
8	3.054	531	533	539	rVB3	463	439	0.04%	0.004%
9	3.189	567	575	577	rBV3	586	917	0.07%	0.009%
10	3.263	595	598	604	rVB2	356	392	0.03%	0.004%
11	3.327	616	618	623	rVB3	244	173	0.01%	0.002%
12	3.375	628	633	637	rBV2	387	397	0.03%	0.004%
13	3.472	659	663	667	rBV2	329	295	0.02%	0.003%
14	3.491	667	669	672	rVV2	275	198	0.02%	0.002%
15	3.697	727	733	735	rBV	267	302	0.02%	0.003%
16	3.796	762	764	768	rVB3	339	251	0.02%	0.003%
17	3.832	770	775	777	rBV	356	273	0.02%	0.003%
18	3.931	802	806	810	rVB2	230	217	0.02%	0.002%
19	4.018	827	833	840	rBV3	397	597	0.05%	0.006%
20	4.189	884	886	890	rVB	310	182	0.01%	0.002%
21	4.224	894	897	901	rVB2	259	218	0.02%	0.002%
22	4.301	917	921	926	rBV	353	256	0.02%	0.003%
23	4.629	1006	1023	1058	rBV	125471	328622	26.41%	3.287%
24	5.066	1141	1159	1180	rBV	231707	499943	40.18%	5.000%
25	5.250	1214	1216	1220	rVB	397	245	0.02%	0.002%
26	5.452	1276	1279	1282	rVB2	233	165	0.01%	0.002%
27	5.478	1282	1287	1289	rBV	312	302	0.02%	0.003%
28	5.729	1341	1365	1394	rBV2	462113	1244198	100.00%	12.444%
29	5.938	1428	1430	1439	rVB	375	322	0.03%	0.003%
30	6.025	1453	1457	1458	rBV2	243	191	0.02%	0.002%
31	6.092	1472	1478	1481	rBV3	311	350	0.03%	0.004%
32	6.128	1483	1489	1492	rVB2	404	451	0.04%	0.005%
33	6.250	1511	1527	1550	rBV	389308	743681	59.77%	7.438%
34	6.529	1606	1614	1626	rVV6	1801	3239	0.26%	0.032%
35	6.597	1633	1635	1638	rVB3	471	281	0.02%	0.003%
36	6.693	1649	1665	1687	rBV	283594	561237	45.11%	5.613%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048114.D
 Acq On : 18 Apr 2022 12:35
 Operator : SY/MD
 Sample : N2387-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.803	1696	1699	1708	rVB3	884	1001	0.08%	0.010%
38	6.857	1713	1716	1721	rVB2	370	295	0.02%	0.003%
39	6.951	1741	1745	1749	rVB2	242	212	0.02%	0.002%
40	6.970	1749	1751	1754	rVB	283	173	0.01%	0.002%
41	7.047	1770	1775	1778	rBV3	321	327	0.03%	0.003%
42	7.118	1791	1797	1798	rBV2	233	230	0.02%	0.002%
43	7.185	1809	1818	1827	rBV3	2181	3588	0.29%	0.036%
44	7.468	1903	1906	1908	rBV2	299	174	0.01%	0.002%
45	7.568	1924	1937	1955	rBV	146830	260211	20.91%	2.603%
46	7.687	1969	1974	1982	rVB5	1359	1824	0.15%	0.018%
47	7.800	2005	2009	2013	rVB3	424	384	0.03%	0.004%
48	7.899	2026	2040	2056	rBV	537614	942252	75.73%	9.424%
49	8.179	2116	2127	2147	rBV	103230	180998	14.55%	1.810%
50	8.472	2206	2218	2229	rBV2	5168	8973	0.72%	0.090%
51	8.581	2250	2252	2255	rBV2	350	232	0.02%	0.002%
52	8.635	2256	2269	2300	rBV	362213	677916	54.49%	6.780%
53	8.980	2374	2376	2379	rBV	339	233	0.02%	0.002%
54	9.160	2429	2432	2434	rBV2	261	199	0.02%	0.002%
55	9.246	2457	2459	2464	rVB	475	274	0.02%	0.003%
56	9.272	2464	2467	2469	rBV2	357	235	0.02%	0.002%
57	9.311	2475	2479	2483	rBV2	305	313	0.03%	0.003%
58	9.349	2488	2491	2497	rBV2	305	305	0.02%	0.003%
59	9.417	2498	2512	2537	rBV	586384	995799	80.04%	9.960%
60	9.568	2555	2559	2563	rBV3	484	425	0.03%	0.004%
61	9.687	2592	2596	2597	rBV2	606	324	0.03%	0.003%
62	9.799	2628	2631	2636	rBV2	173	193	0.02%	0.002%
63	9.979	2682	2687	2691	rVV3	355	439	0.04%	0.004%
64	10.320	2789	2793	2796	rBV	233	191	0.02%	0.002%
65	10.343	2796	2800	2808	rBV2	244	359	0.03%	0.004%
66	10.545	2859	2863	2869	rVB4	562	711	0.06%	0.007%
67	10.674	2895	2903	2913	rVB5	2471	3729	0.30%	0.037%
68	10.758	2916	2929	2951	rBV	440052	704023	56.58%	7.042%
69	10.893	2959	2971	2981	rBV2	8252	13828	1.11%	0.138%
70	10.999	3002	3004	3008	rVB2	274	161	0.01%	0.002%
71	11.031	3012	3014	3017	rBV2	296	225	0.02%	0.002%
72	11.108	3031	3038	3041	rVV4	369	485	0.04%	0.005%
73	11.240	3075	3079	3086	rBV3	258	320	0.03%	0.003%
74	11.459	3140	3147	3157	rVB7	1637	2459	0.20%	0.025%
75	11.574	3178	3183	3188	rBV3	346	376	0.03%	0.004%
76	11.600	3188	3191	3194	rVB	356	245	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048114.D
 Acq On : 18 Apr 2022 12:35
 Operator : SY/MD
 Sample : N2387-07
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.700	3211	3222	3230	rBV5	1489	2289	0.18%	0.023%
78	11.741	3230	3235	3236	rBV	765	476	0.04%	0.005%
79	11.812	3244	3257	3285	rBV	615924	992901	79.80%	9.931%
80	11.973	3303	3307	3313	rVB3	1700	1812	0.15%	0.018%
81	12.063	3327	3335	3346	rBV4	8763	14523	1.17%	0.145%
82	12.131	3354	3356	3359	rBV	392	273	0.02%	0.003%
83	12.195	3362	3376	3394	rVV	550862	931162	74.84%	9.313%
84	12.327	3415	3417	3426	rVB4	971	1025	0.08%	0.010%
85	12.442	3448	3453	3455	rBV	369	341	0.03%	0.003%
86	12.639	3512	3514	3517	rVB	514	281	0.02%	0.003%
87	12.684	3525	3528	3532	rVB2	390	295	0.02%	0.003%
88	12.712	3532	3537	3540	rBV	429	389	0.03%	0.004%
89	12.735	3540	3544	3548	rVB2	367	332	0.03%	0.003%
90	12.780	3548	3558	3563	rBV2	1130	1853	0.15%	0.019%
91	12.822	3568	3571	3572	rBV	290	199	0.02%	0.002%
92	13.005	3625	3628	3632	rVB2	502	451	0.04%	0.005%
93	13.028	3632	3635	3637	rBV	419	267	0.02%	0.003%
94	13.044	3637	3640	3649	rVB3	259	346	0.03%	0.003%
95	13.844	3880	3889	3901	rBV2	10046	15451	1.24%	0.155%
96	14.333	4036	4041	4055	rVB4	2240	3300	0.27%	0.033%
97	14.777	4175	4179	4182	rBV2	381	319	0.03%	0.003%
98	15.028	4255	4257	4261	rBV3	409	241	0.02%	0.002%
99	15.146	4292	4294	4296	rBV2	374	185	0.01%	0.002%
100	15.243	4322	4324	4330	rVB3	512	413	0.03%	0.004%




Sum of corrected areas: 9998149

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048114.D
Acq On : 18 Apr 2022 12:35
Operator : SY/MD
Sample : N2387-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

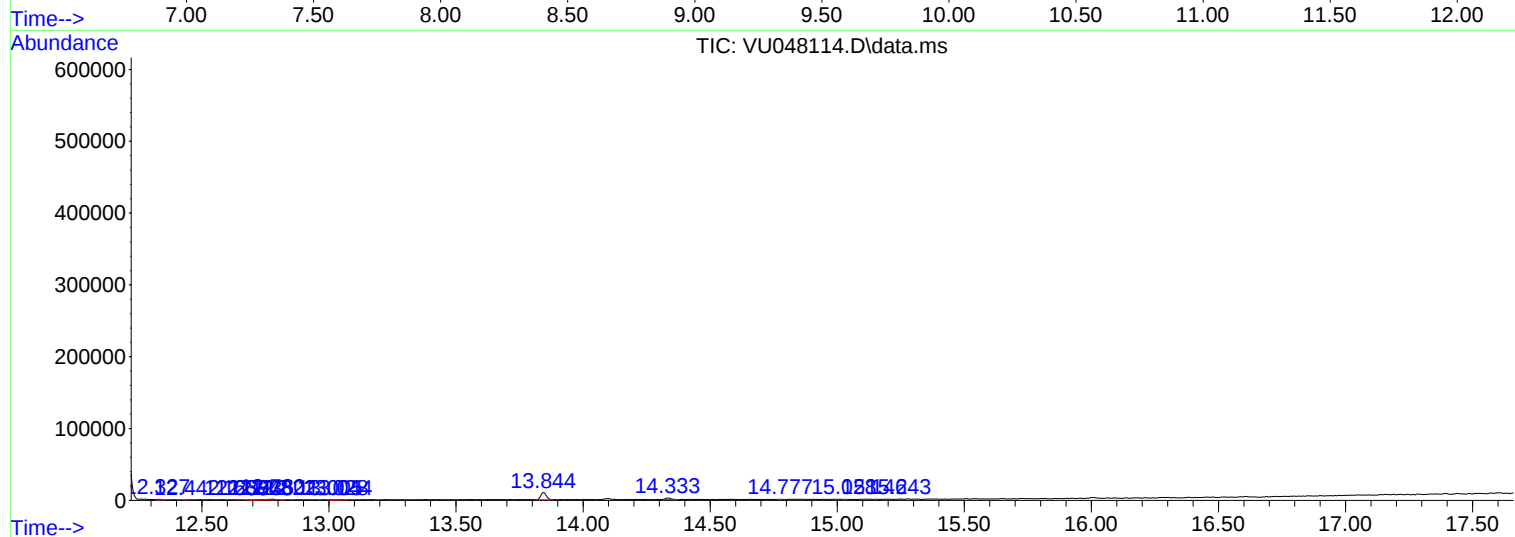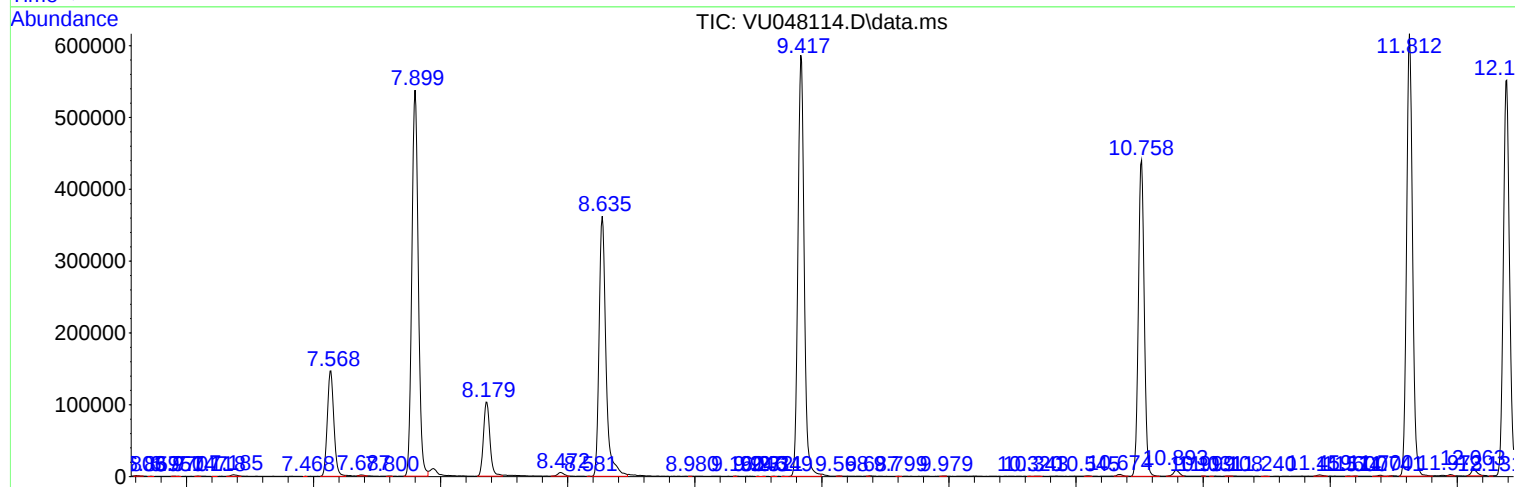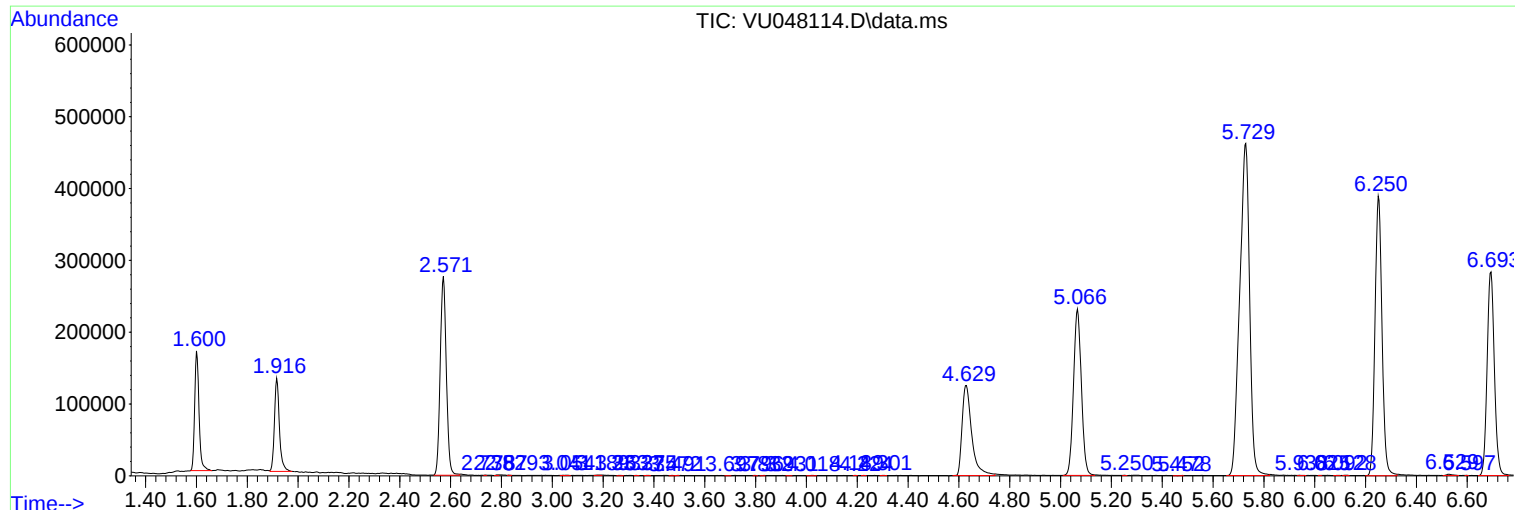

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048114.D
Acq On : 18 Apr 2022 12:35
Operator : SY/MD
Sample : N2387-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048114.D
Acq On : 18 Apr 2022 12:35
Operator : SY/MD
Sample : N2387-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J72

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc