

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048115.D
 Acq On : 18 Apr 2022 12:58
 Operator : SY/MD
 Sample : N2419-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048115.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	98	rBV	161108	190529	15.72%	1.810%
2	1.915	171	179	202	rVB	124846	174276	14.38%	1.655%
3	2.571	370	383	399	rBV	263852	437164	36.07%	4.152%
4	2.726	427	431	435	rBV3	271	248	0.02%	0.002%
5	2.996	512	515	518	rBV	376	223	0.02%	0.002%
6	3.051	529	532	540	rVB3	791	898	0.07%	0.009%
7	3.086	540	543	549	rBV2	301	340	0.03%	0.003%
8	3.141	557	560	564	rVB2	382	299	0.02%	0.003%
9	3.182	564	573	575	rBV4	1497	2076	0.17%	0.020%
10	3.256	594	596	600	rBV2	306	264	0.02%	0.003%
11	3.276	600	602	607	rVB	368	287	0.02%	0.003%
12	3.446	652	655	659	rVB2	255	221	0.02%	0.002%
13	3.468	659	662	664	rBV2	275	205	0.02%	0.002%
14	3.549	683	687	688	rBV2	265	203	0.02%	0.002%
15	3.774	753	757	759	rBV	264	206	0.02%	0.002%
16	3.874	780	788	794	rVV4	546	897	0.07%	0.009%
17	3.986	819	823	826	rBV2	304	220	0.02%	0.002%
18	4.022	831	834	840	rVV3	332	317	0.03%	0.003%
19	4.089	849	855	859	rBV2	223	340	0.03%	0.003%
20	4.134	865	869	872	rBV2	270	293	0.02%	0.003%
21	4.189	883	886	892	rVB2	325	284	0.02%	0.003%
22	4.221	892	896	902	rBV	285	394	0.03%	0.004%
23	4.285	910	916	918	rBV2	276	257	0.02%	0.002%
24	4.369	939	942	945	rVB2	399	241	0.02%	0.002%
25	4.388	945	948	950	rBV2	258	210	0.02%	0.002%
26	4.555	997	1000	1001	rBV2	366	210	0.02%	0.002%
27	4.629	1009	1023	1051	rBV	121560	317573	26.20%	3.016%
28	5.066	1142	1159	1184	rBV	216998	476827	39.34%	4.529%
29	5.285	1223	1227	1229	rBV3	438	338	0.03%	0.003%
30	5.388	1256	1259	1262	rBV2	545	441	0.04%	0.004%
31	5.433	1269	1273	1279	rVB3	272	270	0.02%	0.003%
32	5.530	1293	1303	1313	rVB3	2646	5323	0.44%	0.051%
33	5.610	1323	1328	1330	rBV2	215	210	0.02%	0.002%
34	5.729	1341	1365	1397	rBV2	442539	1201880	99.17%	11.415%
35	6.176	1501	1504	1512	rBV2	140	213	0.02%	0.002%
36	6.250	1512	1527	1556	rBV	403852	775355	63.98%	7.364%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048115.D
 Acq On : 18 Apr 2022 12:58
 Operator : SY/MD
 Sample : N2419-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.491	1600	1602	1606	rBV3	387	335	0.03%	0.003%
38	6.529	1606	1614	1623	rVB5	1508	2620	0.22%	0.025%
39	6.568	1623	1626	1630	rVB3	400	358	0.03%	0.003%
40	6.693	1649	1665	1685	rBV	274044	537115	44.32%	5.101%
41	6.806	1696	1700	1702	rBV3	474	351	0.03%	0.003%
42	7.047	1770	1775	1781	rVB2	407	497	0.04%	0.005%
43	7.192	1806	1820	1833	rBV6	2120	4012	0.33%	0.038%
44	7.308	1851	1856	1861	rBV2	198	276	0.02%	0.003%
45	7.568	1923	1937	1964	rBV	140660	248670	20.52%	2.362%
46	7.677	1966	1971	1972	rBV2	882	610	0.05%	0.006%
47	7.787	2002	2005	2012	rVB3	349	346	0.03%	0.003%
48	7.899	2026	2040	2056	rBV	527472	912065	75.26%	8.663%
49	8.182	2116	2128	2144	rBV	97092	169604	13.99%	1.611%
50	8.475	2210	2219	2226	rBV4	2137	3685	0.30%	0.035%
51	8.552	2238	2243	2252	rVB3	1621	2236	0.18%	0.021%
52	8.635	2256	2269	2304	rBV	369228	693886	57.25%	6.591%
53	9.169	2433	2435	2441	rVB2	424	284	0.02%	0.003%
54	9.330	2478	2485	2488	rBV3	319	350	0.03%	0.003%
55	9.356	2490	2493	2496	rVB	278	202	0.02%	0.002%
56	9.417	2496	2512	2538	rBV2	590246	1211948	100.00%	11.511%
57	9.697	2592	2599	2605	rVB3	1168	1761	0.15%	0.017%
58	9.870	2647	2653	2655	rBV2	301	258	0.02%	0.002%
59	9.899	2660	2662	2667	rVB2	296	212	0.02%	0.002%
60	9.963	2673	2682	2686	rVB2	329	458	0.04%	0.004%
61	10.005	2690	2695	2699	rVB2	245	262	0.02%	0.002%
62	10.102	2720	2725	2729	rBV3	517	571	0.05%	0.005%
63	10.163	2740	2744	2747	rVV2	262	209	0.02%	0.002%
64	10.182	2747	2750	2752	rVV	260	212	0.02%	0.002%
65	10.205	2755	2757	2762	rVV2	279	277	0.02%	0.003%
66	10.240	2766	2768	2771	rVV	410	230	0.02%	0.002%
67	10.372	2804	2809	2812	rBV2	216	210	0.02%	0.002%
68	10.523	2853	2856	2858	rBV2	254	211	0.02%	0.002%
69	10.587	2873	2876	2880	rVB	294	221	0.02%	0.002%
70	10.613	2880	2884	2888	rBV2	199	204	0.02%	0.002%
71	10.671	2895	2902	2911	rBV3	2484	3311	0.27%	0.031%
72	10.758	2916	2929	2948	rBV	416448	667993	55.12%	6.345%
73	10.896	2965	2972	2982	rVB2	4098	6372	0.53%	0.061%
74	11.111	3035	3039	3042	rBV3	465	333	0.03%	0.003%
75	11.246	3076	3081	3087	rVB3	355	401	0.03%	0.004%
76	11.385	3118	3124	3126	rBV2	212	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048115.D
 Acq On : 18 Apr 2022 12:58
 Operator : SY/MD
 Sample : N2419-05
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J52

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.462	3138	3148	3155	rBV6	1642	2878	0.24%	0.027%
78	11.552	3172	3176	3179	rBV2	299	252	0.02%	0.002%
79	11.690	3216	3219	3225	rVB3	659	664	0.05%	0.006%
80	11.745	3225	3236	3245	rBV2	20939	31663	2.61%	0.301%
81	11.812	3245	3257	3281	rVB2	646294	1145540	94.52%	10.880%
82	11.938	3293	3296	3297	rBV	595	318	0.03%	0.003%
83	11.973	3302	3307	3314	rVB6	1433	1887	0.16%	0.018%
84	12.066	3326	3336	3352	rBV3	7304	13887	1.15%	0.132%
85	12.195	3358	3376	3398	rBV2	577786	1096032	90.44%	10.410%
86	12.478	3460	3464	3466	rBV2	288	220	0.02%	0.002%
87	12.603	3499	3503	3508	rBV	353	356	0.03%	0.003%
88	12.684	3525	3528	3529	rBV2	484	239	0.02%	0.002%
89	12.770	3550	3555	3564	rVB2	817	1330	0.11%	0.013%
90	12.928	3601	3604	3608	rBV2	232	234	0.02%	0.002%
91	12.979	3617	3620	3623	rVB3	622	349	0.03%	0.003%
92	13.047	3638	3641	3644	rBV2	315	255	0.02%	0.002%
93	13.221	3687	3695	3705	rVB3	5725	9020	0.74%	0.086%
94	13.841	3877	3888	3901	rBV	73307	112072	9.25%	1.064%
95	13.963	3923	3926	3929	rBV3	379	328	0.03%	0.003%
96	14.330	4031	4040	4055	rBV2	18059	28830	2.38%	0.274%
97	14.677	4145	4148	4151	rBV2	546	296	0.02%	0.003%
98	15.397	4363	4372	4392	rBV4	6519	12243	1.01%	0.116%
99	15.661	4447	4454	4456	rBV5	1011	1354	0.11%	0.013%
100	15.999	4554	4559	4567	rVB5	4219	5412	0.45%	0.051%




Sum of corrected areas: 10528576

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048115.D
Acq On : 18 Apr 2022 12:58
Operator : SY/MD
Sample : N2419-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

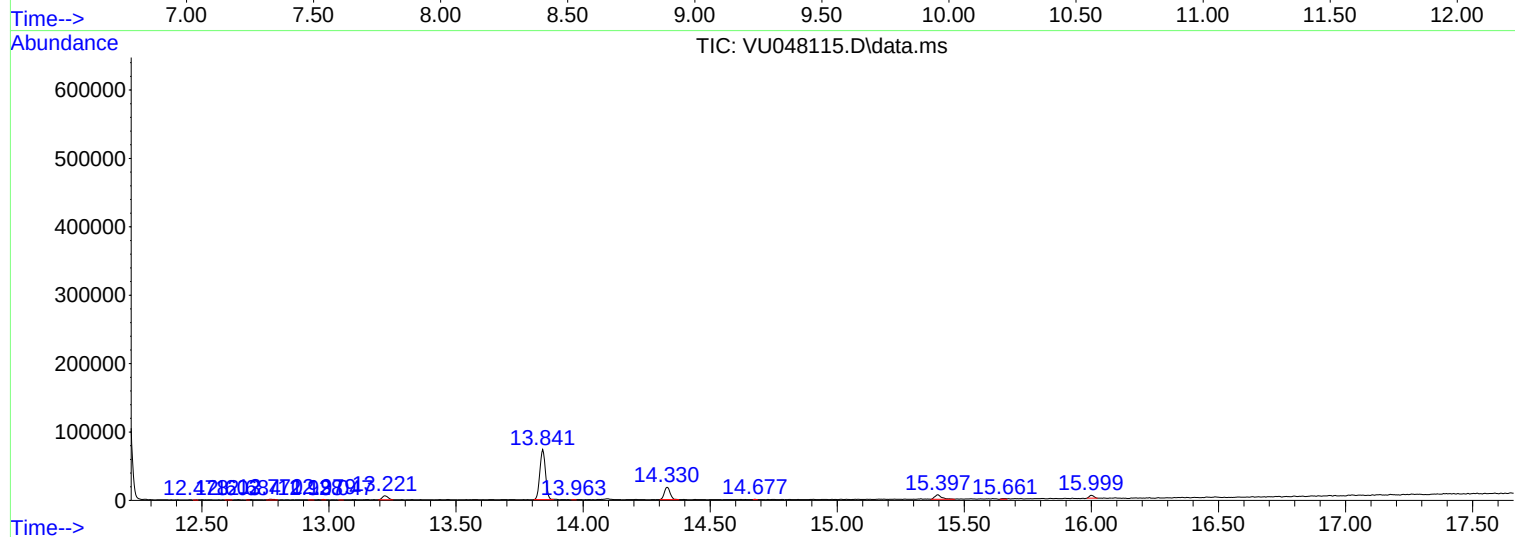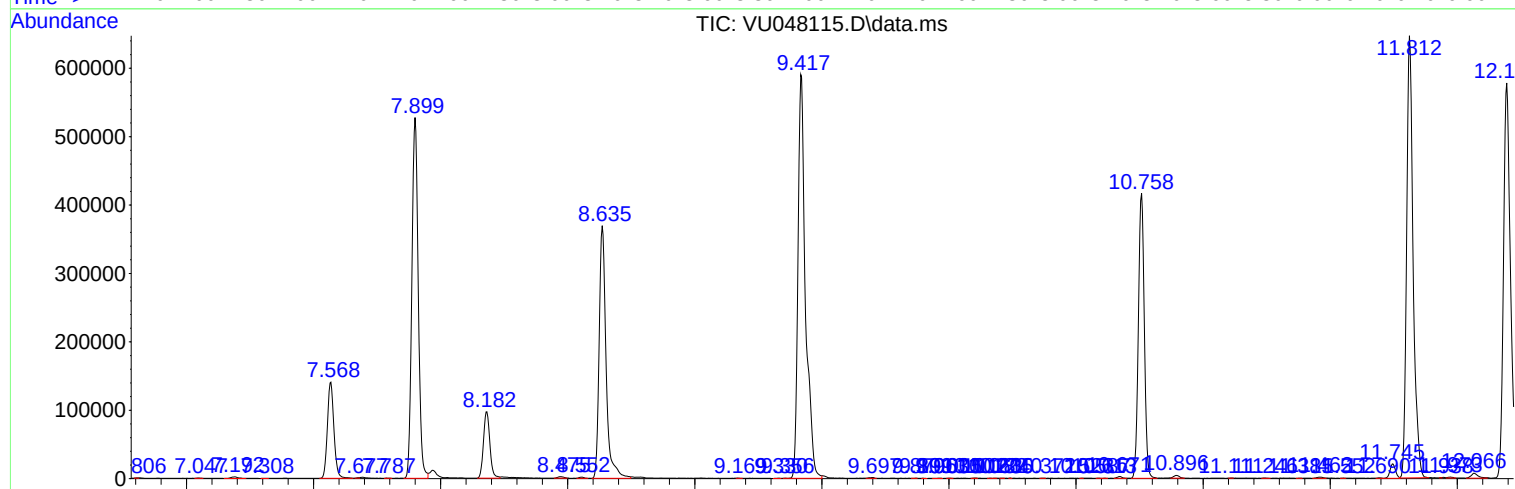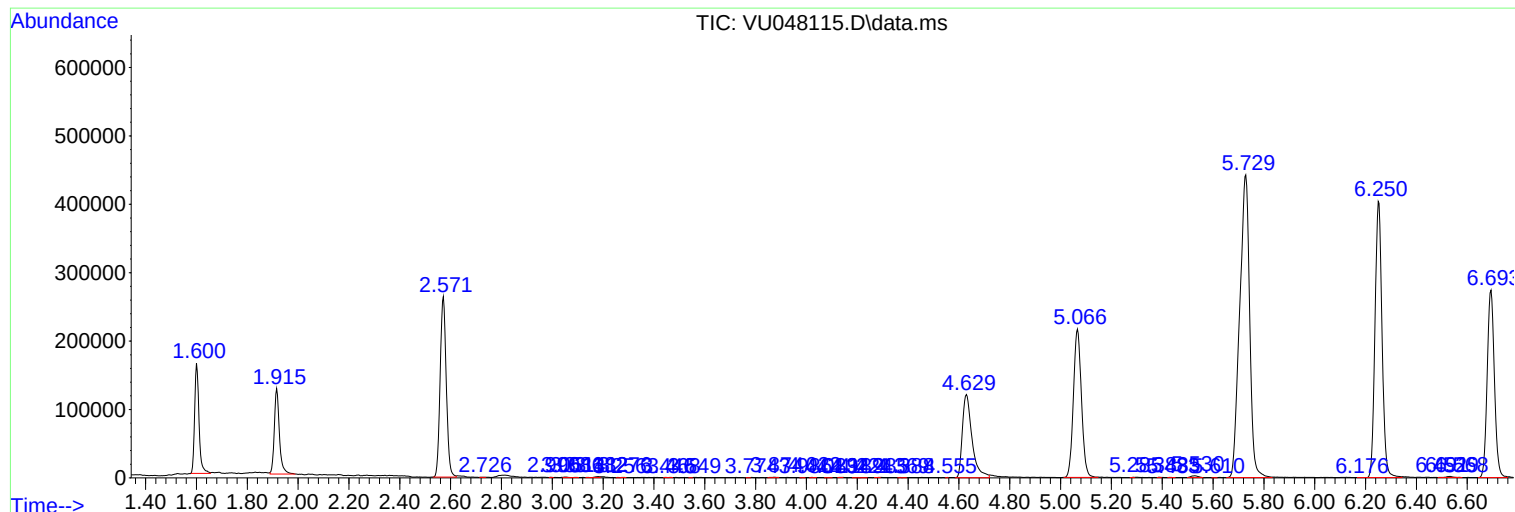

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048115.D
Acq On : 18 Apr 2022 12:58
Operator : SY/MD
Sample : N2419-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048115.D
Acq On : 18 Apr 2022 12:58
Operator : SY/MD
Sample : N2419-05
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J52

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------