

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048116.D
 Acq On : 18 Apr 2022 13:21
 Operator : SY/MD
 Sample : N2387-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048116.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	164113	199102	16.41%	2.025%
2	1.916	171	179	199	rVB	124269	171643	14.15%	1.746%
3	2.504	359	362	365	rBV3	271	282	0.02%	0.003%
4	2.572	369	383	402	rVV	272696	449118	37.02%	4.569%
5	2.742	434	436	439	rVB2	593	345	0.03%	0.004%
6	2.758	439	441	444	rBV2	398	309	0.03%	0.003%
7	2.880	473	479	482	rVB2	440	381	0.03%	0.004%
8	2.957	496	503	507	rBV3	495	574	0.05%	0.006%
9	3.051	524	532	542	rVB6	2106	3597	0.30%	0.037%
10	3.121	550	554	559	rBV2	337	300	0.02%	0.003%
11	3.163	563	567	568	rVV2	382	283	0.02%	0.003%
12	3.186	570	574	584	rVB5	1246	2359	0.19%	0.024%
13	3.253	589	595	600	rBV2	448	525	0.04%	0.005%
14	3.279	600	603	607	rBV2	211	214	0.02%	0.002%
15	3.314	611	614	618	rVB2	290	203	0.02%	0.002%
16	3.469	657	662	666	rBV3	389	444	0.04%	0.005%
17	3.533	678	682	684	rBV2	242	215	0.02%	0.002%
18	3.642	710	716	723	rVB2	338	537	0.04%	0.005%
19	4.089	853	855	861	rVB3	235	202	0.02%	0.002%
20	4.282	911	915	919	rBV2	281	243	0.02%	0.002%
21	4.391	945	949	954	rVB	258	220	0.02%	0.002%
22	4.517	981	988	991	rBV2	178	230	0.02%	0.002%
23	4.552	997	999	1001	rBV	290	191	0.02%	0.002%
24	4.623	1008	1021	1058	rBV	126951	325217	26.81%	3.308%
25	5.067	1142	1159	1180	rBV	223512	490806	40.46%	4.993%
26	5.186	1194	1196	1203	rVB5	315	252	0.02%	0.003%
27	5.285	1224	1227	1230	rBV	367	374	0.03%	0.004%
28	5.359	1247	1250	1252	rBV2	345	259	0.02%	0.003%
29	5.452	1275	1279	1286	rVB2	218	217	0.02%	0.002%
30	5.729	1342	1365	1393	rBV2	455168	1213076	100.00%	12.341%
31	6.028	1453	1458	1459	rBV2	439	294	0.02%	0.003%
32	6.108	1480	1483	1485	rBV3	304	214	0.02%	0.002%
33	6.160	1496	1499	1502	rBV2	270	232	0.02%	0.002%
34	6.250	1511	1527	1553	rBV	387794	745423	61.45%	7.583%
35	6.475	1594	1597	1600	rBV2	266	212	0.02%	0.002%
36	6.526	1606	1613	1621	rVV5	1318	1924	0.16%	0.020%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048116.D
 Acq On : 18 Apr 2022 13:21
 Operator : SY/MD
 Sample : N2387-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.616	1639	1641	1647	rVB3	309	273	0.02%	0.003%
38	6.694	1650	1665	1690	rBV	281127	548142	45.19%	5.576%
39	7.009	1760	1763	1766	rVB	292	214	0.02%	0.002%
40	7.041	1769	1773	1774	rBV2	440	318	0.03%	0.003%
41	7.189	1810	1819	1826	rVV3	2216	3700	0.31%	0.038%
42	7.237	1832	1834	1838	rVB2	321	189	0.02%	0.002%
43	7.568	1923	1937	1955	rBV	140084	250728	20.67%	2.551%
44	7.687	1969	1974	1976	rBV3	1289	1172	0.10%	0.012%
45	7.806	2009	2011	2015	rVB2	404	202	0.02%	0.002%
46	7.899	2026	2040	2056	rBV	526377	922986	76.09%	9.390%
47	8.179	2116	2127	2142	rBV	100978	173933	14.34%	1.769%
48	8.465	2212	2216	2217	rBV2	393	287	0.02%	0.003%
49	8.542	2235	2240	2245	rVB2	318	240	0.02%	0.002%
50	8.587	2250	2254	2256	rBV3	360	262	0.02%	0.003%
51	8.636	2256	2269	2299	rBV	385350	709913	58.52%	7.222%
52	8.902	2349	2352	2354	rBV2	362	268	0.02%	0.003%
53	8.996	2378	2381	2387	rVB3	269	244	0.02%	0.002%
54	9.054	2395	2399	2404	rVB2	244	209	0.02%	0.002%
55	9.079	2404	2407	2410	rBV	365	228	0.02%	0.002%
56	9.160	2428	2432	2436	rBV3	423	416	0.03%	0.004%
57	9.417	2498	2512	2548	rBV	576782	982749	81.01%	9.998%
58	9.565	2555	2558	2564	rBV3	561	604	0.05%	0.006%
59	9.645	2578	2583	2585	rVV2	373	324	0.03%	0.003%
60	9.697	2594	2599	2605	rVB3	810	834	0.07%	0.008%
61	9.790	2623	2628	2630	rBV	237	219	0.02%	0.002%
62	9.915	2665	2667	2674	rVB	206	195	0.02%	0.002%
63	9.960	2677	2681	2687	rBV3	398	503	0.04%	0.005%
64	10.021	2695	2700	2704	rBV2	269	364	0.03%	0.004%
65	10.266	2772	2776	2782	rBV2	291	388	0.03%	0.004%
66	10.340	2797	2799	2803	rVB2	249	206	0.02%	0.002%
67	10.420	2820	2824	2829	rBV	189	223	0.02%	0.002%
68	10.465	2833	2838	2840	rBV2	340	213	0.02%	0.002%
69	10.565	2866	2869	2874	rVB2	314	281	0.02%	0.003%
70	10.613	2881	2884	2888	rVV	276	210	0.02%	0.002%
71	10.671	2893	2902	2909	rBV3	2543	3432	0.28%	0.035%
72	10.706	2909	2913	2916	rBV2	302	221	0.02%	0.002%
73	10.758	2916	2929	2946	rBV	406991	665695	54.88%	6.772%
74	10.893	2963	2971	2977	rVV6	861	1284	0.11%	0.013%
75	10.922	2977	2980	2984	rVV2	281	226	0.02%	0.002%
76	11.111	3034	3039	3040	rBV3	436	313	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048116.D
 Acq On : 18 Apr 2022 13:21
 Operator : SY/MD
 Sample : N2387-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.160	3052	3054	3059	rBV	257	246	0.02%	0.003%
78	11.185	3059	3062	3065	rBV	274	231	0.02%	0.002%
79	11.266	3084	3087	3092	rBV	261	272	0.02%	0.003%
80	11.455	3142	3146	3164	rVB5	1615	2560	0.21%	0.026%
81	11.690	3216	3219	3220	rBV	766	486	0.04%	0.005%
82	11.700	3220	3222	3226	rVB3	961	692	0.06%	0.007%
83	11.751	3236	3238	3244	rVB2	540	350	0.03%	0.004%
84	11.812	3244	3257	3279	rBV	620993	994033	81.94%	10.112%
85	11.947	3292	3299	3303	rBV5	945	1406	0.12%	0.014%
86	12.047	3321	3330	3331	rBV3	453	535	0.04%	0.005%
87	12.063	3331	3335	3336	rVV2	496	364	0.03%	0.004%
88	12.079	3338	3340	3344	rVB2	801	528	0.04%	0.005%
89	12.192	3362	3375	3397	rBV	556340	930773	76.73%	9.469%
90	12.304	3407	3410	3412	rBV	574	365	0.03%	0.004%
91	12.333	3417	3419	3421	rBV3	573	289	0.02%	0.003%
92	12.388	3434	3436	3441	rBV2	421	394	0.03%	0.004%
93	12.484	3464	3466	3469	rVB2	404	229	0.02%	0.002%
94	12.722	3537	3540	3543	rBV3	283	273	0.02%	0.003%
95	12.902	3594	3596	3599	rBV	328	190	0.02%	0.002%
96	13.002	3624	3627	3630	rBV2	274	229	0.02%	0.002%
97	13.089	3649	3654	3655	rBV2	310	277	0.02%	0.003%
98	13.848	3880	3890	3902	rBV2	5503	9509	0.78%	0.097%
99	14.137	3978	3980	3983	rBV3	299	197	0.02%	0.002%
100	14.336	4035	4042	4050	rBV4	2032	2962	0.24%	0.030%




Sum of corrected areas: 9829815

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048116.D
Acq On : 18 Apr 2022 13:21
Operator : SY/MD
Sample : N2387-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

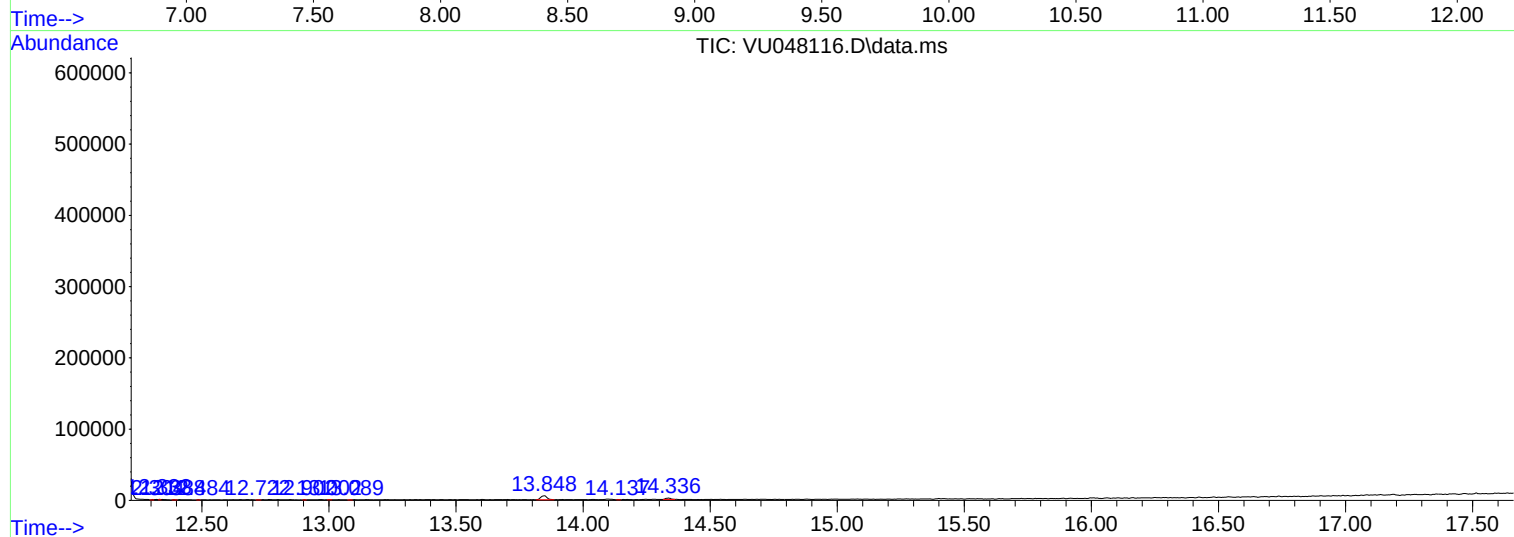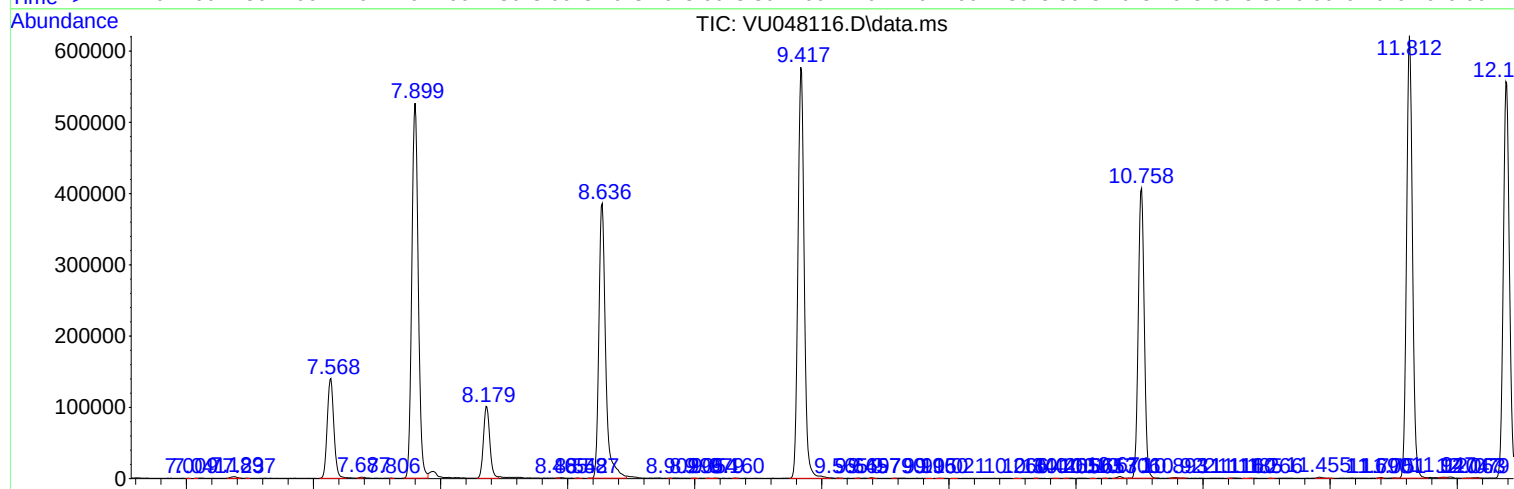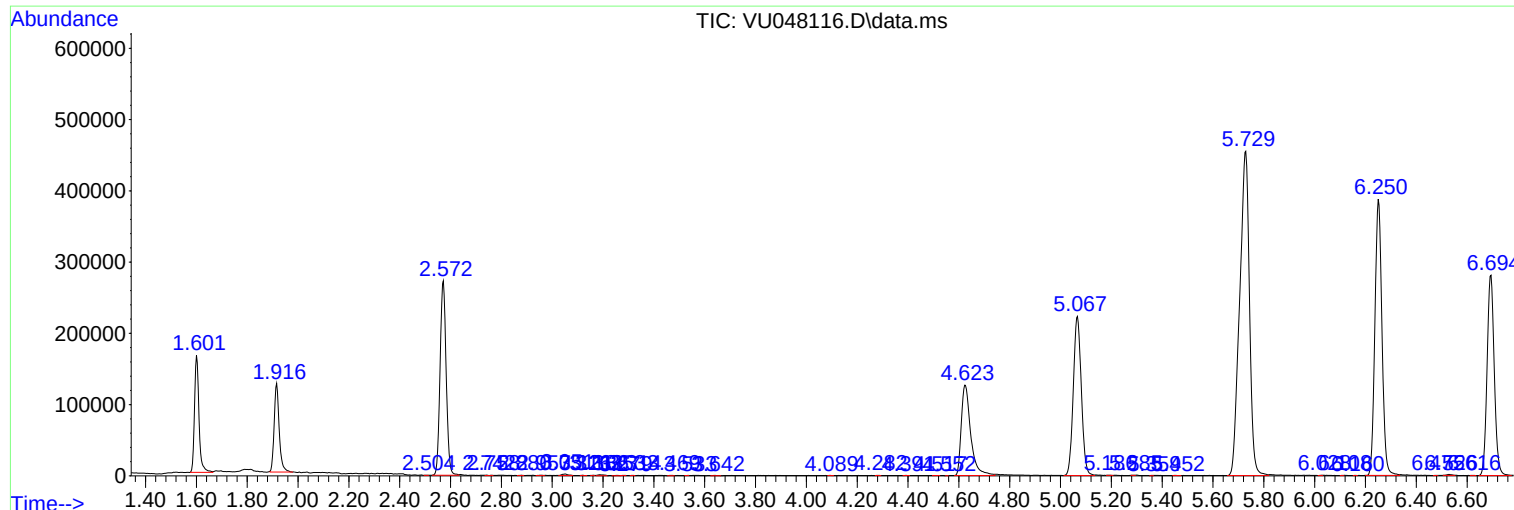

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048116.D
Acq On : 18 Apr 2022 13:21
Operator : SY/MD
Sample : N2387-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048116.D
Acq On : 18 Apr 2022 13:21
Operator : SY/MD
Sample : N2387-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------