

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048119.D
 Acq On : 18 Apr 2022 14:30
 Operator : SY/MD
 Sample : N2419-04DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048119.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	103	rBV	167523	201203	11.55%	1.674%
2	1.916	170	179	203	rVB	125739	182578	10.48%	1.519%
3	2.568	370	382	397	rVV	279053	457401	26.25%	3.806%
4	2.748	430	438	440	rBV7	874	1024	0.06%	0.009%
5	2.819	456	460	463	rBV3	347	238	0.01%	0.002%
6	2.839	463	466	472	rVB2	278	302	0.02%	0.003%
7	2.874	472	477	482	rVB3	461	523	0.03%	0.004%
8	2.948	494	500	504	rBV3	528	586	0.03%	0.005%
9	3.051	520	532	540	rBV6	1764	3111	0.18%	0.026%
10	3.112	546	551	555	rBV3	334	307	0.02%	0.003%
11	3.189	562	575	588	rVV2	19329	43955	2.52%	0.366%
12	3.279	599	603	607	rBV2	319	263	0.02%	0.002%
13	3.366	627	630	636	rVB2	339	247	0.01%	0.002%
14	3.433	645	651	653	rBV	206	215	0.01%	0.002%
15	3.469	658	662	664	rBV2	265	212	0.01%	0.002%
16	3.588	692	699	702	rBV	350	397	0.02%	0.003%
17	3.700	731	734	740	rVB2	296	217	0.01%	0.002%
18	3.739	740	746	749	rVB	269	320	0.02%	0.003%
19	3.758	749	752	757	rBV2	248	281	0.02%	0.002%
20	3.787	759	761	765	rVB	375	204	0.01%	0.002%
21	4.147	867	873	874	rBV2	235	222	0.01%	0.002%
22	4.189	883	886	892	rVV3	308	366	0.02%	0.003%
23	4.346	930	935	939	rBV2	321	337	0.02%	0.003%
24	4.414	952	956	961	rVV3	280	330	0.02%	0.003%
25	4.552	995	999	1003	rVV2	282	301	0.02%	0.003%
26	4.620	1003	1020	1057	rBV	139863	346842	19.91%	2.886%
27	5.067	1142	1159	1184	rBV	228755	500941	28.75%	4.168%
28	5.211	1201	1204	1210	rVB2	395	439	0.03%	0.004%
29	5.289	1222	1228	1230	rBV2	674	750	0.04%	0.006%
30	5.340	1238	1244	1248	rBV2	316	382	0.02%	0.003%
31	5.523	1295	1301	1302	rBV2	488	521	0.03%	0.004%
32	5.726	1341	1364	1374	rBV2	463044	1270972	72.94%	10.576%
33	6.006	1449	1451	1456	rVV3	366	213	0.01%	0.002%
34	6.102	1479	1481	1484	rVB3	370	204	0.01%	0.002%
35	6.125	1484	1488	1492	rBV3	500	402	0.02%	0.003%
36	6.186	1502	1507	1512	rVB2	297	253	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048119.D
 Acq On : 18 Apr 2022 14:30
 Operator : SY/MD
 Sample : N2419-04DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.250	1512	1527	1559	rBV	408739	772431	44.33%	6.427%
38	6.449	1585	1589	1592	rBV3	248	193	0.01%	0.002%
39	6.533	1606	1615	1620	rBV5	1879	2665	0.15%	0.022%
40	6.690	1649	1664	1694	rVV	287222	567602	32.58%	4.723%
41	6.932	1734	1739	1743	rBV2	147	192	0.01%	0.002%
42	7.047	1769	1775	1778	rBV	286	300	0.02%	0.002%
43	7.186	1809	1818	1828	rBV5	2437	4131	0.24%	0.034%
44	7.292	1848	1851	1856	rBV2	387	377	0.02%	0.003%
45	7.565	1923	1936	1954	rBV	146240	258882	14.86%	2.154%
46	7.690	1969	1975	1981	rVB5	1374	1964	0.11%	0.016%
47	7.748	1990	1993	1996	rBV4	266	224	0.01%	0.002%
48	7.787	2002	2005	2009	rVV3	451	262	0.02%	0.002%
49	7.899	2025	2040	2056	rBV	574287	987817	56.69%	8.219%
50	8.179	2116	2127	2144	rBV	104245	176541	10.13%	1.469%
51	8.475	2214	2219	2222	rBV4	358	316	0.02%	0.003%
52	8.520	2231	2233	2240	rVB2	416	299	0.02%	0.002%
53	8.633	2256	2268	2299	rBV	370866	676088	38.80%	5.626%
54	8.819	2323	2326	2331	rVB3	356	341	0.02%	0.003%
55	8.845	2331	2334	2337	rBV2	356	218	0.01%	0.002%
56	8.893	2345	2349	2351	rBV	308	249	0.01%	0.002%
57	8.919	2351	2357	2365	rVB3	580	809	0.05%	0.007%
58	9.224	2449	2452	2454	rBV	424	291	0.02%	0.002%
59	9.288	2468	2472	2477	rVB2	281	266	0.02%	0.002%
60	9.321	2477	2482	2485	rBV	231	278	0.02%	0.002%
61	9.420	2499	2513	2515	rBV	585059	812391	46.63%	6.760%
62	9.690	2591	2597	2603	rBV4	926	1123	0.06%	0.009%
63	9.758	2611	2618	2622	rVB3	373	465	0.03%	0.004%
64	9.787	2622	2627	2632	rVB2	295	252	0.01%	0.002%
65	9.893	2657	2660	2664	rVB	281	194	0.01%	0.002%
66	10.140	2732	2737	2741	rBV2	299	371	0.02%	0.003%
67	10.443	2827	2831	2834	rVB2	269	200	0.01%	0.002%
68	10.552	2862	2865	2869	rVB2	330	247	0.01%	0.002%
69	10.668	2895	2901	2911	rVB4	2419	3424	0.20%	0.028%
70	10.758	2915	2929	2948	rBV	420382	679628	39.01%	5.655%
71	10.867	2958	2963	2965	rBV2	628	448	0.03%	0.004%
72	11.118	3036	3041	3042	rBV4	528	369	0.02%	0.003%
73	11.459	3141	3147	3155	rVB6	1266	1887	0.11%	0.016%
74	11.510	3160	3163	3167	rBV	215	210	0.01%	0.002%
75	11.581	3183	3185	3190	rVB	639	406	0.02%	0.003%
76	11.626	3194	3199	3202	rBV2	263	256	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048119.D
 Acq On : 18 Apr 2022 14:30
 Operator : SY/MD
 Sample : N2419-04DL 200X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J47DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.693	3214	3220	3226	rVB5	891	1131	0.06%	0.009%
78	11.745	3226	3236	3245	rBV	53445	83454	4.79%	0.694%
79	11.816	3245	3258	3283	rVB2	668004	1714239	98.38%	14.264%
80	11.941	3294	3297	3300	rVB4	822	486	0.03%	0.004%
81	11.973	3302	3307	3314	rVB4	2025	2575	0.15%	0.021%
82	12.015	3318	3320	3324	rVB2	525	324	0.02%	0.003%
83	12.198	3361	3377	3397	rBV2	733593	1742382	100.00%	14.498%
84	12.337	3417	3420	3424	rVB3	517	270	0.02%	0.002%
85	12.410	3437	3443	3446	rVB3	583	590	0.03%	0.005%
86	12.436	3446	3451	3453	rBV3	388	380	0.02%	0.003%
87	12.475	3461	3463	3468	rBV2	312	311	0.02%	0.003%
88	12.745	3544	3547	3551	rVB3	521	442	0.03%	0.004%
89	12.767	3551	3554	3556	rBV2	608	464	0.03%	0.004%
90	12.835	3571	3575	3578	rBV	532	488	0.03%	0.004%
91	12.909	3595	3598	3601	rVB3	418	326	0.02%	0.003%
92	12.931	3601	3605	3607	rBV2	344	328	0.02%	0.003%
93	12.973	3611	3618	3629	rVB3	2611	4277	0.25%	0.036%
94	13.263	3706	3708	3711	rBV2	357	219	0.01%	0.002%
95	13.330	3724	3729	3741	rVB8	1444	2498	0.14%	0.021%
96	13.841	3876	3888	3906	rBV	249845	391600	22.47%	3.258%
97	14.330	4030	4040	4055	rBV	63497	98416	5.65%	0.819%
98	14.619	4127	4130	4133	rBV2	411	331	0.02%	0.003%
99	15.031	4255	4258	4260	rBV	536	352	0.02%	0.003%
100	15.324	4346	4349	4351	rBV3	748	511	0.03%	0.004%




Sum of corrected areas: 12018060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048119.D
Acq On : 18 Apr 2022 14:30
Operator : SY/MD
Sample : N2419-04DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

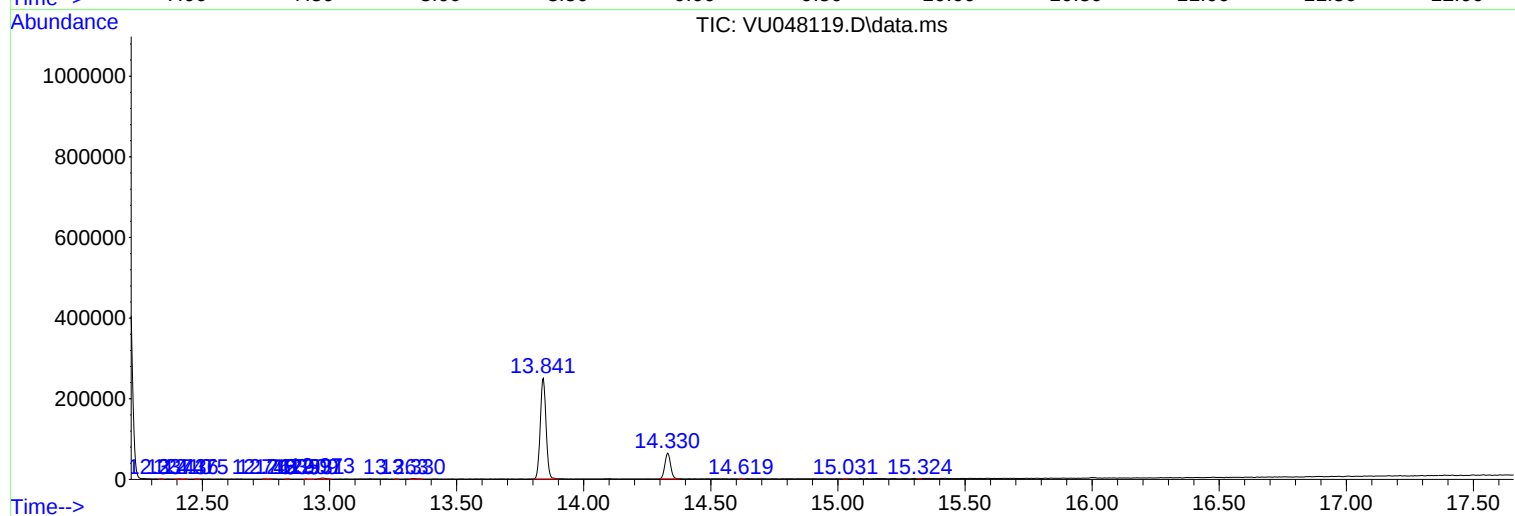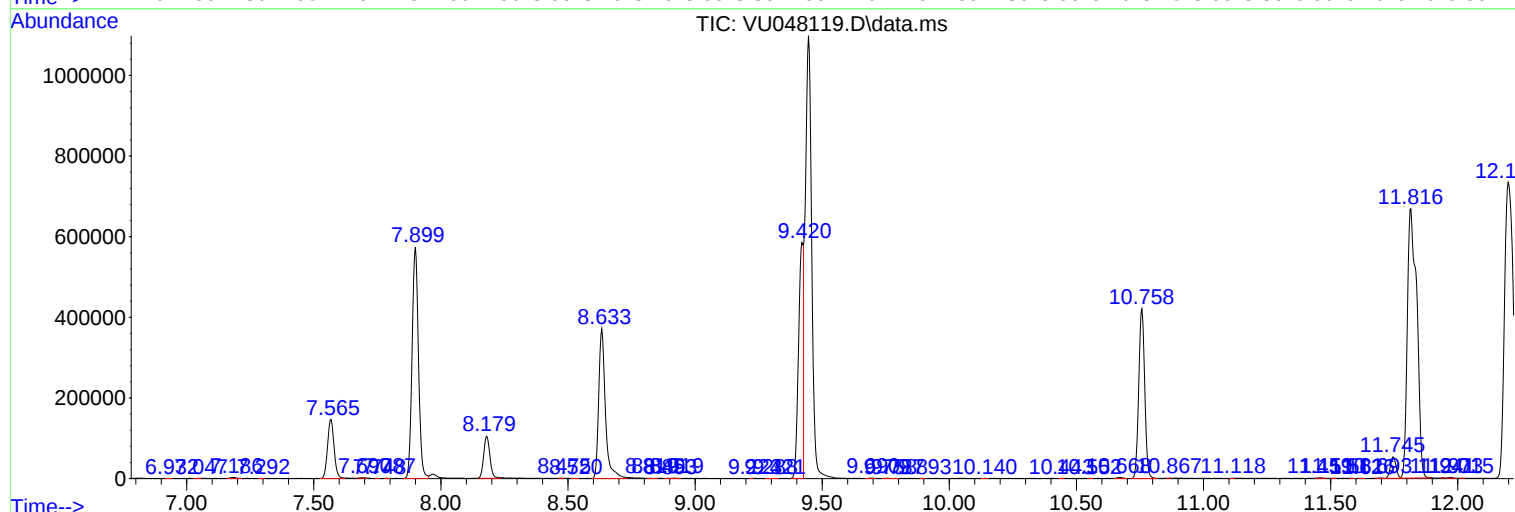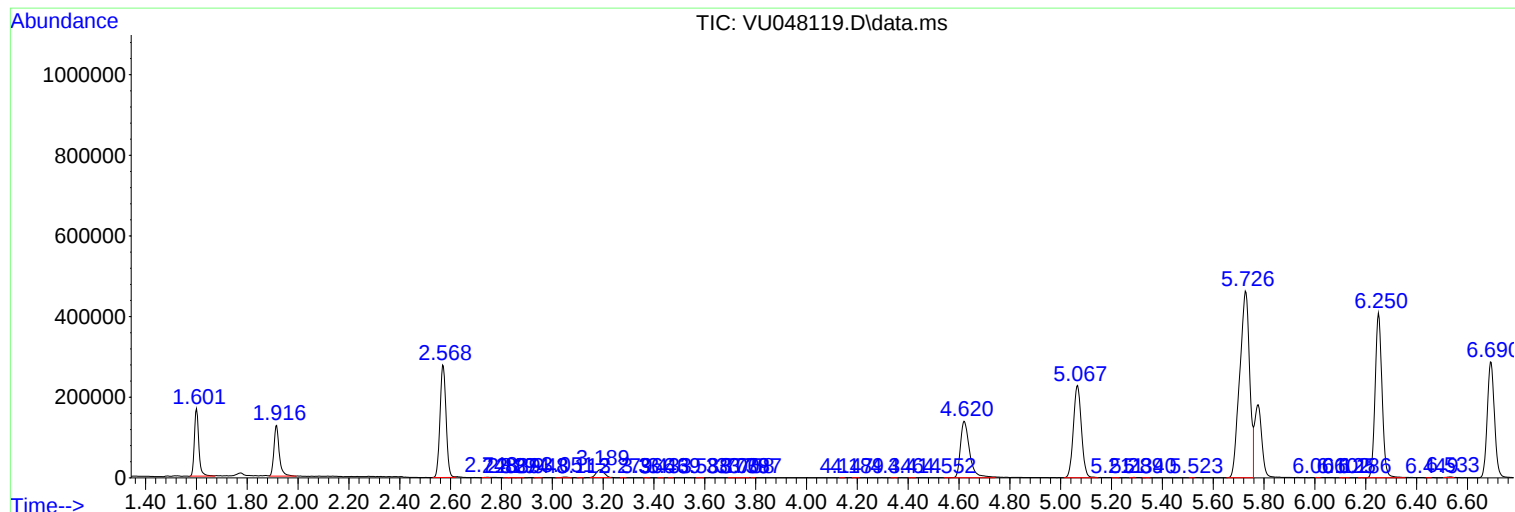

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048119.D
Acq On : 18 Apr 2022 14:30
Operator : SY/MD
Sample : N2419-04DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048119.D
Acq On : 18 Apr 2022 14:30
Operator : SY/MD
Sample : N2419-04DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J47DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc