

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048121.D
 Acq On : 18 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2419-06DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J53DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048121.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	98	rBV	163177	194978	9.87%	1.630%
2	1.912	170	178	200	rVB	120659	170975	8.65%	1.429%
3	2.568	369	382	397	rBV	273135	446532	22.60%	3.733%
4	2.842	462	467	471	rVB3	642	562	0.03%	0.005%
5	2.864	471	474	476	rBV3	308	204	0.01%	0.002%
6	2.922	488	492	495	rVB3	364	310	0.02%	0.003%
7	3.015	517	521	525	rBV2	373	350	0.02%	0.003%
8	3.054	525	533	544	rVB5	1909	3236	0.16%	0.027%
9	3.192	561	576	591	rVB	8130	19108	0.97%	0.160%
10	3.253	592	595	598	rVB	252	193	0.01%	0.002%
11	3.276	598	602	604	rBV2	252	210	0.01%	0.002%
12	3.459	655	659	663	rBV2	492	532	0.03%	0.004%
13	3.556	686	689	693	rVB2	357	251	0.01%	0.002%
14	3.584	693	698	700	rBV2	299	320	0.02%	0.003%
15	3.697	730	733	735	rVV2	330	242	0.01%	0.002%
16	3.745	739	748	750	rBV	301	340	0.02%	0.003%
17	3.787	756	761	763	rBV	270	256	0.01%	0.002%
18	4.006	821	829	832	rBV2	315	329	0.02%	0.003%
19	4.038	835	839	841	rBV2	249	193	0.01%	0.002%
20	4.118	859	864	865	rBV2	293	234	0.01%	0.002%
21	4.176	879	882	886	rBV2	209	186	0.01%	0.002%
22	4.195	886	888	894	rVB	314	261	0.01%	0.002%
23	4.228	894	898	901	rBV2	329	260	0.01%	0.002%
24	4.308	917	923	928	rVB3	364	436	0.02%	0.004%
25	4.340	928	933	936	rBV2	378	451	0.02%	0.004%
26	4.382	943	946	950	rVB2	253	210	0.01%	0.002%
27	4.437	960	963	970	rVV	324	385	0.02%	0.003%
28	4.626	1008	1022	1057	rBV2	128250	329175	16.66%	2.752%
29	4.871	1095	1098	1104	rVV4	380	347	0.02%	0.003%
30	4.906	1108	1109	1111	rVB	481	184	0.01%	0.002%
31	5.067	1141	1159	1183	rBV	225906	498832	25.25%	4.170%
32	5.253	1215	1217	1223	rVB2	276	216	0.01%	0.002%
33	5.292	1223	1229	1231	rBV3	524	634	0.03%	0.005%
34	5.337	1241	1243	1247	rVB2	360	223	0.01%	0.002%
35	5.398	1259	1262	1266	rBV	699	653	0.03%	0.005%
36	5.526	1292	1302	1312	rBV4	1549	2832	0.14%	0.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048121.D
 Acq On : 18 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2419-06DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J53DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.729	1342	1365	1374	rBV2	458665	1249332	63.24%	10.444%
38	6.041	1453	1462	1470	rBV4	654	1106	0.06%	0.009%
39	6.099	1477	1480	1483	rBV2	384	298	0.02%	0.002%
40	6.147	1491	1495	1496	rBV2	337	193	0.01%	0.002%
41	6.182	1503	1506	1508	rBV2	306	248	0.01%	0.002%
42	6.250	1513	1527	1549	rBV	413477	783685	39.67%	6.552%
43	6.523	1604	1612	1614	rBV3	1767	1850	0.09%	0.015%
44	6.694	1650	1665	1686	rBV	279383	549597	27.82%	4.595%
45	6.803	1695	1699	1700	rBV2	465	371	0.02%	0.003%
46	6.887	1722	1725	1728	rBV	376	266	0.01%	0.002%
47	7.054	1769	1777	1783	rBV2	469	754	0.04%	0.006%
48	7.189	1810	1819	1832	rVB5	2195	4324	0.22%	0.036%
49	7.243	1833	1836	1842	rVB	207	180	0.01%	0.002%
50	7.424	1889	1892	1895	rVV	271	199	0.01%	0.002%
51	7.443	1895	1898	1904	rVB3	256	273	0.01%	0.002%
52	7.568	1924	1937	1958	rBV	144155	252923	12.80%	2.114%
53	7.687	1970	1974	1978	rVV5	1027	1071	0.05%	0.009%
54	7.790	2003	2006	2013	rVB3	947	988	0.05%	0.008%
55	7.832	2013	2019	2021	rBV	238	237	0.01%	0.002%
56	7.899	2026	2040	2056	rBV	555890	965008	48.85%	8.067%
57	8.179	2115	2127	2147	rBV	101592	173716	8.79%	1.452%
58	8.533	2235	2237	2244	rVB	443	346	0.02%	0.003%
59	8.632	2255	2268	2304	rBV	360000	662206	33.52%	5.536%
60	8.867	2338	2341	2345	rVB2	586	406	0.02%	0.003%
61	8.912	2345	2355	2356	rBV3	749	962	0.05%	0.008%
62	8.977	2372	2375	2378	rBV2	237	193	0.01%	0.002%
63	9.231	2452	2454	2457	rBV	304	186	0.01%	0.002%
64	9.420	2499	2513	2514	rBV	656766	790070	39.99%	6.605%
65	9.649	2582	2584	2588	rVV3	333	248	0.01%	0.002%
66	9.697	2595	2599	2606	rVB3	746	912	0.05%	0.008%
67	10.118	2725	2730	2735	rBV	305	350	0.02%	0.003%
68	10.195	2752	2754	2758	rVB3	230	184	0.01%	0.002%
69	10.224	2759	2763	2764	rBV3	311	186	0.01%	0.002%
70	10.298	2783	2786	2791	rVB2	220	185	0.01%	0.002%
71	10.607	2878	2882	2884	rBV2	246	214	0.01%	0.002%
72	10.636	2884	2891	2895	rVB2	768	920	0.05%	0.008%
73	10.671	2895	2902	2911	rVB4	3055	4071	0.21%	0.034%
74	10.713	2911	2915	2916	rBV2	368	257	0.01%	0.002%
75	10.758	2916	2929	2949	rVB	412700	670814	33.96%	5.608%
76	10.867	2958	2963	2967	rBV3	622	676	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048121.D
 Acq On : 18 Apr 2022 15:15
 Operator : SY/MD
 Sample : N2419-06DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J53DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.890	2967	2970	2971	rBV3	390	204	0.01%	0.002%
78	10.925	2978	2981	2987	rVB2	380	389	0.02%	0.003%
79	11.031	3011	3014	3018	rVB3	390	246	0.01%	0.002%
80	11.086	3026	3031	3036	rVV2	293	302	0.02%	0.003%
81	11.115	3036	3040	3047	rVB2	600	630	0.03%	0.005%
82	11.298	3091	3097	3100	rBV2	262	303	0.02%	0.003%
83	11.311	3100	3101	3108	rVB	322	234	0.01%	0.002%
84	11.462	3140	3148	3158	rBV6	1427	2936	0.15%	0.025%
85	11.578	3180	3184	3189	rVB3	599	514	0.03%	0.004%
86	11.610	3190	3194	3198	rBV3	339	348	0.02%	0.003%
87	11.700	3215	3222	3226	rVB3	905	1064	0.05%	0.009%
88	11.745	3226	3236	3245	rBV	49498	76025	3.85%	0.636%
89	11.812	3245	3257	3281	rVB2	700807	1851890	93.74%	15.482%
90	11.941	3294	3297	3302	rBV5	701	683	0.03%	0.006%
91	12.079	3338	3340	3343	rVB2	443	232	0.01%	0.002%
92	12.205	3362	3379	3399	rBV2	808078	1975467	100.00%	16.515%
93	12.517	3470	3476	3481	rBV2	490	701	0.04%	0.006%
94	12.690	3524	3530	3532	rBV4	411	445	0.02%	0.004%
95	12.980	3616	3620	3629	rVB3	1153	1182	0.06%	0.010%
96	13.256	3702	3706	3709	rBV2	404	382	0.02%	0.003%
97	13.841	3877	3888	3901	rBV	127370	203507	10.30%	1.701%
98	14.079	3955	3962	3964	rBV4	532	659	0.03%	0.006%
99	14.211	3999	4003	4004	rBV2	419	315	0.02%	0.003%
100	14.330	4029	4040	4052	rBV	30366	48462	2.45%	0.405%




Sum of corrected areas: 11961765

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048121.D
Acq On : 18 Apr 2022 15:15
Operator : SY/MD
Sample : N2419-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J53DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

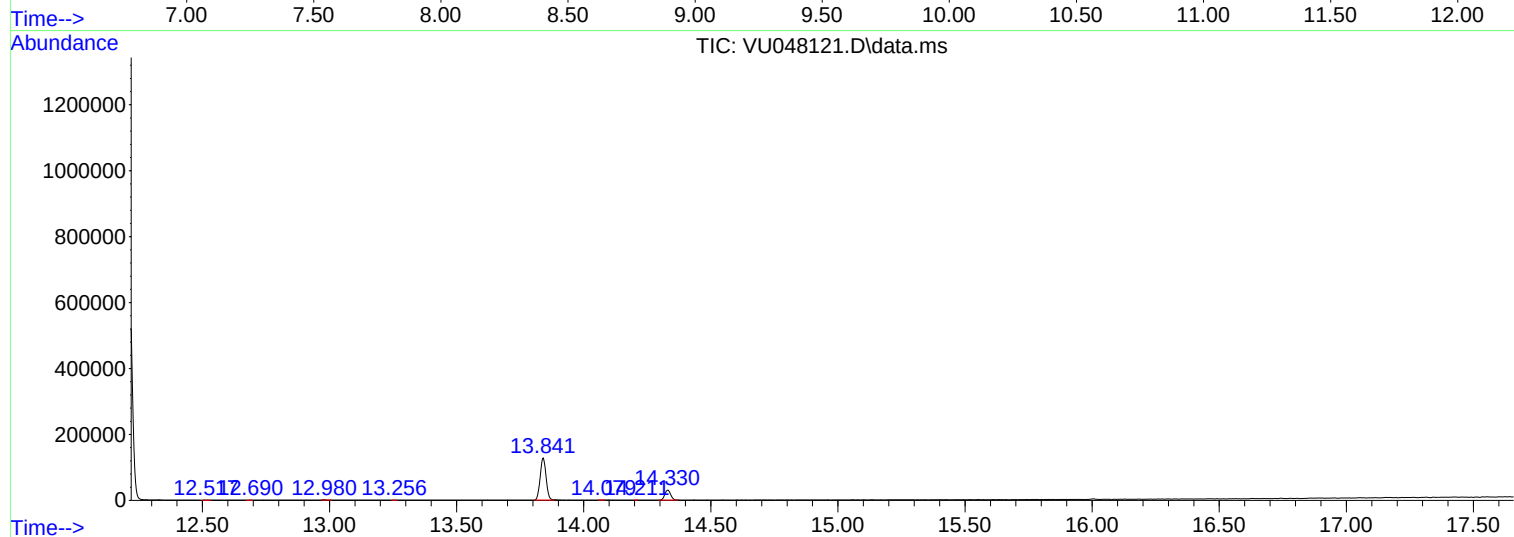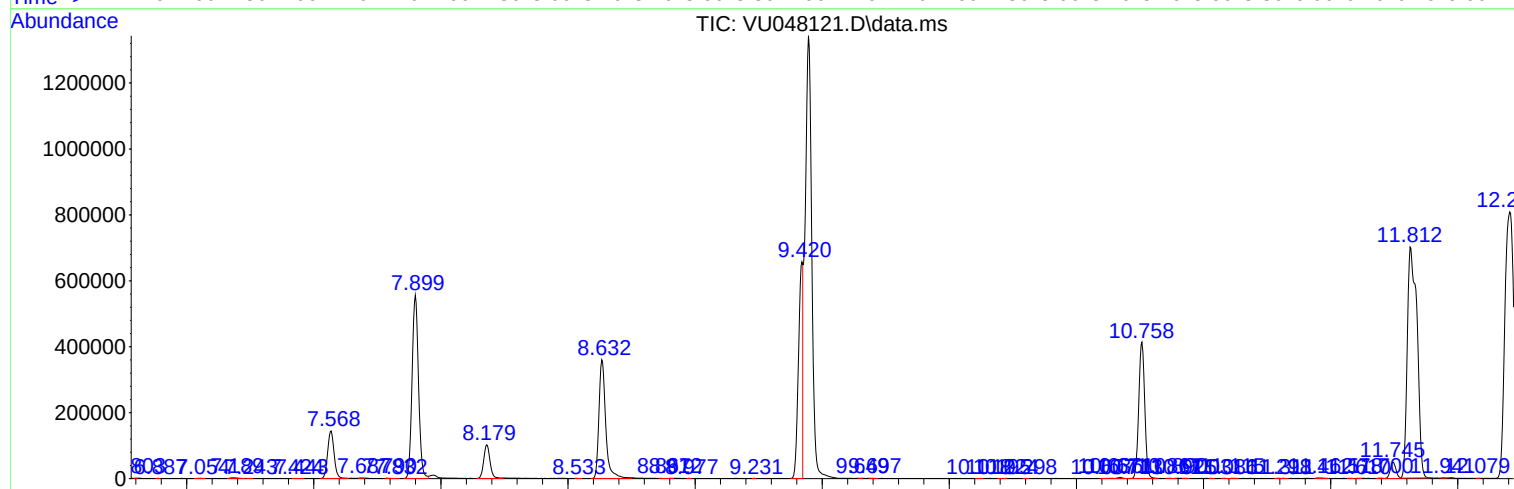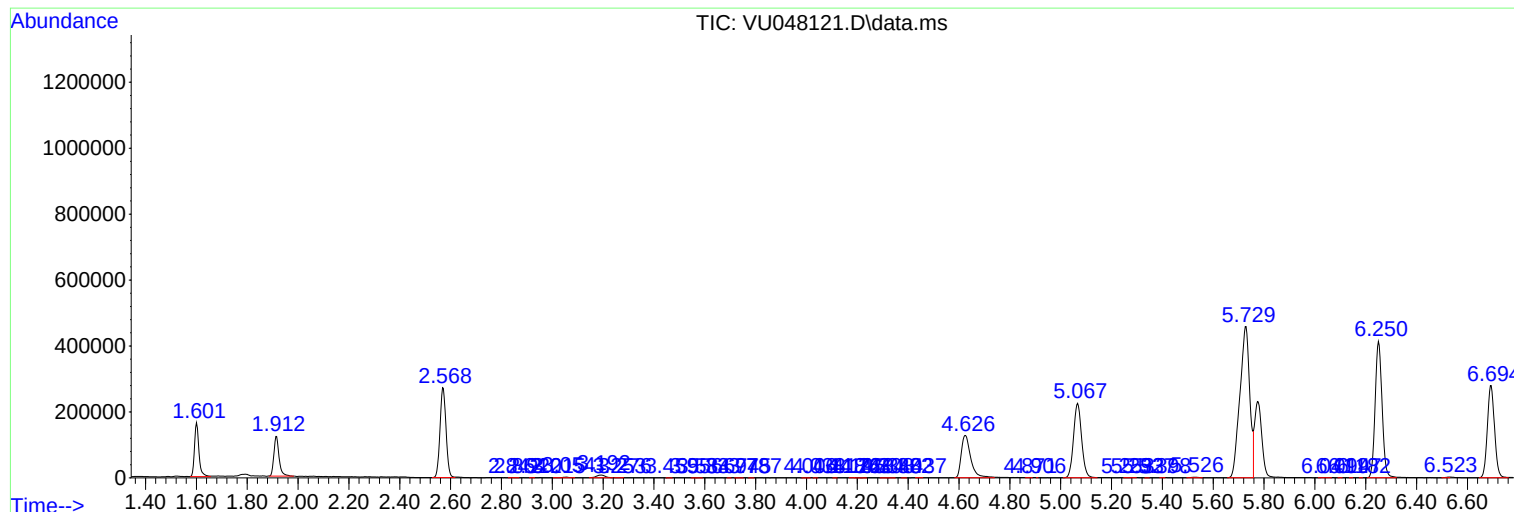

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048121.D
Acq On : 18 Apr 2022 15:15
Operator : SY/MD
Sample : N2419-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J53DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048121.D
Acq On : 18 Apr 2022 15:15
Operator : SY/MD
Sample : N2419-06DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J53DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------