

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048122.D
 Acq On : 18 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2419-07DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J54DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048122.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	101	rBV	164382	193873	8.69%	1.475%
2	1.916	171	179	197	rVB	127112	177753	7.97%	1.352%
3	2.494	355	359	362	rBV2	488	430	0.02%	0.003%
4	2.568	370	382	399	rBV	266370	446727	20.02%	3.398%
5	2.687	417	419	421	rBV2	404	210	0.01%	0.002%
6	2.777	444	447	449	rBV	363	238	0.01%	0.002%
7	2.793	449	452	457	rVB4	400	341	0.02%	0.003%
8	2.822	457	461	464	rBV3	350	293	0.01%	0.002%
9	2.851	465	470	472	rVB2	362	247	0.01%	0.002%
10	2.867	472	475	480	rBV3	383	290	0.01%	0.002%
11	2.932	492	495	499	rBV	228	221	0.01%	0.002%
12	3.051	524	532	543	rVB6	1515	3077	0.14%	0.023%
13	3.125	551	555	557	rBV	268	221	0.01%	0.002%
14	3.186	561	574	590	rBV	8480	17631	0.79%	0.134%
15	3.314	611	614	623	rVB2	389	491	0.02%	0.004%
16	3.510	671	675	678	rBV2	487	275	0.01%	0.002%
17	3.645	714	717	723	rVB3	283	232	0.01%	0.002%
18	3.700	729	734	742	rBV2	465	685	0.03%	0.005%
19	3.742	742	747	748	rBV	298	251	0.01%	0.002%
20	3.777	756	758	764	rBV	205	203	0.01%	0.002%
21	4.112	860	862	866	rBV3	349	318	0.01%	0.002%
22	4.154	870	875	876	rBV	337	207	0.01%	0.002%
23	4.346	931	935	939	rVB2	327	267	0.01%	0.002%
24	4.408	951	954	959	rBV2	211	190	0.01%	0.001%
25	4.559	997	1001	1003	rBV2	307	209	0.01%	0.002%
26	4.633	1008	1024	1052	rBV2	133042	361547	16.20%	2.750%
27	5.002	1135	1139	1142	rBV4	354	332	0.01%	0.003%
28	5.067	1142	1159	1187	rVV	225756	493552	22.12%	3.754%
29	5.186	1192	1196	1200	rVB3	272	264	0.01%	0.002%
30	5.285	1223	1227	1228	rBV2	361	284	0.01%	0.002%
31	5.571	1312	1316	1320	rBV	297	292	0.01%	0.002%
32	5.729	1341	1365	1371	rBV2	461439	1210145	54.23%	9.204%
33	5.777	1372	1380	1413	rVB	1125276	2231676	100.00%	16.974%
34	6.173	1501	1503	1507	rVB	357	199	0.01%	0.002%
35	6.250	1513	1527	1556	rBV	430390	821629	36.82%	6.249%
36	6.526	1606	1613	1626	rVB7	1938	3813	0.17%	0.029%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048122.D
 Acq On : 18 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2419-07DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J54DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	6.600	1631	1636	1641	rVB3	356	399	0.02%	0.003%
38	6.694	1647	1665	1688	rBV	281834	554670	24.85%	4.219%
39	7.131	1796	1801	1804	rBV3	266	254	0.01%	0.002%
40	7.186	1810	1818	1836	rVB5	2531	4647	0.21%	0.035%
41	7.301	1851	1854	1860	rBV2	265	247	0.01%	0.002%
42	7.350	1866	1869	1873	rBV2	305	248	0.01%	0.002%
43	7.472	1901	1907	1913	rBV2	196	255	0.01%	0.002%
44	7.568	1921	1937	1957	rBV	144259	254605	11.41%	1.937%
45	7.661	1963	1966	1969	rBV3	400	279	0.01%	0.002%
46	7.687	1969	1974	1983	rVB5	1473	2176	0.10%	0.017%
47	7.739	1988	1990	1996	rBV3	358	240	0.01%	0.002%
48	7.793	2001	2007	2010	rBV4	858	919	0.04%	0.007%
49	7.845	2020	2023	2026	rBV4	384	256	0.01%	0.002%
50	7.899	2026	2040	2055	rBV	557338	961173	43.07%	7.311%
51	8.179	2116	2127	2148	rVV	99400	174977	7.84%	1.331%
52	8.501	2224	2227	2231	rBV3	282	213	0.01%	0.002%
53	8.636	2256	2269	2303	rBV	381193	716689	32.11%	5.451%
54	8.816	2322	2325	2331	rBV4	282	348	0.02%	0.003%
55	8.919	2348	2357	2366	rBV6	1546	2590	0.12%	0.020%
56	8.996	2377	2381	2385	rBV3	321	260	0.01%	0.002%
57	9.285	2466	2471	2475	rBV3	282	287	0.01%	0.002%
58	9.420	2499	2513	2515	rBV	666020	921906	41.31%	7.012%
59	9.607	2567	2571	2575	rVB3	409	367	0.02%	0.003%
60	9.645	2575	2583	2591	rBV5	730	1257	0.06%	0.010%
61	9.697	2594	2599	2606	rVV4	800	1019	0.05%	0.008%
62	9.732	2607	2610	2615	rVB2	496	328	0.01%	0.002%
63	9.761	2615	2619	2622	rBV2	260	207	0.01%	0.002%
64	9.796	2626	2630	2635	rBV2	247	242	0.01%	0.002%
65	10.034	2701	2704	2706	rVB2	489	259	0.01%	0.002%
66	10.073	2711	2716	2718	rBV2	235	245	0.01%	0.002%
67	10.169	2743	2746	2749	rVB	415	239	0.01%	0.002%
68	10.324	2792	2794	2799	rVB2	265	218	0.01%	0.002%
69	10.510	2850	2852	2859	rVB	361	326	0.01%	0.002%
70	10.549	2859	2864	2868	rBV2	432	427	0.02%	0.003%
71	10.671	2895	2902	2912	rVB4	2479	3864	0.17%	0.029%
72	10.758	2915	2929	2948	rBV	419472	683639	30.63%	5.200%
73	10.864	2959	2962	2965	rVB3	402	310	0.01%	0.002%
74	11.118	3038	3041	3044	rVB4	390	235	0.01%	0.002%
75	11.185	3058	3062	3065	rVB	400	260	0.01%	0.002%
76	11.201	3065	3067	3070	rBV2	351	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048122.D
 Acq On : 18 Apr 2022 15:38
 Operator : SY/MD
 Sample : N2419-07DL 400X
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0J54DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.224	3070	3074	3075	rBV	246	188	0.01%	0.001%
78	11.430	3132	3138	3139	rBV	405	323	0.01%	0.002%
79	11.459	3142	3147	3150	rBV3	1029	969	0.04%	0.007%
80	11.574	3181	3183	3188	rVB2	313	207	0.01%	0.002%
81	11.700	3217	3222	3228	rVB3	970	1006	0.05%	0.008%
82	11.748	3228	3237	3244	rBV3	9538	14615	0.65%	0.111%
83	11.812	3244	3257	3284	rVV2	685936	1540501	69.03%	11.717%
84	11.941	3293	3297	3299	rBV3	692	510	0.02%	0.004%
85	12.031	3324	3325	3329	rVB	428	251	0.01%	0.002%
86	12.195	3358	3376	3396	rBV2	621317	1285494	57.60%	9.777%
87	12.330	3414	3418	3420	rBV3	368	246	0.01%	0.002%
88	12.394	3435	3438	3443	rBV4	394	377	0.02%	0.003%
89	12.989	3619	3623	3627	rBV2	489	517	0.02%	0.004%
90	13.053	3635	3643	3645	rBV3	511	682	0.03%	0.005%
91	13.214	3691	3693	3700	rVB4	535	534	0.02%	0.004%
92	13.275	3707	3712	3716	rBV2	380	423	0.02%	0.003%
93	13.385	3742	3746	3749	rBV2	393	330	0.01%	0.003%
94	13.844	3879	3889	3901	rBV	20151	32617	1.46%	0.248%
95	14.066	3954	3958	3960	rBV2	428	354	0.02%	0.003%
96	14.333	4033	4041	4050	rVB5	4029	6293	0.28%	0.048%
97	14.372	4050	4053	4057	rBV2	306	265	0.01%	0.002%
98	14.488	4087	4089	4092	rBV2	348	203	0.01%	0.002%
99	14.568	4111	4114	4117	rBV2	555	486	0.02%	0.004%
100	14.941	4226	4230	4232	rBV2	472	353	0.02%	0.003%




Sum of corrected areas: 13147659

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048122.D
Acq On : 18 Apr 2022 15:38
Operator : SY/MD
Sample : N2419-07DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J54DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

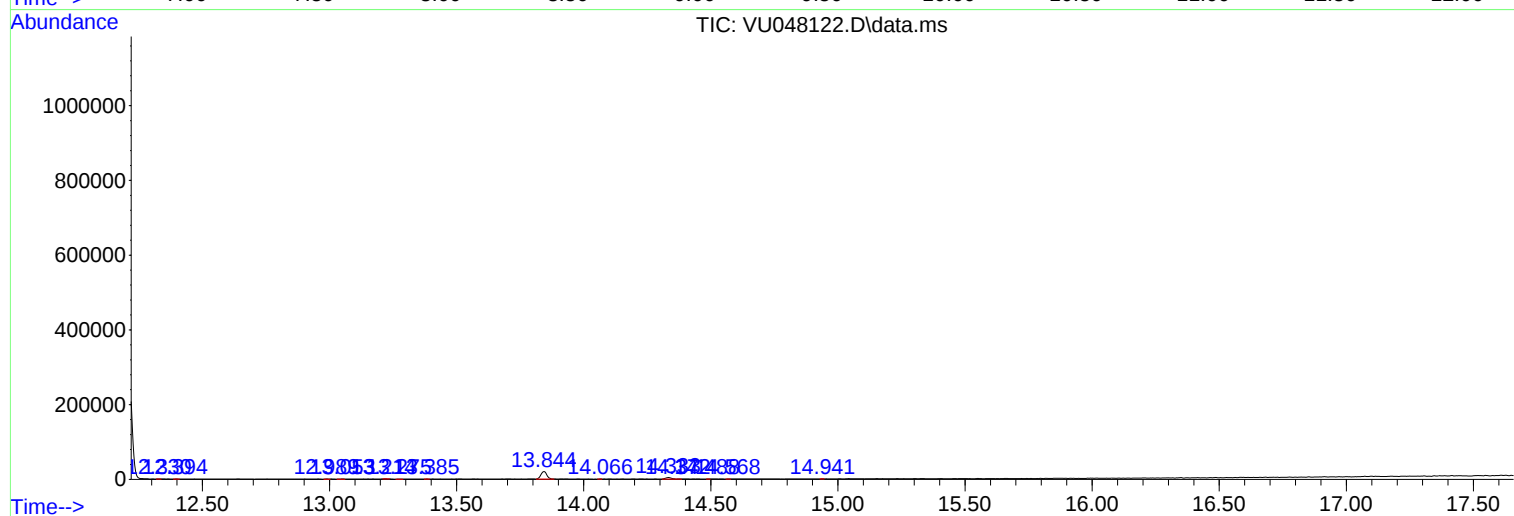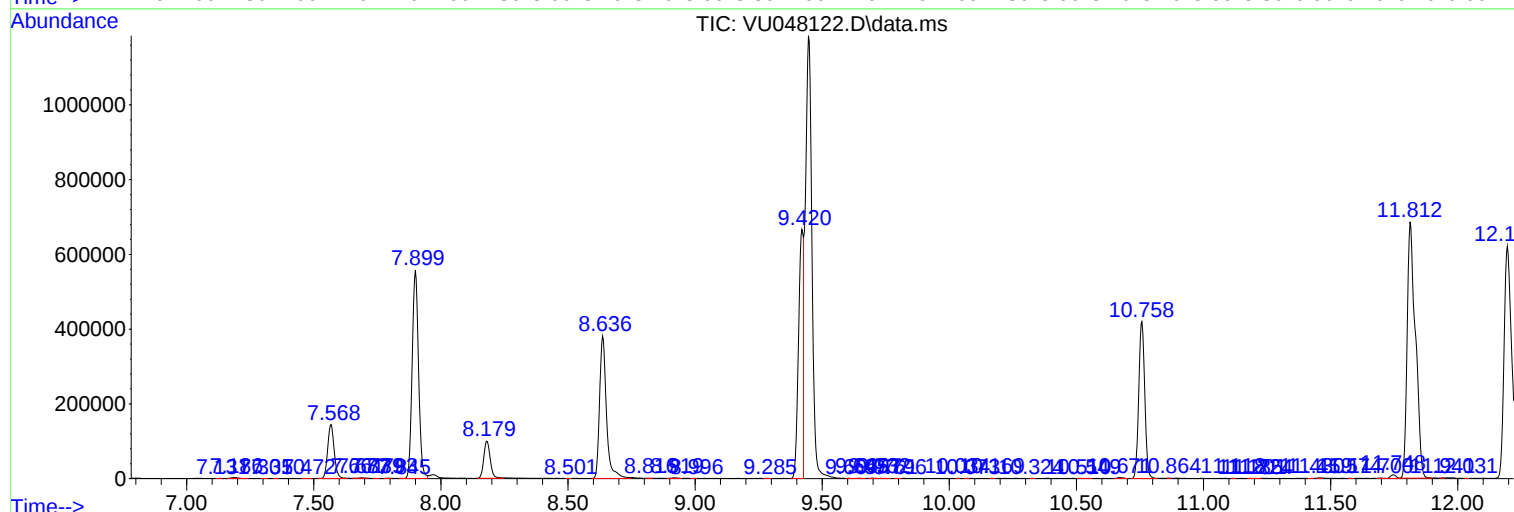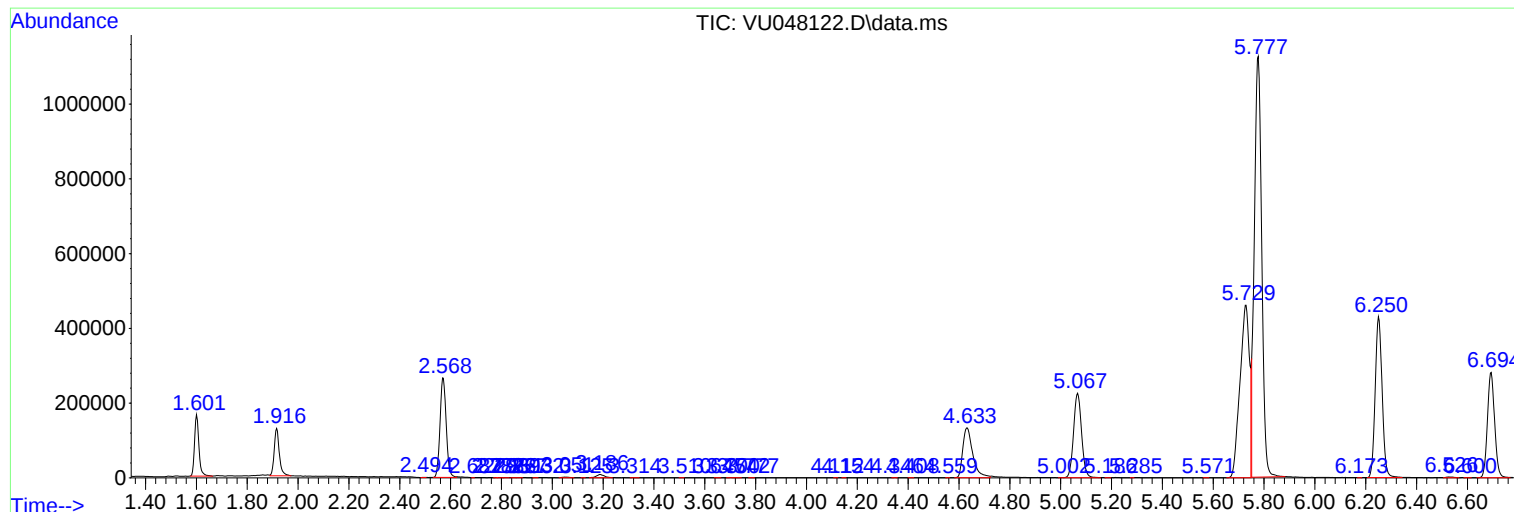

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048122.D
Acq On : 18 Apr 2022 15:38
Operator : SY/MD
Sample : N2419-07DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J54DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048122.D
Acq On : 18 Apr 2022 15:38
Operator : SY/MD
Sample : N2419-07DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0J54DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------