

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048124.D
 Acq On : 18 Apr 2022 16:24
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M

Title : VOC Analysis

Signal : TIC: VU048124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	73	81	98	rBV	149749	179114	16.35%	1.970%
2	1.916	171	179	198	rVB	112898	154561	14.11%	1.700%
3	2.504	358	362	363	rBV	335	218	0.02%	0.002%
4	2.571	368	383	397	rBV	213615	353744	32.28%	3.891%
5	2.697	419	422	426	rVB3	533	440	0.04%	0.005%
6	2.732	430	433	435	rBV2	357	260	0.02%	0.003%
7	2.797	445	453	463	rVB4	1243	2126	0.19%	0.023%
8	2.842	463	467	473	rVB4	466	615	0.06%	0.007%
9	2.893	473	483	485	rBV3	404	475	0.04%	0.005%
10	2.980	508	510	514	rVB2	353	213	0.02%	0.002%
11	3.047	523	531	539	rBV4	911	1393	0.13%	0.015%
12	3.189	560	575	591	rVV	4424	10020	0.91%	0.110%
13	3.289	603	606	611	rBV	342	345	0.03%	0.004%
14	3.359	625	628	629	rBV2	364	209	0.02%	0.002%
15	3.523	676	679	683	rVB2	264	199	0.02%	0.002%
16	3.562	683	691	693	rBV	316	286	0.03%	0.003%
17	3.578	693	696	698	rBV	397	212	0.02%	0.002%
18	3.758	748	752	757	rVB3	322	301	0.03%	0.003%
19	3.787	757	761	764	rVB2	360	232	0.02%	0.003%
20	3.809	764	768	771	rBV2	279	257	0.02%	0.003%
21	3.906	795	798	801	rVB2	420	289	0.03%	0.003%
22	3.941	806	809	811	rVV2	234	197	0.02%	0.002%
23	3.957	811	814	819	rVB2	349	295	0.03%	0.003%
24	4.006	826	829	838	rVB3	385	557	0.05%	0.006%
25	4.096	854	857	860	rBV	271	197	0.02%	0.002%
26	4.157	871	876	879	rBV	325	239	0.02%	0.003%
27	4.221	893	896	904	rVV2	296	352	0.03%	0.004%
28	4.295	915	919	922	rBV2	227	250	0.02%	0.003%
29	4.375	940	944	947	rVV2	251	203	0.02%	0.002%
30	4.452	965	968	972	rBV2	371	322	0.03%	0.004%
31	4.488	976	979	983	rVB2	323	201	0.02%	0.002%
32	4.510	983	986	988	rBV2	313	180	0.02%	0.002%
33	4.626	1008	1022	1056	rBV	117382	295827	27.00%	3.254%
34	5.067	1143	1159	1183	rBV	199818	438923	40.06%	4.827%
35	5.288	1221	1228	1239	rBV4	1163	2024	0.18%	0.022%
36	5.382	1253	1257	1263	rVB2	229	235	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048124.D
 Acq On : 18 Apr 2022 16:24
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	5.726	1342	1364	1392	rBV2	404580	1095717	100.00%	12.051%
38	5.896	1414	1417	1423	rVB3	404	447	0.04%	0.005%
39	5.980	1437	1443	1448	rVB2	497	512	0.05%	0.006%
40	6.134	1487	1491	1492	rBV3	317	189	0.02%	0.002%
41	6.147	1492	1495	1502	rVB4	863	804	0.07%	0.009%
42	6.250	1512	1527	1561	rBV	278516	534132	48.75%	5.875%
43	6.417	1576	1579	1583	rVB2	348	221	0.02%	0.002%
44	6.443	1583	1587	1591	rBV4	308	311	0.03%	0.003%
45	6.530	1607	1614	1622	rBV5	1458	2467	0.23%	0.027%
46	6.620	1636	1642	1646	rBV2	165	233	0.02%	0.003%
47	6.694	1650	1665	1687	rBV	251331	492731	44.97%	5.419%
48	6.812	1698	1702	1711	rVB5	845	1003	0.09%	0.011%
49	6.883	1721	1724	1734	rVV4	926	1085	0.10%	0.012%
50	7.047	1773	1775	1782	rVB2	483	459	0.04%	0.005%
51	7.189	1810	1819	1824	rBV6	2045	3273	0.30%	0.036%
52	7.337	1858	1865	1869	rVB3	476	683	0.06%	0.008%
53	7.359	1869	1872	1875	rBV2	224	186	0.02%	0.002%
54	7.430	1889	1894	1897	rBV2	179	217	0.02%	0.002%
55	7.565	1924	1936	1959	rBV	125964	226115	20.64%	2.487%
56	7.687	1970	1974	1981	rVB4	1404	1331	0.12%	0.015%
57	7.899	2023	2040	2056	rBV	484158	840972	76.75%	9.249%
58	8.079	2093	2096	2103	rVB2	672	564	0.05%	0.006%
59	8.179	2116	2127	2145	rVV	88326	153720	14.03%	1.691%
60	8.320	2168	2171	2174	rVB4	378	242	0.02%	0.003%
61	8.349	2177	2180	2184	rVB4	559	394	0.04%	0.004%
62	8.504	2226	2228	2236	rVB2	216	185	0.02%	0.002%
63	8.632	2256	2268	2303	rBV	331187	619848	56.57%	6.817%
64	8.787	2308	2316	2331	rVB2	17835	30031	2.74%	0.330%
65	9.166	2430	2434	2437	rVB2	351	328	0.03%	0.004%
66	9.185	2437	2440	2443	rBV2	273	210	0.02%	0.002%
67	9.234	2447	2455	2461	rBV3	453	567	0.05%	0.006%
68	9.288	2468	2472	2475	rVB3	330	295	0.03%	0.003%
69	9.417	2499	2512	2551	rBV2	417235	988823	90.24%	10.875%
70	9.574	2558	2561	2564	rVB2	431	260	0.02%	0.003%
71	9.600	2567	2569	2574	rVB2	273	185	0.02%	0.002%
72	9.690	2591	2597	2607	rBV3	777	1171	0.11%	0.013%
73	10.025	2699	2701	2705	rVB	303	217	0.02%	0.002%
74	10.050	2705	2709	2715	rBV2	318	369	0.03%	0.004%
75	10.099	2722	2724	2730	rVB3	285	210	0.02%	0.002%
76	10.349	2795	2802	2805	rBV2	491	635	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048124.D
 Acq On : 18 Apr 2022 16:24
 Operator : SY/MD
 Sample : N2386-06
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	10.674	2895	2903	2910	rVB4	2209	3077	0.28%	0.034%
78	10.758	2915	2929	2948	rVV	379772	612782	55.93%	6.740%
79	10.861	2955	2961	2965	rBV3	710	760	0.07%	0.008%
80	10.896	2967	2972	2978	rVB2	1366	1479	0.13%	0.016%
81	11.025	3010	3012	3020	rVV4	259	269	0.02%	0.003%
82	11.070	3024	3026	3029	rVB	392	193	0.02%	0.002%
83	11.327	3100	3106	3110	rBV2	478	506	0.05%	0.006%
84	11.414	3130	3133	3139	rVB2	366	301	0.03%	0.003%
85	11.455	3139	3146	3154	rBV4	1116	1929	0.18%	0.021%
86	11.578	3181	3184	3186	rBV2	366	260	0.02%	0.003%
87	11.639	3198	3203	3211	rBV3	340	518	0.05%	0.006%
88	11.693	3215	3220	3226	rBV3	986	1066	0.10%	0.012%
89	11.745	3226	3236	3246	rBV	41910	67012	6.12%	0.737%
90	11.812	3246	3257	3279	rVB2	443807	985462	89.94%	10.838%
91	11.941	3294	3297	3298	rBV3	417	253	0.02%	0.003%
92	11.970	3302	3306	3307	rBV2	998	631	0.06%	0.007%
93	12.063	3326	3335	3349	rBV3	11209	20924	1.91%	0.230%
94	12.195	3361	3376	3397	rBV2	507832	941165	85.89%	10.351%
95	12.327	3413	3417	3418	rBV2	424	286	0.03%	0.003%
96	12.423	3442	3447	3450	rBV3	427	425	0.04%	0.005%
97	12.629	3508	3511	3513	rBV	269	230	0.02%	0.003%
98	12.918	3597	3601	3605	rBV3	268	322	0.03%	0.004%
99	13.217	3691	3694	3696	rBV3	687	444	0.04%	0.005%
100	13.844	3881	3889	3898	rVB4	3362	5208	0.48%	0.057%




Sum of corrected areas: 9092355

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048124.D
Acq On : 18 Apr 2022 16:24
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

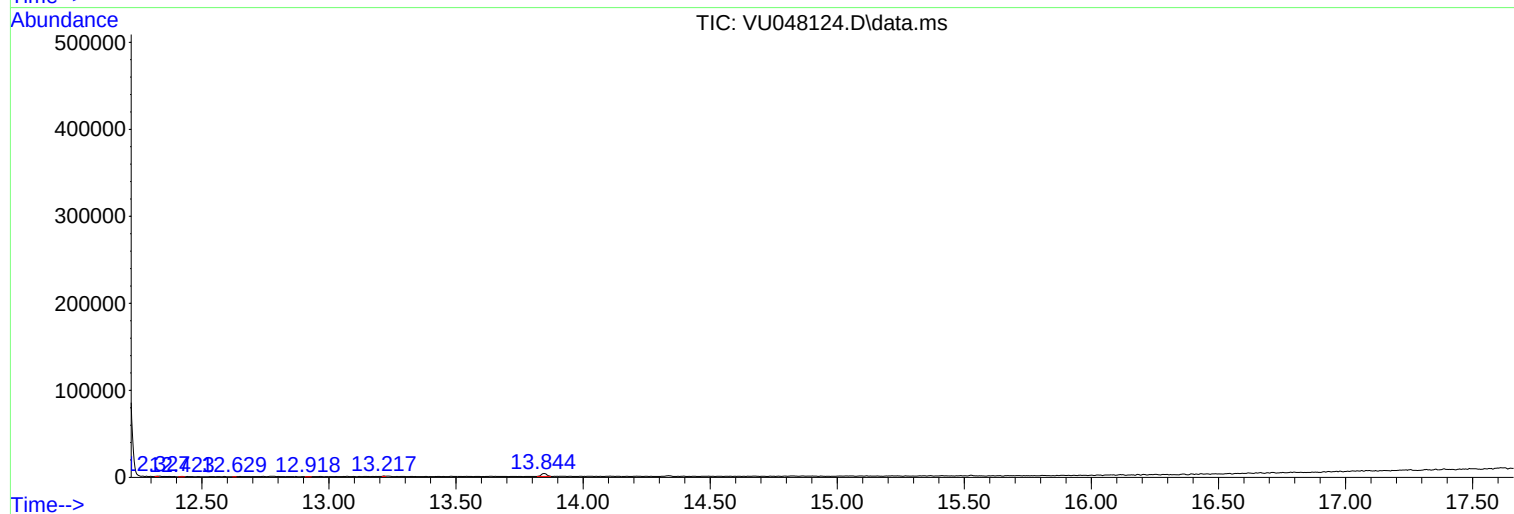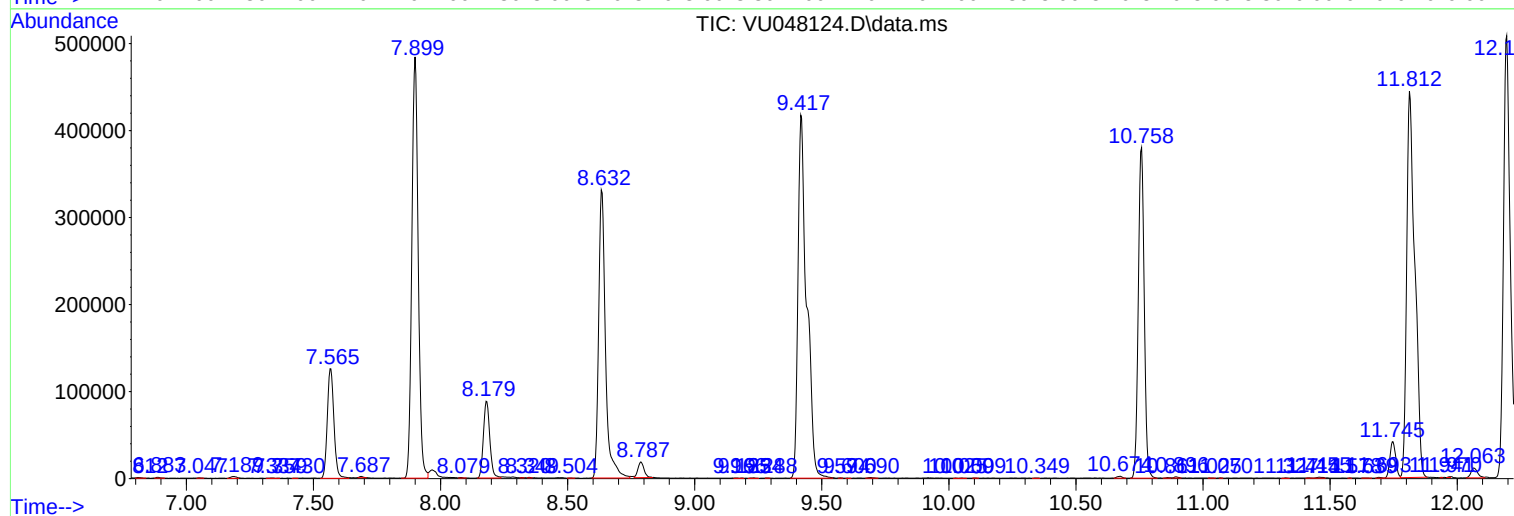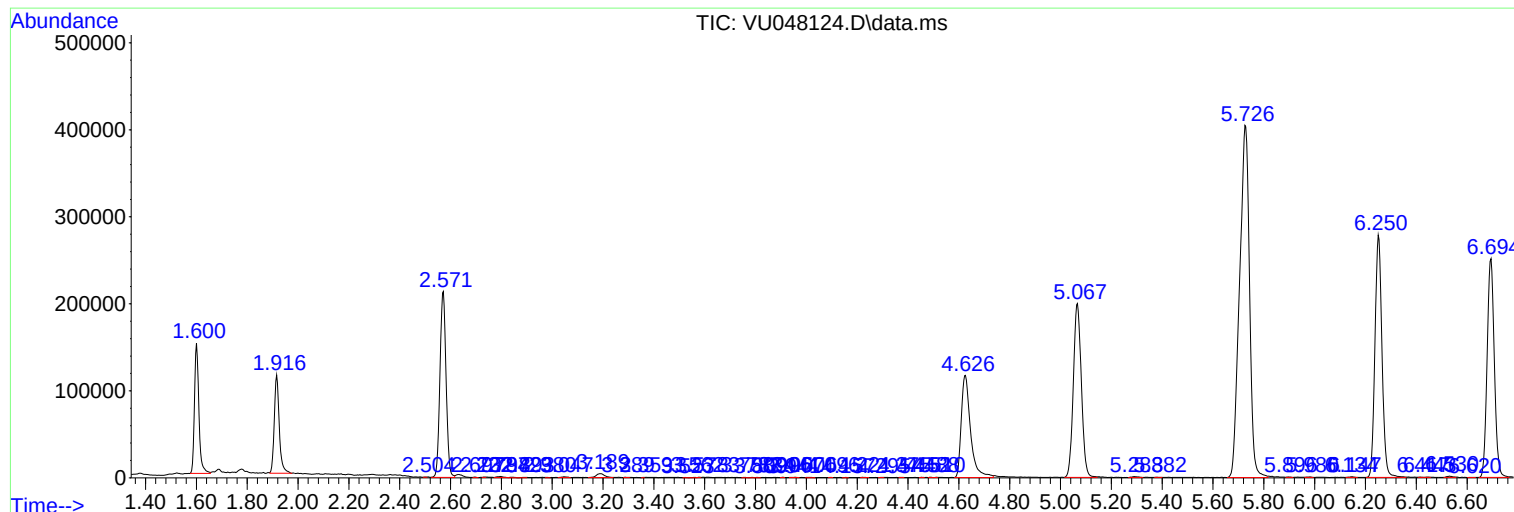

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048124.D
Acq On : 18 Apr 2022 16:24
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048124.D
Acq On : 18 Apr 2022 16:24
Operator : SY/MD
Sample : N2386-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------