

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048125.D
 Acq On : 18 Apr 2022 16:47
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

Signal : TIC: VU048125.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	75	81	95	rBV	167081	216827	16.61%	2.070%
2	1.916	172	179	198	rVB	125915	176563	13.53%	1.686%
3	2.568	368	382	395	rBV	267028	445469	34.13%	4.253%
4	2.790	447	451	464	rVB2	1674	2743	0.21%	0.026%
5	2.838	464	466	472	rBV3	335	303	0.02%	0.003%
6	2.906	483	487	490	rBV3	446	420	0.03%	0.004%
7	3.047	527	531	532	rBV3	798	638	0.05%	0.006%
8	3.192	565	576	587	rBV4	2186	4925	0.38%	0.047%
9	3.832	772	775	779	rVB2	408	278	0.02%	0.003%
10	3.948	808	811	816	rVV3	373	308	0.02%	0.003%
11	3.993	821	825	830	rVB	394	382	0.03%	0.004%
12	4.202	887	890	897	rBV2	254	260	0.02%	0.002%
13	4.401	950	952	959	rVB2	255	228	0.02%	0.002%
14	4.565	1000	1003	1006	rBV2	269	230	0.02%	0.002%
15	4.623	1007	1021	1047	rBV	123990	315574	24.18%	3.013%
16	5.067	1139	1159	1179	rBV2	222637	489176	37.48%	4.671%
17	5.289	1223	1228	1229	rBV2	498	356	0.03%	0.003%
18	5.729	1342	1365	1404	rBV2	450105	1222468	93.66%	11.672%
19	5.880	1409	1412	1415	rBV2	281	209	0.02%	0.002%
20	5.964	1435	1438	1441	rVV3	612	486	0.04%	0.005%
21	5.989	1443	1446	1449	rVB2	483	239	0.02%	0.002%
22	6.096	1477	1479	1482	rBV2	292	205	0.02%	0.002%
23	6.115	1482	1485	1488	rBV3	568	366	0.03%	0.003%
24	6.141	1488	1493	1494	rBV2	311	253	0.02%	0.002%
25	6.250	1510	1527	1556	rBV	399122	762381	58.41%	7.279%
26	6.417	1577	1579	1583	rVB2	452	318	0.02%	0.003%
27	6.530	1607	1614	1625	rVB7	1626	3258	0.25%	0.031%
28	6.578	1625	1629	1633	rBV3	309	271	0.02%	0.003%
29	6.694	1650	1665	1685	rBV	280162	554478	42.48%	5.294%
30	6.806	1697	1700	1703	rBV2	528	434	0.03%	0.004%
31	6.842	1708	1711	1714	rVB3	487	285	0.02%	0.003%
32	6.880	1719	1723	1725	rBV2	624	349	0.03%	0.003%
33	6.967	1747	1750	1757	rVB	299	289	0.02%	0.003%
34	7.041	1768	1773	1774	rBV2	366	264	0.02%	0.003%
35	7.057	1774	1778	1783	rVB3	721	663	0.05%	0.006%
36	7.124	1793	1799	1801	rBV2	234	229	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048125.D
 Acq On : 18 Apr 2022 16:47
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

37	7.182	1810	1817	1828	rBV3	2267	3904	0.30%	0.037%
38	7.250	1833	1838	1844	rVB2	283	238	0.02%	0.002%
39	7.301	1852	1854	1858	rVB2	321	275	0.02%	0.003%
40	7.327	1858	1862	1865	rBV2	342	335	0.03%	0.003%
41	7.488	1909	1912	1916	rBV3	302	284	0.02%	0.003%
42	7.565	1924	1936	1954	rBV	141365	251957	19.30%	2.406%
43	7.687	1972	1974	1980	rVB4	891	743	0.06%	0.007%
44	7.742	1985	1991	1993	rVB2	358	289	0.02%	0.003%
45	7.899	2025	2040	2056	rBV	546427	947976	72.63%	9.051%
46	8.179	2116	2127	2143	rBV	100943	173160	13.27%	1.653%
47	8.472	2216	2218	2227	rVB	922	1183	0.09%	0.011%
48	8.536	2234	2238	2242	rVB3	521	340	0.03%	0.003%
49	8.555	2242	2244	2248	rVB3	365	250	0.02%	0.002%
50	8.578	2248	2251	2252	rBV2	374	223	0.02%	0.002%
51	8.636	2256	2269	2305	rBV	380633	712849	54.61%	6.806%
52	8.790	2310	2317	2328	rVB5	6010	10447	0.80%	0.100%
53	8.954	2364	2368	2373	rVB2	346	310	0.02%	0.003%
54	9.076	2404	2406	2412	rVB2	509	256	0.02%	0.002%
55	9.163	2429	2433	2437	rBV4	356	345	0.03%	0.003%
56	9.227	2448	2453	2457	rBV2	188	216	0.02%	0.002%
57	9.420	2498	2513	2516	rBV	631149	984905	75.46%	9.404%
58	9.645	2580	2583	2584	rBV	482	263	0.02%	0.003%
59	9.684	2592	2595	2596	rVV	550	284	0.02%	0.003%
60	9.697	2596	2599	2604	rVV3	1052	867	0.07%	0.008%
61	9.732	2608	2610	2614	rVV2	285	219	0.02%	0.002%
62	9.880	2652	2656	2658	rBV2	300	263	0.02%	0.003%
63	10.237	2763	2767	2771	rBV3	316	319	0.02%	0.003%
64	10.607	2878	2882	2883	rBV	287	243	0.02%	0.002%
65	10.671	2891	2902	2908	rBV5	2742	3567	0.27%	0.034%
66	10.758	2915	2929	2946	rBV	410016	664075	50.88%	6.340%
67	10.854	2956	2959	2960	rBV	368	212	0.02%	0.002%
68	10.890	2967	2970	2982	rVB5	1387	2001	0.15%	0.019%
69	11.079	3026	3029	3033	rBV	341	205	0.02%	0.002%
70	11.105	3034	3037	3039	rVV	361	252	0.02%	0.002%
71	11.234	3072	3077	3083	rBV2	281	300	0.02%	0.003%
72	11.462	3139	3148	3157	rVV4	1752	2906	0.22%	0.028%
73	11.584	3182	3186	3188	rVB2	319	240	0.02%	0.002%
74	11.690	3215	3219	3220	rBV	849	518	0.04%	0.005%
75	11.748	3226	3237	3245	rBV	36921	59121	4.53%	0.564%
76	11.812	3245	3257	3281	rVB2	648067	1305256	100.00%	12.462%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048125.D
 Acq On : 18 Apr 2022 16:47
 Operator : SY/MD
 Sample : N2386-04
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0HY6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis

77	11.973	3302	3307	3314	rVB6	2315	3085	0.24%	0.029%
78	12.066	3326	3336	3350	rBV2	7294	13843	1.06%	0.132%
79	12.195	3362	3376	3397	rVB2	599666	1112252	85.21%	10.620%
80	12.324	3412	3416	3418	rBV4	643	516	0.04%	0.005%
81	12.472	3460	3462	3465	rVV2	381	205	0.02%	0.002%
82	12.497	3466	3470	3473	rVB3	366	318	0.02%	0.003%
83	12.533	3479	3481	3485	rVB3	316	214	0.02%	0.002%
84	12.568	3490	3492	3496	rBV	391	240	0.02%	0.002%
85	12.636	3508	3513	3516	rBV	783	788	0.06%	0.008%
86	12.735	3541	3544	3547	rBV2	409	267	0.02%	0.003%
87	12.774	3552	3556	3558	rBV3	560	437	0.03%	0.004%
88	12.838	3571	3576	3579	rVB2	296	273	0.02%	0.003%
89	13.073	3644	3649	3650	rBV3	356	279	0.02%	0.003%
90	13.189	3679	3685	3686	rBV2	300	265	0.02%	0.003%
91	13.291	3715	3717	3720	rVB	398	230	0.02%	0.002%
92	13.356	3735	3737	3742	rVB	334	222	0.02%	0.002%
93	13.378	3742	3744	3746	rBV2	331	206	0.02%	0.002%
94	13.472	3771	3773	3778	rBV2	220	249	0.02%	0.002%
95	13.629	3819	3822	3823	rBV2	379	232	0.02%	0.002%
96	13.848	3883	3890	3898	rVB6	2510	3628	0.28%	0.035%
97	14.327	4036	4039	4047	rVB3	791	864	0.07%	0.008%
98	14.854	4201	4203	4208	rBV3	439	370	0.03%	0.004%
99	15.008	4249	4251	4255	rVB	580	272	0.02%	0.003%
100	15.401	4370	4373	4375	rBV2	886	663	0.05%	0.006%




Sum of corrected areas: 10473639

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048125.D
Acq On : 18 Apr 2022 16:47
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COHY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

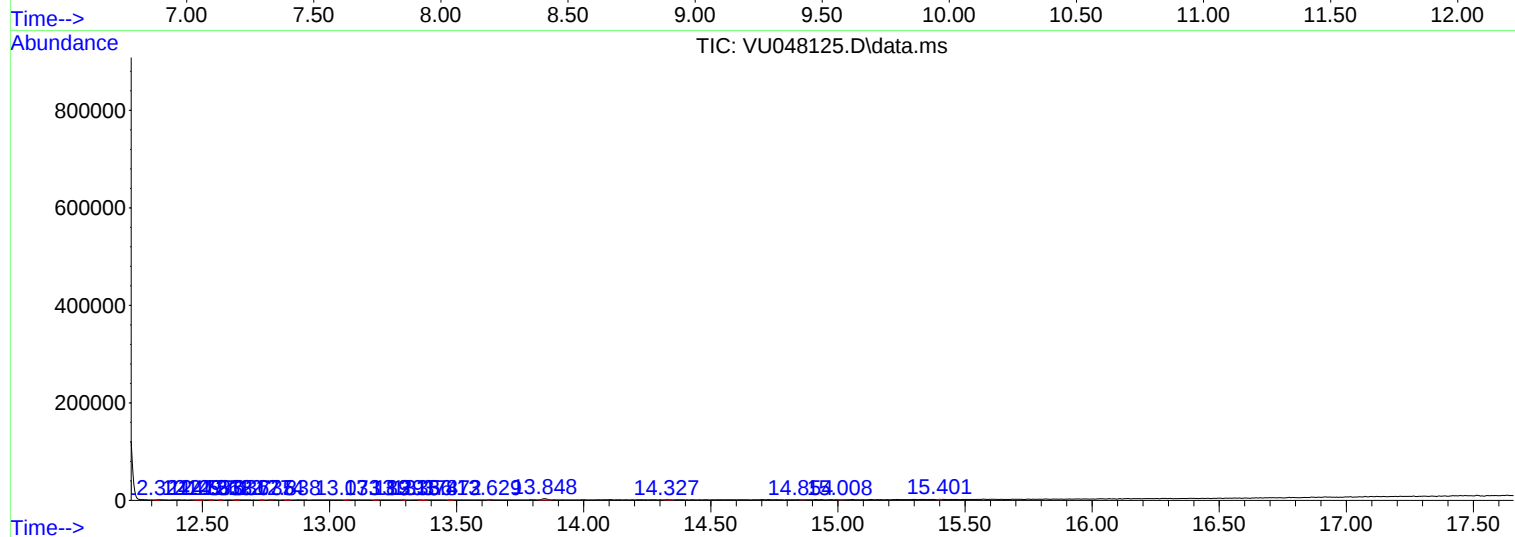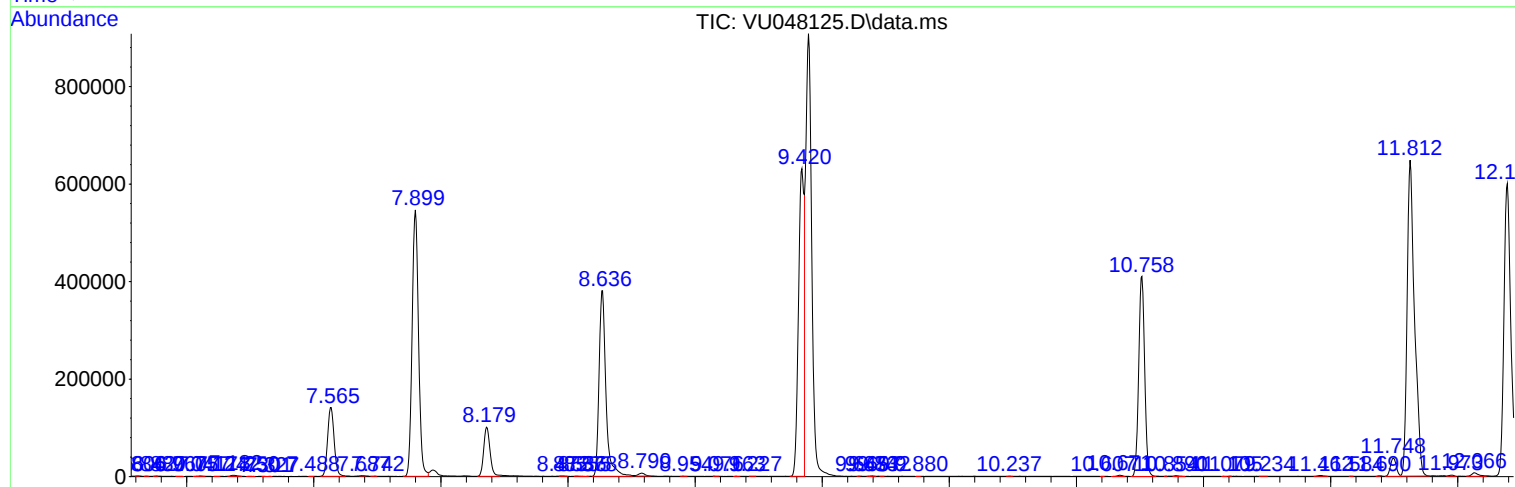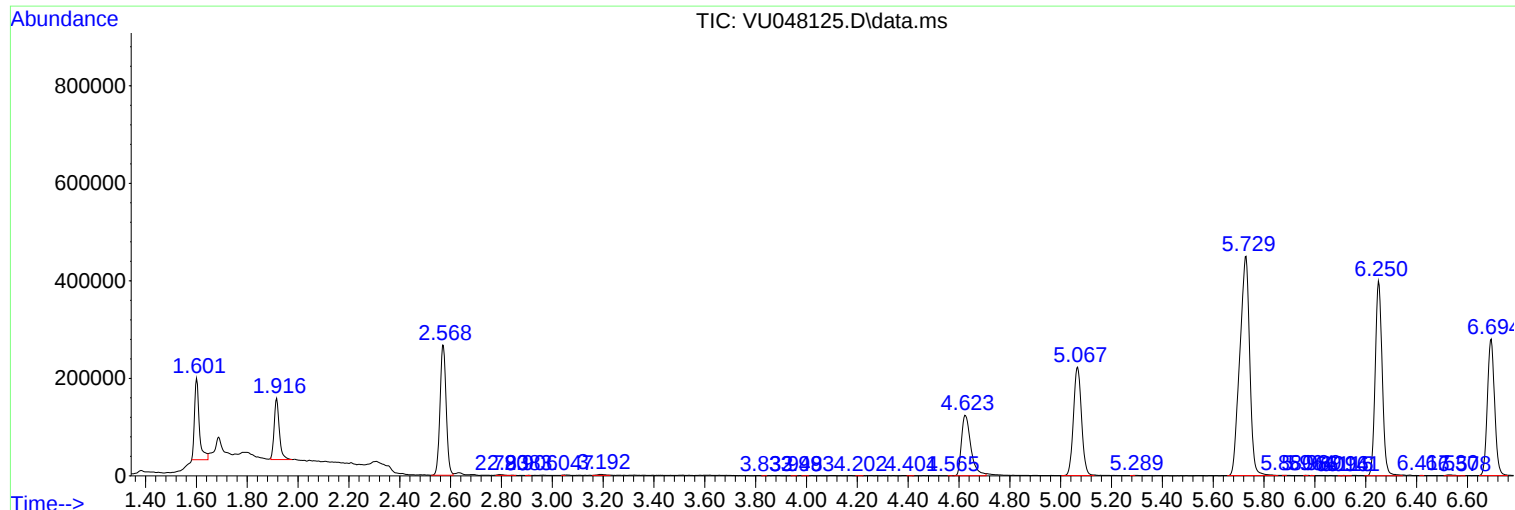

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048125.D
Acq On : 18 Apr 2022 16:47
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
Data File : VU048125.D
Acq On : 18 Apr 2022 16:47
Operator : SY/MD
Sample : N2386-04
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0HY6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------