


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041822\
 Data File : VU048108.D
 Acq On : 18 Apr 2022 09:49
 Operator : SY/MD
 Sample : BFB066
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB066

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM032422WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 22 02:51:38 2022

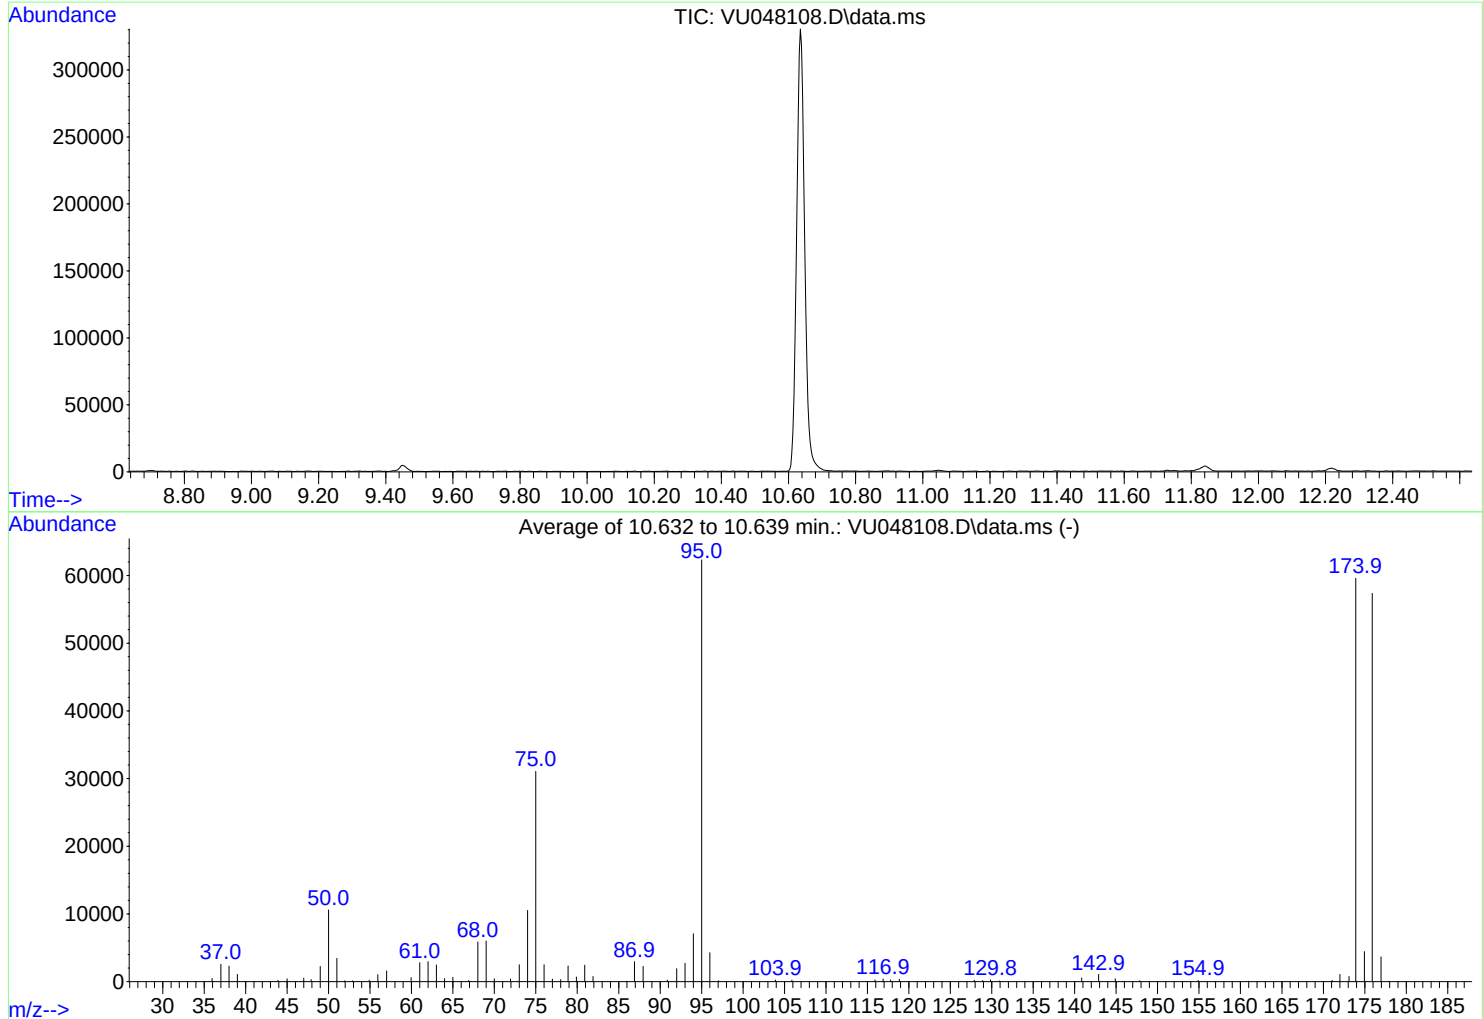

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	10583	PASS
75	95	30	80	49.9	31069	PASS
95	95	100	100	100.0	62309	PASS
96	95	5	9	6.9	4288	PASS
173	174	0.00	2	1.3	762	PASS
174	95	50	120	95.6	59581	PASS
175	174	5	9	7.4	4434	PASS
176	174	95	101	96.3	57371	PASS
177	176	5	9	6.4	3667	PASS

m/z	Abundance
39.90	128.0
43.90	410.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
36.00	502.0
37.00	2557.0
38.00	2359.0
39.00	954.0
39.90	144.0
44.00	605.0
45.00	402.0
47.00	544.0
47.90	322.0
49.00	2236.0
50.00	10663.0
51.00	3269.0
52.00	121.0
52.90	134.0
54.90	211.0
55.90	1032.0
57.00	1584.0
59.90	579.0
61.00	2791.0
62.00	2908.0
63.00	2387.0
64.00	458.0
65.00	656.0
66.90	173.0
68.00	5583.0
69.00	5831.0
70.00	420.0
71.90	357.0
73.00	2408.0
74.00	10398.0
75.00	30608.0
76.00	2379.0
77.00	360.0
78.00	341.0
78.90	2333.0
79.90	726.0
80.90	2537.0
81.90	746.0
85.90	117.0
86.90	2739.0
88.00	2436.0
90.90	233.0
92.00	1980.0
93.00	2641.0
94.00	6956.0
95.00	60416.0
96.00	4324.0
97.00	107.0
103.90	268.0
105.90	222.0
115.90	259.0
116.90	430.0
117.80	266.0
118.90	344.0
127.90	225.0
128.90	178.0
129.90	264.0
130.90	130.0
140.80	539.0
142.90	1046.0
144.90	386.0
145.80	112.0
147.90	158.0
154.90	173.0
171.10	213.0
172.00	920.0
173.10	612.0
173.90	57992.0
175.00	4407.0
175.90	55200.0
176.90	3661.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
36.00	468.0
37.00	2703.0
38.00	2357.0
39.00	1094.0
39.90	170.0
44.00	603.0
45.00	431.0
47.00	529.0
47.90	311.0
49.00	2313.0
50.00	10933.0
51.00	3528.0
51.90	118.0
52.90	122.0
54.90	222.0
56.00	1104.0
57.00	1648.0
59.90	616.0
61.00	2891.0
62.00	3053.0
63.00	2550.0
64.00	456.0
65.00	651.0
66.90	165.0
68.00	6079.0
69.00	6167.0
70.00	436.0
72.00	413.0
73.00	2560.0
74.00	10874.0
75.00	32128.0
76.00	2567.0
77.00	396.0
78.00	323.0
78.90	2376.0
79.90	693.0
80.90	2506.0
81.90	800.0
85.90	105.0
86.90	3058.0
88.00	2231.0
90.90	230.0
92.00	1991.0
93.00	2802.0
94.00	7342.0
95.00	64248.0
96.00	4435.0
97.10	143.0
103.90	253.0
105.90	226.0
115.90	264.0
116.90	408.0
117.80	283.0
118.80	363.0
127.90	231.0
128.90	186.0
129.80	253.0
130.90	145.0
140.90	566.0
142.90	1105.0
144.90	459.0
146.00	129.0
147.90	141.0
154.90	218.0
156.90	102.0
161.00	126.0
171.00	196.0
172.00	1067.0
173.10	781.0
173.90	61600.0
174.90	4581.0
175.90	59040.0
177.00	3774.0
177.90	100.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066

m/z	Abundance
35.90	462.0
37.00	2498.0
38.00	2179.0
39.00	1176.0
39.90	202.0
43.90	575.0
45.00	426.0
47.00	507.0
47.90	289.0
49.00	2190.0
50.00	10154.0
51.00	3538.0
51.90	125.0
52.90	105.0
54.90	205.0
56.00	1006.0
57.00	1525.0
60.00	557.0
61.00	2778.0
62.00	2883.0
63.00	2460.0
64.00	422.0
65.00	603.0
66.90	137.0
68.00	5930.0
69.00	6003.0
70.00	433.0
72.00	408.0
73.00	2555.0
74.00	10265.0
75.00	30472.0
76.00	2601.0
77.00	347.0
78.00	254.0
78.90	2213.0
79.90	628.0
80.90	2282.0
81.90	747.0
86.90	3062.0
87.90	2070.0
90.80	251.0
92.00	1744.0
93.00	2732.0
94.00	6919.0
95.00	62264.0
96.00	4104.0
97.10	155.0
103.90	219.0
105.90	233.0
115.90	232.0
116.90	378.0
117.80	265.0
118.90	374.0
127.90	213.0
128.90	154.0
129.80	238.0
130.90	116.0
140.90	535.0
142.90	1032.0
144.90	455.0
146.00	113.0
147.80	119.0
154.90	205.0
161.00	110.0
171.00	152.0
172.00	1221.0
173.10	894.0
173.90	59152.0
174.90	4313.0
175.90	57872.0
176.90	3565.0
177.90	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB066