
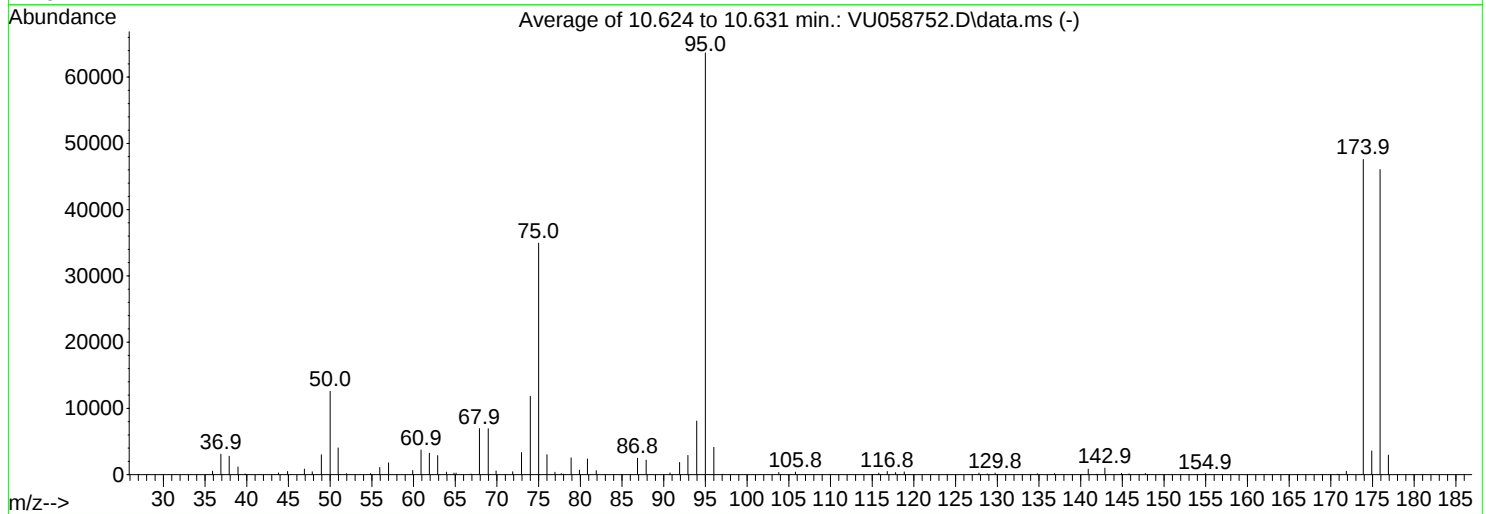


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041824\
Data File : VU058752.D
Acq On : 18 Apr 2024 08:45
Operator : MD/SY
Sample : BFB146
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB146

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR040424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 18 05:04:53 2024

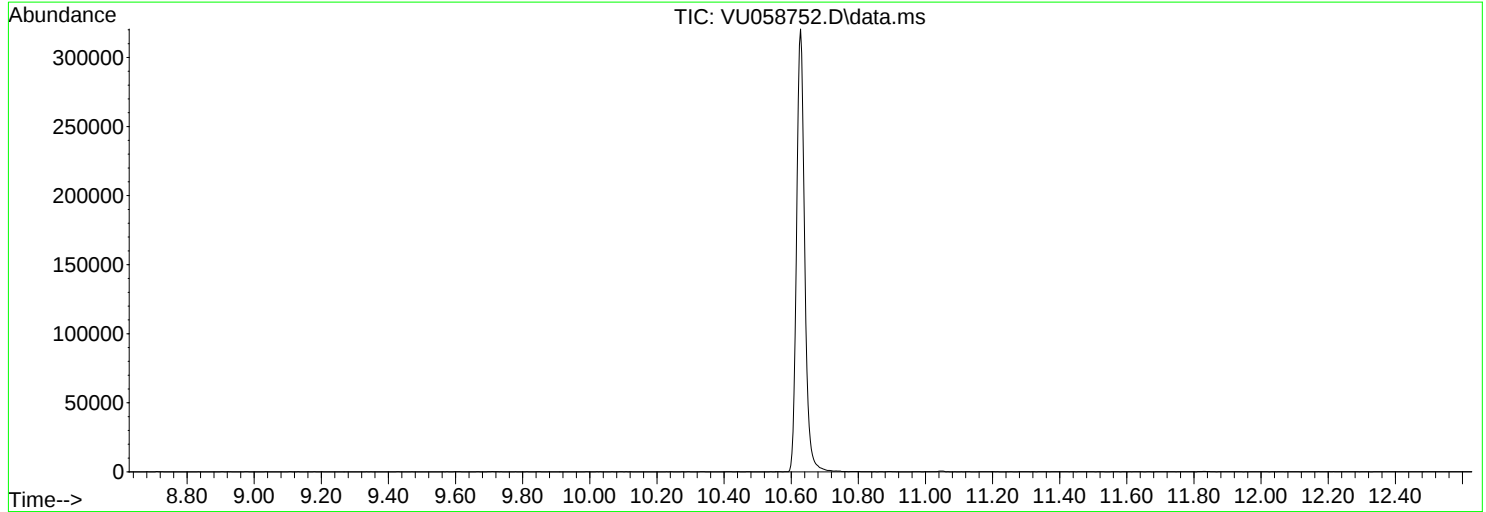

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	12572	PASS
75	95	30	80	54.9	34941	PASS
95	95	100	100	100.0	63664	PASS
96	95	5	9	6.5	4142	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.7	47579	PASS
175	174	5	9	7.5	3564	PASS
176	174	95	101	96.8	46059	PASS
177	176	5	9	6.4	2952	PASS

m/z	Abundance
43.80	140.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	527.0
36.90	3061.0
37.90	2798.0
39.00	1134.0
39.80	115.0
43.90	428.0
44.90	509.0
46.90	830.0
47.80	444.0
48.90	3038.0
50.00	12755.0
50.90	4150.0
51.90	152.0
54.90	142.0
55.90	1126.0
57.00	1838.0
59.90	694.0
60.90	3749.0
61.90	3337.0
62.90	2989.0
64.00	420.0
65.10	379.0
66.90	162.0
67.90	6795.0
68.90	6971.0
69.90	539.0
71.90	460.0
73.00	3419.0
74.00	11825.0
75.00	34888.0
76.00	3107.0
76.90	344.0
77.70	240.0
78.90	2529.0
79.90	672.0
80.90	2349.0
81.90	573.0
86.90	2486.0
87.90	2158.0
90.70	261.0
91.90	1870.0
92.90	2800.0
93.90	8175.0
95.00	63608.0
96.00	4237.0
97.00	118.0
103.80	331.0
105.80	367.0
115.80	267.0
116.80	491.0
117.80	294.0
118.80	372.0
127.80	211.0
128.80	136.0
129.70	226.0
134.80	152.0
136.90	168.0
140.90	834.0
141.90	115.0
142.90	969.0
144.90	205.0
145.80	110.0
147.70	159.0
154.90	151.0
170.80	121.0
171.90	514.0
173.90	46496.0
174.90	3487.0
175.90	44656.0
176.90	2979.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	549.0
36.90	3190.0
37.90	2892.0
38.90	1170.0
39.80	126.0
43.80	399.0
44.90	503.0
46.90	886.0
47.90	434.0
49.00	3113.0
50.00	13010.0
51.00	4137.0
51.90	149.0
54.80	187.0
56.00	1143.0
57.00	1810.0
59.90	641.0
60.90	3809.0
61.90	3330.0
62.90	2971.0
63.90	394.0
64.80	356.0
65.10	361.0
67.90	7219.0
69.00	7125.0
69.90	583.0
71.90	446.0
73.00	3446.0
74.00	12225.0
75.00	36000.0
76.00	3113.0
77.00	353.0
77.70	233.0
78.90	2632.0
79.90	689.0
80.80	2442.0
81.90	629.0
86.80	2547.0
87.90	2280.0
90.70	277.0
91.90	1886.0
92.90	2951.0
93.90	8318.0
95.00	65584.0
96.00	4263.0
97.00	105.0
103.80	356.0
105.80	409.0
115.80	254.0
116.80	500.0
117.80	312.0
118.80	408.0
127.80	237.0
128.80	135.0
129.70	246.0
134.80	135.0
136.80	161.0
140.90	828.0
142.00	132.0
142.90	1026.0
144.90	195.0
145.80	118.0
147.70	182.0
155.00	163.0
170.80	103.0
171.90	521.0
173.90	49056.0
174.90	3696.0
175.90	47480.0
176.90	3029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146

m/z	Abundance
35.90	535.0
36.90	3018.0
37.90	2632.0
38.90	1139.0
39.80	107.0
43.80	372.0
44.90	442.0
46.90	802.0
47.80	425.0
49.00	2847.0
50.00	11952.0
51.00	3807.0
52.00	135.0
54.80	210.0
56.00	1025.0
57.00	1719.0
59.90	576.0
60.90	3586.0
61.90	3071.0
62.90	2672.0
63.90	366.0
64.90	368.0
66.90	144.0
67.90	6877.0
69.00	6724.0
69.90	548.0
71.90	394.0
72.90	3161.0
74.00	11449.0
75.00	33936.0
76.00	2830.0
77.00	394.0
78.00	247.0
78.90	2452.0
79.90	658.0
80.80	2313.0
81.90	590.0
86.80	2410.0
87.90	2195.0
90.80	265.0
91.90	1749.0
92.90	2924.0
94.00	7789.0
95.00	61800.0
96.00	3926.0
103.80	317.0
105.80	367.0
115.80	214.0
116.80	458.0
117.80	320.0
118.90	420.0
127.80	249.0
128.80	129.0
129.80	236.0
134.80	141.0
136.80	153.0
140.90	797.0
142.90	1002.0
144.90	172.0
145.80	111.0
147.80	178.0
154.90	165.0
171.80	480.0
173.90	47184.0
174.90	3510.0
175.90	46040.0
176.90	2849.0

Instrument :
MSVOA_U
ClientSampleId :
BFB146