

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041923\
 Data File : VU053784.D
 Acq On : 19 Apr 2023 16:09
 Operator : JC/MD
 Sample : VU0419WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0419WBL01

Quant Time: Apr 21 09:25:19 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U041923DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Fri Apr 21 09:18:21 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.105	96	27407	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.632	95	9855	0.917	ug/l	0.00
Spiked Amount 1.000			Recovery	=	92.000%	
68) 1,2-Dichlorobenzene-d4	12.188	152	11423	0.894	ug/l	0.00
Spiked Amount 1.000			Recovery	=	89.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041923\
Data File : VU053784.D
Acq On : 19 Apr 2023 16:09
Operator : JC/MD
Sample : VU0419WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0419WBL01

Quant Time: Apr 21 09:25:19 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U041923DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Fri Apr 21 09:18:21 2023
Response via : Initial Calibration




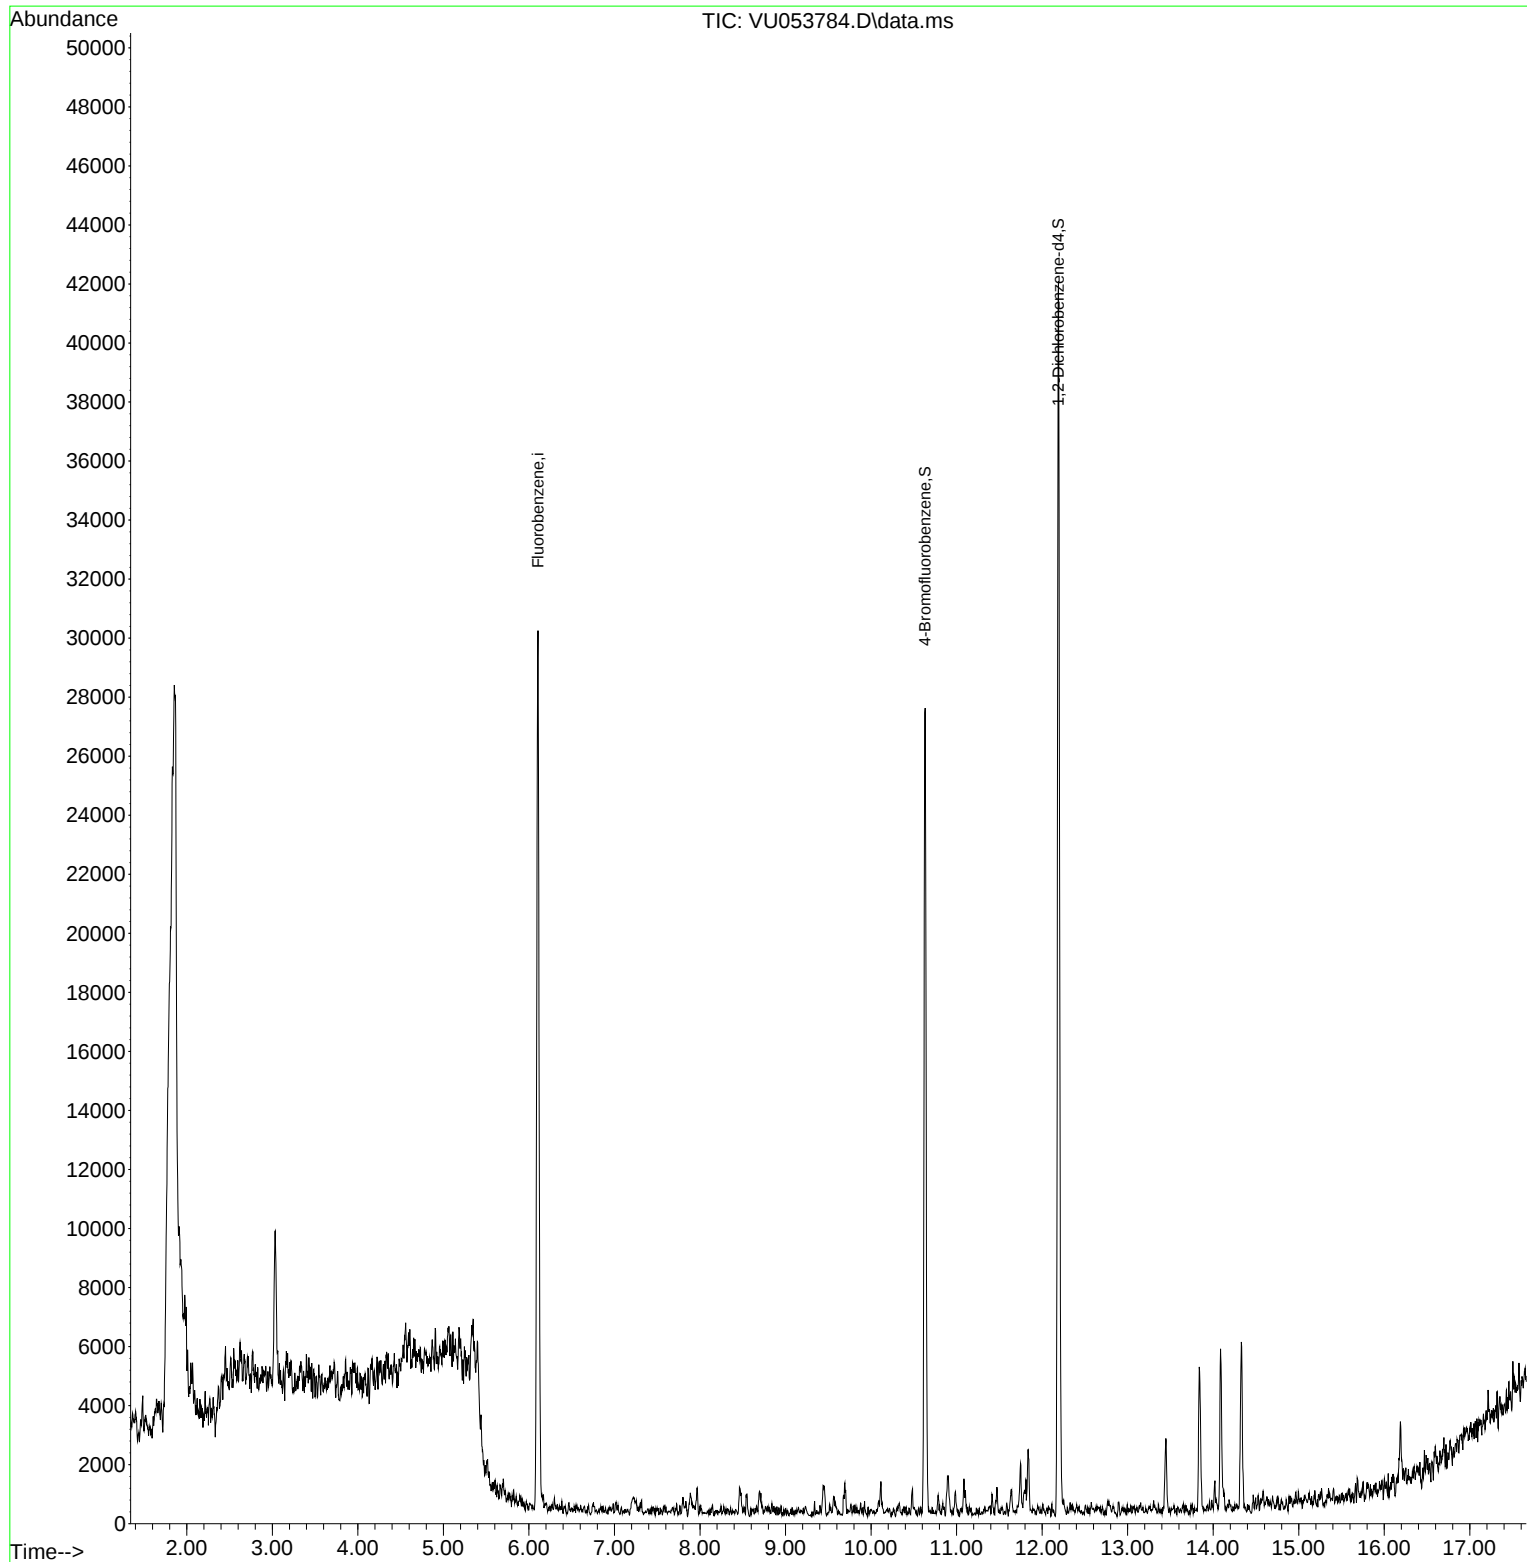


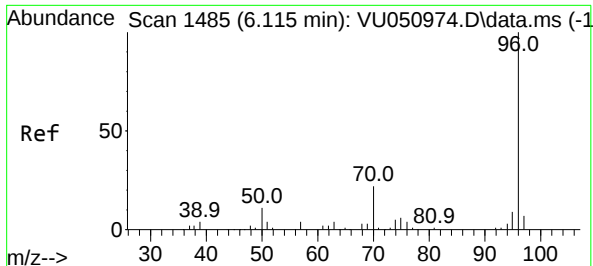

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.105 min Scan# 1482
Delta R.T. -0.003 min
Lab File: VU053784.D
Acq: 19 Apr 2023 16:09




Instrument :
MSVOA_U
ClientSampleId :
VU0419WBL01


Tgt Ion: 96	Resp: 27407
Ion Ratio	Lower Upper
96 100	
70 20.9	16.5 24.7
95 9.2	7.4 11.0
97 6.2	0.0 0.0

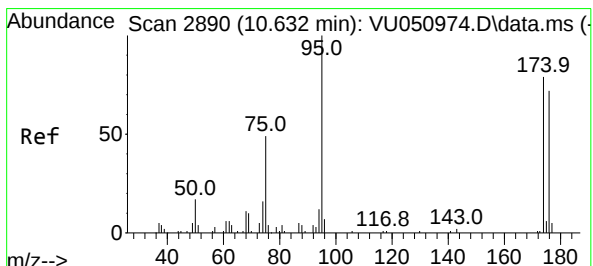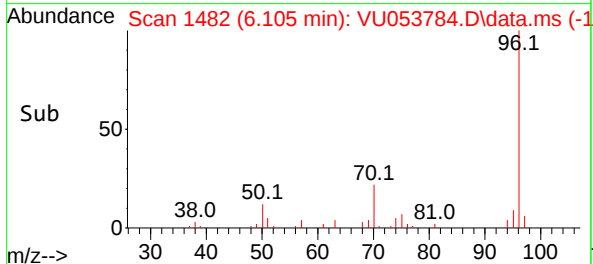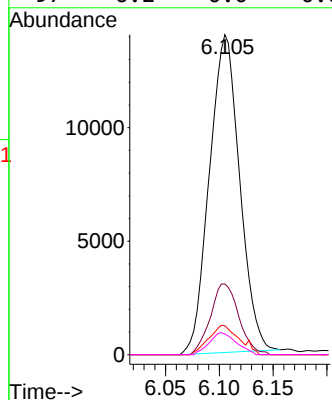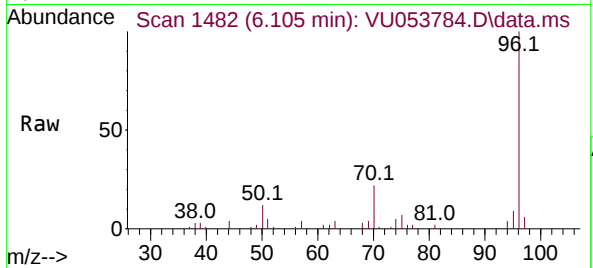

#57
4-Bromofluorobenzene
Concen: 0.917 ug/l
RT: 10.632 min Scan# 2890
Delta R.T. -0.000 min
Lab File: VU053784.D
Acq: 19 Apr 2023 16:09


Tgt Ion: 95	Resp: 9855
Ion Ratio	Lower Upper
95 100	
174 85.1	63.3 94.9
176 76.4	59.3 88.9

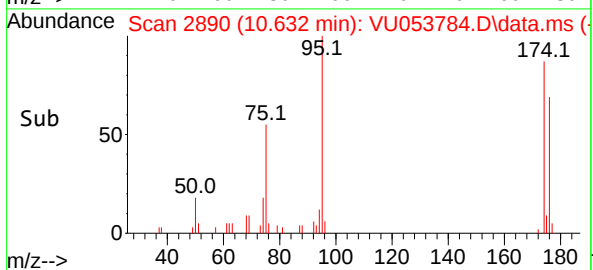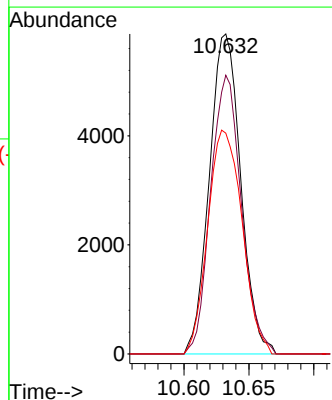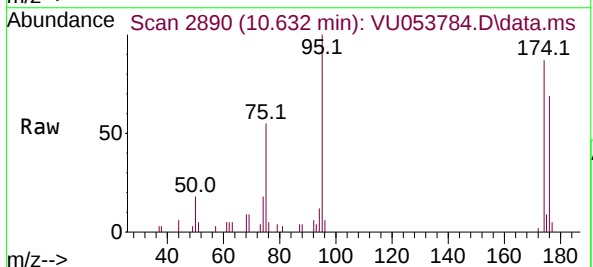

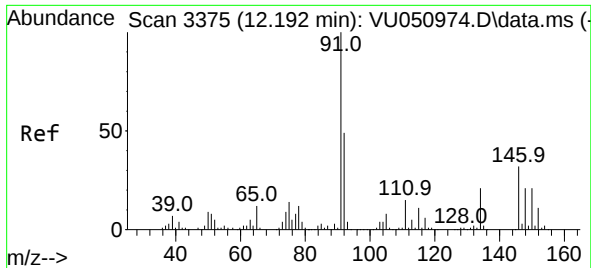

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.894 ug/l
 RT: 12.188 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VU053784.D
 Acq: 19 Apr 2023 16:09

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0419WBL01

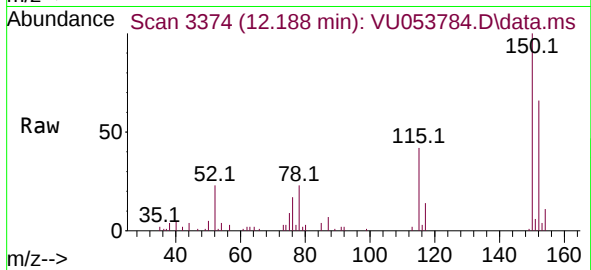

Tgt Ion:	152	Resp:	11423
Ion	Ratio	Lower	Upper
152	100		
115	67.0	0.0	308.8
150	160.6	0.0	635.0

