


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU041923\
 Data File : VU053773.D
 Acq On : 19 Apr 2023 09:49
 Operator : JC/MD
 Sample : BFB
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR032423WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Wed Apr 19 04:58:28 2023

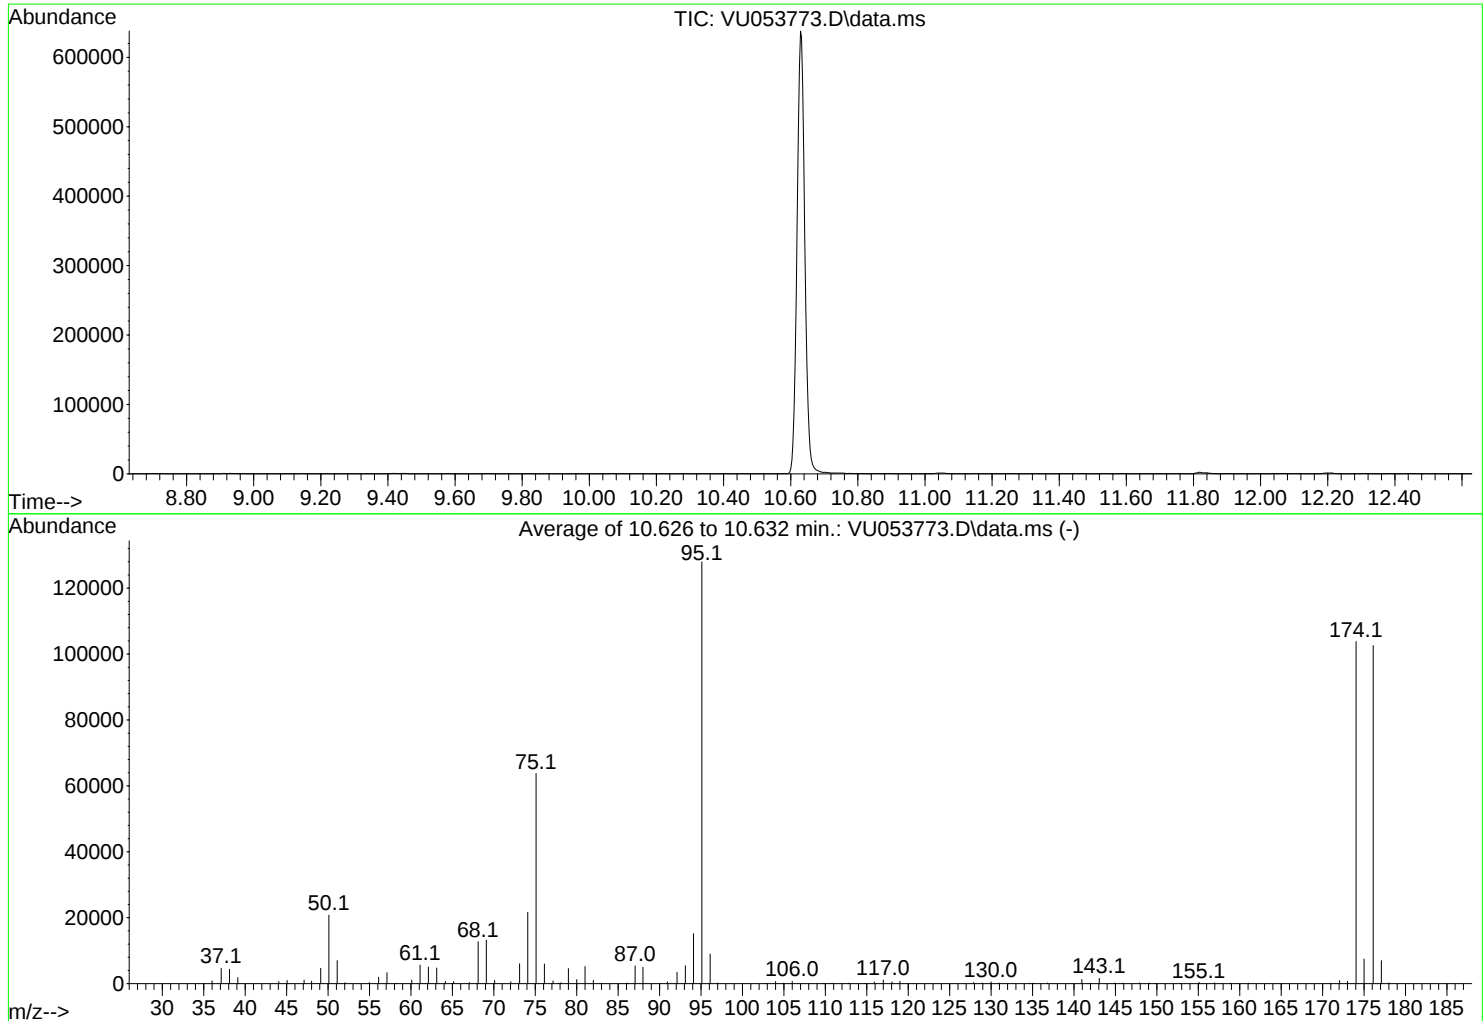

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.2	20781	PASS
75	95	30	80	49.8	63784	PASS
95	95	100	100	100.0	127984	PASS
96	95	5	9	7.0	9004	PASS
173	174	0.00	2	0.7	707	PASS
174	95	50	120	81.1	103803	PASS
175	174	5	9	7.2	7465	PASS
176	174	95	101	98.8	102605	PASS
177	176	5	9	6.8	6970	PASS