


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042224\
Data File : VU058762.D
Acq On : 22 Apr 2024 10:22
Operator : MD/SY
Sample : BFB147
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB147

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 24 00:34:42 2024

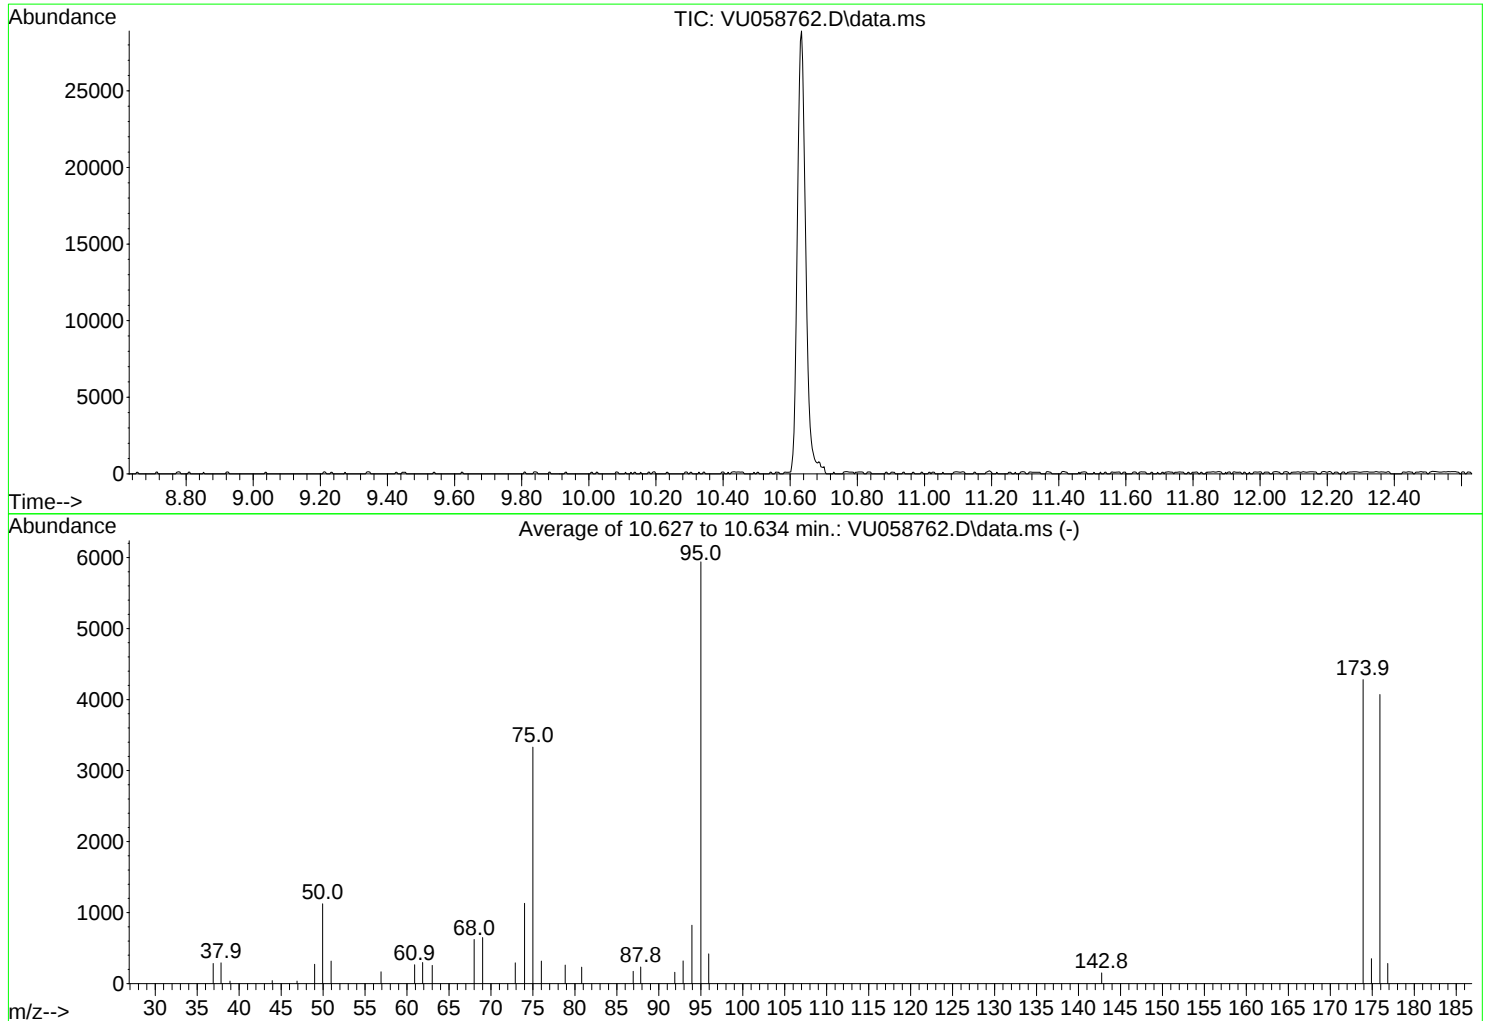

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2894

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.9	1125	PASS
75	95	30	80	56.1	3330	PASS
95	95	100	100	100.0	5939	PASS
96	95	5	9	7.0	418	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.1	4280	PASS
175	174	5	9	8.2	352	PASS
176	174	95	101	95.1	4071	PASS
177	176	5	9	7.0	283	PASS

m/z	Abundance
43.90	109.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.90	249.0
37.90	281.0
38.90	104.0
44.00	166.0
49.00	259.0
49.90	1121.0
51.00	348.0
56.90	159.0
60.90	241.0
61.80	280.0
63.00	242.0
68.00	600.0
69.00	569.0
72.90	235.0
74.00	1024.0
75.00	3032.0
76.00	298.0
78.80	233.0
80.80	230.0
86.90	130.0
87.80	269.0
91.90	159.0
92.90	273.0
94.00	728.0
95.00	5636.0
95.90	412.0
142.80	148.0
173.90	3838.0
174.90	357.0
175.90	3640.0
176.80	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.90	288.0
37.80	299.0
44.00	156.0
49.00	286.0
50.00	1127.0
51.00	320.0
56.90	178.0
60.90	269.0
61.90	293.0
63.00	266.0
68.00	656.0
69.00	661.0
72.90	294.0
74.00	1181.0
75.00	3430.0
76.00	329.0
78.80	269.0
80.80	236.0
86.90	166.0
87.90	240.0
91.90	157.0
92.90	337.0
93.90	860.0
95.00	6139.0
95.90	434.0
142.70	163.0
173.90	4380.0
174.90	360.0
175.90	4162.0
176.80	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147

m/z	Abundance
36.90	311.0
37.80	300.0
44.00	136.0
46.90	109.0
49.00	274.0
49.90	1128.0
50.90	285.0
56.90	164.0
60.90	287.0
61.90	322.0
63.00	267.0
68.00	611.0
69.00	719.0
72.90	352.0
74.00	1192.0
75.00	3529.0
76.00	325.0
78.90	282.0
80.80	226.0
87.00	226.0
87.90	197.0
91.90	166.0
92.90	351.0
93.90	879.0
95.00	6043.0
96.00	408.0
142.70	142.0
173.90	4621.0
174.90	340.0
175.90	4410.0
176.90	286.0

Instrument :
MSVOA_U
ClientSampleId :
BFB147