


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042320\
 Data File : VU037856.D
 Acq On : 23 Apr 2020 08:54
 Operator : JC/MD
 Sample : BFB41
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB41

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 23 12:05:26 2020

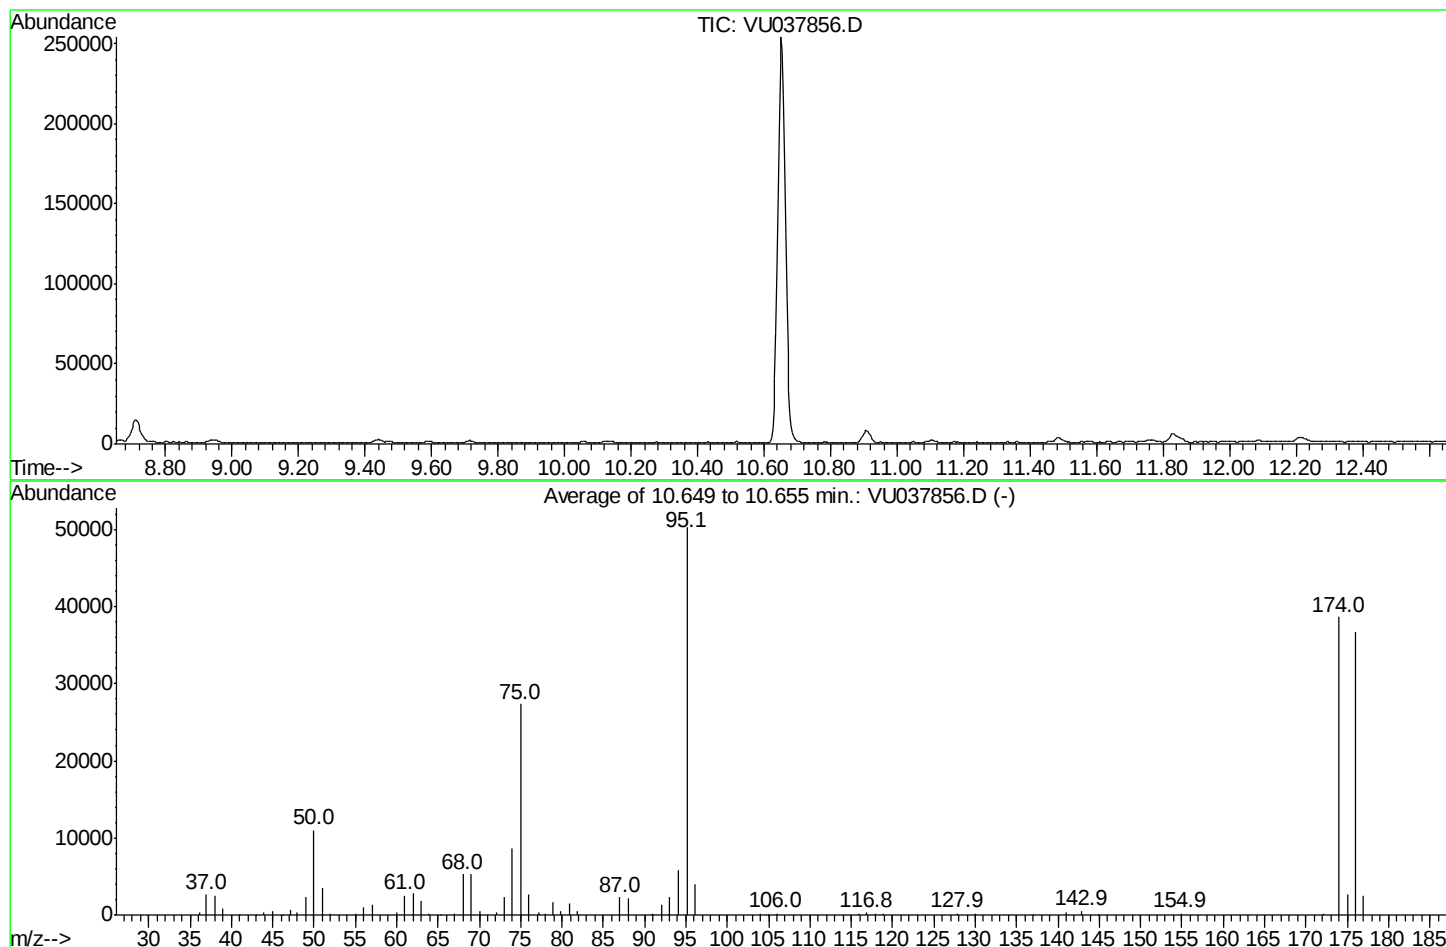

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2884

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	10985	PASS
75	95	30	80	54.4	27352	PASS
95	95	100	100	100.0	50290	PASS
96	95	5	9	8.0	4017	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.8	38624	PASS
175	174	5	9	7.0	2720	PASS
176	174	95	101	95.2	36784	PASS
177	176	5	9	7.0	2568	PASS

m/z	Abundance
36.10	383.0
37.00	2600.0
38.00	2657.0
39.00	834.0
39.90	203.0
41.00	122.0
44.00	1020.0
45.00	396.0
46.20	122.0
47.10	657.0
48.00	311.0
49.00	2254.0
50.00	10535.0
51.00	3472.0
52.00	124.0
55.00	214.0
56.00	1003.0
57.00	1317.0
60.00	320.0
61.00	2425.0
62.00	2740.0
63.00	1826.0
67.00	214.0
68.00	5313.0
69.00	5339.0
70.00	476.0
72.10	333.0
73.00	2238.0
74.00	8291.0
75.00	26000.0
76.00	2669.0
77.20	302.0
77.80	163.0
78.90	1791.0
79.90	468.0
80.90	1482.0
81.90	449.0
87.00	2194.0
88.00	1886.0
91.10	243.0
92.00	1276.0
93.10	2171.0
94.00	5989.0
95.10	48528.0
96.00	4149.0
104.00	220.0
104.90	135.0
106.00	236.0
116.80	269.0
117.80	169.0
118.90	189.0
127.90	161.0
130.10	174.0
136.90	105.0
141.00	405.0
142.90	568.0
144.80	110.0
154.90	177.0
172.20	138.0
174.00	36592.0
175.00	2702.0
176.00	34984.0
177.00	2393.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.20	424.0
37.00	2687.0
38.00	2570.0
39.00	850.0
40.00	198.0
40.90	120.0
44.00	1149.0
45.00	473.0
46.20	127.0
47.10	675.0
48.00	389.0
49.00	2358.0
50.00	11345.0
51.00	3530.0
52.00	154.0
55.10	206.0
56.00	1009.0
57.00	1380.0
60.10	338.0
61.00	2595.0
62.00	2947.0
63.00	1889.0
63.90	177.0
65.20	109.0
66.90	212.0
68.00	5506.0
69.00	5449.0
70.00	497.0
72.10	275.0
73.00	2454.0
74.00	8861.0
75.00	28368.0
76.00	2739.0
77.20	331.0
77.90	250.0
78.90	1722.0
79.90	470.0
80.90	1576.0
81.90	437.0
87.00	2301.0
88.00	2224.0
91.00	240.0
92.00	1296.0
93.10	2375.0
94.10	6024.0
95.10	52016.0
96.10	4210.0
104.00	209.0
105.00	123.0
106.00	213.0
115.90	148.0
116.90	301.0
117.90	179.0
118.80	229.0
127.90	205.0
130.00	189.0
140.90	388.0
142.90	545.0
144.90	107.0
154.90	236.0
172.10	118.0
174.00	39928.0
175.00	2836.0
176.00	38032.0
177.00	2687.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

m/z	Abundance
36.10	366.0
37.00	2534.0
38.00	2431.0
39.00	833.0
40.00	247.0
43.00	114.0
44.00	1284.0
45.00	511.0
47.10	612.0
48.00	415.0
49.00	2284.0
50.00	11076.0
51.00	3355.0
52.00	157.0
55.10	151.0
56.00	935.0
57.00	1442.0
60.10	350.0
61.00	2514.0
62.00	2787.0
63.00	1914.0
63.90	220.0
66.90	160.0
68.00	5013.0
69.00	5284.0
70.00	410.0
71.90	245.0
73.00	2404.0
74.00	8741.0
75.00	27688.0
76.00	2500.0
77.20	267.0
78.00	286.0
78.90	1466.0
79.90	473.0
80.90	1520.0
81.90	387.0
87.00	2358.0
88.00	2422.0
90.80	206.0
92.00	1240.0
93.00	2348.0
94.00	5555.0
95.10	50328.0
96.10	3692.0
103.80	205.0
106.00	200.0
115.90	160.0
116.90	272.0
117.90	185.0
118.80	251.0
127.90	203.0
130.00	177.0
140.90	367.0
142.90	492.0
154.90	221.0
172.10	105.0
174.00	39352.0
175.00	2623.0
176.00	37336.0
177.00	2626.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41

Scan 2884 (10.613 min): VU037856.D
BFB41

m/z	Abundance
39.90	231.0
43.90	782.0

Instrument :
MSVOA_U
ClientSampleId :
BFB41