


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042324\
Data File : VU058774.D
Acq On : 23 Apr 2024 08:24
Operator : MD/SY
Sample : BFB148
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB148

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Apr 24 00:34:42 2024

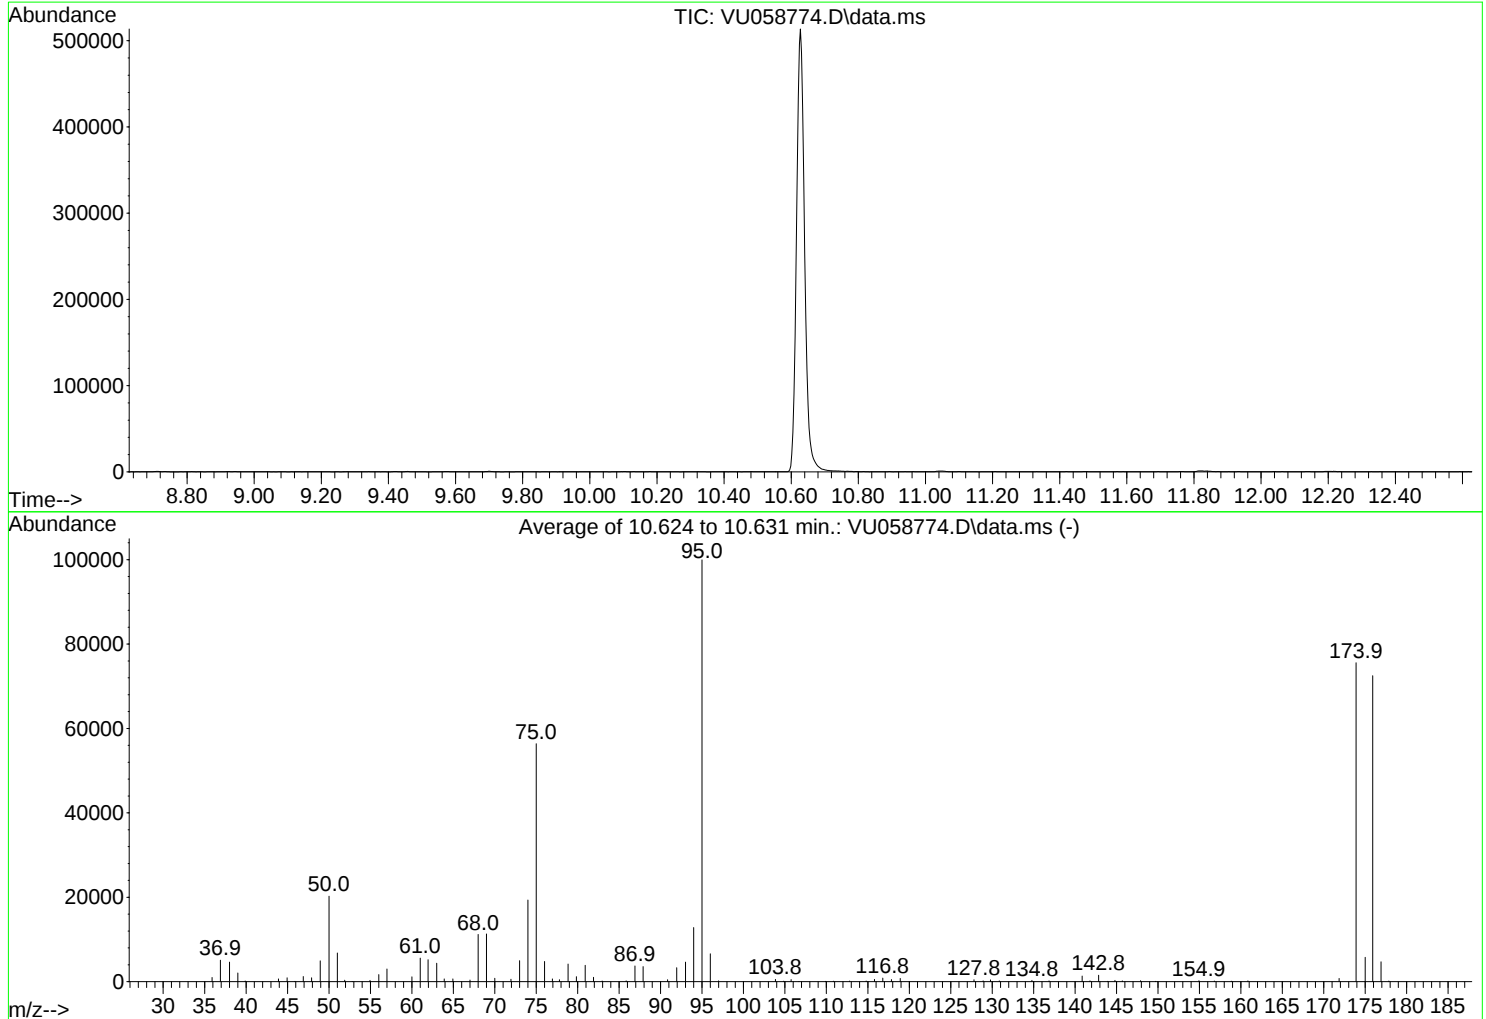

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.3	20253	PASS
75	95	30	80	56.4	56373	PASS
95	95	100	100	100.0	99968	PASS
96	95	5	9	6.6	6611	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	75.6	75595	PASS
175	174	5	9	7.6	5761	PASS
176	174	95	101	95.9	72488	PASS
177	176	5	9	6.5	4699	PASS

m/z	Abundance
43.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
35.90	984.0
36.90	5219.0
38.00	4564.0
39.00	2098.0
39.90	170.0
44.00	796.0
45.00	965.0
45.90	148.0
46.90	1263.0
47.90	844.0
48.90	5013.0
50.00	20560.0
51.00	6618.0
51.90	343.0
52.80	122.0
55.00	294.0
56.00	1654.0
57.00	2980.0
60.00	1137.0
61.00	5645.0
61.90	5338.0
63.00	4265.0
63.90	733.0
65.00	678.0
67.00	368.0
68.00	11189.0
69.00	11342.0
70.00	803.0
71.90	624.0
73.00	4927.0
74.00	19688.0
75.00	56472.0
76.00	4870.0
77.00	599.0
77.80	478.0
78.90	4103.0
79.90	1186.0
80.90	3810.0
81.90	1006.0
82.90	137.0
85.80	170.0
86.90	3674.0
87.90	3718.0
90.90	438.0
91.90	3387.0
93.00	4583.0
94.00	12411.0
95.00	100392.0
96.00	6698.0
97.00	188.0
103.90	544.0
104.80	142.0
105.80	499.0
109.90	103.0
110.90	134.0
112.80	138.0
114.80	170.0
115.80	547.0
116.80	791.0
117.90	518.0
118.90	774.0
127.80	473.0
128.90	164.0
129.80	417.0
130.90	156.0
134.80	302.0
136.80	158.0
140.80	1260.0
141.80	219.0
142.80	1485.0
143.90	117.0
144.80	279.0
145.70	133.0
147.90	238.0
149.70	131.0
154.90	229.0
156.80	157.0
158.80	114.0
160.80	196.0
171.90	745.0
173.90	73424.0
175.00	5603.0
175.90	71192.0
176.90	4564.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
35.90	1004.0
36.90	5277.0
38.00	4770.0
39.00	2115.0
39.90	156.0
44.00	788.0
45.00	960.0
45.90	127.0
46.90	1266.0
47.90	976.0
49.00	5122.0
50.00	20800.0
51.00	7091.0
51.90	339.0
55.00	290.0
56.00	1716.0
57.00	3124.0
60.00	1222.0
61.00	5749.0
62.00	5284.0
63.00	4502.0
63.90	679.0
65.00	646.0
67.00	392.0
68.00	11493.0
69.00	11690.0
70.00	800.0
71.90	570.0
73.00	5088.0
74.00	19952.0
75.00	58184.0
76.00	4892.0
76.90	645.0
77.80	465.0
78.90	4311.0
79.80	1213.0
80.90	3983.0
81.90	1076.0
83.00	140.0
85.80	208.0
86.90	3788.0
87.90	3641.0
90.90	482.0
92.00	3395.0
93.00	4786.0
94.00	13208.0
95.00	102800.0
96.00	6845.0
97.00	203.0
103.80	555.0
104.90	137.0
105.80	528.0
109.90	114.0
110.90	124.0
112.80	155.0
114.80	141.0
115.80	545.0
116.80	845.0
117.80	501.0
118.90	778.0
127.80	470.0
128.90	196.0
129.80	415.0
130.80	180.0
134.80	298.0
136.90	211.0
140.80	1349.0
141.80	200.0
142.90	1546.0
144.00	112.0
144.80	304.0
145.70	205.0
147.90	241.0
149.70	134.0
155.00	251.0
156.80	174.0
158.90	100.0
160.90	214.0
171.90	770.0
173.90	77848.0
175.00	5927.0
175.90	74664.0
176.90	4870.0
177.90	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148

m/z	Abundance
35.90	940.0
36.90	4736.0
38.00	4511.0
39.00	1923.0
39.90	130.0
43.90	795.0
44.90	847.0
46.90	1154.0
47.90	949.0
49.00	4702.0
50.00	19400.0
51.00	6641.0
51.90	345.0
54.80	295.0
56.00	1629.0
57.00	2875.0
60.00	1108.0
61.00	5297.0
62.00	4989.0
63.00	4300.0
63.90	527.0
64.90	610.0
67.00	340.0
68.00	10875.0
69.00	10912.0
70.00	753.0
72.00	505.0
73.00	4910.0
74.00	18376.0
75.00	54464.0
76.00	4580.0
76.90	678.0
77.80	383.0
78.80	4057.0
79.80	1160.0
80.90	3828.0
81.90	983.0
83.00	139.0
85.90	203.0
86.90	3718.0
87.90	3292.0
90.80	492.0
92.00	3093.0
93.00	4528.0
94.00	12791.0
95.00	96712.0
96.00	6289.0
97.00	212.0
103.80	529.0
104.90	114.0
105.70	488.0
106.70	104.0
110.70	120.0
112.80	154.0
114.80	121.0
115.80	473.0
116.80	839.0
117.80	423.0
118.90	690.0
127.80	430.0
128.90	210.0
129.80	389.0
130.90	199.0
134.80	271.0
136.90	232.0
140.90	1362.0
141.80	134.0
142.90	1531.0
144.80	287.0
145.70	233.0
147.90	201.0
149.90	140.0
155.00	236.0
156.80	170.0
158.90	107.0
160.80	201.0
171.80	723.0
173.90	75512.0
175.00	5753.0
175.90	71608.0
176.90	4662.0
177.80	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB148