

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042424\
 Data File : VU058791.D
 Acq On : 24 Apr 2024 13:33
 Operator : MD/SY
 Sample : VU0424WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: Apr 25 01:42:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM042424.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Apr 25 01:37:46 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	3983	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.419	117	5856	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	1822	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.590	65	971	0.495	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	100.000%
4) 1,2-Dichloroethane-d4	5.685	65	1745	0.522	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	104.000%
7) 1,2-Dichloropropane-d6	6.687	67	1664	0.504	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	100.000%
8) Toluene-d8	7.887	98	4168	0.498	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	1179	0.518	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
					Qvalue	
6) Trichloroethene	6.544	95	73	0.020	ug/L #	92
13) 1,2-Dibromo-3-chloropr...	12.751	75	74	0.219	ug/L #	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042424\
Data File : VU058791.D
Acq On : 24 Apr 2024 13:33
Operator : MD/SY
Sample : VU0424WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: Apr 25 01:42:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM042424.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Apr 25 01:37:46 2024
Response via : Initial Calibration

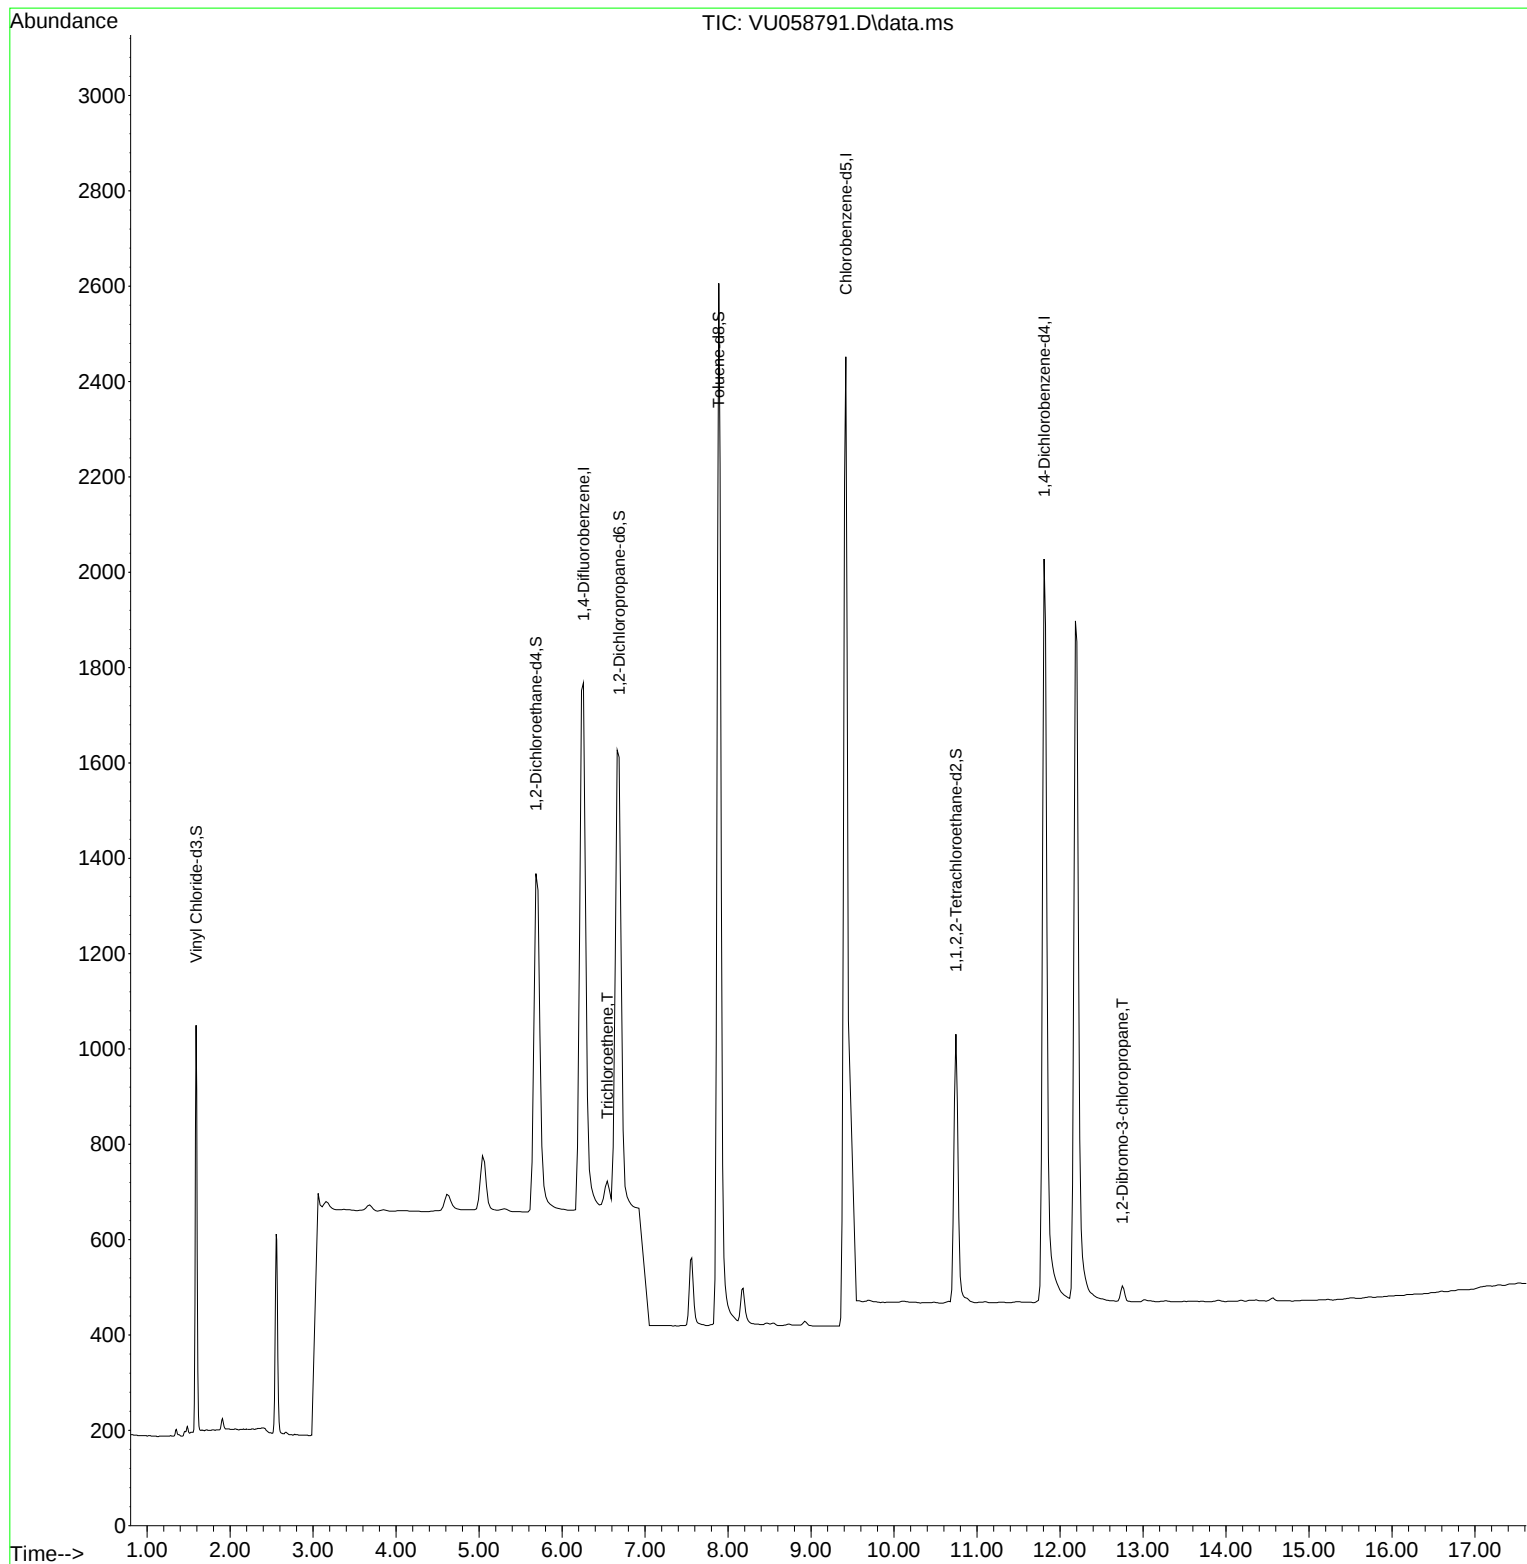

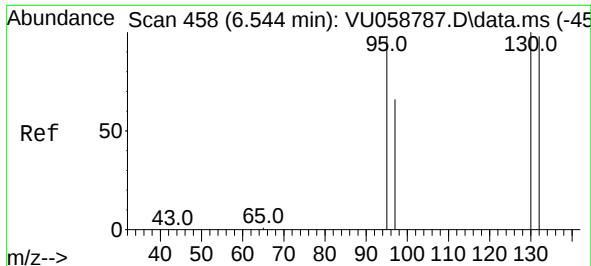




#6
Trichloroethene
Concen: 0.020 ug/L
RT: 6.544 min Scan# 458
Delta R.T. 0.000 min
Lab File: VU058791.D
Acq: 24 Apr 2024 13:33

Instrument :
MSVOA_U
ClientSampleId :

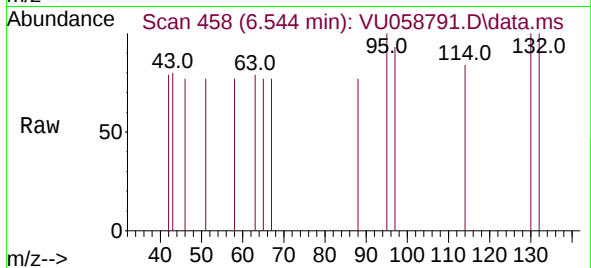

Tgt Ion: 95 Resp: 73

Ion	Ratio	Lower	Upper
95	100		
97	93.4	49.3	91.5#
132	100.0	70.1	130.3
130	100.0	71.2	132.2

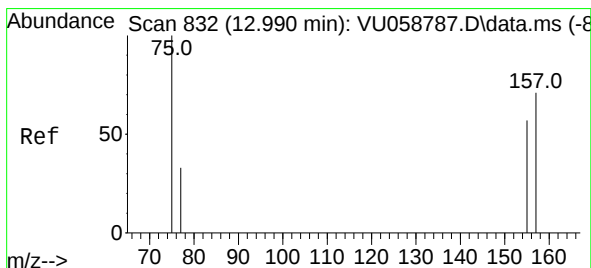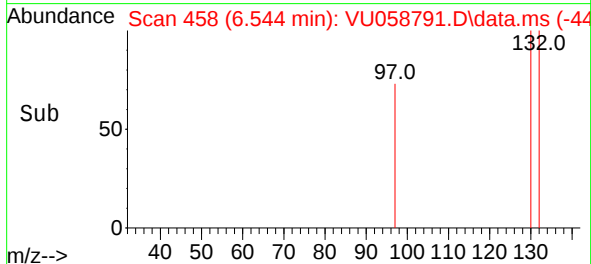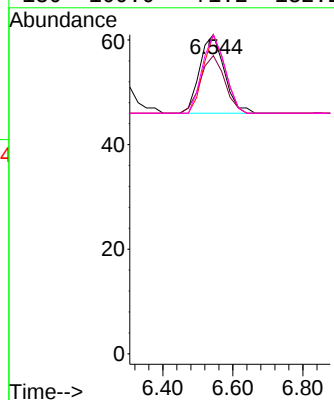

#13
1,2-Dibromo-3-chloropropane
Concen: 0.219 ug/L
RT: 12.751 min Scan# 818
Delta R.T. -0.240 min
Lab File: VU058791.D
Acq: 24 Apr 2024 13:33

Tgt Ion: 75 Resp: 74

Ion	Ratio	Lower	Upper
75	100		
157	63.9	67.5	101.3#
155	68.1	61.7	92.5

