


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042424\
Data File : VU058784.D
Acq On : 24 Apr 2024 08:58
Operator : MD/SY
Sample : BFB005
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB005

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM042424.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 25 01:37:46 2024

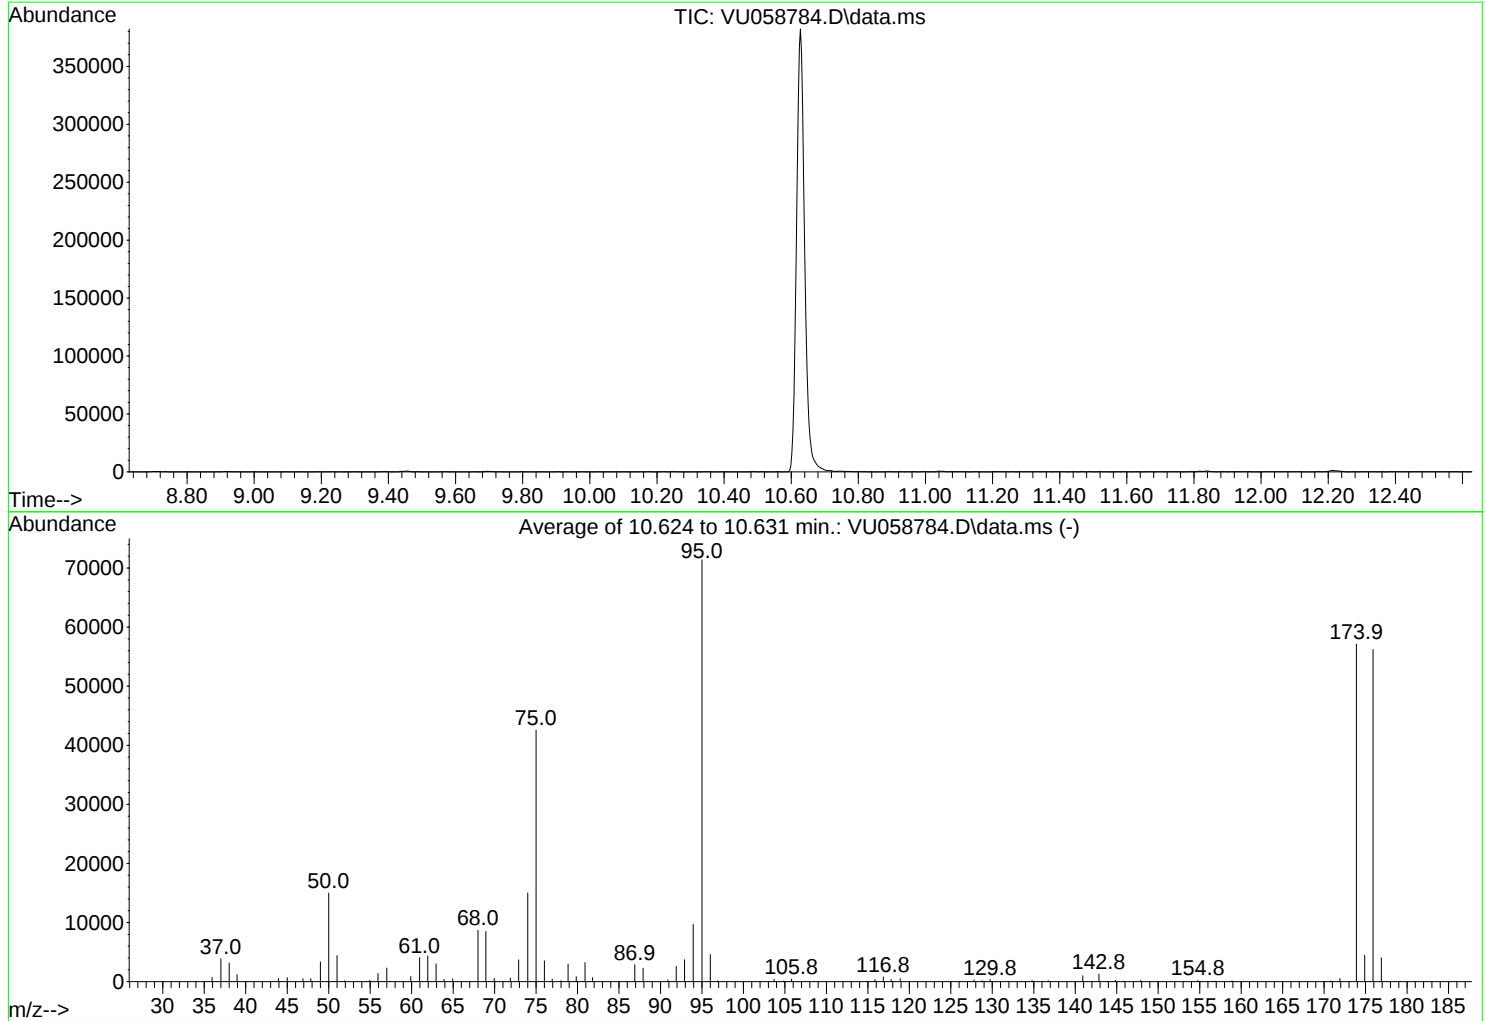

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	14974	PASS
75	95	30	80	59.6	42568	PASS
95	95	100	100	100.0	71376	PASS
96	95	5	9	6.4	4590	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.0	57128	PASS
175	174	5	9	7.8	4432	PASS
176	174	95	101	98.4	56221	PASS
177	176	5	9	7.1	4002	PASS

m/z	Abundance
73.90	116.0
74.90	299.0
95.00	396.0
173.90	315.0
175.90	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	768.0
37.00	3798.0
38.00	3160.0
38.90	1194.0
43.90	535.0
45.00	625.0
46.90	518.0
47.90	530.0
49.00	3375.0
50.00	14907.0
51.00	4574.0
51.90	198.0
54.90	221.0
55.90	1409.0
57.00	2358.0
59.90	787.0
61.00	3968.0
62.00	4270.0
63.00	3123.0
63.90	413.0
64.90	428.0
67.10	213.0
68.00	8654.0
69.00	8435.0
70.00	574.0
71.90	663.0
72.90	3537.0
74.00	15267.0
75.00	42520.0
76.00	3561.0
76.90	494.0
78.00	248.0
78.80	2948.0
79.90	836.0
80.90	3236.0
81.80	636.0
86.90	2906.0
87.90	2304.0
90.90	305.0
91.90	2646.0
92.90	3745.0
94.00	9415.0
95.00	71440.0
96.00	4438.0
96.90	117.0
103.70	354.0
104.90	114.0
105.80	433.0
115.80	349.0
116.80	837.0
117.80	311.0
118.90	582.0
127.80	316.0
128.80	176.0
129.80	396.0
134.70	203.0
136.80	162.0
140.90	1012.0
142.90	1178.0
144.90	225.0
147.90	268.0
154.80	255.0
156.90	134.0
158.90	120.0
170.80	100.0
171.90	476.0
173.90	56144.0
174.90	4316.0
175.90	54800.0
176.90	3900.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
35.90	782.0
37.00	3936.0
38.00	3209.0
38.90	1225.0
40.00	102.0
43.90	538.0
45.00	682.0
46.90	497.0
47.80	505.0
49.00	3405.0
50.00	15547.0
51.00	4549.0
51.90	175.0
55.00	204.0
56.00	1401.0
57.00	2396.0
59.90	887.0
60.90	4214.0
61.90	4539.0
63.00	3090.0
63.90	415.0
65.00	488.0
68.00	9055.0
68.90	8717.0
70.00	602.0
71.90	636.0
72.90	3836.0
74.00	15453.0
75.00	44120.0
76.00	3664.0
77.00	470.0
78.00	281.0
78.90	3068.0
79.80	862.0
80.90	3343.0
81.80	708.0
86.90	3060.0
87.90	2351.0
90.90	310.0
91.90	2640.0
92.90	3873.0
93.90	10033.0
95.00	73312.0
96.00	4771.0
96.90	149.0
103.70	427.0
104.80	122.0
105.80	471.0
114.90	124.0
115.80	339.0
116.90	836.0
117.80	367.0
118.90	537.0
127.80	311.0
128.80	164.0
129.80	367.0
130.50	107.0
134.80	222.0
136.70	151.0
140.90	1008.0
142.90	1304.0
144.90	216.0
145.80	101.0
147.90	243.0
154.80	274.0
156.60	120.0
157.00	112.0
158.90	146.0
170.80	124.0
171.90	547.0
173.90	58720.0
174.90	4517.0
175.90	58000.0
176.90	4149.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005

m/z	Abundance
36.00	673.0
37.00	3854.0
38.00	3040.0
39.00	1170.0
40.00	103.0
44.00	513.0
45.00	713.0
46.90	487.0
47.80	508.0
49.00	3223.0
50.00	14469.0
51.00	4091.0
51.90	141.0
55.00	203.0
56.00	1324.0
57.00	2156.0
59.90	912.0
60.90	4005.0
61.90	4257.0
62.90	2782.0
63.90	349.0
65.00	545.0
68.00	8359.0
68.90	8344.0
69.90	543.0
71.90	521.0
72.90	3707.0
74.00	14310.0
75.00	41064.0
76.00	3344.0
77.00	363.0
78.90	2940.0
79.80	852.0
80.90	3079.0
81.80	728.0
86.90	2669.0
87.90	2211.0
90.90	282.0
91.90	2418.0
92.90	3549.0
93.90	9598.0
95.00	69376.0
96.00	4562.0
96.90	171.0
103.70	466.0
104.80	120.0
105.80	438.0
106.70	111.0
114.90	117.0
115.90	340.0
116.90	731.0
117.80	361.0
118.90	466.0
127.80	266.0
128.70	140.0
129.70	311.0
130.50	105.0
134.90	225.0
136.70	143.0
140.90	961.0
142.80	1326.0
143.90	108.0
144.80	203.0
145.80	139.0
147.90	222.0
154.80	231.0
156.60	122.0
156.90	114.0
158.90	126.0
170.80	109.0
171.90	567.0
173.90	56520.0
174.90	4464.0
175.90	55864.0
176.90	3957.0

Instrument :
MSVOA_U
ClientSampleId :
BFB005