

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053968.D
 Acq On : 28 Apr 2023 14:10
 Operator : JC/MD
 Sample : 02549-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	94	rVB	105961	126005	15.74%	2.031%
2	1.912	170	178	191	rBV	105745	144720	18.08%	2.333%
3	2.565	369	381	399	rBV	176286	286717	35.81%	4.622%
4	2.848	465	469	470	rBV	257	157	0.02%	0.003%
5	3.041	523	529	536	rBV2	1030	1385	0.17%	0.022%
6	3.096	543	546	550	rBV	304	172	0.02%	0.003%
7	3.182	564	573	575	rBV2	1561	1967	0.25%	0.032%
8	3.343	619	623	626	rBB	173	168	0.02%	0.003%
9	3.359	626	628	630	rBV	307	190	0.02%	0.003%
10	3.452	656	657	661	rBV	220	144	0.02%	0.002%
11	3.616	705	708	710	rBV	239	188	0.02%	0.003%
12	3.713	733	738	742	rBV2	224	252	0.03%	0.004%
13	3.941	805	809	811	rBV	204	144	0.02%	0.002%
14	4.073	847	850	853	rBV2	263	229	0.03%	0.004%
15	4.115	861	863	867	rVB	395	266	0.03%	0.004%
16	4.211	891	893	898	rVB	308	225	0.03%	0.004%
17	4.298	918	920	928	rVV	177	207	0.03%	0.003%
18	4.388	945	948	952	rBB2	253	229	0.03%	0.004%
19	4.555	996	1000	1002	rBB	182	141	0.02%	0.002%
20	4.571	1003	1005	1010	rBV	272	213	0.03%	0.003%
21	4.626	1010	1022	1048	rBV	45171	119130	14.88%	1.920%
22	4.867	1095	1097	1100	rVB2	391	222	0.03%	0.004%
23	4.944	1119	1121	1126	rVB2	306	242	0.03%	0.004%
24	5.060	1140	1157	1181	rBV2	156384	339712	42.43%	5.476%
25	5.243	1211	1214	1216	rBV2	425	276	0.03%	0.004%
26	5.295	1226	1230	1231	rBV	213	137	0.02%	0.002%
27	5.314	1234	1236	1240	rVB2	299	200	0.02%	0.003%
28	5.337	1240	1243	1245	rBV2	395	250	0.03%	0.004%
29	5.378	1253	1256	1259	rBB	208	161	0.02%	0.003%
30	5.559	1308	1312	1315	rBB	165	162	0.02%	0.003%
31	5.581	1316	1319	1322	rBV2	415	304	0.04%	0.005%
32	5.722	1342	1363	1384	rBV2	295565	800648	100.00%	12.906%
33	5.948	1429	1433	1434	rBV2	194	165	0.02%	0.003%
34	5.989	1444	1446	1449	rVB	313	153	0.02%	0.002%
35	6.015	1449	1454	1456	rBB2	348	259	0.03%	0.004%
36	6.041	1460	1462	1465	rVB	453	228	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053968.D
 Acq On : 28 Apr 2023 14:10
 Operator : JC/MD
 Sample : 02549-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.128	1483	1489	1492	rBB2	458	404	0.05%	0.007%
38	6.147	1493	1495	1501	rBB	154	175	0.02%	0.003%
39	6.247	1509	1526	1544	rBV	273437	526019	65.70%	8.479%
40	6.394	1569	1572	1575	rBV2	223	171	0.02%	0.003%
41	6.459	1590	1592	1594	rVB2	351	164	0.02%	0.003%
42	6.491	1599	1602	1606	rVV2	306	223	0.03%	0.004%
43	6.533	1606	1615	1624	rVB8	2296	4211	0.53%	0.068%
44	6.687	1649	1663	1684	rBV	180431	353738	44.18%	5.702%
45	6.800	1694	1698	1700	rBV2	476	352	0.04%	0.006%
46	6.819	1702	1704	1707	rVB2	792	447	0.06%	0.007%
47	7.240	1831	1835	1837	rBV2	247	202	0.03%	0.003%
48	7.256	1837	1840	1843	rVB	275	187	0.02%	0.003%
49	7.497	1910	1915	1916	rBV	156	133	0.02%	0.002%
50	7.510	1916	1919	1922	rVB	238	141	0.02%	0.002%
51	7.562	1922	1935	1952	rBV	102670	182407	22.78%	2.940%
52	7.758	1993	1996	1998	rBV	190	152	0.02%	0.002%
53	7.793	2003	2007	2011	rVV2	209	209	0.03%	0.003%
54	7.893	2025	2038	2068	rVV	383098	669002	83.56%	10.784%
55	8.111	2102	2106	2107	rBV2	255	157	0.02%	0.003%
56	8.176	2113	2126	2142	rBV2	71479	121716	15.20%	1.962%
57	8.462	2206	2215	2216	rBV	919	877	0.11%	0.014%
58	8.552	2231	2243	2252	rBB7	7024	11565	1.44%	0.186%
59	8.629	2256	2267	2298	rBV	146596	276591	34.55%	4.458%
60	8.828	2327	2329	2332	rBV	229	149	0.02%	0.002%
61	8.848	2332	2335	2338	rVV	258	192	0.02%	0.003%
62	9.021	2380	2389	2394	rBV2	325	558	0.07%	0.009%
63	9.086	2406	2409	2412	rBV	227	186	0.02%	0.003%
64	9.163	2430	2433	2436	rBV	200	173	0.02%	0.003%
65	9.211	2445	2448	2452	rBV	201	169	0.02%	0.003%
66	9.330	2480	2485	2486	rBV	207	209	0.03%	0.003%
67	9.414	2497	2511	2532	rBV	378753	621658	77.64%	10.021%
68	9.571	2558	2560	2565	rVB2	390	300	0.04%	0.005%
69	9.690	2595	2597	2600	rVV	289	144	0.02%	0.002%
70	9.709	2601	2603	2610	rVB3	498	403	0.05%	0.006%
71	9.748	2610	2615	2618	rBV	246	268	0.03%	0.004%
72	10.041	2701	2706	2708	rBV	184	215	0.03%	0.003%
73	10.102	2723	2725	2727	rVV	361	135	0.02%	0.002%
74	10.115	2727	2729	2732	rVB	337	164	0.02%	0.003%
75	10.150	2737	2740	2745	rBV	256	298	0.04%	0.005%
76	10.285	2780	2782	2788	rVB	202	139	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053968.D
 Acq On : 28 Apr 2023 14:10
 Operator : JC/MD
 Sample : 02549-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DCCT2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	10.311	2788	2790	2795	rBV	200	134	0.02%	0.002%
78	10.385	2810	2813	2821	rBV2	164	188	0.02%	0.003%
79	10.491	2844	2846	2849	rBV	237	149	0.02%	0.002%
80	10.536	2857	2860	2863	rBV	299	235	0.03%	0.004%
81	10.632	2887	2890	2891	rBV	308	136	0.02%	0.002%
82	10.751	2914	2927	2942	rBV	248901	400744	50.05%	6.460%
83	10.886	2963	2969	2971	rBV2	1043	1058	0.13%	0.017%
84	11.471	3148	3151	3153	rBB2	308	174	0.02%	0.003%
85	11.552	3173	3176	3181	rBV	197	186	0.02%	0.003%
86	11.738	3232	3234	3235	rBV	404	159	0.02%	0.003%
87	11.806	3244	3255	3275	rBV	374979	597328	74.61%	9.628%
88	12.188	3362	3374	3390	rBV	373509	599162	74.83%	9.658%
89	12.346	3421	3423	3426	rVB	269	137	0.02%	0.002%
90	12.471	3459	3462	3464	rBV	233	137	0.02%	0.002%
91	12.754	3547	3550	3552	rBV2	259	165	0.02%	0.003%
92	12.883	3587	3590	3595	rBV	312	203	0.03%	0.003%
93	13.352	3733	3736	3738	rBV2	338	174	0.02%	0.003%
94	13.703	3843	3845	3847	rBV2	333	182	0.02%	0.003%
95	13.841	3883	3888	3890	rBV2	1042	807	0.10%	0.013%
96	14.201	3996	4000	4006	rBV3	483	528	0.07%	0.009%
97	14.256	4013	4017	4020	rBV	410	331	0.04%	0.005%
98	14.385	4054	4057	4058	rBV	333	228	0.03%	0.004%
99	14.757	4171	4173	4178	rBV2	301	219	0.03%	0.004%
100	14.905	4216	4219	4225	rBV2	457	496	0.06%	0.008%




Sum of corrected areas: 6203831

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053968.D
Acq On : 28 Apr 2023 14:10
Operator : JC/MD
Sample : 02549-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

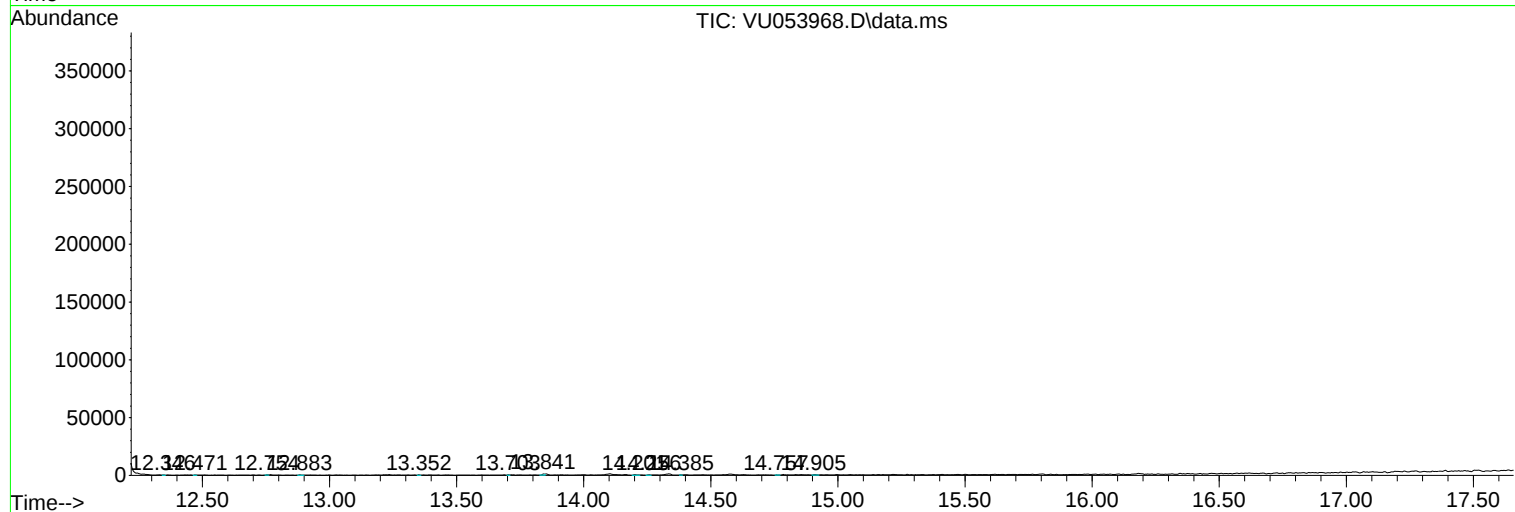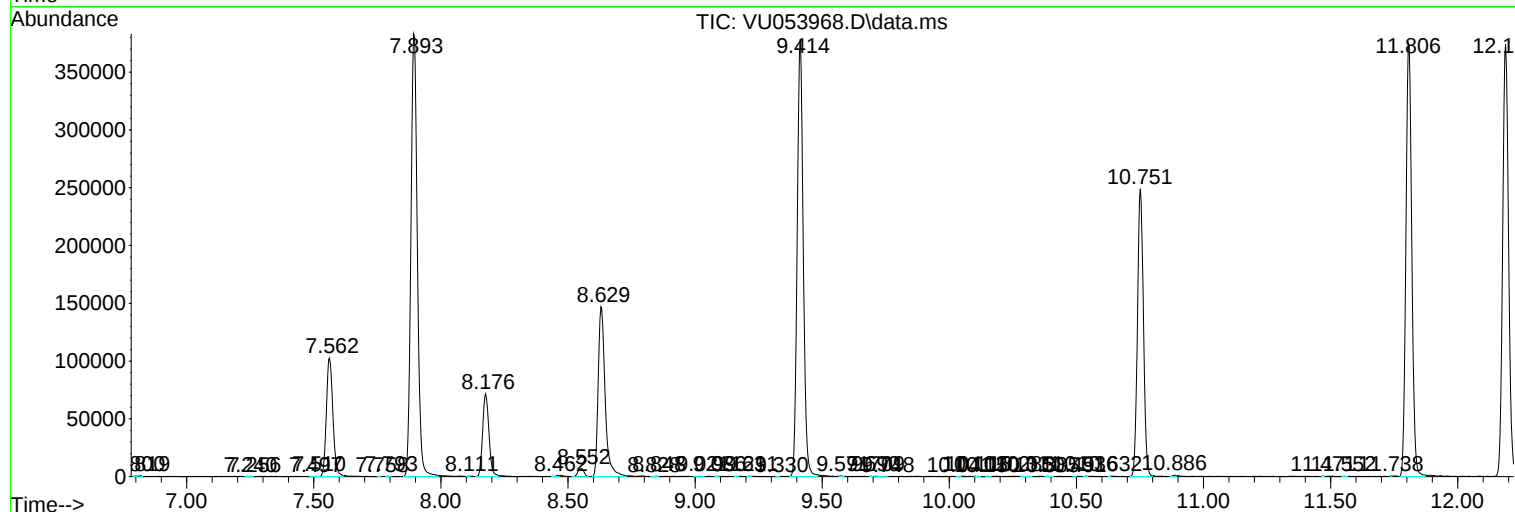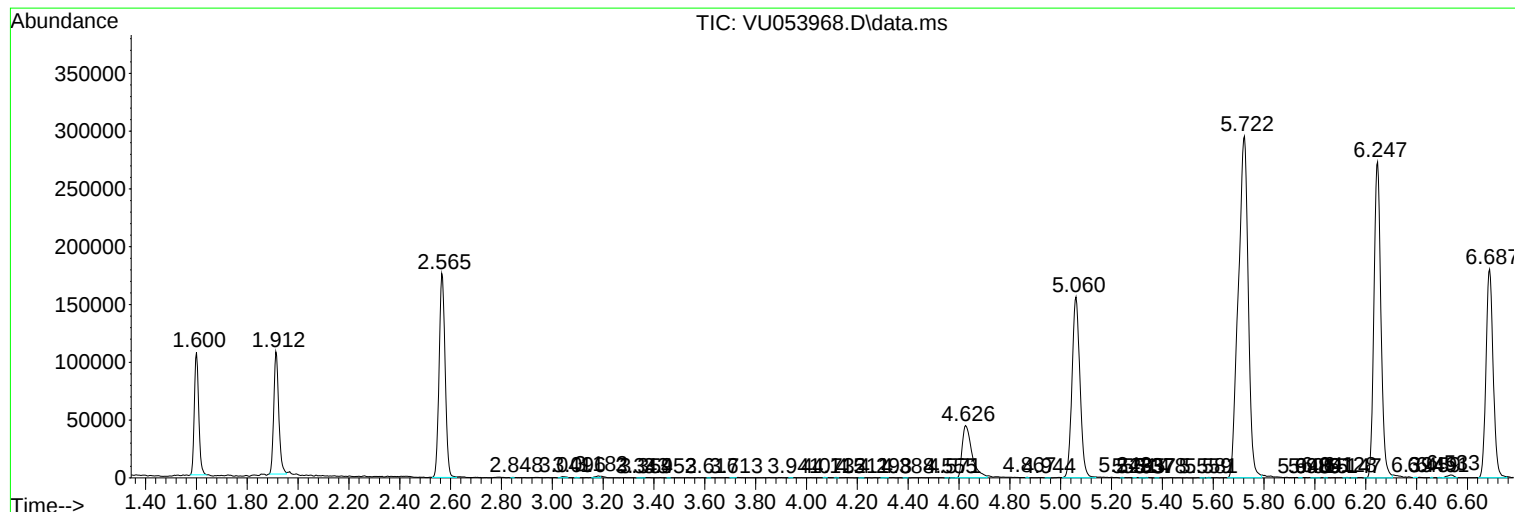

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053968.D
Acq On : 28 Apr 2023 14:10
Operator : JC/MD
Sample : 02549-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053968.D
Acq On : 28 Apr 2023 14:10
Operator : JC/MD
Sample : 02549-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DCCT2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------