

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053969.D
 Acq On : 28 Apr 2023 14:34
 Operator : JC/MD
 Sample : 02549-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

Signal : TIC: VU053969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	99	rBV	105331	123604	15.90%	2.064%
2	1.912	170	178	196	rVB	104187	142263	18.30%	2.376%
3	2.565	369	381	402	rBV	165897	268996	34.61%	4.492%
4	2.729	430	432	436	rVB	312	167	0.02%	0.003%
5	2.784	447	449	455	rBV	273	333	0.04%	0.006%
6	2.948	497	500	506	rBV	293	170	0.02%	0.003%
7	2.990	510	513	517	rBV2	233	177	0.02%	0.003%
8	3.047	521	531	540	rVB5	2400	4640	0.60%	0.077%
9	3.543	681	685	692	rBB	322	444	0.06%	0.007%
10	3.581	693	697	699	rBV2	276	189	0.02%	0.003%
11	3.604	702	704	709	rVB	268	216	0.03%	0.004%
12	3.655	718	720	724	rBV	198	191	0.02%	0.003%
13	3.896	793	795	797	rBB	266	123	0.02%	0.002%
14	3.919	798	802	809	rBV	200	289	0.04%	0.005%
15	4.080	849	852	853	rBV	240	142	0.02%	0.002%
16	4.128	865	867	869	rBV	260	170	0.02%	0.003%
17	4.144	870	872	877	rVB2	377	312	0.04%	0.005%
18	4.173	878	881	886	rBV	162	193	0.02%	0.003%
19	4.240	899	902	903	rBV	189	124	0.02%	0.002%
20	4.324	926	928	937	rBV	218	330	0.04%	0.006%
21	4.417	955	957	959	rBV	199	136	0.02%	0.002%
22	4.623	1011	1021	1048	rBV2	47267	123652	15.91%	2.065%
23	4.890	1099	1104	1106	rBV2	284	239	0.03%	0.004%
24	5.060	1139	1157	1178	rBV	145757	318541	40.98%	5.320%
25	5.337	1240	1243	1246	rVB	495	254	0.03%	0.004%
26	5.362	1247	1251	1253	rBV2	243	156	0.02%	0.003%
27	5.462	1279	1282	1284	rBV	228	133	0.02%	0.002%
28	5.559	1306	1312	1315	rBV	200	237	0.03%	0.004%
29	5.575	1315	1317	1321	rVB	307	198	0.03%	0.003%
30	5.636	1327	1336	1340	rBV2	291	409	0.05%	0.007%
31	5.719	1340	1362	1389	rBV2	283571	777293	100.00%	12.980%
32	6.047	1462	1464	1466	rBV	283	162	0.02%	0.003%
33	6.105	1479	1482	1484	rBV	290	163	0.02%	0.003%
34	6.166	1497	1501	1506	rBV	263	303	0.04%	0.005%
35	6.243	1512	1525	1548	rBV	258137	493659	63.51%	8.244%
36	6.459	1589	1592	1594	rBV	244	145	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053969.D
 Acq On : 28 Apr 2023 14:34
 Operator : JC/MD
 Sample : 02549-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	6.526	1604	1613	1614	rBV2	2500	2568	0.33%	0.043%
38	6.588	1628	1632	1635	rBB	218	193	0.02%	0.003%
39	6.684	1647	1662	1685	rBV	176438	345741	44.48%	5.774%
40	6.803	1697	1699	1705	rVB2	280	249	0.03%	0.004%
41	6.880	1721	1723	1725	rBV	208	135	0.02%	0.002%
42	6.922	1732	1736	1740	rBV	338	328	0.04%	0.005%
43	6.970	1747	1751	1756	rBV2	270	295	0.04%	0.005%
44	6.996	1756	1759	1762	rVB	238	132	0.02%	0.002%
45	7.044	1770	1774	1777	rVB2	348	272	0.03%	0.005%
46	7.063	1778	1780	1785	rBB	183	148	0.02%	0.002%
47	7.134	1800	1802	1805	rVB	264	126	0.02%	0.002%
48	7.157	1805	1809	1813	rBB	266	229	0.03%	0.004%
49	7.202	1818	1823	1826	rBV3	414	393	0.05%	0.007%
50	7.243	1833	1836	1840	rBB	162	152	0.02%	0.003%
51	7.301	1850	1854	1858	rBV2	355	380	0.05%	0.006%
52	7.388	1878	1881	1887	rVV2	217	186	0.02%	0.003%
53	7.456	1900	1902	1903	rBV2	255	128	0.02%	0.002%
54	7.504	1914	1917	1920	rBV	198	190	0.02%	0.003%
55	7.562	1923	1935	1963	rVB2	100979	179526	23.10%	2.998%
56	7.697	1974	1977	1980	rBV2	417	272	0.03%	0.005%
57	7.893	2025	2038	2061	rBV	364319	638038	82.08%	10.655%
58	8.176	2115	2126	2139	rBV	71148	117883	15.17%	1.969%
59	8.301	2161	2165	2170	rBB	192	236	0.03%	0.004%
60	8.327	2170	2173	2174	rBV	233	123	0.02%	0.002%
61	8.372	2184	2187	2191	rBV	262	183	0.02%	0.003%
62	8.452	2207	2212	2214	rBV	279	249	0.03%	0.004%
63	8.510	2226	2230	2232	rBV	192	184	0.02%	0.003%
64	8.549	2233	2242	2256	rVB5	8061	13260	1.71%	0.221%
65	8.629	2256	2267	2301	rBV	151032	284963	36.66%	4.759%
66	8.793	2316	2318	2323	rVB	344	287	0.04%	0.005%
67	8.816	2323	2325	2327	rBV2	360	231	0.03%	0.004%
68	8.938	2361	2363	2366	rVV	222	129	0.02%	0.002%
69	8.980	2374	2376	2377	rBV	256	122	0.02%	0.002%
70	9.015	2382	2387	2392	rBV2	226	301	0.04%	0.005%
71	9.131	2420	2423	2427	rBV	269	194	0.02%	0.003%
72	9.243	2455	2458	2460	rBV	347	198	0.03%	0.003%
73	9.414	2498	2511	2533	rBV	351674	586413	75.44%	9.793%
74	9.568	2556	2559	2563	rVB2	539	392	0.05%	0.007%
75	9.594	2563	2567	2569	rBV2	344	257	0.03%	0.004%
76	9.610	2569	2572	2575	rVB2	239	133	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053969.D
 Acq On : 28 Apr 2023 14:34
 Operator : JC/MD
 Sample : 02549-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	9.645	2580	2583	2585	rBB	225	149	0.02%	0.002%
78	9.661	2586	2588	2590	rBV	184	120	0.02%	0.002%
79	9.751	2614	2616	2623	rVB	209	151	0.02%	0.003%
80	9.784	2623	2626	2630	rVB	299	229	0.03%	0.004%
81	9.803	2630	2632	2635	rBV	157	136	0.02%	0.002%
82	10.285	2779	2782	2785	rBV2	335	272	0.03%	0.005%
83	10.462	2833	2837	2838	rBV	199	147	0.02%	0.002%
84	10.629	2887	2889	2894	rVB3	313	189	0.02%	0.003%
85	10.751	2914	2927	2947	rVV	247035	401918	51.71%	6.712%
86	10.857	2958	2960	2965	rBV	210	140	0.02%	0.002%
87	10.957	2989	2991	2999	rVB	226	164	0.02%	0.003%
88	11.044	3015	3018	3021	rBV	243	146	0.02%	0.002%
89	11.472	3146	3151	3155	rVB2	253	287	0.04%	0.005%
90	11.623	3195	3198	3201	rBV	200	172	0.02%	0.003%
91	11.806	3244	3255	3271	rBV	354706	564060	72.57%	9.420%
92	12.037	3324	3327	3330	rBV2	191	127	0.02%	0.002%
93	12.189	3361	3374	3391	rBV	368129	582744	74.97%	9.732%
94	12.578	3492	3495	3499	rBV	232	167	0.02%	0.003%
95	13.224	3694	3696	3699	rVB	337	228	0.03%	0.004%
96	14.098	3961	3968	3971	rBV2	993	1324	0.17%	0.022%
97	14.324	4035	4038	4040	rBV3	463	385	0.05%	0.006%
98	14.417	4064	4067	4069	rBV	183	121	0.02%	0.002%
99	14.488	4087	4089	4092	rBV	320	166	0.02%	0.003%
100	15.031	4255	4258	4263	rBV2	401	456	0.06%	0.008%




Sum of corrected areas: 5988170

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053969.D
Acq On : 28 Apr 2023 14:34
Operator : JC/MD
Sample : 02549-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

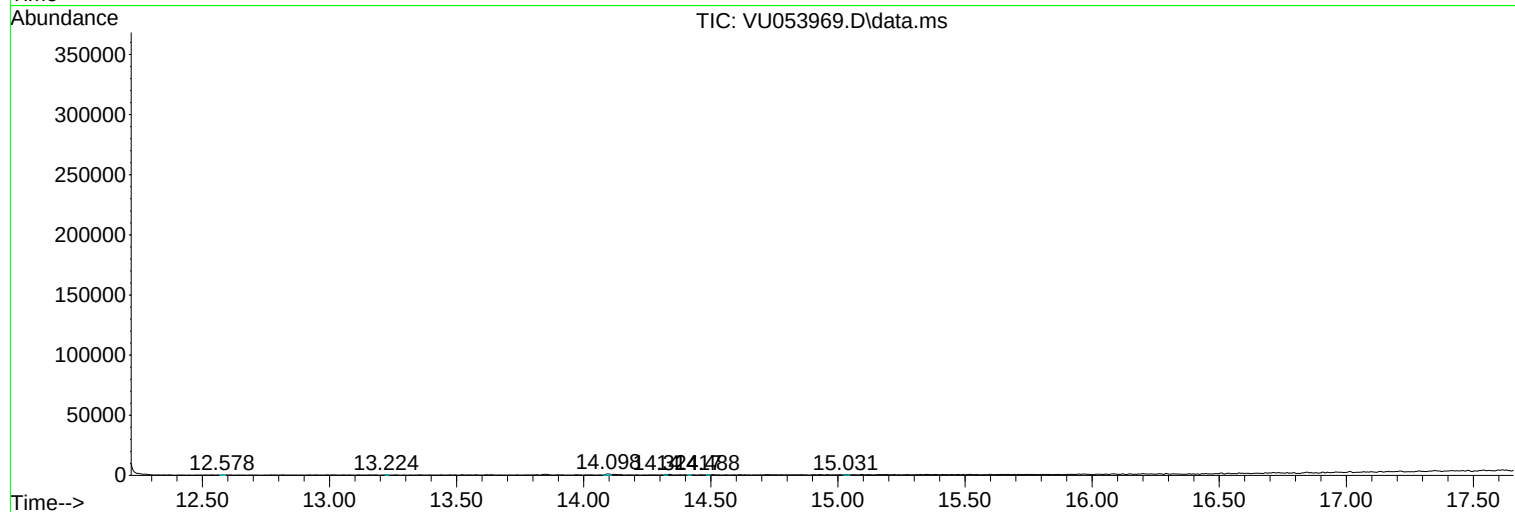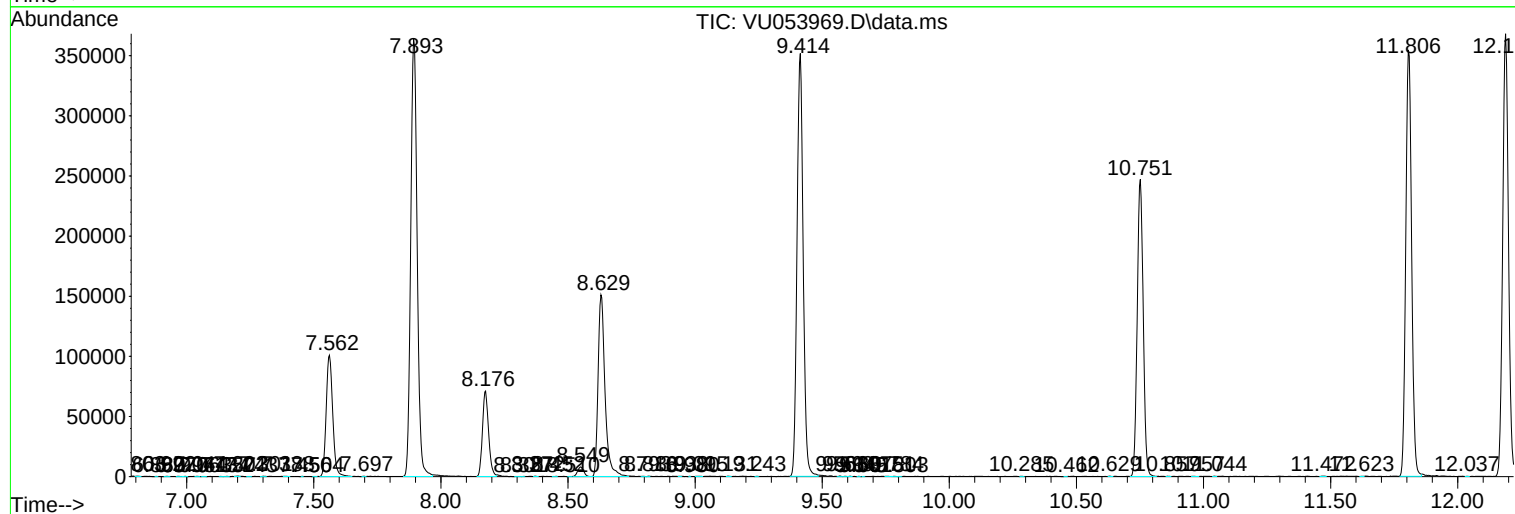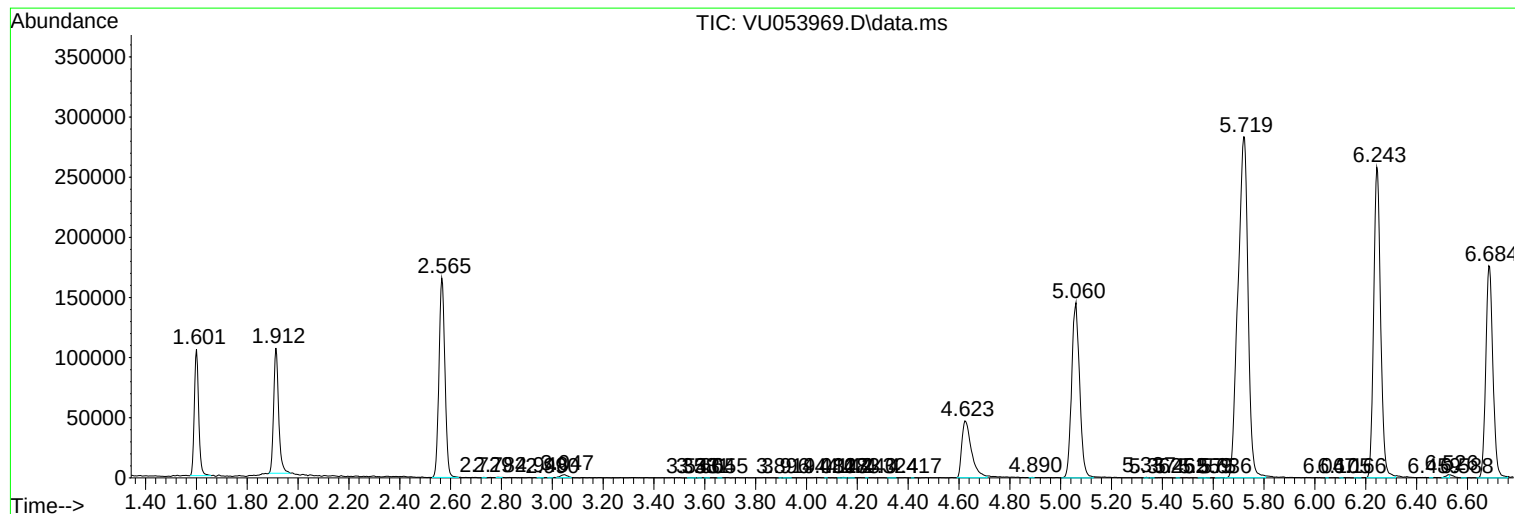

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053969.D
Acq On : 28 Apr 2023 14:34
Operator : JC/MD
Sample : 02549-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053969.D
Acq On : 28 Apr 2023 14:34
Operator : JC/MD
Sample : 02549-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc