

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053975.D
 Acq On : 28 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02548-47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M

Title : VOC Analysis

Signal : TIC: VU053975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	73	80	93	rBV	95518	117296	14.63%	1.927%
2	1.912	171	178	195	rVB	108285	144707	18.05%	2.378%
3	2.475	351	353	355	rBV	430	186	0.02%	0.003%
4	2.565	368	381	398	rBV	160923	263275	32.84%	4.326%
5	2.922	488	492	493	rBV	321	215	0.03%	0.004%
6	2.980	507	510	515	rBV2	193	199	0.02%	0.003%
7	3.044	523	530	541	rVB4	1768	2936	0.37%	0.048%
8	3.125	552	555	560	rVB	279	192	0.02%	0.003%
9	3.186	562	574	583	rBV3	2398	4703	0.59%	0.077%
10	3.314	611	614	617	rVV	387	281	0.04%	0.005%
11	3.420	645	647	650	rBB	276	150	0.02%	0.002%
12	3.491	668	669	673	rVB	270	154	0.02%	0.003%
13	3.890	790	793	799	rBV	202	290	0.04%	0.005%
14	3.945	807	810	812	rBV	188	152	0.02%	0.002%
15	4.060	844	846	849	rVV	265	163	0.02%	0.003%
16	4.080	849	852	854	rVV2	267	150	0.02%	0.002%
17	4.109	857	861	865	rBV	216	276	0.03%	0.005%
18	4.160	874	877	879	rBV	259	185	0.02%	0.003%
19	4.256	905	907	909	rBV	328	214	0.03%	0.004%
20	4.334	929	931	935	rVB2	344	252	0.03%	0.004%
21	4.401	946	952	955	rVV	319	333	0.04%	0.005%
22	4.472	972	974	978	rBV2	350	285	0.04%	0.005%
23	4.626	1009	1022	1044	rBV	50256	127535	15.91%	2.096%
24	4.848	1088	1091	1093	rBV	276	163	0.02%	0.003%
25	4.906	1106	1109	1111	rBV	357	201	0.03%	0.003%
26	5.057	1140	1156	1177	rBV	154149	336283	41.95%	5.526%
27	5.208	1200	1203	1206	rVB2	455	374	0.05%	0.006%
28	5.227	1206	1209	1212	rVB2	303	223	0.03%	0.004%
29	5.247	1212	1215	1216	rBV	335	204	0.03%	0.003%
30	5.266	1219	1221	1225	rVB	320	220	0.03%	0.004%
31	5.289	1225	1228	1231	rBB2	368	205	0.03%	0.003%
32	5.317	1234	1237	1239	rBV	185	156	0.02%	0.003%
33	5.330	1239	1241	1245	rVB2	355	212	0.03%	0.003%
34	5.356	1246	1249	1253	rBB	165	155	0.02%	0.003%
35	5.379	1254	1256	1261	rBV	172	196	0.02%	0.003%
36	5.430	1269	1272	1275	rBV2	318	285	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053975.D
 Acq On : 28 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02548-47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

37	5.514	1295	1298	1301	rBV2	310	242	0.03%	0.004%
38	5.719	1340	1362	1385	rBV2	293233	801623	100.00%	13.172%
39	5.916	1420	1423	1427	rVB2	347	285	0.04%	0.005%
40	5.951	1430	1434	1435	rBV2	240	158	0.02%	0.003%
41	6.009	1449	1452	1454	rBV	311	226	0.03%	0.004%
42	6.125	1484	1488	1491	rVB2	304	276	0.03%	0.005%
43	6.144	1491	1494	1498	rBV2	224	181	0.02%	0.003%
44	6.179	1503	1505	1509	rVB	321	182	0.02%	0.003%
45	6.243	1512	1525	1545	rBV	258282	490850	61.23%	8.066%
46	6.446	1585	1588	1589	rBV2	280	180	0.02%	0.003%
47	6.530	1605	1614	1623	rBV6	2234	4273	0.53%	0.070%
48	6.588	1629	1632	1638	rVB	336	326	0.04%	0.005%
49	6.684	1649	1662	1681	rBV	182312	357597	44.61%	5.876%
50	7.134	1799	1802	1805	rBV	253	149	0.02%	0.002%
51	7.182	1814	1817	1818	rBV	288	191	0.02%	0.003%
52	7.198	1818	1822	1825	rVV	352	331	0.04%	0.005%
53	7.260	1838	1841	1845	rVV	304	251	0.03%	0.004%
54	7.282	1845	1848	1850	rVV2	354	251	0.03%	0.004%
55	7.301	1852	1854	1857	rVB	293	161	0.02%	0.003%
56	7.369	1869	1875	1879	rBV	207	307	0.04%	0.005%
57	7.388	1879	1881	1884	rVV	383	167	0.02%	0.003%
58	7.562	1922	1935	1955	rBV	100710	179347	22.37%	2.947%
59	7.694	1971	1976	1981	rVB4	671	756	0.09%	0.012%
60	7.893	2025	2038	2066	rVV	375288	651112	81.22%	10.699%
61	8.176	2115	2126	2145	rBV	71129	121167	15.12%	1.991%
62	8.385	2188	2191	2196	rBV	228	270	0.03%	0.004%
63	8.462	2207	2215	2224	rVV3	644	1308	0.16%	0.021%
64	8.549	2234	2242	2252	rVB4	6327	9674	1.21%	0.159%
65	8.632	2256	2268	2302	rBV	158878	299274	37.33%	4.918%
66	8.886	2344	2347	2353	rBB2	422	402	0.05%	0.007%
67	8.922	2354	2358	2366	rBV2	297	479	0.06%	0.008%
68	9.038	2390	2394	2397	rBV2	349	280	0.03%	0.005%
69	9.076	2403	2406	2410	rVB2	325	243	0.03%	0.004%
70	9.108	2414	2416	2421	rVB	294	209	0.03%	0.003%
71	9.147	2422	2428	2430	rBV	190	200	0.02%	0.003%
72	9.276	2465	2468	2471	rVB2	210	149	0.02%	0.002%
73	9.414	2498	2511	2545	rBV	350769	584047	72.86%	9.597%
74	9.636	2578	2580	2583	rBB	271	163	0.02%	0.003%
75	9.655	2583	2586	2589	rBV2	334	261	0.03%	0.004%
76	9.825	2635	2639	2642	rVB	449	378	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
 Data File : VU053975.D
 Acq On : 28 Apr 2023 17:34
 Operator : JC/MD
 Sample : 02548-47
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
 Title : VOC Analysis

77	9.845	2642	2645	2649	rBV2	261	250	0.03%	0.004%
78	9.915	2662	2667	2670	rBV	215	284	0.04%	0.005%
79	10.095	2721	2723	2729	rBV2	540	463	0.06%	0.008%
80	10.134	2732	2735	2738	rBV	259	232	0.03%	0.004%
81	10.369	2805	2808	2810	rBV	197	145	0.02%	0.002%
82	10.417	2820	2823	2828	rVB2	394	396	0.05%	0.007%
83	10.452	2829	2834	2836	rBV	215	247	0.03%	0.004%
84	10.494	2844	2847	2852	rVB	361	319	0.04%	0.005%
85	10.526	2852	2857	2862	rBV2	433	636	0.08%	0.010%
86	10.751	2914	2927	2948	rBV	264045	422125	52.66%	6.936%
87	10.944	2984	2987	2990	rVB2	251	182	0.02%	0.003%
88	11.433	3135	3139	3140	rBV	208	164	0.02%	0.003%
89	11.806	3243	3255	3273	rBV	347903	554318	69.15%	9.108%
90	12.009	3315	3318	3321	rBV	335	190	0.02%	0.003%
91	12.060	3331	3334	3337	rBV	235	180	0.02%	0.003%
92	12.079	3337	3340	3344	rVV4	515	351	0.04%	0.006%
93	12.189	3361	3374	3400	rBV	364618	592085	73.86%	9.729%
94	12.340	3418	3421	3425	rVB	391	219	0.03%	0.004%
95	12.980	3617	3620	3623	rBV2	222	163	0.02%	0.003%
96	13.533	3789	3792	3794	rVB	417	207	0.03%	0.003%
97	13.680	3833	3838	3841	rBV2	324	310	0.04%	0.005%
98	14.346	4037	4045	4047	rBV2	451	546	0.07%	0.009%
99	14.520	4097	4099	4104	rBV	305	212	0.03%	0.003%
100	14.561	4108	4112	4116	rBV3	563	588	0.07%	0.010%




Sum of corrected areas: 6085744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053975.D
Acq On : 28 Apr 2023 17:34
Operator : JC/MD
Sample : 02548-47
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

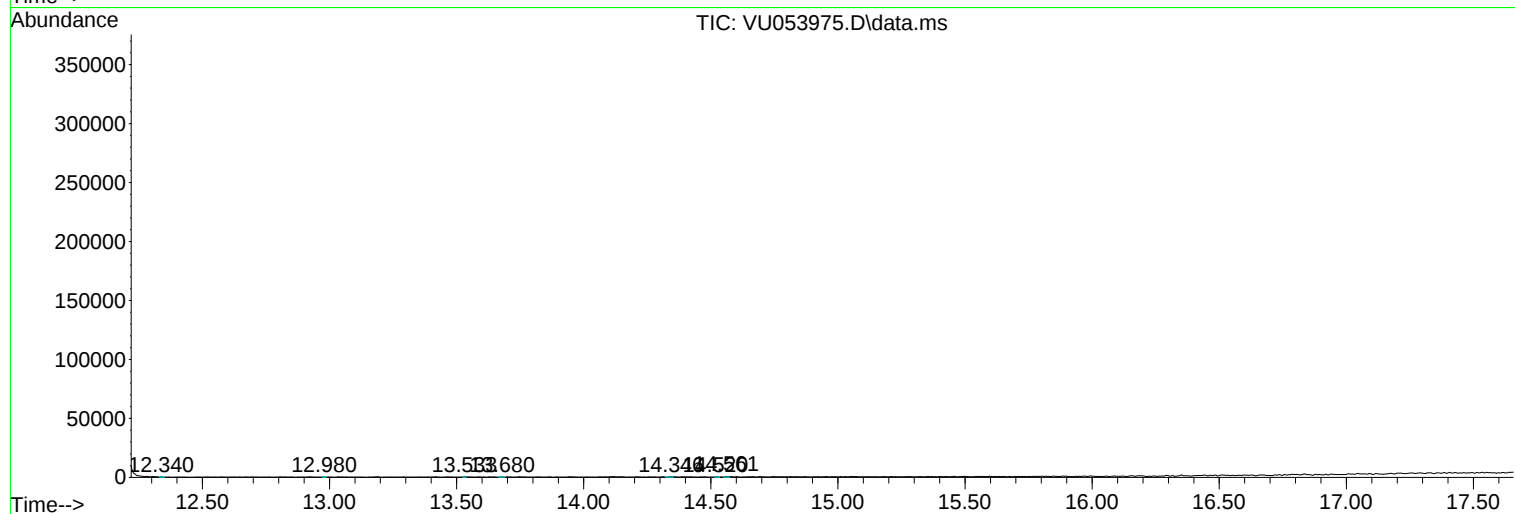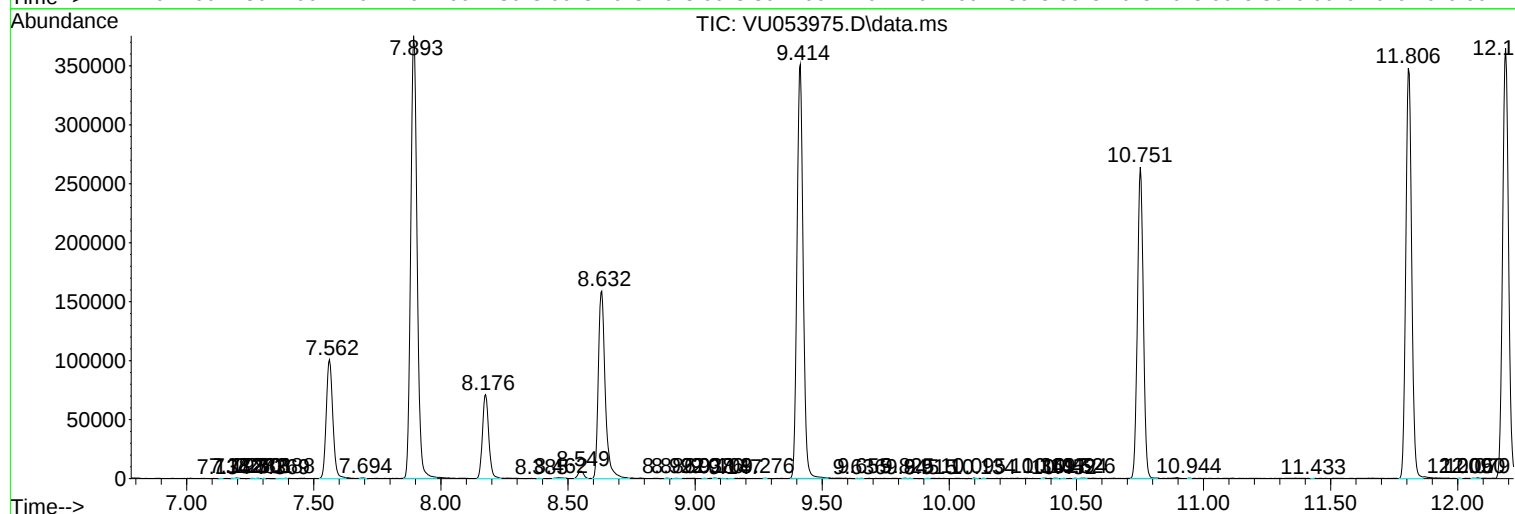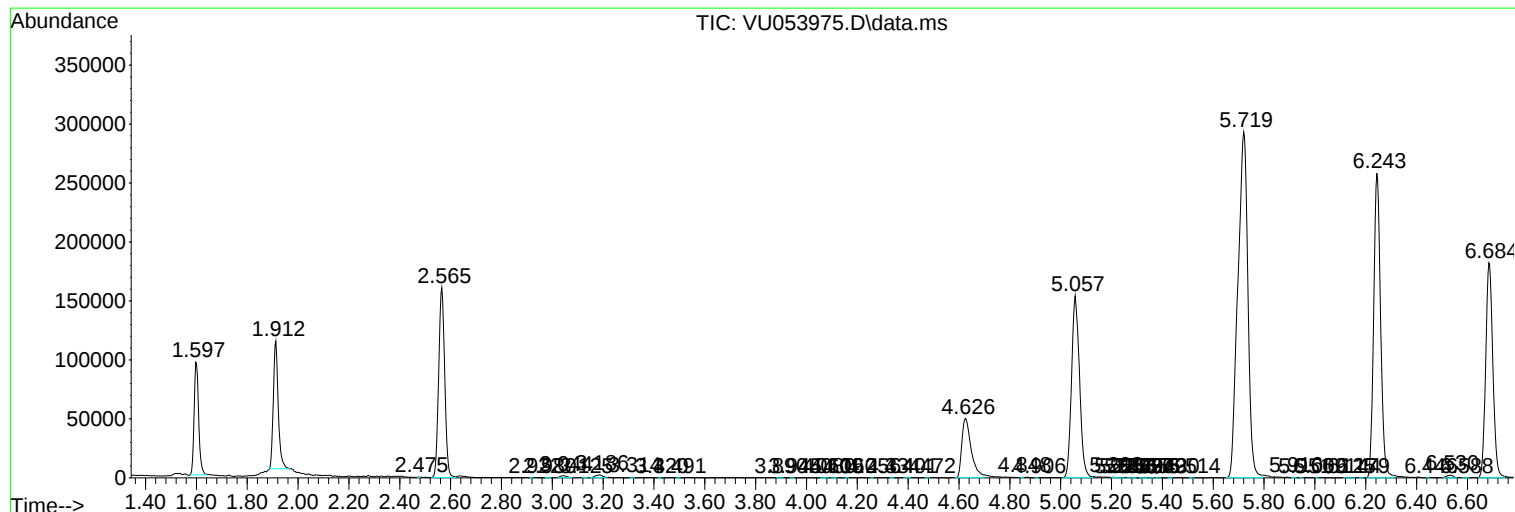

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053975.D
Acq On : 28 Apr 2023 17:34
Operator : JC/MD
Sample : 02548-47
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042923\
Data File : VU053975.D
Acq On : 28 Apr 2023 17:34
Operator : JC/MD
Sample : 02548-47
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM033123WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------