

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037951.D
 Acq On : 30 Apr 2020 15:02
 Operator : JC/MD
 Sample : L2395-01 800X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	76	84	99	rBV2	515953	569246	18.64%	2.363%
2	1.925	173	182	196	rVB	348027	459435	15.04%	1.907%
3	2.588	376	388	404	rBV2	634704	1072214	35.11%	4.451%
4	2.713	424	427	430	rBV4	1184	868	0.03%	0.004%
5	2.819	456	460	472	rVB3	2996	3987	0.13%	0.017%
6	2.861	472	473	478	rVB2	591	382	0.01%	0.002%
7	2.974	504	508	512	rBV3	600	583	0.02%	0.002%
8	2.996	512	515	519	rVB	630	434	0.01%	0.002%
9	3.070	532	538	540	rBV5	2187	2376	0.08%	0.010%
10	3.215	571	583	596	rBV2	6075	14225	0.47%	0.059%
11	3.263	596	598	604	rVB2	1138	683	0.02%	0.003%
12	3.388	626	637	649	rVB3	7013	13875	0.45%	0.058%
13	3.446	649	655	658	rBV4	553	556	0.02%	0.002%
14	3.588	695	699	703	rVB4	468	473	0.02%	0.002%
15	3.678	723	727	733	rVB3	696	630	0.02%	0.003%
16	3.829	770	774	777	rBV3	534	357	0.01%	0.001%
17	3.909	788	799	812	rVB3	4992	10876	0.36%	0.045%
18	3.980	819	821	825	rVB2	495	402	0.01%	0.002%
19	4.009	825	830	834	rVB4	488	519	0.02%	0.002%
20	4.044	839	841	844	rBV2	491	395	0.01%	0.002%
21	4.202	888	890	895	rVB	556	407	0.01%	0.002%
22	4.568	1000	1004	1008	rVB3	662	562	0.02%	0.002%
23	4.665	1017	1034	1039	rBV	344379	726501	23.79%	3.016%
24	4.919	1111	1113	1117	rVB2	723	394	0.01%	0.002%
25	4.945	1117	1121	1126	rVB4	578	540	0.02%	0.002%
26	4.973	1126	1130	1135	rVB5	704	627	0.02%	0.003%
27	5.015	1138	1143	1145	rBV4	526	424	0.01%	0.002%
28	5.102	1150	1170	1193	rBV	509900	1150555	37.67%	4.776%
29	5.289	1226	1228	1232	rVB3	835	555	0.02%	0.002%
30	5.353	1232	1248	1260	rBV5	10924	25841	0.85%	0.107%
31	5.520	1295	1300	1304	rBV3	608	781	0.03%	0.003%
32	5.588	1318	1321	1326	rVB2	770	512	0.02%	0.002%
33	5.758	1352	1374	1404	rVV2	1160753	3054260	100.00%	12.678%
34	5.941	1429	1431	1437	rVB5	934	551	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037951.D
 Acq On : 30 Apr 2020 15:02
 Operator : JC/MD
 Sample : L2395-01 800X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	6.044	1460	1463	1464	rBV	878	466	0.02%	0.002%
36	6.131	1486	1490	1491	rBV3	717	531	0.02%	0.002%
37	6.279	1520	1536	1569	rBV	945392	1787542	58.53%	7.420%
38	6.475	1594	1597	1599	rBV2	691	450	0.01%	0.002%
39	6.568	1613	1626	1641	rBV9	15386	39134	1.28%	0.162%
40	6.719	1658	1673	1694	rBV	721917	1403458	45.95%	5.826%
41	6.922	1732	1736	1739	rBV4	768	488	0.02%	0.002%
42	7.070	1780	1782	1787	rVB	534	396	0.01%	0.002%
43	7.195	1817	1821	1825	rBV4	1501	1724	0.06%	0.007%
44	7.382	1875	1879	1884	rBV3	538	498	0.02%	0.002%
45	7.591	1930	1944	1963	rVV	428432	731724	23.96%	3.037%
46	7.661	1963	1966	1972	rVB3	917	727	0.02%	0.003%
47	7.700	1975	1978	1981	rBV4	888	726	0.02%	0.003%
48	7.816	2008	2014	2025	rVB4	2595	4135	0.14%	0.017%
49	7.922	2032	2047	2082	rBV	1385142	2531018	82.87%	10.506%
50	8.202	2121	2134	2152	rBV	292105	484017	15.85%	2.009%
51	8.420	2196	2202	2203	rBV2	1064	888	0.03%	0.004%
52	8.491	2218	2224	2230	rBV4	1158	1356	0.04%	0.006%
53	8.575	2241	2250	2261	rBV3	12883	20854	0.68%	0.087%
54	8.655	2261	2275	2315	rBV	914166	1731060	56.68%	7.186%
55	8.935	2353	2362	2371	rBV6	6715	13214	0.43%	0.055%
56	9.057	2397	2400	2405	rVB4	739	698	0.02%	0.003%
57	9.185	2431	2440	2446	rBV5	1835	2758	0.09%	0.011%
58	9.211	2446	2448	2454	rVB2	648	464	0.02%	0.002%
59	9.436	2503	2518	2556	rBV	1321327	2261981	74.06%	9.390%
60	9.591	2559	2566	2570	rBV7	2051	2963	0.10%	0.012%
61	9.649	2582	2584	2586	rBV2	928	589	0.02%	0.002%
62	9.713	2594	2604	2615	rVB5	8093	14986	0.49%	0.062%
63	9.829	2636	2640	2644	rBV2	440	407	0.01%	0.002%
64	9.857	2646	2649	2653	rVV2	435	395	0.01%	0.002%
65	10.034	2702	2704	2710	rVB	459	371	0.01%	0.002%
66	10.118	2720	2730	2742	rVV6	9072	16565	0.54%	0.069%
67	10.230	2759	2765	2767	rBV2	509	610	0.02%	0.003%
68	10.433	2825	2828	2832	rBV2	442	400	0.01%	0.002%
69	10.501	2841	2849	2863	rVB2	9651	15507	0.51%	0.064%
70	10.771	2918	2933	2952	rVV	925607	1476517	48.34%	6.129%
71	11.044	3013	3018	3019	rBV2	445	358	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037951.D
 Acq On : 30 Apr 2020 15:02
 Operator : JC/MD
 Sample : L2395-01 800X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	11.124	3030	3043	3055	rBV	30516	45825	1.50%	0.190%
73	11.247	3077	3081	3083	rBV	476	364	0.01%	0.002%
74	11.430	3134	3138	3143	rBV3	636	612	0.02%	0.003%
75	11.481	3147	3154	3165	rVB5	2325	3229	0.11%	0.013%
76	11.607	3190	3193	3195	rBV3	629	412	0.01%	0.002%
77	11.690	3215	3219	3222	rVB2	509	402	0.01%	0.002%
78	11.713	3222	3226	3228	rBV3	526	449	0.01%	0.002%
79	11.758	3231	3240	3248	rVV4	13161	19296	0.63%	0.080%
80	11.825	3248	3261	3282	rVB	1338299	2138003	70.00%	8.875%
81	12.083	3336	3341	3344	rBV4	633	615	0.02%	0.003%
82	12.150	3359	3362	3366	rVB2	596	456	0.01%	0.002%
83	12.205	3366	3379	3395	rBV	1355203	2135671	69.92%	8.865%
84	12.462	3454	3459	3460	rBV	484	445	0.01%	0.002%
85	12.591	3495	3499	3506	rVB2	621	683	0.02%	0.003%
86	12.626	3506	3510	3515	rVB2	474	372	0.01%	0.002%
87	12.658	3516	3520	3522	rBV3	628	477	0.02%	0.002%
88	12.742	3543	3546	3549	rBV2	590	461	0.02%	0.002%
89	12.787	3557	3560	3561	rBV2	723	389	0.01%	0.002%
90	12.935	3602	3606	3610	rBV4	575	545	0.02%	0.002%
91	13.240	3692	3701	3709	rBV6	3685	5885	0.19%	0.024%
92	13.584	3805	3808	3811	rBV2	894	672	0.02%	0.003%
93	13.661	3830	3832	3834	rBV	722	369	0.01%	0.002%
94	13.719	3848	3850	3854	rBV	539	359	0.01%	0.001%
95	13.742	3854	3857	3861	rBV2	561	409	0.01%	0.002%
96	13.864	3886	3895	3906	rVV	33828	51483	1.69%	0.214%
97	13.909	3906	3909	3913	rVB2	936	698	0.02%	0.003%
98	14.111	3966	3972	3981	rVB3	6579	8959	0.29%	0.037%
99	14.359	4042	4049	4059	rVB7	4297	6850	0.22%	0.028%
100	14.925	4222	4225	4229	rBV4	818	717	0.02%	0.003%


Sum of corrected areas: 24090108

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037951.D
Acq On : 30 Apr 2020 15:02
Operator : JC/MD
Sample : L2395-01 800X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

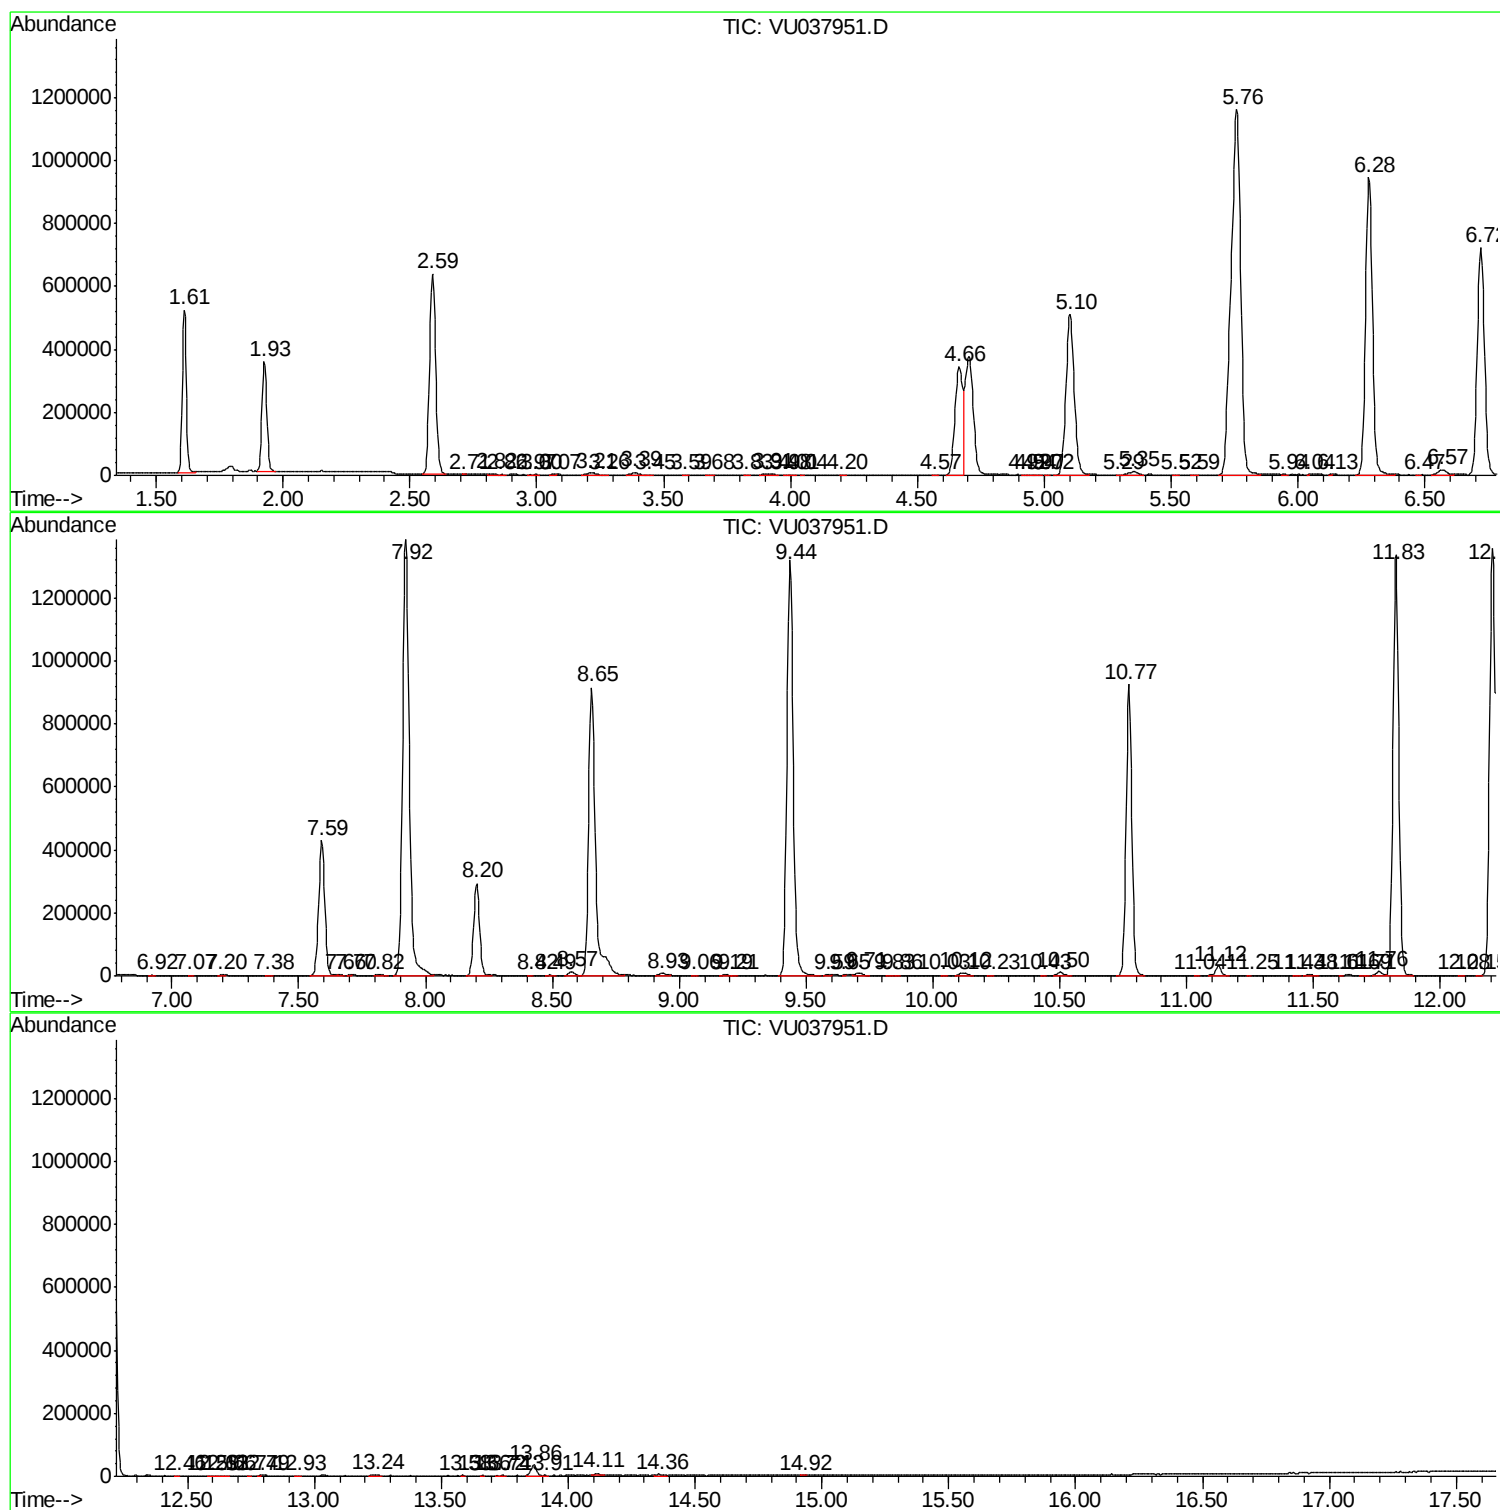

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037951.D
Acq On : 30 Apr 2020 15:02
Operator : JC/MD
Sample : L2395-01 800X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037951.D
Acq On : 30 Apr 2020 15:02
Operator : JC/MD
Sample : L2395-01 800X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
