

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037953.D
 Acq On : 30 Apr 2020 15:48
 Operator : JC/MD
 Sample : L2395-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	76	84	100	rBV2	560353	635734	21.45%	2.472%
2	1.925	174	182	199	rVB	339512	464941	15.69%	1.808%
3	2.591	376	389	405	rBV2	623559	1055927	35.64%	4.106%
4	2.707	420	425	440	rVB7	5876	11272	0.38%	0.044%
5	2.784	446	449	451	rBV3	1026	735	0.02%	0.003%
6	2.925	486	493	500	rVB6	1016	1833	0.06%	0.007%
7	3.012	515	520	521	rBV2	584	480	0.02%	0.002%
8	3.076	526	540	556	rVB	188464	349767	11.80%	1.360%
9	3.221	572	585	603	rVB3	8166	20408	0.69%	0.079%
10	3.289	603	606	609	rBV2	611	506	0.02%	0.002%
11	3.321	613	616	621	rVB2	473	507	0.02%	0.002%
12	3.375	629	633	634	rBV	1470	896	0.03%	0.003%
13	3.543	681	685	688	rVB2	802	613	0.02%	0.002%
14	3.565	688	692	696	rBV3	521	430	0.01%	0.002%
15	3.736	740	745	751	rVB2	687	895	0.03%	0.003%
16	3.771	751	756	758	rBV2	536	529	0.02%	0.002%
17	3.909	780	799	818	rVB2	51752	123139	4.16%	0.479%
18	4.121	859	865	868	rBV	474	435	0.01%	0.002%
19	4.382	941	946	948	rBV2	556	470	0.02%	0.002%
20	4.607	1005	1016	1018	rBV2	3146	4773	0.16%	0.019%
21	4.665	1019	1034	1038	rBV	329294	640683	21.62%	2.491%
22	4.890	1101	1104	1108	rVB6	660	569	0.02%	0.002%
23	4.970	1127	1129	1132	rBV3	627	395	0.01%	0.002%
24	5.102	1153	1170	1196	rBV	493937	1103663	37.25%	4.292%
25	5.353	1226	1248	1265	rVV	135120	305035	10.29%	1.186%
26	5.414	1265	1267	1275	rVB5	1668	1801	0.06%	0.007%
27	5.517	1296	1299	1304	rVB2	1019	726	0.02%	0.003%
28	5.555	1309	1311	1316	rVB3	799	710	0.02%	0.003%
29	5.581	1316	1319	1323	rBV3	862	634	0.02%	0.002%
30	5.671	1344	1347	1351	rVB2	501	374	0.01%	0.001%
31	5.758	1351	1374	1408	rBV2	1118028	2963110	100.00%	11.522%
32	6.060	1463	1468	1469	rBV2	1818	1474	0.05%	0.006%
33	6.173	1499	1503	1506	rVB4	685	532	0.02%	0.002%
34	6.192	1506	1509	1512	rVB2	679	448	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037953.D
 Acq On : 30 Apr 2020 15:48
 Operator : JC/MD
 Sample : L2395-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	6.279	1521	1536	1565	rBV	898402	1715466	57.89%	6.671%
36	6.491	1598	1602	1606	rBV4	737	841	0.03%	0.003%
37	6.571	1606	1627	1655	rVV	711985	1356138	45.77%	5.274%
38	6.723	1658	1674	1695	rVV	691704	1344805	45.38%	5.229%
39	6.948	1741	1744	1751	rVV3	605	713	0.02%	0.003%
40	6.993	1751	1758	1774	rVB6	2854	5727	0.19%	0.022%
41	7.099	1788	1791	1797	rVB4	459	422	0.01%	0.002%
42	7.205	1814	1824	1834	rBV8	1895	3632	0.12%	0.014%
43	7.250	1834	1838	1842	rVB3	428	407	0.01%	0.002%
44	7.298	1850	1853	1858	rBV3	554	522	0.02%	0.002%
45	7.491	1907	1913	1915	rBV2	489	437	0.01%	0.002%
46	7.591	1925	1944	1969	rBV	402209	702765	23.72%	2.733%
47	7.806	2004	2011	2012	rBV3	1703	1398	0.05%	0.005%
48	7.922	2030	2047	2065	rBV	1337025	2425277	81.85%	9.431%
49	8.202	2118	2134	2149	rBV	289858	472081	15.93%	1.836%
50	8.423	2195	2203	2210	rVB5	2442	4090	0.14%	0.016%
51	8.494	2219	2225	2229	rBV5	1944	2127	0.07%	0.008%
52	8.575	2241	2250	2259	rBV3	9578	15149	0.51%	0.059%
53	8.655	2262	2275	2314	rBV	857268	1650003	55.68%	6.416%
54	8.931	2350	2361	2372	rBV7	7170	13860	0.47%	0.054%
55	9.099	2409	2413	2417	rBV2	820	732	0.02%	0.003%
56	9.185	2432	2440	2445	rBV4	1670	2020	0.07%	0.008%
57	9.333	2481	2486	2488	rBV3	453	398	0.01%	0.002%
58	9.436	2501	2518	2551	rBV	1263071	2180841	73.60%	8.481%
59	9.587	2555	2565	2581	rVV	56091	90325	3.05%	0.351%
60	9.710	2591	2603	2622	rBV	175096	298491	10.07%	1.161%
61	9.877	2653	2655	2661	rVB3	743	450	0.02%	0.002%
62	10.060	2708	2712	2715	rBV2	465	502	0.02%	0.002%
63	10.118	2718	2730	2744	rVV2	61915	103065	3.48%	0.401%
64	10.243	2767	2769	2775	rVB2	698	702	0.02%	0.003%
65	10.388	2809	2814	2818	rBV4	411	381	0.01%	0.001%
66	10.501	2840	2849	2860	rVB2	10468	15497	0.52%	0.060%
67	10.581	2871	2874	2876	rBV3	1145	850	0.03%	0.003%
68	10.697	2905	2910	2915	rBV3	469	486	0.02%	0.002%
69	10.771	2920	2933	2952	rBV	878251	1399592	47.23%	5.443%
70	10.925	2969	2981	2982	rBV7	3890	5463	0.18%	0.021%
71	10.999	3002	3004	3010	rBV3	809	954	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037953.D
 Acq On : 30 Apr 2020 15:48
 Operator : JC/MD
 Sample : L2395-11DL 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D96DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	11.124	3034	3043	3051	rVB3	7702	12127	0.41%	0.047%
73	11.160	3051	3054	3061	rVB3	677	589	0.02%	0.002%
74	11.269	3086	3088	3095	rVB3	797	582	0.02%	0.002%
75	11.301	3095	3098	3100	rBV3	547	368	0.01%	0.001%
76	11.423	3132	3136	3142	rVV6	637	744	0.03%	0.003%
77	11.484	3145	3155	3168	rVB6	5709	9808	0.33%	0.038%
78	11.581	3182	3185	3190	rBV3	391	385	0.01%	0.001%
79	11.648	3204	3206	3211	rVB	631	493	0.02%	0.002%
80	11.758	3232	3240	3248	rVB5	4569	6829	0.23%	0.027%
81	11.825	3248	3261	3278	rBV	1287571	2056749	69.41%	7.998%
82	11.899	3279	3284	3286	rBV3	1154	947	0.03%	0.004%
83	12.156	3360	3364	3365	rBV2	656	422	0.01%	0.002%
84	12.205	3365	3379	3394	rVV	1299801	2073534	69.98%	8.063%
85	12.340	3417	3421	3430	rVV7	1118	1193	0.04%	0.005%
86	12.661	3517	3521	3525	rBV	654	638	0.02%	0.002%
87	12.751	3546	3549	3551	rBV2	715	510	0.02%	0.002%
88	12.796	3558	3563	3570	rVB3	1051	1365	0.05%	0.005%
89	12.838	3573	3576	3580	rBV3	589	466	0.02%	0.002%
90	12.970	3613	3617	3624	rVB6	2285	2891	0.10%	0.011%
91	13.041	3636	3639	3643	rVB3	839	555	0.02%	0.002%
92	13.237	3694	3700	3707	rBV4	3289	4076	0.14%	0.016%
93	13.491	3776	3779	3783	rBV	733	558	0.02%	0.002%
94	13.545	3790	3796	3799	rBV5	869	1049	0.04%	0.004%
95	13.732	3851	3854	3856	rBV3	598	388	0.01%	0.002%
96	13.764	3859	3864	3870	rVB7	1619	1782	0.06%	0.007%
97	13.864	3887	3895	3903	rBV3	12449	16831	0.57%	0.065%
98	14.111	3966	3972	3981	rVB3	5804	7941	0.27%	0.031%
99	14.291	4025	4028	4031	rBV3	794	630	0.02%	0.002%
100	14.507	4093	4095	4099	rBV	627	405	0.01%	0.002%


Sum of corrected areas: 25715908

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037953.D
Acq On : 30 Apr 2020 15:48
Operator : JC/MD
Sample : L2395-11DL 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D96DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

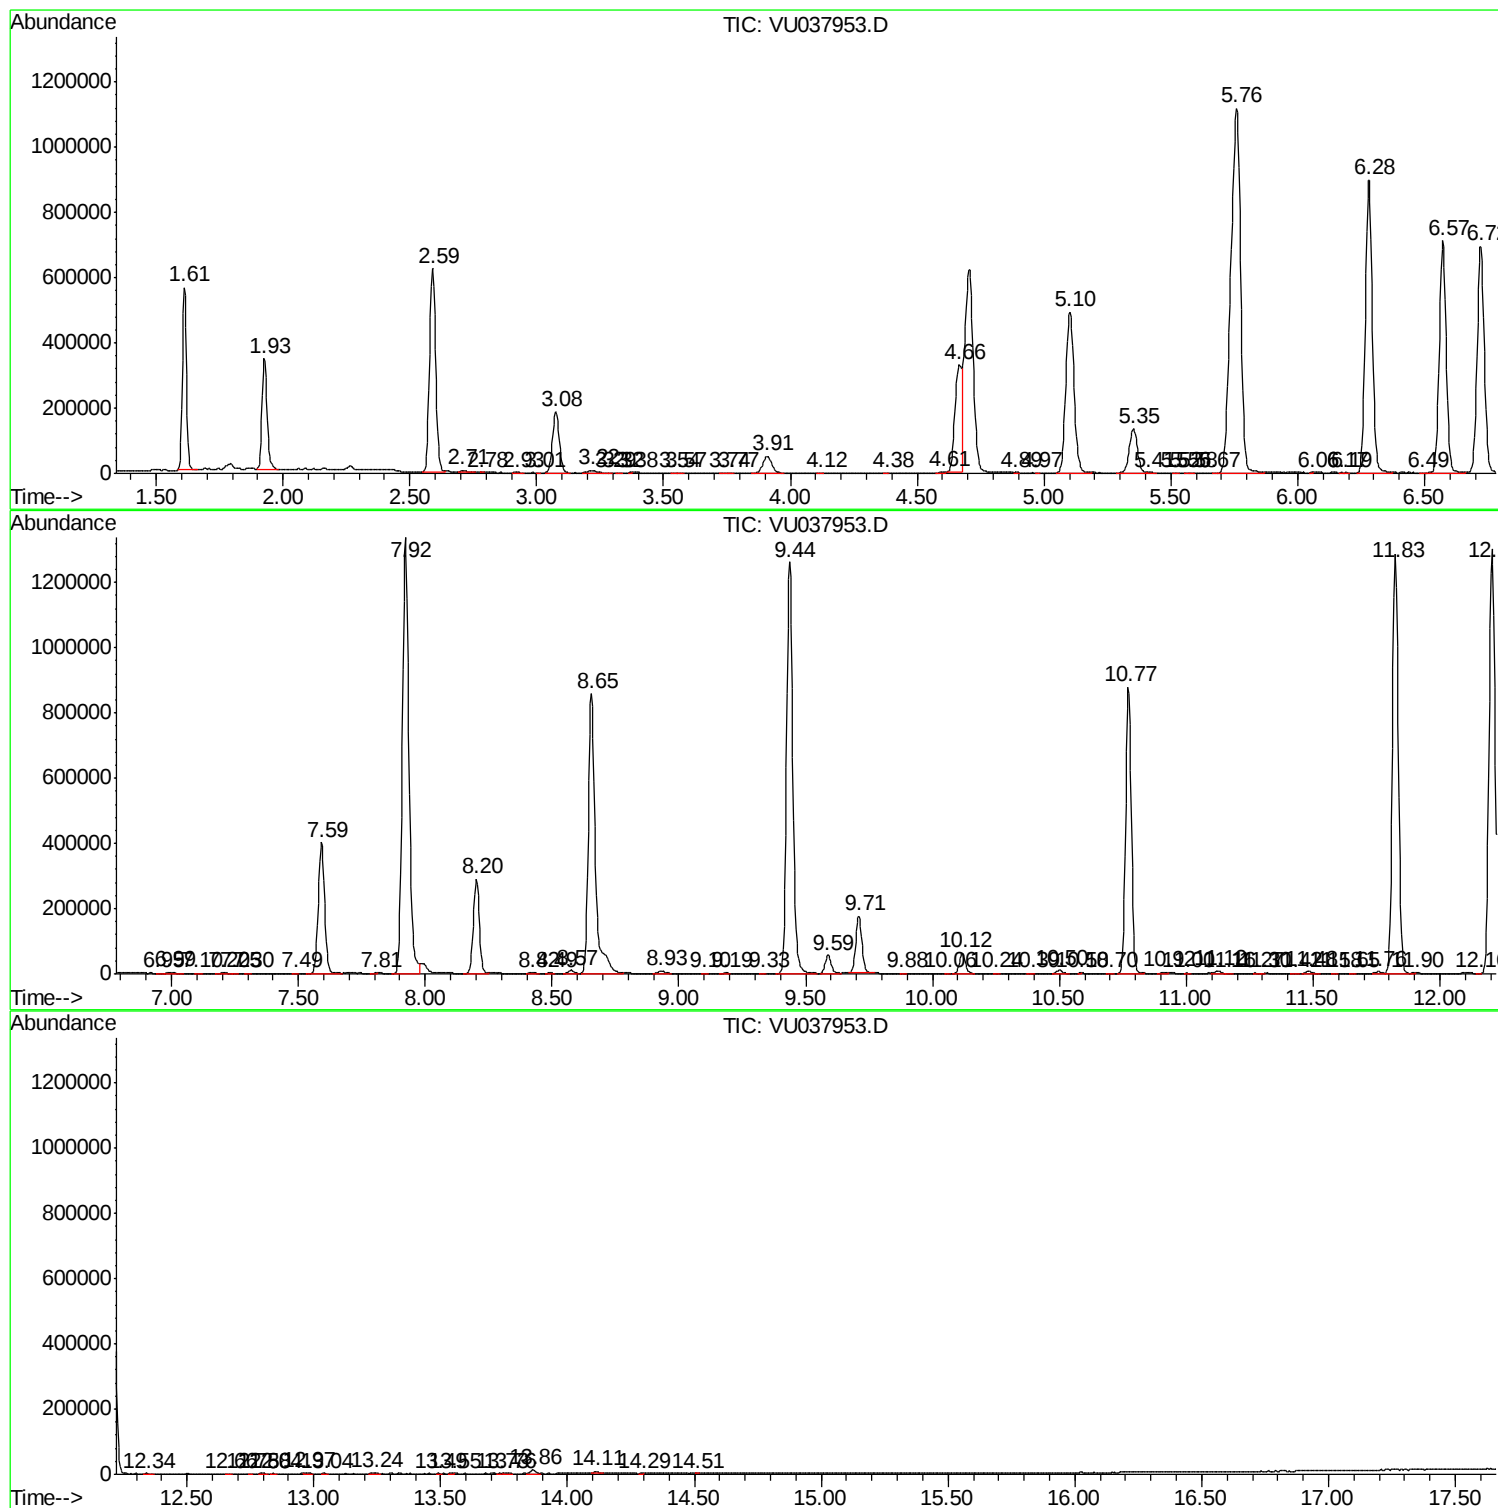

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037953.D
Acq On : 30 Apr 2020 15:48
Operator : JC/MD
Sample : L2395-11DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D96DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037953.D
Acq On : 30 Apr 2020 15:48
Operator : JC/MD
Sample : L2395-11DL 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D96DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc