

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037957.D
 Acq On : 30 Apr 2020 17:19
 Operator : JC/MD
 Sample : L2395-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	94	rBV	411775	435772	9.54%	1.544%
2	1.929	175	183	200	rVB	318022	413324	9.05%	1.464%
3	2.591	377	389	407	rBV3	643758	1198472	26.24%	4.245%
4	2.900	482	485	486	rBV3	1006	490	0.01%	0.002%
5	3.076	526	540	559	rVB	241287	453332	9.93%	1.606%
6	3.282	598	604	605	rBV3	630	570	0.01%	0.002%
7	3.343	620	623	626	rBV3	651	449	0.01%	0.002%
8	3.382	626	635	648	rVB7	4485	9677	0.21%	0.034%
9	3.469	659	662	665	rBV3	470	316	0.01%	0.001%
10	3.485	665	667	669	rBV	283	145	0.00%	0.001%
11	3.510	674	675	679	rVB3	584	276	0.01%	0.001%
12	3.536	680	683	688	rBV4	421	443	0.01%	0.002%
13	3.594	699	701	702	rBV	499	237	0.01%	0.001%
14	3.613	705	707	709	rVV2	387	180	0.00%	0.001%
15	3.652	716	719	721	rBV2	636	392	0.01%	0.001%
16	3.678	724	727	729	rVV3	372	234	0.01%	0.001%
17	3.719	737	740	741	rBV2	407	231	0.01%	0.001%
18	3.909	785	799	812	rBV2	21243	48231	1.06%	0.171%
19	3.980	818	821	826	rBV2	605	600	0.01%	0.002%
20	4.035	835	838	841	rVB3	297	198	0.00%	0.001%
21	4.051	841	843	846	rBV2	210	132	0.00%	0.000%
22	4.096	853	857	859	rBV2	277	197	0.00%	0.001%
23	4.118	859	864	867	rVB3	476	390	0.01%	0.001%
24	4.154	871	875	878	rVB2	319	230	0.01%	0.001%
25	4.173	878	881	883	rBV2	537	343	0.01%	0.001%
26	4.202	886	890	892	rBV2	198	168	0.00%	0.001%
27	4.260	906	908	911	rVB2	306	133	0.00%	0.000%
28	4.301	919	921	922	rBV	327	144	0.00%	0.001%
29	4.372	941	943	947	rVB	372	275	0.01%	0.001%
30	4.398	948	951	953	rBV	389	253	0.01%	0.001%
31	4.427	957	960	961	rBV	280	164	0.00%	0.001%
32	4.465	966	972	979	rBV5	551	952	0.02%	0.003%
33	4.581	1006	1008	1013	rBV2	419	212	0.00%	0.001%
34	4.703	1018	1046	1070	rBV2	798488	2410098	52.77%	8.537%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037957.D
 Acq On : 30 Apr 2020 17:19
 Operator : JC/MD
 Sample : L2395-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	5.102	1154	1170	1193	rBV	468923	1041479	22.81%	3.689%
36	5.353	1231	1248	1265	rBV	221857	503828	11.03%	1.785%
37	5.462	1280	1282	1284	rBV2	326	135	0.00%	0.000%
38	5.633	1331	1335	1337	rBV3	888	598	0.01%	0.002%
39	5.758	1351	1374	1413	rBV2	1015936	2729953	59.78%	9.670%
40	6.279	1522	1536	1566	rBV	817591	1555146	34.05%	5.508%
41	6.571	1611	1627	1646	rBV	2469749	4566827	100.00%	16.176%
42	6.723	1661	1674	1691	rVB	648820	1245420	27.27%	4.411%
43	7.060	1776	1779	1781	rBV3	542	338	0.01%	0.001%
44	7.073	1781	1783	1789	rVB3	775	528	0.01%	0.002%
45	7.108	1792	1794	1796	rBV2	389	218	0.00%	0.001%
46	7.173	1813	1814	1818	rBV2	371	174	0.00%	0.001%
47	7.211	1818	1826	1835	rVV7	2165	3798	0.08%	0.013%
48	7.243	1835	1836	1839	rVB	405	183	0.00%	0.001%
49	7.279	1845	1847	1849	rBV	275	156	0.00%	0.001%
50	7.321	1854	1860	1866	rVB3	563	671	0.01%	0.002%
51	7.356	1866	1871	1874	rBV3	394	370	0.01%	0.001%
52	7.388	1874	1881	1886	rBV4	459	561	0.01%	0.002%
53	7.436	1893	1896	1897	rBV2	380	171	0.00%	0.001%
54	7.591	1931	1944	1964	rBV	294094	504074	11.04%	1.785%
55	7.845	2019	2023	2026	rVB2	436	261	0.01%	0.001%
56	7.861	2026	2028	2030	rBV2	250	167	0.00%	0.001%
57	7.922	2032	2047	2082	rBV	1190526	2195382	48.07%	7.776%
58	8.202	2121	2134	2150	rBV2	204750	341041	7.47%	1.208%
59	8.362	2180	2184	2188	rBV3	662	639	0.01%	0.002%
60	8.423	2195	2203	2212	rBV3	8526	13241	0.29%	0.047%
61	8.575	2240	2250	2260	rBV4	7812	12533	0.27%	0.044%
62	8.655	2260	2275	2315	rBV2	791934	1554496	34.04%	5.506%
63	8.848	2332	2335	2337	rBV	393	255	0.01%	0.001%
64	8.886	2344	2347	2349	rVB2	694	302	0.01%	0.001%
65	8.983	2373	2377	2380	rVB2	581	457	0.01%	0.002%
66	9.002	2380	2383	2384	rBV	625	270	0.01%	0.001%
67	9.012	2384	2386	2389	rVB2	332	135	0.00%	0.000%
68	9.025	2389	2390	2393	rBV2	157	89	0.00%	0.000%
69	9.050	2395	2398	2400	rBV	300	152	0.00%	0.001%
70	9.076	2401	2406	2409	rBV3	602	750	0.02%	0.003%
71	9.121	2417	2420	2424	rBV3	476	336	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037957.D
 Acq On : 30 Apr 2020 17:19
 Operator : JC/MD
 Sample : L2395-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D92

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	9.179	2431	2438	2442	rBV4	931	1285	0.03%	0.005%
73	9.240	2454	2457	2459	rBV2	353	282	0.01%	0.001%
74	9.256	2460	2462	2465	rVV2	535	233	0.01%	0.001%
75	9.436	2504	2518	2549	rBV	1144012	1961238	42.95%	6.947%
76	9.761	2616	2619	2622	rBV	645	529	0.01%	0.002%
77	9.800	2629	2631	2637	rBV2	343	357	0.01%	0.001%
78	9.874	2652	2654	2656	rBV	247	89	0.00%	0.000%
79	10.118	2724	2730	2737	rBV7	1511	2485	0.05%	0.009%
80	10.173	2745	2747	2749	rBV2	382	229	0.01%	0.001%
81	10.237	2763	2767	2769	rBV2	542	460	0.01%	0.002%
82	10.359	2803	2805	2808	rBV	655	383	0.01%	0.001%
83	10.391	2812	2815	2818	rBV3	588	330	0.01%	0.001%
84	10.414	2818	2822	2823	rBV	297	191	0.00%	0.001%
85	10.472	2834	2840	2841	rBV2	690	691	0.02%	0.002%
86	10.597	2876	2879	2884	rBV4	522	389	0.01%	0.001%
87	10.722	2916	2918	2919	rBV4	331	145	0.00%	0.001%
88	10.771	2920	2933	2959	rVB	813951	1323519	28.98%	4.688%
89	10.864	2959	2962	2967	rBV	510	480	0.01%	0.002%
90	11.099	3032	3035	3038	rBV3	882	665	0.01%	0.002%
91	11.484	3149	3155	3159	rBV3	1606	2080	0.05%	0.007%
92	11.626	3195	3199	3200	rBV2	652	524	0.01%	0.002%
93	11.825	3248	3261	3277	rBV	1144610	1813108	39.70%	6.422%
94	12.205	3366	3379	3398	rVB	1152992	1858636	40.70%	6.583%
95	13.028	3628	3635	3645	rBV4	5244	8704	0.19%	0.031%
96	13.237	3695	3700	3707	rBV5	2502	3001	0.07%	0.011%


Sum of corrected areas: 28232427

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037957.D
Acq On : 30 Apr 2020 17:19
Operator : JC/MD
Sample : L2395-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D92

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

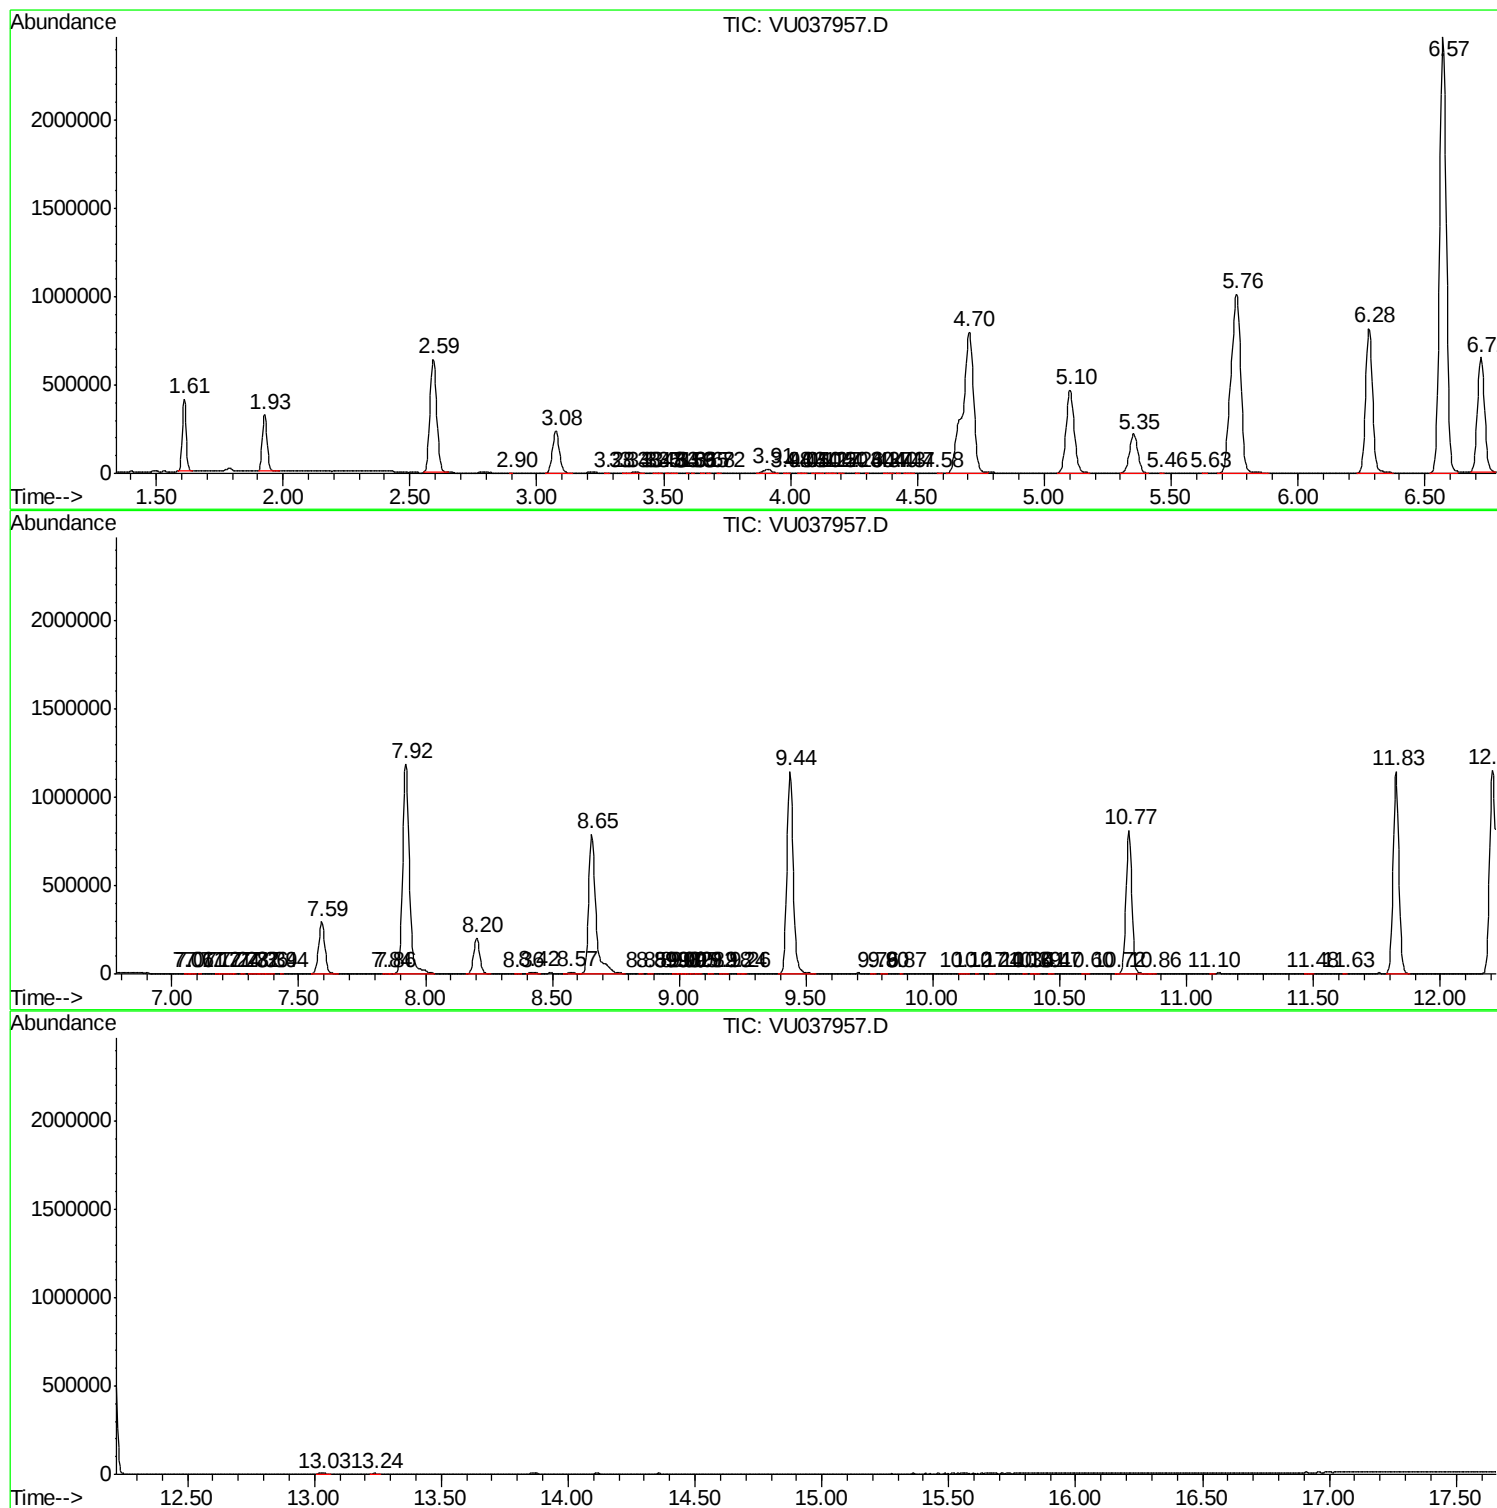

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037957.D
Acq On : 30 Apr 2020 17:19
Operator : JC/MD
Sample : L2395-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D92

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037957.D
Acq On : 30 Apr 2020 17:19
Operator : JC/MD
Sample : L2395-07
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D92

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc