

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037961.D
 Acq On : 30 Apr 2020 19:35
 Operator : JC/MD
 Sample : L2395-01 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	76	85	96	rBV2	627459	723161	19.10%	2.788%
2	1.925	174	182	195	rVB	324061	425587	11.24%	1.641%
3	2.591	375	389	408	rBV2	642499	1153221	30.46%	4.445%
4	2.710	423	426	427	rBV3	968	571	0.02%	0.002%
5	3.073	533	539	550	rBV6	2513	3667	0.10%	0.014%
6	3.160	559	566	569	rBV2	706	817	0.02%	0.003%
7	3.221	570	585	599	rVV	10927	25164	0.66%	0.097%
8	3.272	599	601	604	rVB2	558	337	0.01%	0.001%
9	3.385	623	636	648	rBV6	7035	14927	0.39%	0.058%
10	3.459	656	659	664	rVB4	605	418	0.01%	0.002%
11	3.735	742	745	751	rVB3	485	425	0.01%	0.002%
12	3.906	781	798	818	rVB2	21647	52150	1.38%	0.201%
13	3.986	818	823	827	rBV3	558	547	0.01%	0.002%
14	4.060	842	846	853	rVB3	579	759	0.02%	0.003%
15	4.195	884	888	893	rVB2	654	585	0.02%	0.002%
16	4.234	893	900	903	rBV2	469	476	0.01%	0.002%
17	4.584	1004	1009	1012	rBV3	435	443	0.01%	0.002%
18	4.706	1018	1047	1073	rBV2	1374193	3785436	100.00%	14.592%
19	5.009	1138	1141	1144	rBV2	673	468	0.01%	0.002%
20	5.102	1153	1170	1194	rBV	473525	1058894	27.97%	4.082%
21	5.353	1232	1248	1261	rBV3	38768	87733	2.32%	0.338%
22	5.443	1271	1276	1281	rVB5	946	1039	0.03%	0.004%
23	5.465	1281	1283	1288	rBV2	408	340	0.01%	0.001%
24	5.758	1352	1374	1409	rBV2	1072473	2847731	75.23%	10.977%
25	5.957	1434	1436	1439	rBV4	667	434	0.01%	0.002%
26	6.005	1449	1451	1454	rVB3	928	392	0.01%	0.002%
27	6.060	1463	1468	1469	rBV2	1136	938	0.02%	0.004%
28	6.279	1520	1536	1574	rBV	881263	1703096	44.99%	6.565%
29	6.571	1611	1627	1642	rBV8	28656	67854	1.79%	0.262%
30	6.722	1658	1674	1694	rBV	664357	1297860	34.29%	5.003%
31	6.928	1736	1738	1742	rBV3	649	427	0.01%	0.002%
32	7.047	1771	1775	1778	rBV	484	445	0.01%	0.002%
33	7.089	1784	1788	1791	rVB2	422	346	0.01%	0.001%
34	7.208	1813	1825	1827	rBV3	2147	2851	0.08%	0.011%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037961.D
 Acq On : 30 Apr 2020 19:35
 Operator : JC/MD
 Sample : L2395-01 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	7.455	1899	1902	1905	rBV2	488	348	0.01%	0.001%
36	7.526	1919	1924	1928	rBV3	362	384	0.01%	0.001%
37	7.591	1928	1944	1966	rBV	385661	668612	17.66%	2.577%
38	7.706	1972	1980	1984	rBV8	1473	2348	0.06%	0.009%
39	7.819	2008	2015	2023	rVB4	3088	4725	0.12%	0.018%
40	7.861	2023	2028	2032	rVB4	617	491	0.01%	0.002%
41	7.922	2032	2047	2080	rBV	1282533	2340711	61.83%	9.023%
42	8.201	2121	2134	2149	rBV	268859	446410	11.79%	1.721%
43	8.420	2194	2202	2213	rVB3	4573	6821	0.18%	0.026%
44	8.468	2213	2217	2220	rBV3	836	672	0.02%	0.003%
45	8.491	2220	2224	2228	rVB3	925	851	0.02%	0.003%
46	8.574	2241	2250	2261	rVB6	6195	9953	0.26%	0.038%
47	8.655	2261	2275	2290	rBV	825878	1497928	39.57%	5.774%
48	8.880	2342	2345	2347	rVV3	504	343	0.01%	0.001%
49	8.931	2353	2361	2371	rVV6	5735	10023	0.26%	0.039%
50	8.973	2371	2374	2378	rVB4	960	782	0.02%	0.003%
51	9.031	2388	2392	2393	rBV2	613	365	0.01%	0.001%
52	9.082	2403	2408	2412	rBV2	362	336	0.01%	0.001%
53	9.176	2433	2437	2439	rBV3	863	709	0.02%	0.003%
54	9.375	2494	2499	2504	rBV2	606	844	0.02%	0.003%
55	9.436	2504	2518	2553	rVB	1245792	2159951	57.06%	8.326%
56	9.590	2553	2566	2576	rBV	6329	11327	0.30%	0.044%
57	9.709	2594	2603	2616	rVB2	22143	37421	0.99%	0.144%
58	9.758	2616	2618	2620	rBV2	586	377	0.01%	0.001%
59	9.774	2620	2623	2626	rVB4	635	421	0.01%	0.002%
60	9.844	2642	2645	2649	rVV3	518	384	0.01%	0.001%
61	9.938	2671	2674	2680	rVB3	664	505	0.01%	0.002%
62	10.002	2690	2694	2697	rVB2	440	342	0.01%	0.001%
63	10.050	2704	2709	2711	rBV2	436	404	0.01%	0.002%
64	10.118	2720	2730	2743	rVV2	16364	27046	0.71%	0.104%
65	10.455	2833	2835	2841	rBV2	420	339	0.01%	0.001%
66	10.500	2842	2849	2855	rVV5	1664	2115	0.06%	0.008%
67	10.552	2859	2865	2869	rBV3	784	769	0.02%	0.003%
68	10.587	2869	2876	2884	rVV5	2601	3437	0.09%	0.013%
69	10.770	2919	2933	2950	rBV	843443	1357355	35.86%	5.232%
70	10.880	2965	2967	2972	rVB2	681	421	0.01%	0.002%
71	10.909	2972	2976	2978	rBV2	594	514	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037961.D
 Acq On : 30 Apr 2020 19:35
 Operator : JC/MD
 Sample : L2395-01 200X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	10.938	2982	2985	2989	rVB2	779	588	0.02%	0.002%
73	10.999	3002	3004	3008	rBV2	510	344	0.01%	0.001%
74	11.230	3070	3076	3080	rBV	614	631	0.02%	0.002%
75	11.343	3105	3111	3114	rBV2	453	524	0.01%	0.002%
76	11.426	3134	3137	3141	rVV3	625	421	0.01%	0.002%
77	11.481	3147	3154	3165	rVB4	1469	2402	0.06%	0.009%
78	11.655	3205	3208	3213	rBV	531	566	0.01%	0.002%
79	11.713	3222	3226	3227	rBV2	589	381	0.01%	0.001%
80	11.758	3234	3240	3248	rVB4	3287	4623	0.12%	0.018%
81	11.825	3248	3261	3280	rBV	1274744	2046111	54.05%	7.887%
82	12.008	3310	3318	3322	rBV3	491	477	0.01%	0.002%
83	12.204	3364	3379	3397	rBV	1233713	1992470	52.64%	7.681%
84	12.304	3406	3410	3412	rBV2	643	487	0.01%	0.002%
85	12.327	3413	3417	3422	rVV3	681	709	0.02%	0.003%
86	12.413	3440	3444	3448	rBV2	463	444	0.01%	0.002%
87	12.838	3571	3576	3580	rBV2	574	597	0.02%	0.002%
88	12.915	3594	3600	3606	rBV4	888	1144	0.03%	0.004%
89	13.240	3694	3701	3710	rVV6	3441	4575	0.12%	0.018%
90	13.352	3734	3736	3740	rVV2	389	351	0.01%	0.001%
91	13.815	3877	3880	3883	rBV2	872	713	0.02%	0.003%
92	13.864	3888	3895	3904	rVB6	6375	9977	0.26%	0.038%
93	13.928	3909	3915	3916	rBV2	854	784	0.02%	0.003%
94	14.111	3964	3972	3981	rBV2	5343	8239	0.22%	0.032%
95	14.282	4023	4025	4030	rVB2	627	384	0.01%	0.001%
96	14.356	4042	4048	4058	rVB5	3527	5130	0.14%	0.020%
97	14.683	4148	4150	4153	rBV3	601	366	0.01%	0.001%
98	14.864	4204	4206	4209	rBV2	818	459	0.01%	0.002%
99	14.883	4209	4212	4214	rBV2	1137	688	0.02%	0.003%
100	14.973	4236	4240	4243	rBV2	1031	932	0.02%	0.004%


Sum of corrected areas: 25941840

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037961.D
Acq On : 30 Apr 2020 19:35
Operator : JC/MD
Sample : L2395-01 200X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

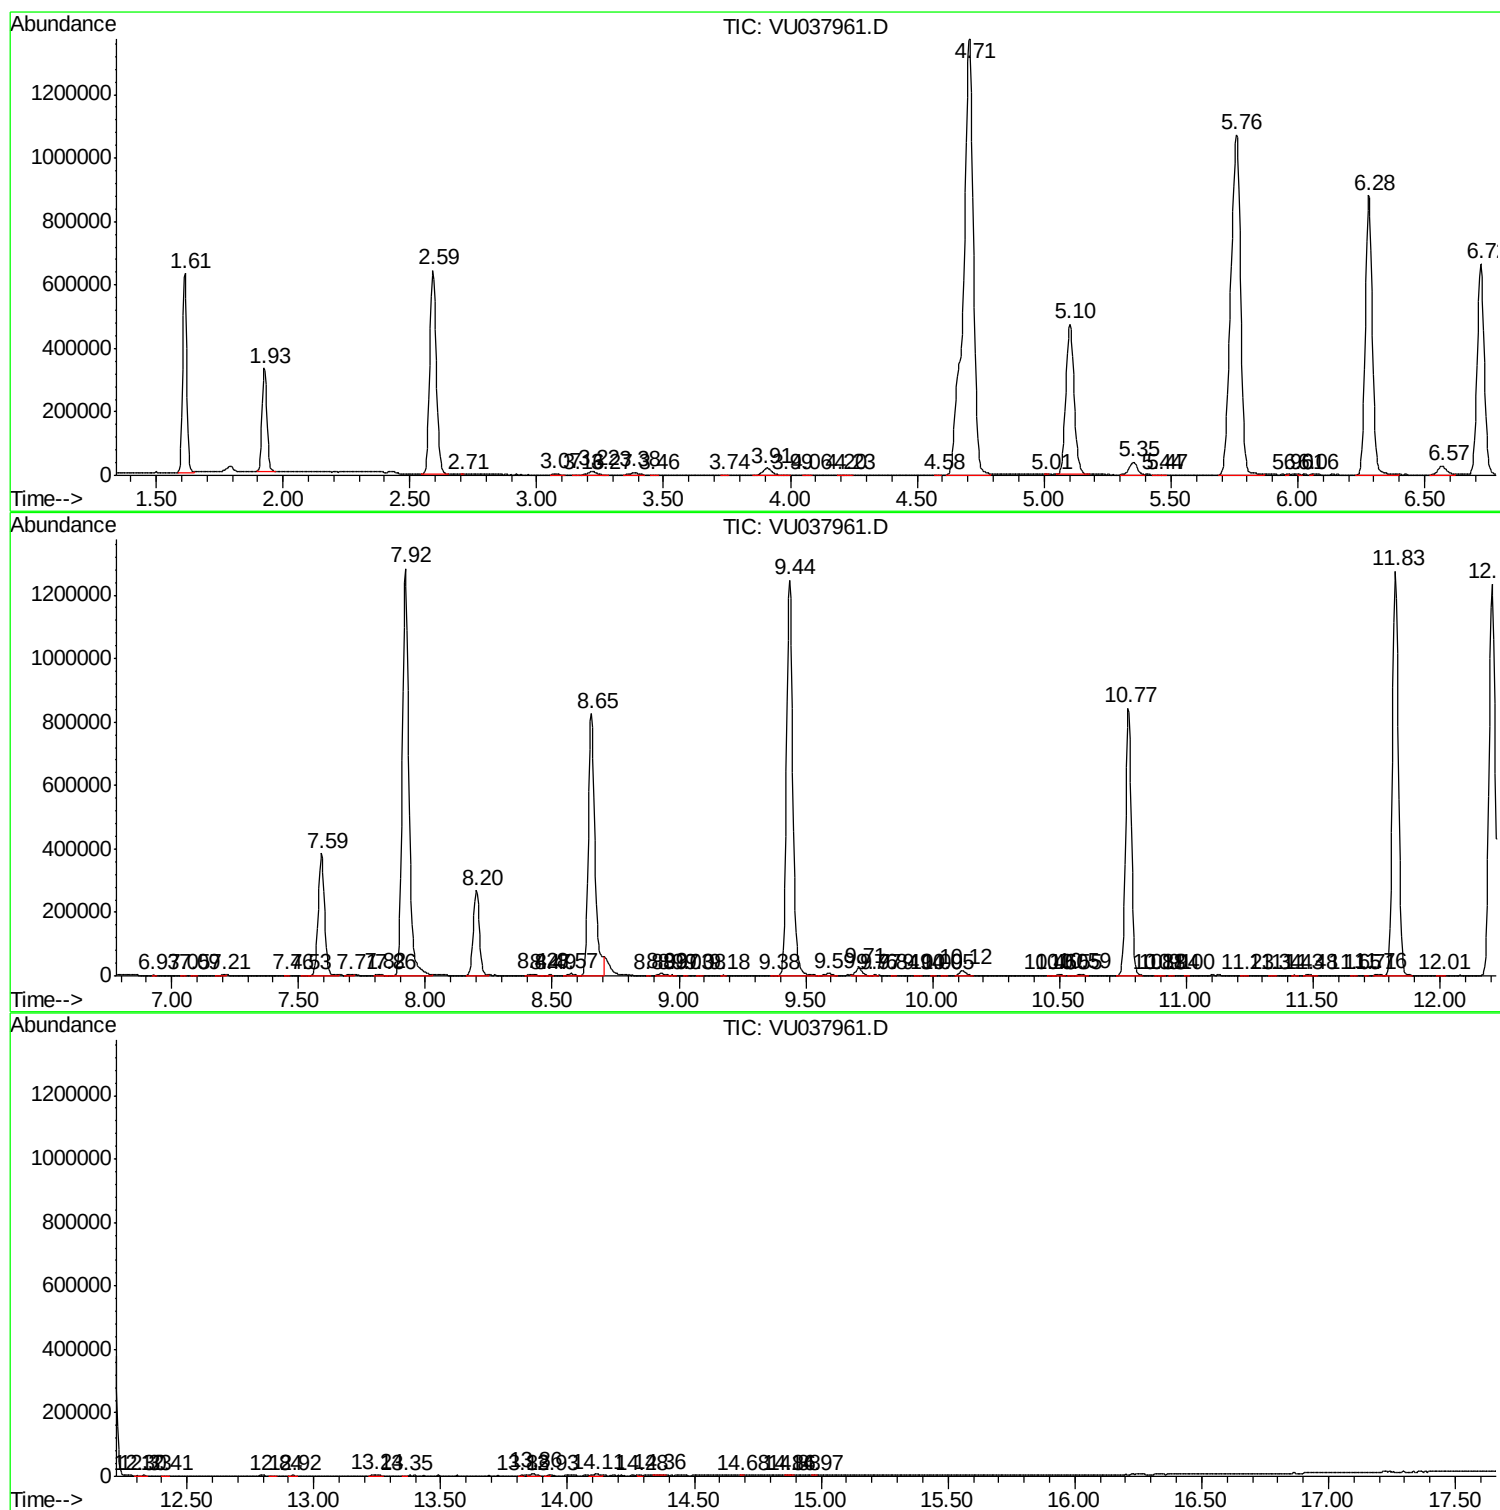

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037961.D
Acq On : 30 Apr 2020 19:35
Operator : JC/MD
Sample : L2395-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037961.D
Acq On : 30 Apr 2020 19:35
Operator : JC/MD
Sample : L2395-01 200X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc