

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037974.D
 Acq On : 01 May 2020 01:13
 Operator : JC/MD
 Sample : L2410-10DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBEF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	76	84	99	rBV	432927	465804	16.12%	1.897%
2	1.925	174	182	199	rVB	327381	436604	15.11%	1.778%
3	2.507	358	363	366	rBV5	1930	2095	0.07%	0.009%
4	2.591	377	389	407	rVB	581041	953517	32.99%	3.883%
5	2.720	422	429	437	rBV7	1342	2382	0.08%	0.010%
6	2.861	471	473	478	rBV2	750	595	0.02%	0.002%
7	2.964	501	505	506	rBV	632	460	0.02%	0.002%
8	3.215	570	583	598	rBV2	12883	28235	0.98%	0.115%
9	3.369	626	631	632	rBV2	680	537	0.02%	0.002%
10	3.459	656	659	661	rBV	470	329	0.01%	0.001%
11	3.475	661	664	670	rVB4	502	478	0.02%	0.002%
12	3.591	698	700	704	rVB	508	373	0.01%	0.002%
13	3.720	737	740	743	rVB2	675	470	0.02%	0.002%
14	3.745	743	748	749	rBV2	536	407	0.01%	0.002%
15	3.765	749	754	756	rBV3	530	424	0.01%	0.002%
16	3.938	803	808	811	rBV2	736	544	0.02%	0.002%
17	3.961	811	815	822	rVB3	805	1146	0.04%	0.005%
18	4.002	822	828	829	rBV	527	479	0.02%	0.002%
19	4.134	862	869	872	rBV	404	455	0.02%	0.002%
20	4.173	877	881	885	rBV2	495	410	0.01%	0.002%
21	4.559	999	1001	1006	rVB2	625	458	0.02%	0.002%
22	4.594	1010	1012	1016	rVB2	608	394	0.01%	0.002%
23	4.662	1016	1033	1074	rBV	338143	864003	29.90%	3.518%
24	4.999	1132	1138	1140	rBV4	471	396	0.01%	0.002%
25	5.102	1153	1170	1191	rVV	494515	1082633	37.46%	4.408%
26	5.199	1198	1200	1204	rVV3	842	533	0.02%	0.002%
27	5.324	1230	1239	1244	rBV5	1792	3180	0.11%	0.013%
28	5.395	1255	1261	1263	rBV4	827	786	0.03%	0.003%
29	5.478	1285	1287	1294	rVB2	501	441	0.02%	0.002%
30	5.520	1296	1300	1301	rBV	402	330	0.01%	0.001%
31	5.594	1318	1323	1327	rVB2	550	473	0.02%	0.002%
32	5.758	1352	1374	1404	rBV2	1087333	2890003	100.00%	11.768%
33	5.996	1446	1448	1450	rBV	759	445	0.02%	0.002%
34	6.076	1464	1473	1483	rBV7	2833	4757	0.16%	0.019%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037974.D
 Acq On : 01 May 2020 01:13
 Operator : JC/MD
 Sample : L2410-10DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBEF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	6.208	1510	1514	1516	rBV2	465	381	0.01%	0.002%
36	6.279	1521	1536	1571	rBV	896804	1751285	60.60%	7.131%
37	6.491	1600	1602	1607	rVB4	689	518	0.02%	0.002%
38	6.565	1613	1625	1636	rBV7	14984	35402	1.22%	0.144%
39	6.723	1658	1674	1698	rVB	685340	1328005	45.95%	5.408%
40	6.835	1703	1709	1718	rBV7	1634	2670	0.09%	0.011%
41	7.208	1817	1825	1833	rVV6	2321	4190	0.14%	0.017%
42	7.591	1929	1944	1958	rBV	386715	662903	22.94%	2.699%
43	7.809	2008	2012	2013	rBV4	761	510	0.02%	0.002%
44	7.922	2029	2047	2081	rBV	1293603	2401251	83.09%	9.778%
45	8.202	2120	2134	2151	rBV	259799	435163	15.06%	1.772%
46	8.359	2181	2183	2187	rVB3	578	341	0.01%	0.001%
47	8.427	2200	2204	2207	rVB4	636	375	0.01%	0.002%
48	8.575	2235	2250	2264	rVV	1000508	1731176	59.90%	7.049%
49	8.655	2264	2275	2319	rVB2	833494	1670376	57.80%	6.802%
50	8.893	2345	2349	2350	rBV	618	377	0.01%	0.002%
51	8.928	2355	2360	2361	rVV4	732	554	0.02%	0.002%
52	9.134	2422	2424	2428	rVB	604	329	0.01%	0.001%
53	9.179	2435	2438	2444	rVB4	811	905	0.03%	0.004%
54	9.218	2444	2450	2452	rBV2	435	442	0.02%	0.002%
55	9.337	2486	2487	2493	rVB	415	353	0.01%	0.001%
56	9.372	2493	2498	2500	rBV2	463	336	0.01%	0.001%
57	9.436	2503	2518	2554	rVB	1275978	2217069	76.72%	9.028%
58	9.591	2562	2566	2568	rBV3	989	765	0.03%	0.003%
59	9.655	2583	2586	2587	rBV2	770	372	0.01%	0.002%
60	9.690	2592	2597	2598	rBV2	1514	1349	0.05%	0.005%
61	9.800	2627	2631	2635	rBV3	440	381	0.01%	0.002%
62	9.893	2656	2660	2667	rVB3	729	845	0.03%	0.003%
63	10.317	2787	2792	2796	rBV	477	381	0.01%	0.002%
64	10.568	2866	2870	2874	rVB3	537	391	0.01%	0.002%
65	10.665	2894	2900	2903	rBV	492	583	0.02%	0.002%
66	10.710	2911	2914	2916	rVV3	772	488	0.02%	0.002%
67	10.771	2920	2933	2955	rVB	866529	1394875	48.27%	5.680%
68	10.893	2969	2971	2978	rVB4	604	634	0.02%	0.003%
69	10.948	2984	2988	2990	rBV2	557	382	0.01%	0.002%
70	11.012	3004	3008	3013	rVB2	656	691	0.02%	0.003%
71	11.047	3013	3019	3022	rBV2	417	476	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037974.D
 Acq On : 01 May 2020 01:13
 Operator : JC/MD
 Sample : L2410-10DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBEF9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	11.169	3053	3057	3063	rVB	400	390	0.01%	0.002%
73	11.327	3104	3106	3112	rVB3	761	607	0.02%	0.002%
74	11.427	3133	3137	3139	rBV3	945	672	0.02%	0.003%
75	11.575	3179	3183	3186	rBV2	636	584	0.02%	0.002%
76	11.655	3206	3208	3212	rVB2	526	333	0.01%	0.001%
77	11.681	3212	3216	3218	rBV3	576	374	0.01%	0.002%
78	11.742	3231	3235	3238	rBV3	641	429	0.01%	0.002%
79	11.825	3246	3261	3282	rBV	1305197	2098696	72.62%	8.546%
80	11.925	3288	3292	3295	rBV4	716	603	0.02%	0.002%
81	12.054	3329	3332	3335	rBV2	497	372	0.01%	0.002%
82	12.205	3365	3379	3401	rBV	1266554	2051244	70.98%	8.352%
83	12.369	3427	3430	3431	rBV	570	334	0.01%	0.001%
84	12.459	3453	3458	3462	rBV3	662	758	0.03%	0.003%
85	12.546	3480	3485	3486	rBV2	718	600	0.02%	0.002%
86	12.684	3523	3528	3531	rBV2	575	590	0.02%	0.002%
87	12.738	3541	3545	3546	rBV	723	484	0.02%	0.002%
88	12.873	3583	3587	3590	rVB2	576	440	0.02%	0.002%
89	12.938	3603	3607	3611	rBV	779	609	0.02%	0.002%
90	13.015	3628	3631	3634	rBV3	814	491	0.02%	0.002%
91	13.140	3667	3670	3675	rBV3	559	548	0.02%	0.002%
92	13.185	3680	3684	3689	rVB4	629	481	0.02%	0.002%
93	13.227	3694	3697	3698	rBV2	598	341	0.01%	0.001%
94	13.240	3698	3701	3706	rVB3	1081	728	0.03%	0.003%
95	13.497	3777	3781	3783	rBV4	598	523	0.02%	0.002%
96	13.864	3889	3895	3904	rVB6	2049	2830	0.10%	0.012%
97	14.018	3940	3943	3948	rBV3	685	759	0.03%	0.003%
98	14.066	3955	3958	3960	rBV2	769	444	0.02%	0.002%
99	14.279	4021	4024	4028	rBV2	809	571	0.02%	0.002%
100	14.565	4111	4113	4118	rBV4	611	587	0.02%	0.002%


Sum of corrected areas: 24558522

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037974.D
Acq On : 01 May 2020 01:13
Operator : JC/MD
Sample : L2410-10DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBEF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

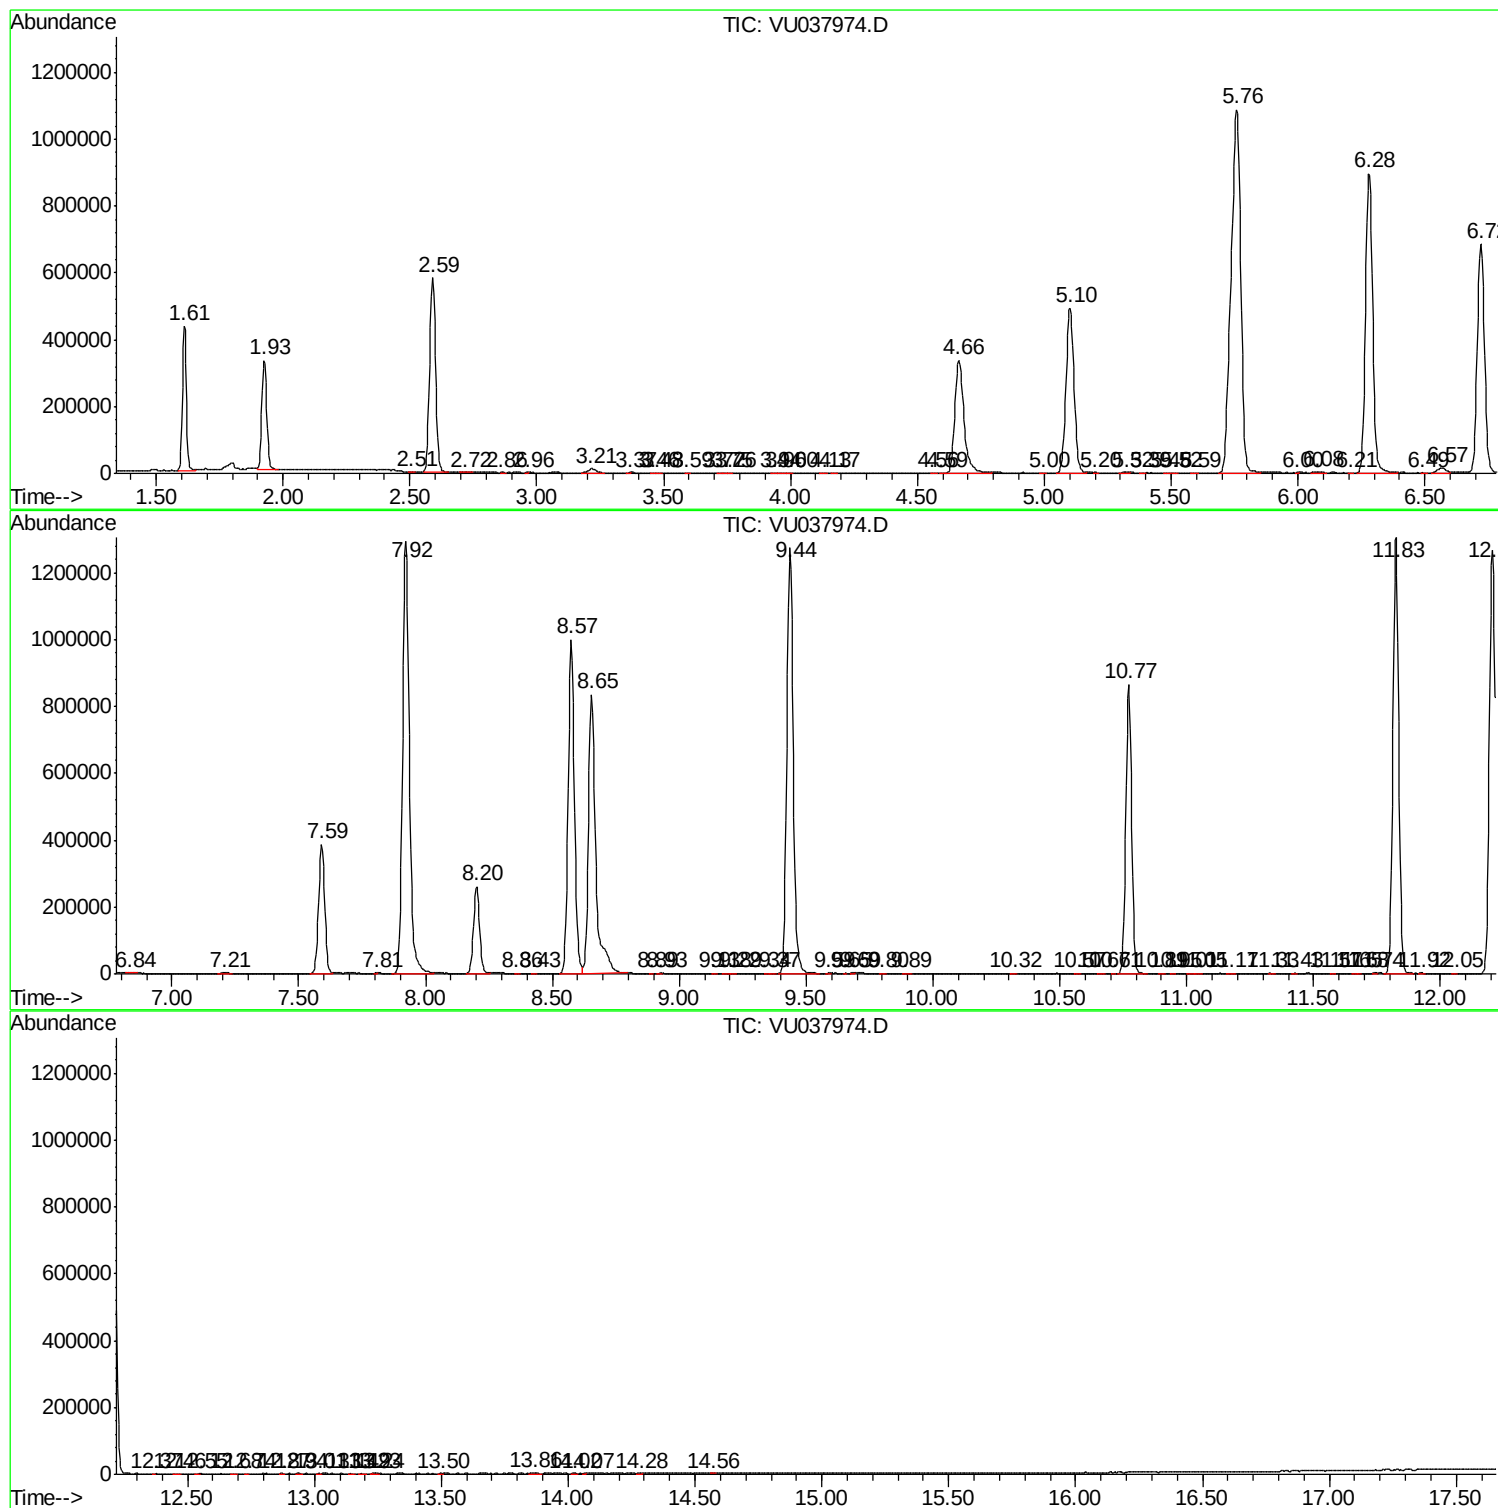

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037974.D
Acq On : 01 May 2020 01:13
Operator : JC/MD
Sample : L2410-10DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBEF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037974.D
Acq On : 01 May 2020 01:13
Operator : JC/MD
Sample : L2410-10DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBEF9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc