

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037979.D
 Acq On : 01 May 2020 03:06
 Operator : JC/MD
 Sample : L2395-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	101	rBV	392457	423732	15.42%	1.952%
2	1.928	175	183	198	rVB	303964	400859	14.59%	1.847%
3	2.591	377	389	409	rVB	545507	894921	32.56%	4.123%
4	3.218	577	584	597	rVB2	6810	13825	0.50%	0.064%
5	3.395	637	639	642	rVB2	657	293	0.01%	0.001%
6	3.575	693	695	699	rBV3	451	252	0.01%	0.001%
7	3.684	726	729	732	rBV2	428	357	0.01%	0.002%
8	3.710	735	737	740	rVV2	260	138	0.01%	0.001%
9	3.761	752	753	756	rBV2	328	220	0.01%	0.001%
10	3.854	779	782	785	rBV3	432	342	0.01%	0.002%
11	3.915	796	801	805	rBV2	782	631	0.02%	0.003%
12	3.941	805	809	812	rBV3	781	588	0.02%	0.003%
13	4.022	831	834	839	rVB3	237	152	0.01%	0.001%
14	4.050	839	843	844	rBV	316	229	0.01%	0.001%
15	4.124	862	866	868	rBV2	253	199	0.01%	0.001%
16	4.205	889	891	893	rBV2	445	249	0.01%	0.001%
17	4.314	922	925	928	rBV2	387	224	0.01%	0.001%
18	4.337	928	932	936	rBV2	610	585	0.02%	0.003%
19	4.417	954	957	960	rBV	389	293	0.01%	0.001%
20	4.446	965	966	969	rBV2	183	106	0.00%	0.000%
21	4.491	978	980	983	rVB	596	354	0.01%	0.002%
22	4.510	983	986	987	rBV2	100	60	0.00%	0.000%
23	4.530	989	992	994	rBV	293	199	0.01%	0.001%
24	4.575	999	1006	1007	rBV2	357	277	0.01%	0.001%
25	4.661	1017	1033	1072	rBV	326749	804921	29.29%	3.708%
26	4.899	1105	1107	1109	rVB	754	339	0.01%	0.002%
27	5.102	1153	1170	1191	rBV	467945	1032424	37.57%	4.757%
28	5.285	1224	1227	1228	rBV2	459	303	0.01%	0.001%
29	5.394	1257	1261	1263	rBV2	918	720	0.03%	0.003%
30	5.459	1279	1281	1286	rVB4	459	345	0.01%	0.002%
31	5.529	1300	1303	1306	rVB	447	226	0.01%	0.001%
32	5.558	1306	1312	1317	rBV4	587	599	0.02%	0.003%
33	5.632	1333	1335	1341	rVB2	340	298	0.01%	0.001%
34	5.658	1341	1343	1345	rBV2	349	207	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U043020\
 Data File : VU037979.D
 Acq On : 01 May 2020 03:06
 Operator : JC/MD
 Sample : L2395-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	5.758	1352	1374	1401	rBV2	1035563	2748173	100.00%	12.661%
36	6.111	1481	1484	1487	rBV2	675	484	0.02%	0.002%
37	6.282	1520	1537	1570	rBV	885783	1715005	62.41%	7.901%
38	6.507	1604	1607	1611	rBV2	653	584	0.02%	0.003%
39	6.722	1659	1674	1693	rBV	654897	1265353	46.04%	5.830%
40	6.970	1750	1751	1757	rVB2	371	235	0.01%	0.001%
41	6.996	1757	1759	1760	rBV	296	115	0.00%	0.001%
42	7.034	1766	1771	1773	rBV4	582	454	0.02%	0.002%
43	7.070	1778	1782	1783	rBV	283	175	0.01%	0.001%
44	7.092	1787	1789	1792	rBV3	306	154	0.01%	0.001%
45	7.144	1799	1805	1811	rBV2	385	493	0.02%	0.002%
46	7.208	1817	1825	1832	rBV6	1818	3095	0.11%	0.014%
47	7.266	1839	1843	1844	rBV2	479	311	0.01%	0.001%
48	7.275	1844	1846	1851	rVB2	697	462	0.02%	0.002%
49	7.301	1851	1854	1855	rBV	266	104	0.00%	0.000%
50	7.311	1855	1857	1858	rBV	351	121	0.00%	0.001%
51	7.356	1867	1871	1872	rBV	294	246	0.01%	0.001%
52	7.398	1883	1884	1889	rBV2	296	240	0.01%	0.001%
53	7.478	1905	1909	1913	rBV2	343	332	0.01%	0.002%
54	7.504	1914	1917	1921	rVB2	478	294	0.01%	0.001%
55	7.526	1921	1924	1930	rBV3	418	445	0.02%	0.002%
56	7.591	1930	1944	1961	rBV	361494	619971	22.56%	2.856%
57	7.816	2005	2014	2021	rBV8	1846	3123	0.11%	0.014%
58	7.922	2033	2047	2077	rBV	1208718	2245283	81.70%	10.344%
59	8.150	2115	2118	2121	rVB	511	331	0.01%	0.002%
60	8.201	2121	2134	2156	rBV	252853	414104	15.07%	1.908%
61	8.410	2197	2199	2202	rBV2	284	163	0.01%	0.001%
62	8.475	2214	2219	2220	rBV2	693	495	0.02%	0.002%
63	8.574	2242	2250	2259	rVB8	5888	9899	0.36%	0.046%
64	8.655	2262	2275	2323	rVV2	811463	1606874	58.47%	7.403%
65	8.877	2342	2344	2346	rBV	353	214	0.01%	0.001%
66	8.931	2352	2361	2373	rVB7	3907	7317	0.27%	0.034%
67	9.008	2383	2385	2387	rVB2	333	107	0.00%	0.000%
68	9.057	2398	2400	2402	rBV	353	184	0.01%	0.001%
69	9.098	2411	2413	2414	rBV	169	75	0.00%	0.000%
70	9.115	2414	2418	2420	rVV	377	243	0.01%	0.001%
71	9.156	2429	2431	2434	rBV	354	222	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU043020\
 Data File : VU037979.D
 Acq On : 01 May 2020 03:06
 Operator : JC/MD
 Sample : L2395-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK01

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	9.227	2449	2453	2457	rVB3	615	409	0.01%	0.002%
73	9.259	2461	2463	2465	rBV	231	91	0.00%	0.000%
74	9.279	2467	2469	2472	rBV2	293	154	0.01%	0.001%
75	9.343	2486	2489	2494	rVB2	482	360	0.01%	0.002%
76	9.388	2499	2503	2504	rBV	604	434	0.02%	0.002%
77	9.436	2504	2518	2549	rVV	1242384	2164071	78.75%	9.970%
78	9.590	2562	2566	2570	rBV3	1295	1132	0.04%	0.005%
79	9.652	2581	2585	2587	rBV2	564	539	0.02%	0.002%
80	9.780	2623	2625	2627	rBV	323	174	0.01%	0.001%
81	9.848	2643	2646	2647	rBV	356	167	0.01%	0.001%
82	9.960	2677	2681	2684	rBV2	606	586	0.02%	0.003%
83	10.002	2691	2694	2698	rBV2	618	430	0.02%	0.002%
84	10.037	2702	2705	2709	rVB	536	408	0.01%	0.002%
85	10.089	2718	2721	2722	rBV	337	122	0.00%	0.001%
86	10.185	2747	2751	2754	rBV3	738	569	0.02%	0.003%
87	10.288	2778	2783	2784	rBV	441	389	0.01%	0.002%
88	10.394	2812	2816	2818	rBV	568	453	0.02%	0.002%
89	10.410	2818	2821	2824	rVB	528	385	0.01%	0.002%
90	10.594	2875	2878	2880	rBV2	391	250	0.01%	0.001%
91	10.770	2920	2933	2959	rVB	834391	1342809	48.86%	6.187%
92	10.992	2999	3002	3004	rBV2	396	250	0.01%	0.001%
93	11.098	3032	3035	3039	rBV4	757	524	0.02%	0.002%
94	11.327	3103	3106	3109	rBV2	589	436	0.02%	0.002%
95	11.825	3248	3261	3280	rBV	1277170	2029597	73.85%	9.351%
96	12.204	3366	3379	3394	rBV	1203049	1935582	70.43%	8.918%


Sum of corrected areas: 21705268

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU043020\
Data File : VU037979.D
Acq On : 01 May 2020 03:06
Operator : JC/MD
Sample : L2395-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

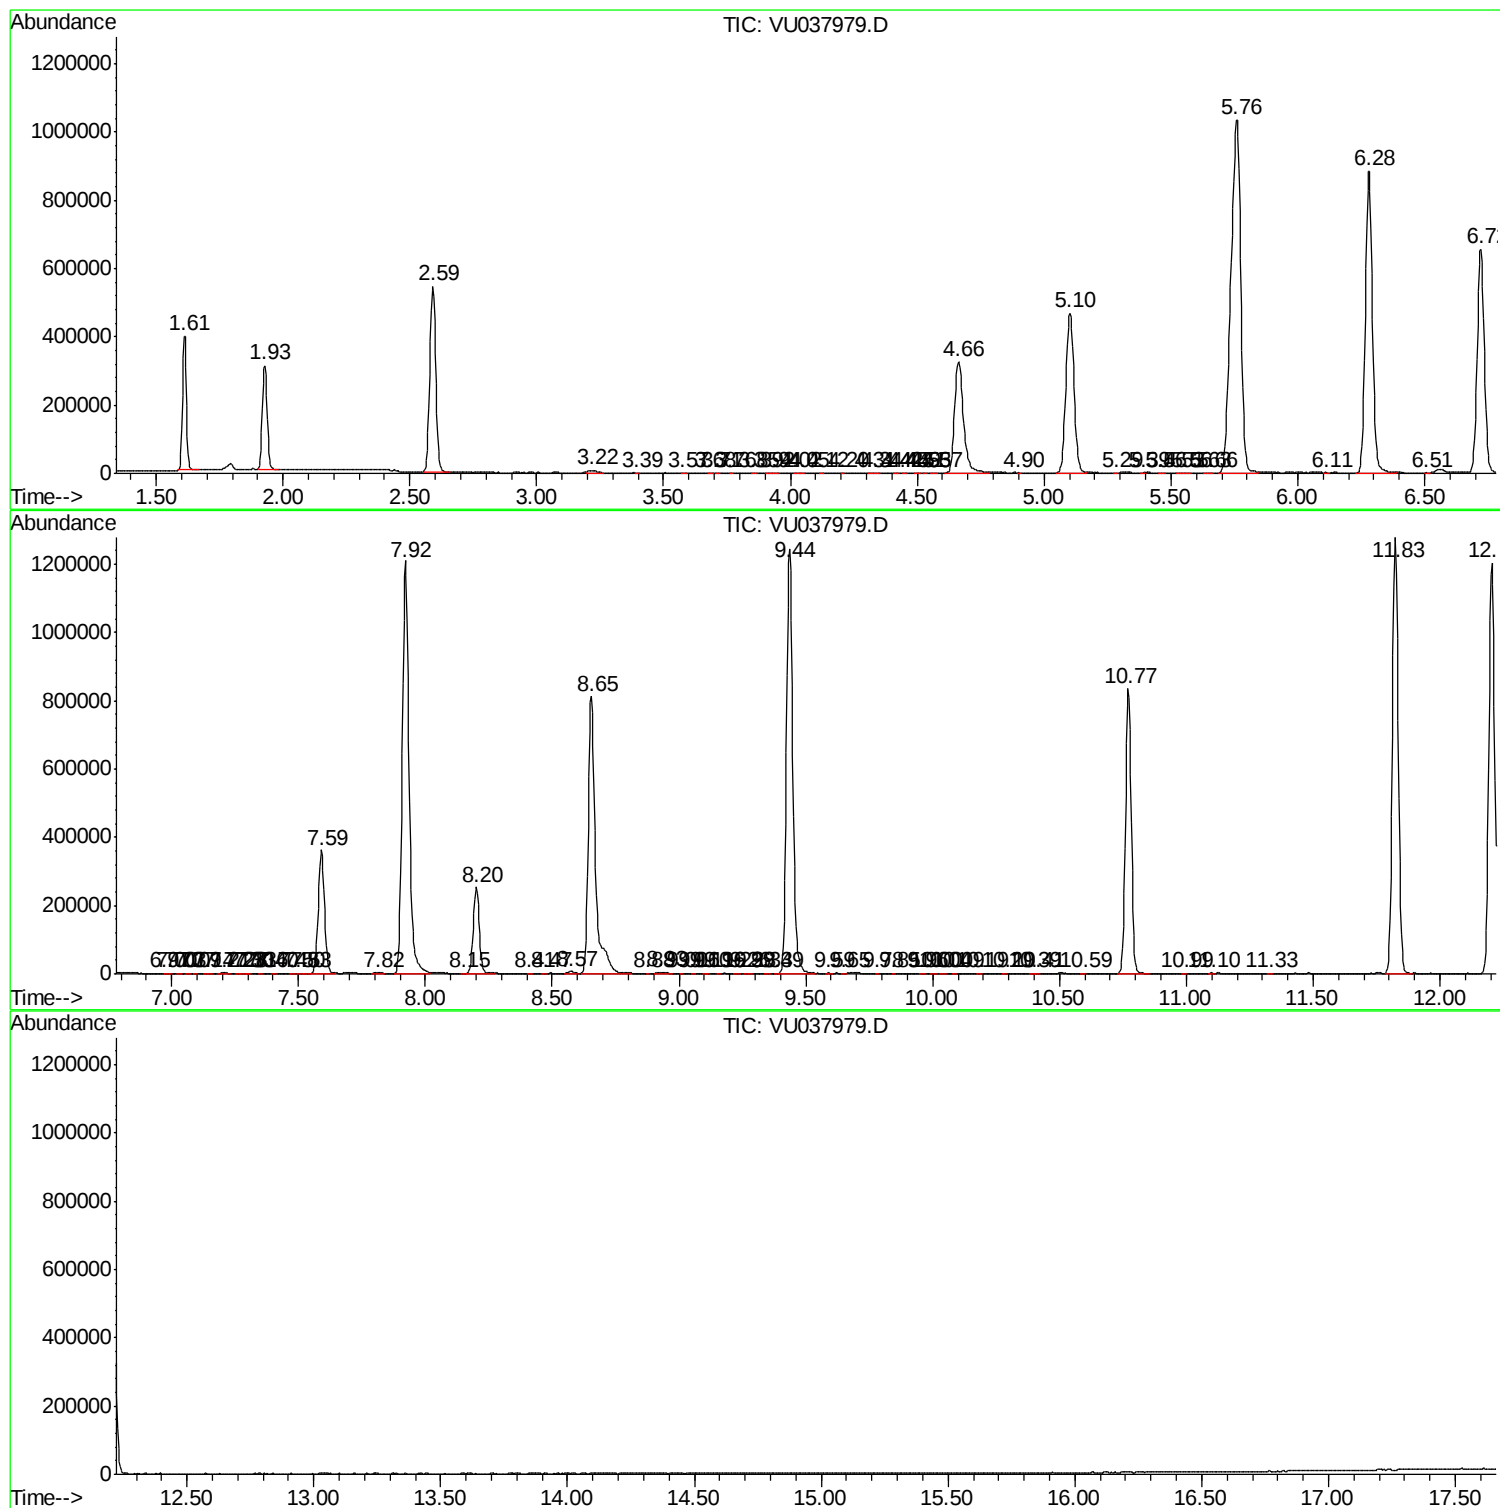

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037979.D
Acq On : 01 May 2020 03:06
Operator : JC/MD
Sample : L2395-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU043020\
Data File : VU037979.D
Acq On : 01 May 2020 03:06
Operator : JC/MD
Sample : L2395-21
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK01

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc