


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU043020\
 Data File : VU037942.D
 Acq On : 30 Apr 2020 08:37
 Operator : JC/MD
 Sample : BFB45
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB45

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 30 09:48:08 2020

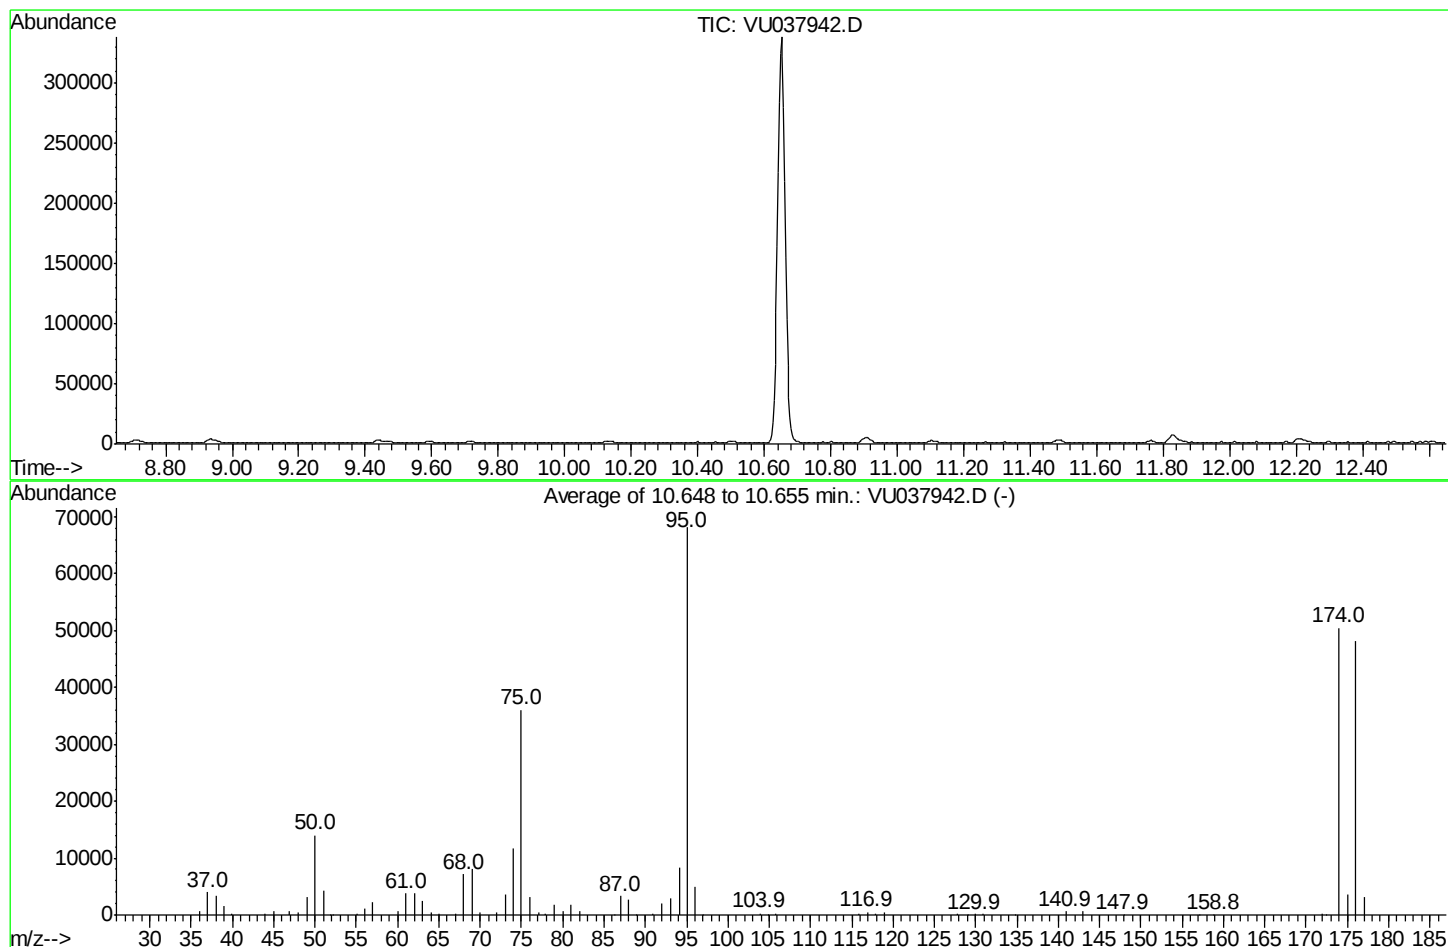

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	13984	PASS
75	95	30	80	52.9	36061	PASS
95	95	100	100	100.0	68152	PASS
96	95	5	9	7.3	4968	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.0	50461	PASS
175	174	5	9	7.1	3580	PASS
176	174	95	101	95.6	48258	PASS
177	176	5	9	6.5	3120	PASS

m/z	Abundance
35.90	547.0
37.00	4033.0
38.00	3222.0
39.00	1396.0
39.90	435.0
43.90	1233.0
45.00	844.0
46.90	596.0
47.90	434.0
49.00	2941.0
50.00	14325.0
51.00	4278.0
51.90	158.0
55.00	251.0
56.00	1279.0
57.00	2310.0
60.00	855.0
61.00	3649.0
62.00	4136.0
63.00	2437.0
64.00	331.0
65.00	264.0
67.10	209.0
68.00	7016.0
69.00	7834.0
70.00	526.0
72.00	409.0
73.00	3749.0
74.10	11708.0
75.00	36080.0
76.00	3296.0
77.10	477.0
77.80	274.0
78.90	1844.0
80.00	669.0
81.00	1830.0
82.00	620.0
86.20	211.0
87.00	3206.0
88.00	2572.0
88.80	151.0
90.80	238.0
92.00	2079.0
93.00	2893.0
94.10	7957.0
95.00	67280.0
96.00	5077.0
103.90	250.0
105.80	265.0
115.90	242.0
116.90	515.0
117.90	169.0
118.90	359.0
127.80	156.0
129.90	201.0
131.00	174.0
140.90	627.0
143.00	639.0
147.90	109.0
157.10	126.0
158.80	101.0
172.00	195.0
174.00	49408.0
175.00	3484.0
176.00	46640.0
177.00	3069.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
35.90	635.0
37.00	4217.0
38.00	3439.0
39.00	1600.0
39.90	426.0
43.90	1205.0
45.00	751.0
46.90	631.0
47.90	401.0
49.00	3252.0
50.00	14219.0
51.00	4447.0
51.90	119.0
52.10	122.0
55.00	236.0
56.00	1310.0
57.00	2325.0
60.00	756.0
61.00	3890.0
62.00	4024.0
63.10	2456.0
64.00	439.0
64.90	230.0
66.90	192.0
68.00	7306.0
69.00	8273.0
70.00	528.0
72.00	396.0
73.00	3726.0
74.10	12045.0
75.00	37288.0
76.00	3145.0
77.10	498.0
77.90	319.0
78.90	1793.0
80.00	770.0
81.00	1879.0
82.00	631.0
87.00	3478.0
88.00	2771.0
90.80	300.0
92.00	2065.0
93.00	2945.0
94.10	8598.0
95.00	70072.0
96.00	5113.0
96.90	116.0
103.90	298.0
104.80	127.0
105.80	250.0
115.90	225.0
116.90	455.0
117.90	167.0
118.90	427.0
127.80	161.0
129.90	158.0
131.00	178.0
140.90	656.0
143.00	595.0
147.90	116.0
158.90	102.0
172.00	229.0
174.00	52072.0
175.00	3648.0
176.00	49792.0
177.00	3214.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

m/z	Abundance
36.00	640.0
37.00	3786.0
38.00	3256.0
39.00	1562.0
39.90	421.0
43.90	1151.0
45.00	627.0
46.90	635.0
48.00	338.0
49.00	3267.0
50.00	13408.0
51.00	4270.0
52.10	159.0
55.10	208.0
56.00	1140.0
57.00	2065.0
60.10	594.0
61.00	3725.0
62.00	3501.0
63.10	2238.0
64.00	483.0
64.90	237.0
66.80	188.0
68.00	7132.0
69.00	8068.0
70.00	480.0
72.00	340.0
73.00	3578.0
74.00	11490.0
75.00	34816.0
76.10	2774.0
77.00	437.0
77.90	305.0
79.00	1695.0
80.00	701.0
81.00	1812.0
82.00	520.0
87.00	3339.0
88.00	2794.0
90.90	315.0
92.10	1821.0
93.00	2663.0
94.10	8152.0
95.00	67104.0
96.10	4715.0
96.90	112.0
103.90	314.0
104.80	121.0
105.80	213.0
115.90	204.0
116.90	393.0
117.90	168.0
118.90	432.0
127.80	156.0
129.00	118.0
130.00	132.0
130.90	130.0
134.80	106.0
140.90	604.0
143.00	542.0
147.90	101.0
158.90	112.0
172.00	244.0
172.40	174.0
174.00	49904.0
175.00	3608.0
176.00	48344.0
177.00	3077.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45

Scan 2883 (10.610 min): VU037942.D
BFB45

m/z	Abundance
39.90	264.0
43.00	136.0
43.90	997.0

Instrument :
MSVOA_U
ClientSampleId :
BFB45