

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
Data File : VU037989.D
Acq On : 01 May 2020 15:07
Operator : JC/MD
Sample : L2471-06
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y19

Manual Integrations
APPROVED

Sam
5/4/2020 2:15:41 PM

Quant Time: May 02 00:12:09 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 02 00:09:57 2020
Response via : Initial Calibration

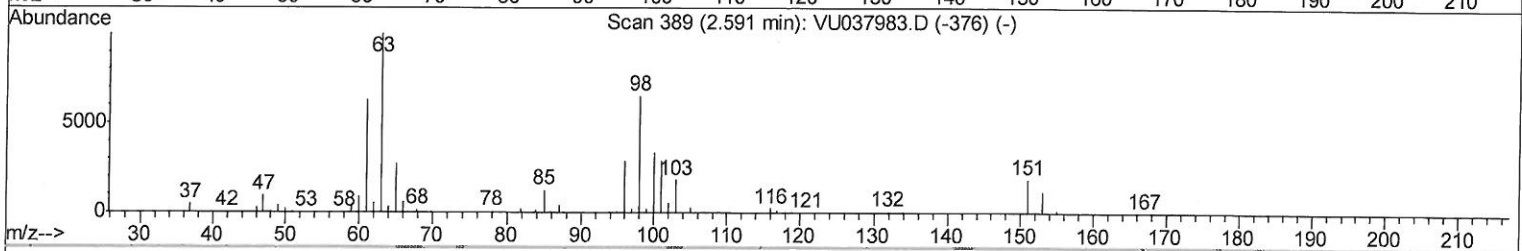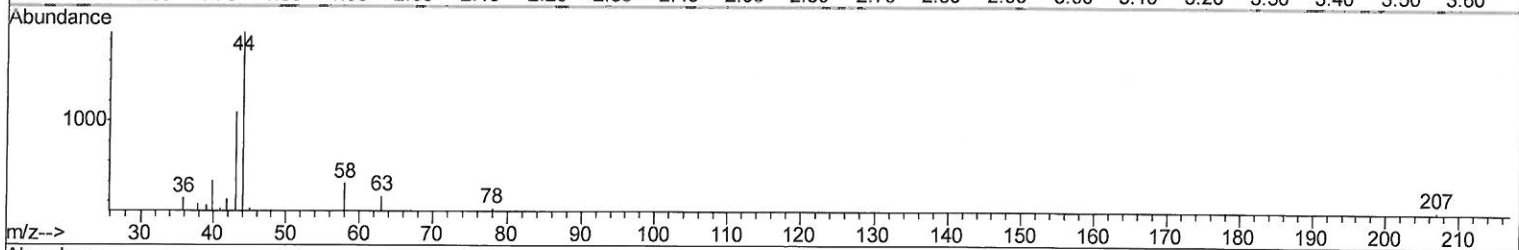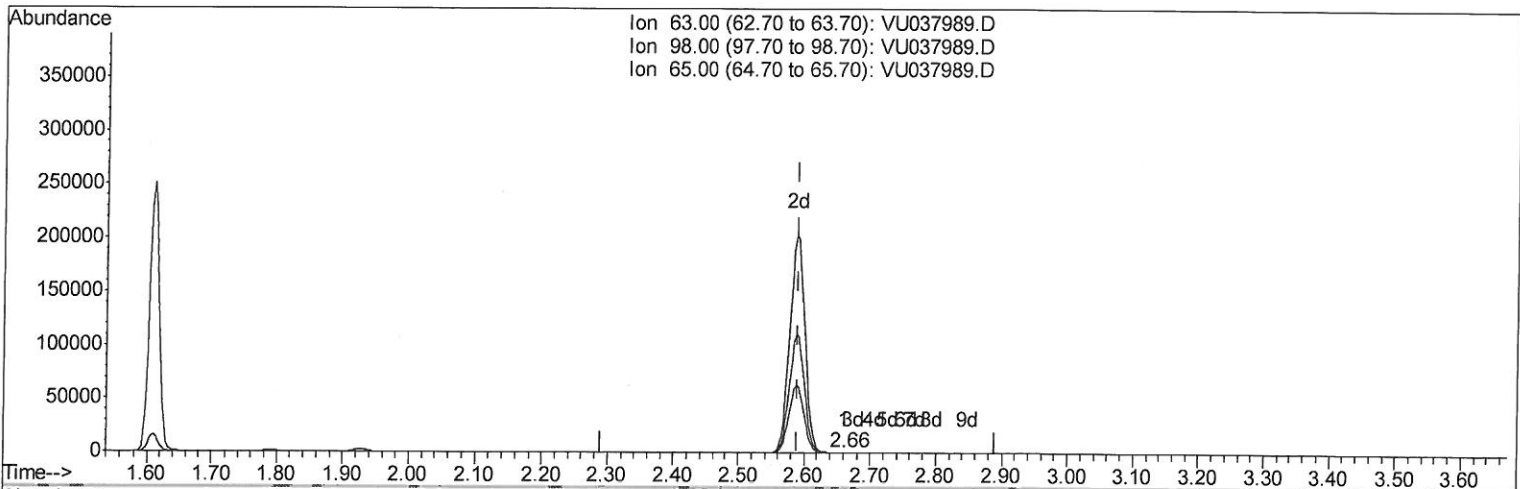

TIC: VU037989.D

(11) 1,1-Dichloroethene-d2 (S)

2.662min (+0.071) 0.02ug/L

response 191

Ion	Exp%	Act%
63.00	100	100
98.00	68.90	79.58
65.00	23.20	21.99
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
 Data File : VU037989.D
 Acq On : 01 May 2020 15:07
 Operator : JC/MD
 Sample : L2471-06
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y19

Manual Integrations
 APPROVED

Sam
 5/4/2020 2:15:41 PM

Quant Time: May 02 00:12:09 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 02 00:09:57 2020
 Response via : Initial Calibration

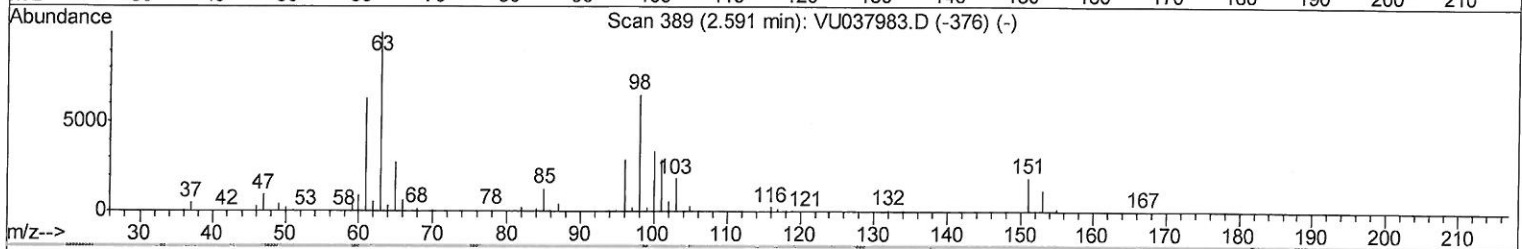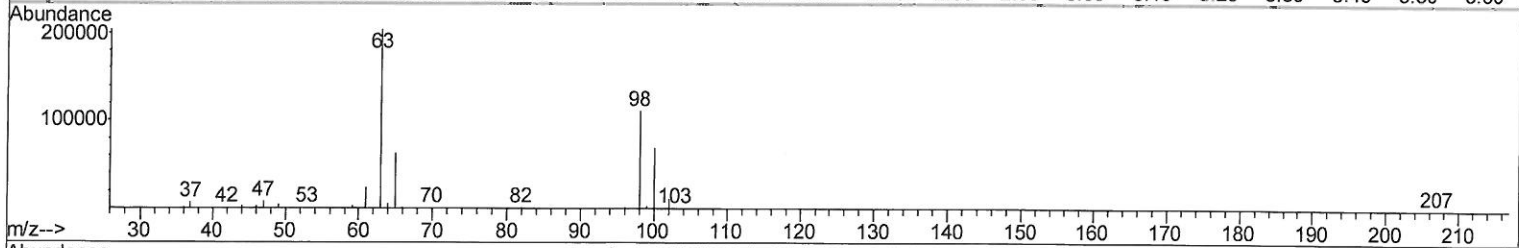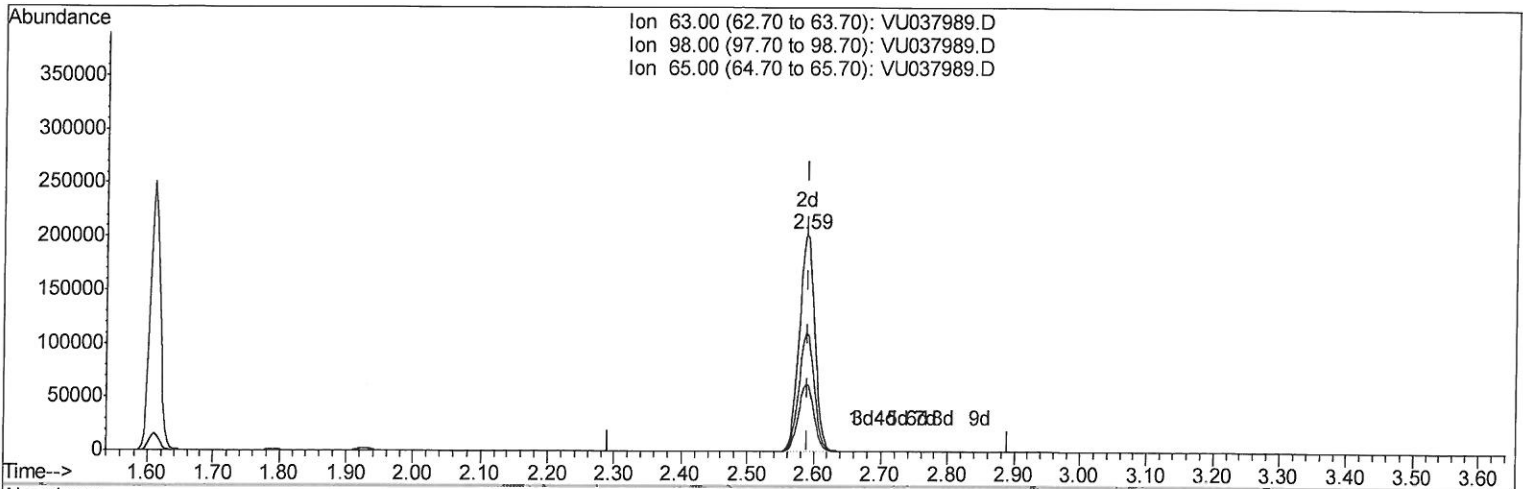

TIC: VU037989.D

(11) 1,1-Dichloroethene-d2 (S)

2.588min (-0.003) 32.90ug/L m

response 327160

Ion	Exp%	Act%
63.00	100	100
98.00	68.90	0.05#
65.00	23.20	0.01#
0.00	0.00	0.00

05/04/20 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050120\
Quantitation Report (LSC Reviewed)

Data File : VU037989.D
Acq On : 01 May 2020 15:07
Operator : JC/MD
Sample : L2471-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y19

Manual Integrations
APPROVED

sam
5/4/2020 2:15:41 PM

Quant Time: May 04 14:41:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 02 00:09:57 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	691118	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	675714	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	303818	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	263748	43.39	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	86.78%		
7) Chloroethane-d5	1.93	69	222211	44.94	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	89.88%		
11) 1,1-Dichloroethene-d2	2.59	63	327160m	32.90	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	65.80%		
21) 2-Butanone-d5	4.66	46	381966	80.39	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	80.39%		
24) Chloroform-d	5.10	84	400242	42.52	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	85.04%		
26) 1,2-Dichloroethane-d4	5.74	65	304608	46.58	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.16%		
32) Benzene-d6	5.76	84	923560	46.37	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.74%		
36) 1,2-Dichloropropane-d6	6.72	67	308880	46.77	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.54%		
41) Toluene-d8	7.92	98	829891	45.42	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	90.84%		
43) trans-1,3-Dichloropropene-	8.20	79	136706	44.15	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	88.30%		
47) 2-Hexanone-d5	8.65	63	282113	98.23	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.23%		
57) 1,1,2,2-Tetrachloroethane-	10.77	84	420151	44.15	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.30%		
64) 1,2-Dichlorobenzene-d4	12.20	152	292482	46.04	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	92.08%		

Target Compounds					Qvalue
9) Trichlorofluoromethane	2.16	101	27297	3.793	ug/L 98
20) cis-1,2-Dichloroethene	4.71	96	8122	1.503	ug/L 91
34) Trichloroethene	6.57	95	162205	31.667	ug/L 99
46) Tetrachloroethene	8.57	164	71413	19.096	ug/L 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

05/04/2020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050120\
Quantitation Report (LSC Reviewed)

Data File : VU037989.D
Acq On : 01 May 2020 15:07
Operator : JC/MD
Sample : L2471-06
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y19

Manual Integrations
APPROVED

sam
5/4/2020 2:15:41 PM

Quant Time: May 04 14:41:36 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 02 00:09:57 2020
Response via : Initial Calibration

