

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
 Data File : VU037990.D
 Acq On : 01 May 2020 15:30
 Operator : JC/MD
 Sample : L2471-07
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y20

Quant Time: May 04 14:42:20 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat May 02 00:09:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	6.28	114	695027	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.44	117	681433	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.83	152	306485	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.61	65	257050	42.05	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	84.10%
7) Chloroethane-d5	1.93	69	222690	44.78	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.56%
11) 1,1-Dichloroethene-d2	2.59	63	325901	32.59	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	65.18%
21) 2-Butanone-d5	4.66	46	419425	87.78	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.78%
24) Chloroform-d	5.10	84	407898	43.09	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	86.18%
26) 1,2-Dichloroethane-d4	5.74	65	298401	45.38	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.76%
32) Benzene-d6	5.76	84	918907	45.75	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.50%
36) 1,2-Dichloropropane-d6	6.72	67	306172	45.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	91.94%
41) Toluene-d8	7.92	98	823266	44.68	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	89.36%
43) trans-1,3-Dichloropropene-	8.20	79	135660	43.44	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.88%
47) 2-Hexanone-d5	8.66	63	276057	95.31	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	95.31%
57) 1,1,2,2-Tetrachloroethane-	10.77	84	416501	43.40	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.80%
64) 1,2-Dichlorobenzene-d4	12.20	152	291682	45.52	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	91.04%


Target Compounds					Ovalue
9) Trichlorofluoromethane	2.16	101	108481	14.989 ug/L	99
34) Trichloroethene	6.57	95	9746	1.887 ug/L	95
46) Tetrachloroethene	8.57	164	210868	55.912 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050120\
Data File : VU037990.D
Acq On : 01 May 2020 15:30
Operator : JC/MD
Sample : L2471-07
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0Y20

Quant Time: May 04 14:42:20 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis
QLast Update : Sat May 02 00:09:57 2020
Response via : Initial Calibration

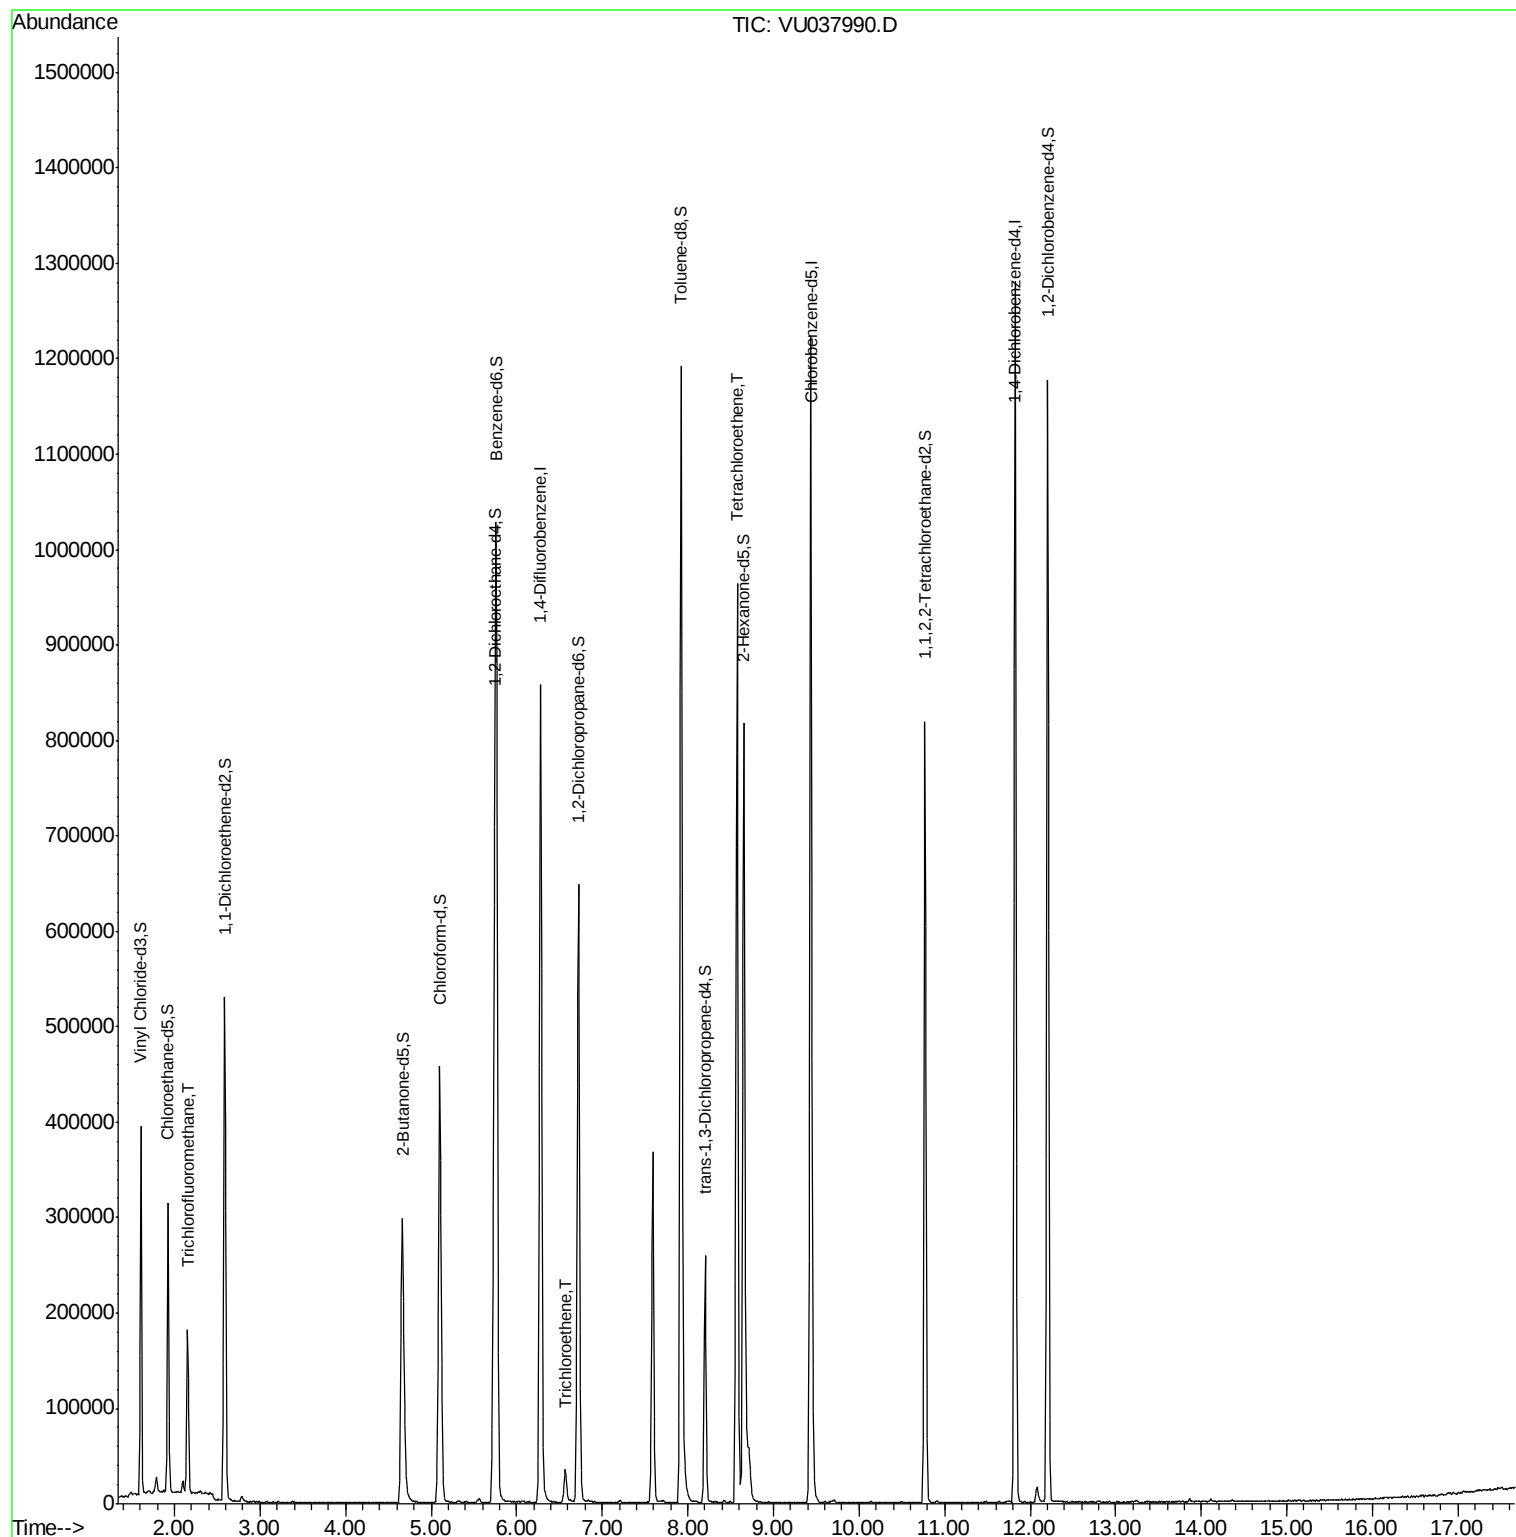




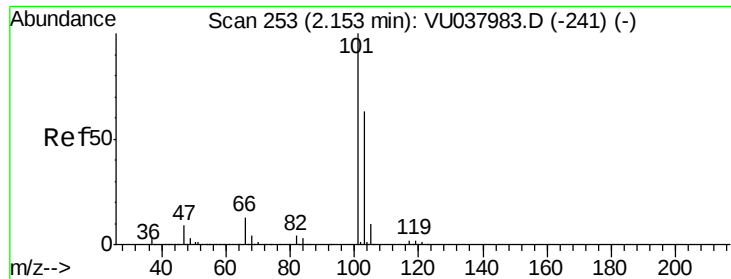


#9

Trichlorofluoromethane
 Concen: 14.989 ug/L
 RT: 2.16 min Scan# 254
 Delta R.T. 0.00 min
 Lab File: VU037990.D
 Acq: 01 May 2020 15:30

Instrument :
 MSVOA_U
 ClientSampleId :
 C0Y20




Tot Ion:101 Resp: 108481
 Ion Ratio Lower Upper
 101 100
 103 64.8 51.4 77.0

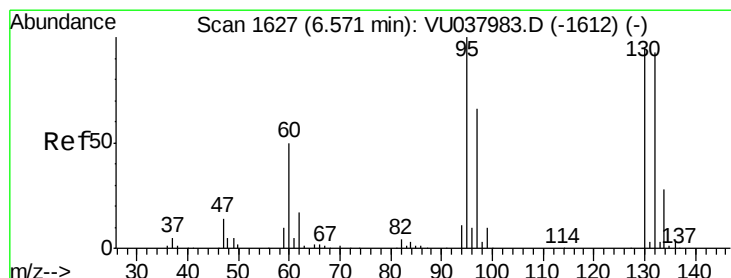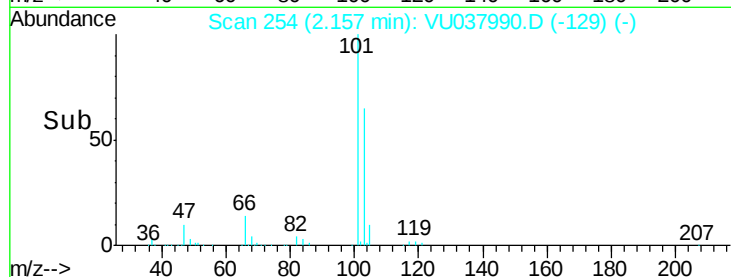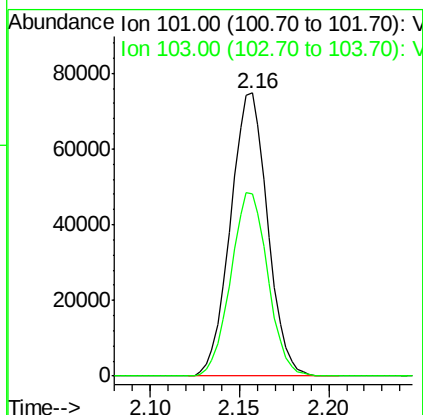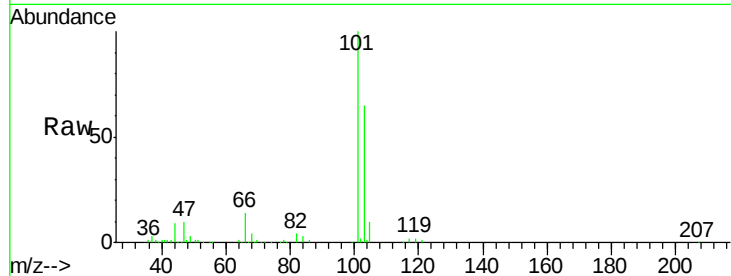


#34

Trichloroethene
 Concen: 1.887 ug/L
 RT: 6.57 min Scan# 1627
 Delta R.T. 0.00 min
 Lab File: VU037990.D
 Acq: 01 May 2020 15:30

Tgt Ion: 95 Resp: 9746
 Ion Ratio Lower Upper
 95 100
 97 66.2 44.9 83.5
 132 84.7 63.2 117.4
 130 87.6 65.9 122.3

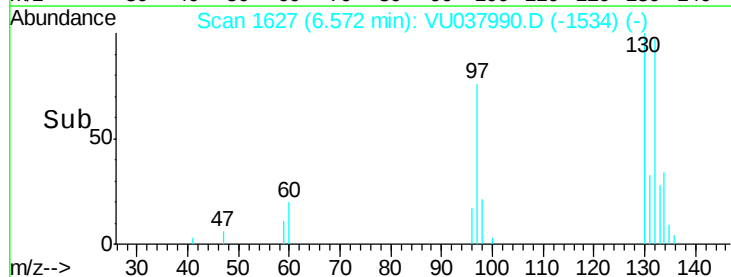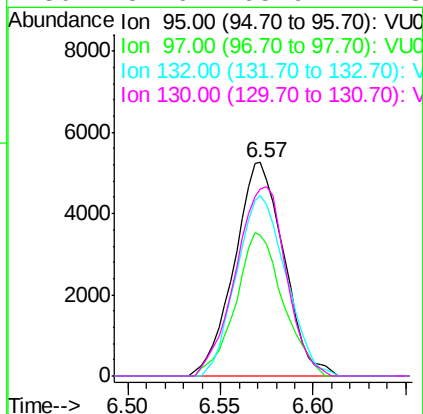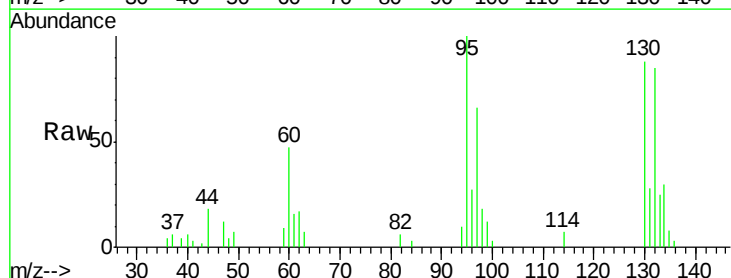

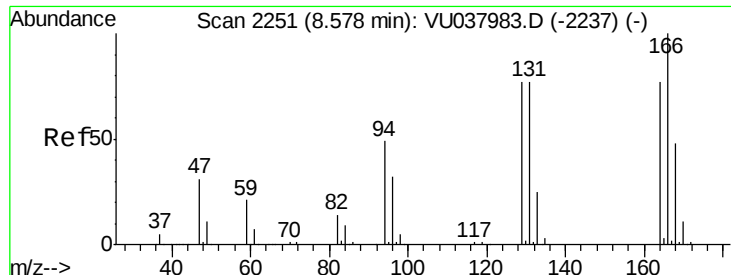

#46

Tetrachloroethene

Concen: 55.912 ug/L

RT: 8.57 min Scan# 2250

Delta R.T. -0.00 min

Lab File: VU037990.D


Acq: 01 May 2020 15:30

Instrument :

MSVOA_U

ClientSampleId :

C0Y20

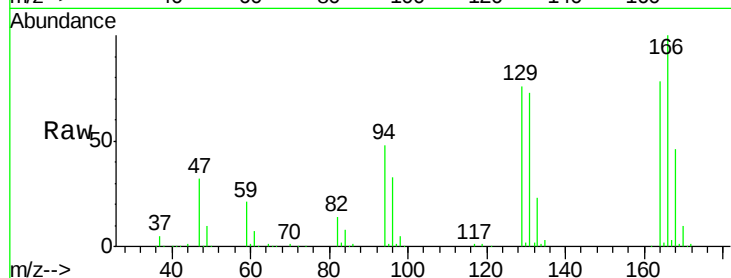

Tot Ion:164 Resp: 210868

Ion Ratio Lower Upper

164 100

129 97.1 68.4 127.0

131 93.6 65.7 122.1

166 128.6 86.7 161.1

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

