

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
 Data File : VU037986.D
 Acq On : 01 May 2020 13:59
 Operator : JC/MD
 Sample : L2410-19DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.366	3	8	18	rVB	19869	19111	0.73%	0.082%
2	1.610	75	84	99	rBV	388437	422248	16.15%	1.821%
3	1.890	165	171	187	rVB	301652	415902	15.91%	1.794%
4	2.578	373	385	405	rVB	511878	835506	31.96%	3.604%
5	2.813	450	458	462	rBV4	2246	3738	0.14%	0.016%
6	2.893	480	483	488	rBV6	713	541	0.02%	0.002%
7	3.034	523	527	529	rBV4	762	513	0.02%	0.002%
8	3.070	529	538	546	rVV4	2617	4853	0.19%	0.021%
9	3.105	546	549	552	rVB3	752	478	0.02%	0.002%
10	3.214	569	583	602	rBV	27144	68580	2.62%	0.296%
11	3.366	626	630	633	rVV3	1141	818	0.03%	0.004%
12	3.385	634	636	638	rBV3	896	454	0.02%	0.002%
13	3.436	648	652	656	rBV4	549	503	0.02%	0.002%
14	3.623	707	710	715	rVB4	1020	935	0.04%	0.004%
15	3.800	763	765	772	rVB3	432	412	0.02%	0.002%
16	3.951	807	812	816	rBV3	633	523	0.02%	0.002%
17	4.018	828	833	836	rBV3	684	505	0.02%	0.002%
18	4.105	854	860	862	rBV2	611	481	0.02%	0.002%
19	4.440	960	964	971	rVB2	440	484	0.02%	0.002%
20	4.581	1002	1008	1010	rVV3	705	775	0.03%	0.003%
21	4.665	1016	1034	1067	rBV2	265874	726881	27.80%	3.135%
22	5.099	1151	1169	1190	rBV	438342	987284	37.76%	4.259%
23	5.317	1230	1237	1241	rBV3	1869	2261	0.09%	0.010%
24	5.375	1252	1255	1258	rVB3	793	548	0.02%	0.002%
25	5.404	1258	1264	1268	rBV5	1527	2065	0.08%	0.009%
26	5.484	1287	1289	1294	rVB3	755	525	0.02%	0.002%
27	5.755	1350	1373	1397	rBV2	1000719	2614454	100.00%	11.277%
28	5.999	1443	1449	1450	rBV3	2118	1689	0.06%	0.007%
29	6.057	1464	1467	1469	rBV2	753	521	0.02%	0.002%
30	6.134	1484	1491	1492	rBV	733	678	0.03%	0.003%
31	6.279	1518	1536	1562	rBV	850265	1630619	62.37%	7.033%
32	6.558	1612	1623	1636	rBV8	12409	28551	1.09%	0.123%
33	6.719	1657	1673	1691	rBV	630160	1209776	46.27%	5.218%
34	6.902	1725	1730	1731	rBV	539	432	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
 Data File : VU037986.D
 Acq On : 01 May 2020 13:59
 Operator : JC/MD
 Sample : L2410-19DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

35	7.002	1756	1761	1762	rBV2	560	423	0.02%	0.002%
36	7.208	1817	1825	1829	rBV7	2794	3696	0.14%	0.016%
37	7.375	1873	1877	1879	rBV2	519	406	0.02%	0.002%
38	7.587	1929	1943	1960	rBV	357231	618915	23.67%	2.670%
39	7.706	1975	1980	1983	rBV3	1301	1510	0.06%	0.007%
40	7.819	2001	2015	2025	rBV6	3185	6348	0.24%	0.027%
41	7.922	2029	2047	2086	rBV	1194290	2159226	82.59%	9.314%
42	8.201	2121	2134	2153	rVV	251904	419474	16.04%	1.809%
43	8.365	2182	2185	2191	rBV4	664	527	0.02%	0.002%
44	8.488	2217	2223	2236	rVB4	1943	3423	0.13%	0.015%
45	8.571	2236	2249	2264	rBV	931375	1613339	61.71%	6.959%
46	8.658	2265	2276	2290	rBV	865529	1497120	57.26%	6.458%
47	8.841	2331	2333	2336	rVB2	869	404	0.02%	0.002%
48	8.873	2338	2343	2348	rVB5	872	863	0.03%	0.004%
49	8.918	2354	2357	2361	rBV3	664	496	0.02%	0.002%
50	8.951	2364	2367	2372	rVB6	768	617	0.02%	0.003%
51	9.012	2384	2386	2391	rVB3	673	430	0.02%	0.002%
52	9.436	2504	2518	2555	rVB	1225044	2111220	80.75%	9.106%
53	9.584	2558	2564	2571	rBV3	1999	2199	0.08%	0.009%
54	9.661	2583	2588	2590	rBV4	1356	1066	0.04%	0.005%
55	9.706	2600	2602	2610	rVB6	3455	3620	0.14%	0.016%
56	9.902	2658	2663	2673	rVB4	928	1122	0.04%	0.005%
57	9.947	2673	2677	2679	rBV	582	407	0.02%	0.002%
58	10.025	2700	2701	2710	rVB3	517	499	0.02%	0.002%
59	10.079	2714	2718	2722	rBV2	493	405	0.02%	0.002%
60	10.124	2722	2732	2741	rVV7	3085	5291	0.20%	0.023%
61	10.205	2753	2757	2760	rBV2	445	409	0.02%	0.002%
62	10.285	2778	2782	2787	rBV2	2305	2235	0.09%	0.010%
63	10.311	2787	2790	2793	rVV	1243	952	0.04%	0.004%
64	10.330	2794	2796	2801	rVV	942	810	0.03%	0.003%
65	10.365	2801	2807	2810	rVV	2081	2281	0.09%	0.010%
66	10.391	2810	2815	2818	rVV2	1558	1675	0.06%	0.007%
67	10.410	2819	2821	2827	rVV	1809	1434	0.05%	0.006%
68	10.455	2831	2835	2841	rVV	1342	1642	0.06%	0.007%
69	10.500	2841	2849	2856	rVV5	2257	3378	0.13%	0.015%
70	10.555	2864	2866	2869	rVB	995	541	0.02%	0.002%
71	10.571	2869	2871	2876	rVB2	465	433	0.02%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU050120\
 Data File : VU037986.D
 Acq On : 01 May 2020 13:59
 Operator : JC/MD
 Sample : L2410-19DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF5DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis

72	10.603	2877	2881	2883	rBV	975	614	0.02%	0.003%
73	10.774	2919	2934	2951	rBV	904372	1453819	55.61%	6.271%
74	11.095	3028	3034	3036	rBV4	1262	1274	0.05%	0.005%
75	11.298	3094	3097	3101	rVV2	641	418	0.02%	0.002%
76	11.320	3101	3104	3110	rVB3	1054	786	0.03%	0.003%
77	11.481	3147	3154	3160	rBV4	2303	2625	0.10%	0.011%
78	11.526	3165	3168	3173	rVB3	595	547	0.02%	0.002%
79	11.754	3233	3239	3248	rVB6	2906	4656	0.18%	0.020%
80	11.825	3248	3261	3279	rBV	1361141	2169072	82.96%	9.356%
81	12.015	3317	3320	3324	rVB	763	428	0.02%	0.002%
82	12.134	3354	3357	3360	rVB2	903	480	0.02%	0.002%
83	12.204	3365	3379	3397	rVV	1269566	2059516	78.77%	8.883%
84	12.336	3416	3420	3427	rVB3	870	1121	0.04%	0.005%
85	12.397	3434	3439	3442	rBV2	747	739	0.03%	0.003%
86	12.439	3449	3452	3459	rVB3	1084	1010	0.04%	0.004%
87	12.536	3477	3482	3486	rBV3	632	670	0.03%	0.003%
88	12.796	3560	3563	3567	rVB2	1030	647	0.02%	0.003%
89	13.015	3629	3631	3634	rBV2	661	435	0.02%	0.002%
90	13.147	3667	3672	3675	rBV3	430	437	0.02%	0.002%
91	13.240	3693	3701	3711	rVB7	3768	5871	0.22%	0.025%
92	13.368	3737	3741	3743	rBV	520	433	0.02%	0.002%
93	13.436	3760	3762	3768	rVB3	630	591	0.02%	0.003%
94	13.468	3768	3772	3777	rBV2	549	633	0.02%	0.003%
95	13.867	3888	3896	3904	rBV6	4803	7808	0.30%	0.034%
96	13.986	3930	3933	3936	rBV2	725	471	0.02%	0.002%
97	14.114	3966	3973	3981	rBV3	5604	8971	0.34%	0.039%
98	14.362	4044	4050	4062	rVB9	3540	5641	0.22%	0.024%
99	14.417	4065	4067	4071	rBV	728	400	0.02%	0.002%
100	15.127	4285	4288	4293	rVB3	1160	1082	0.04%	0.005%


Sum of corrected areas: 23183675

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU050120\
Data File : VU037986.D
Acq On : 01 May 2020 13:59
Operator : JC/MD
Sample : L2410-19DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

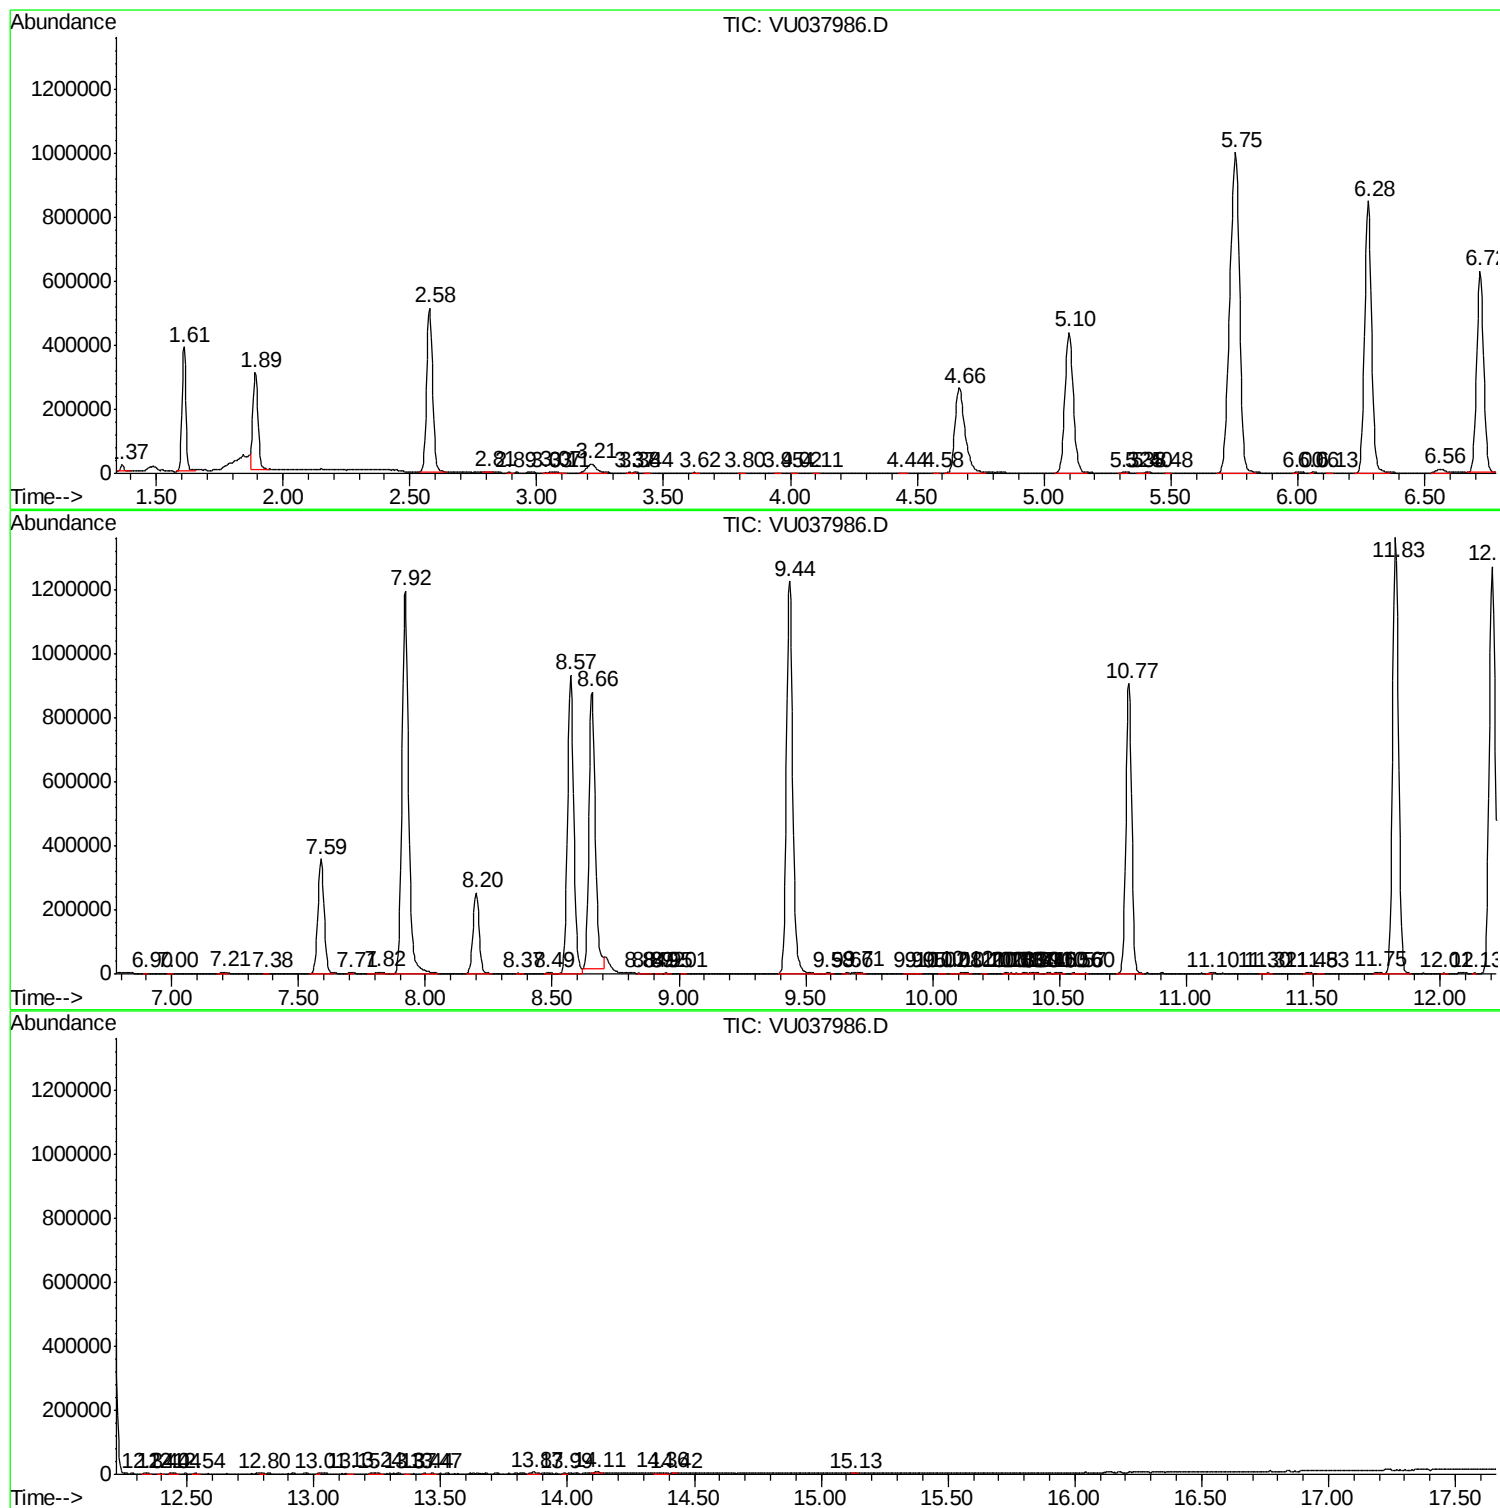

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU050120\
Data File : VU037986.D
Acq On : 01 May 2020 13:59
Operator : JC/MD
Sample : L2410-19DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF5DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU050120\
Data File : VU037986.D
Acq On : 01 May 2020 13:59
Operator : JC/MD
Sample : L2410-19DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF5DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc