


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU050620\
 Data File : VU038016.D
 Acq On : 06 May 2020 10:21
 Operator : JC/MD
 Sample : BFB47
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM043020WMA.M
 Title : VOC Analysis
 Last Update : Thu May 07 01:04:11 2020

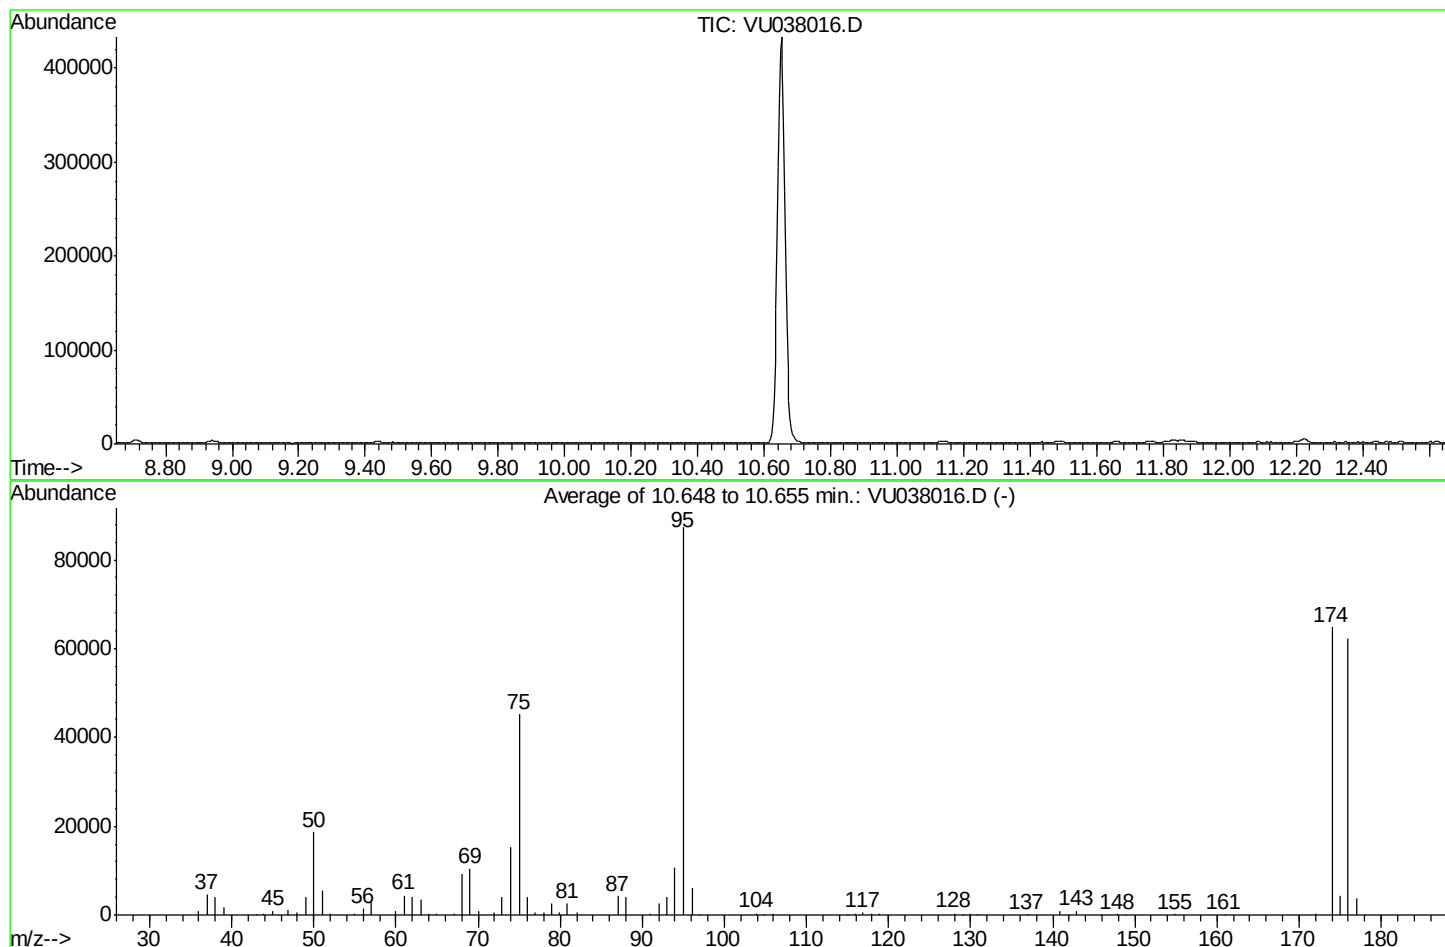

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	18645	PASS
75	95	30	80	51.7	45152	PASS
95	95	100	100	100.0	87336	PASS
96	95	5	9	6.8	5940	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	74.2	64800	PASS
175	174	5	9	6.9	4448	PASS
176	174	95	101	96.1	62280	PASS
177	176	5	9	5.9	3679	PASS

m/z	Abundance
36.00	878.0
37.00	4705.0
38.00	3816.0
39.00	1843.0
39.90	273.0
43.90	1344.0
45.00	870.0
46.90	1126.0
48.00	707.0
49.00	4296.0
50.00	19032.0
51.00	5487.0
52.10	200.0
54.90	256.0
56.00	1456.0
57.00	2825.0
60.00	667.0
61.00	4734.0
62.00	3936.0
63.00	3226.0
64.00	330.0
65.00	291.0
67.00	293.0
68.00	9289.0
69.00	10827.0
70.10	772.0
72.00	567.0
72.90	4216.0
74.00	15747.0
75.00	45456.0
76.00	3931.0
77.00	586.0
77.90	532.0
78.90	2539.0
79.90	696.0
80.90	2449.0
82.00	501.0
87.00	4307.0
88.00	3961.0
90.90	183.0
92.00	2629.0
93.00	4101.0
94.00	10560.0
95.00	87552.0
96.10	6113.0
96.90	147.0
103.90	405.0
104.80	117.0
105.90	343.0
115.00	119.0
115.80	284.0
116.90	558.0
117.90	338.0
118.90	440.0
128.00	300.0
129.00	113.0
129.90	274.0
130.80	153.0
137.00	127.0
140.90	831.0
142.90	807.0
145.90	120.0
147.90	272.0
148.80	162.0
154.90	189.0
172.00	362.0
174.00	63768.0
175.00	4662.0
176.00	61112.0
177.00	3318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
36.00	868.0
37.00	4679.0
38.00	4110.0
39.00	1855.0
39.90	314.0
44.00	1327.0
45.00	937.0
46.90	1147.0
48.00	704.0
49.00	4351.0
50.00	19224.0
51.00	5730.0
52.10	173.0
54.90	252.0
56.00	1429.0
57.00	2906.0
60.00	771.0
61.00	4540.0
62.00	4029.0
63.00	3492.0
63.90	330.0
65.00	273.0
67.10	245.0
68.00	9479.0
69.00	10828.0
70.10	748.0
71.90	516.0
73.00	4266.0
74.00	15658.0
75.00	46600.0
76.00	4124.0
77.00	632.0
78.00	509.0
78.90	2722.0
79.90	687.0
80.90	2655.0
82.00	476.0
87.00	4455.0
88.00	4203.0
90.90	210.0
92.00	2744.0
93.00	4185.0
94.00	11002.0
95.00	90288.0
96.10	6115.0
96.90	142.0
104.00	395.0
104.80	109.0
105.90	290.0
115.80	303.0
116.90	605.0
117.90	367.0
118.90	469.0
128.00	317.0
129.00	127.0
129.90	297.0
130.80	147.0
136.90	160.0
140.90	761.0
141.90	106.0
142.90	927.0
145.90	121.0
147.90	236.0
148.90	121.0
154.90	216.0
160.90	119.0
172.00	297.0
174.00	66904.0
175.00	4559.0
176.00	64432.0
177.00	3826.0
178.00	123.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

m/z	Abundance
35.00	773.0
37.00	4243.0
38.00	3886.0
39.00	1747.0
40.00	350.0
43.00	134.0
44.00	1379.0
45.00	900.0
46.00	1040.0
48.00	608.0
49.00	3915.0
50.00	17680.0
51.00	5466.0
52.00	167.0
54.00	228.0
56.00	1370.0
57.00	2619.0
59.00	790.0
61.00	3902.0
62.00	3886.0
63.00	3296.0
63.00	281.0
65.00	264.0
68.00	9069.0
69.00	9507.0
70.00	803.0
71.00	466.0
73.00	4033.0
74.00	14507.0
75.00	43400.0
76.00	3996.0
76.00	621.0
77.00	452.0
78.00	2478.0
79.00	655.0
80.00	2677.0
82.00	417.0
87.00	4065.0
88.00	3966.0
90.00	231.0
92.00	2533.0
93.00	3911.0
94.00	10073.0
95.00	84168.0
96.00	5592.0
97.00	110.0
104.00	343.0
104.00	112.0
105.00	258.0
115.00	281.0
116.00	546.0
117.00	345.0
118.00	409.0
128.00	292.0
128.00	149.0
129.00	271.0
136.00	179.0
140.00	654.0
142.00	962.0
147.00	159.0
155.00	238.0
160.00	120.0
172.00	223.0
174.00	63728.0
175.00	4125.0
176.00	61296.0
177.00	3893.0
177.00	101.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47

Scan 2882 (10.607 min): VU038016.D
BFB47

m/z	Abundance
39.00	117.0
40.00	312.0
43.90	922.0

Instrument :
MSVOA_U
ClientSampleId :
BFB47