


Dichlorodifluoromethane

Response Ratio

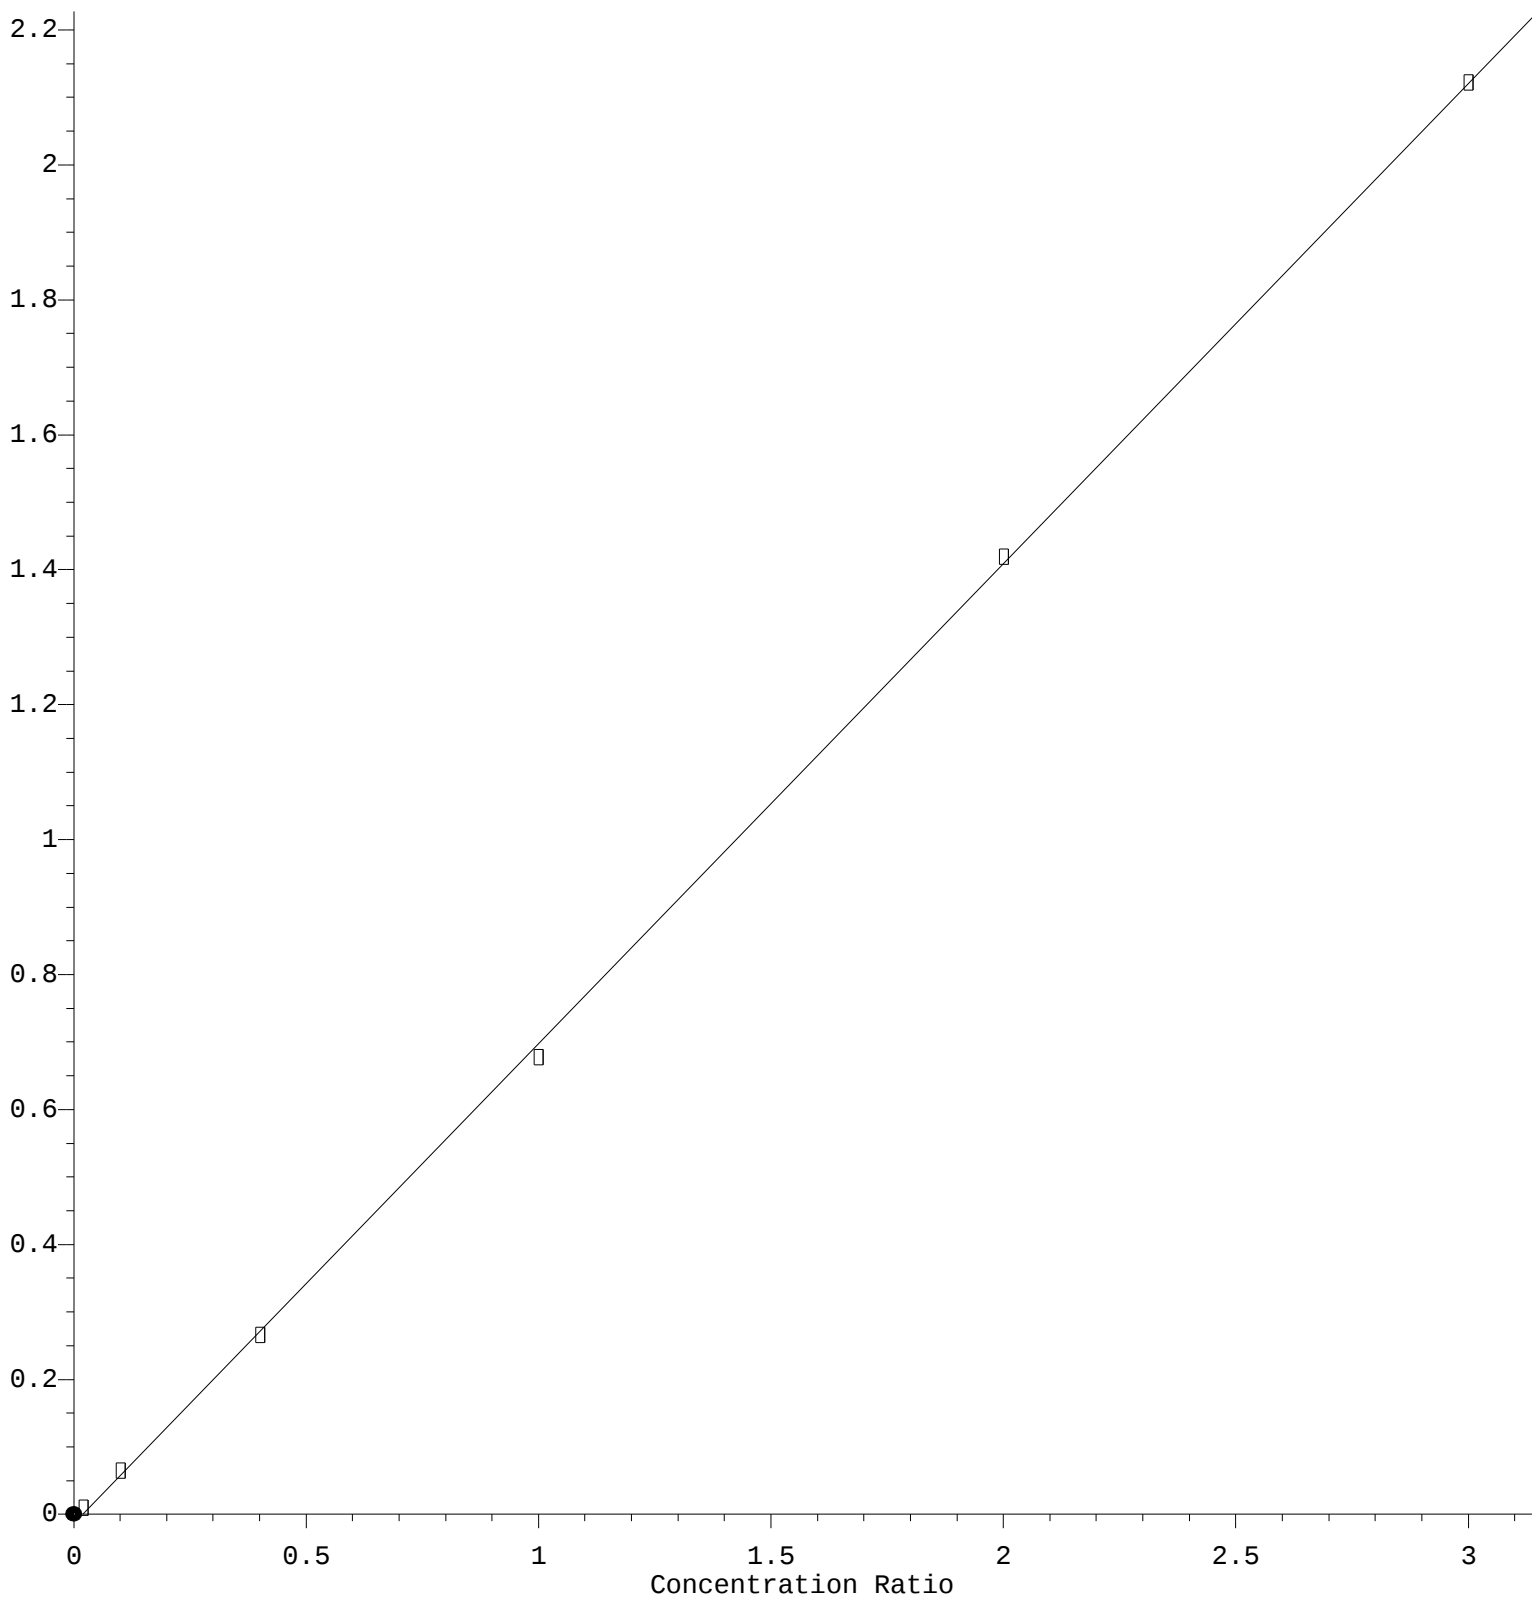

$$\text{Response} = 7.114\text{e-}001 * \text{Amt} - 1.363\text{e-}002$$


Coef of Det (r^2) = 0.999820 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Chloromethane

Response Ratio

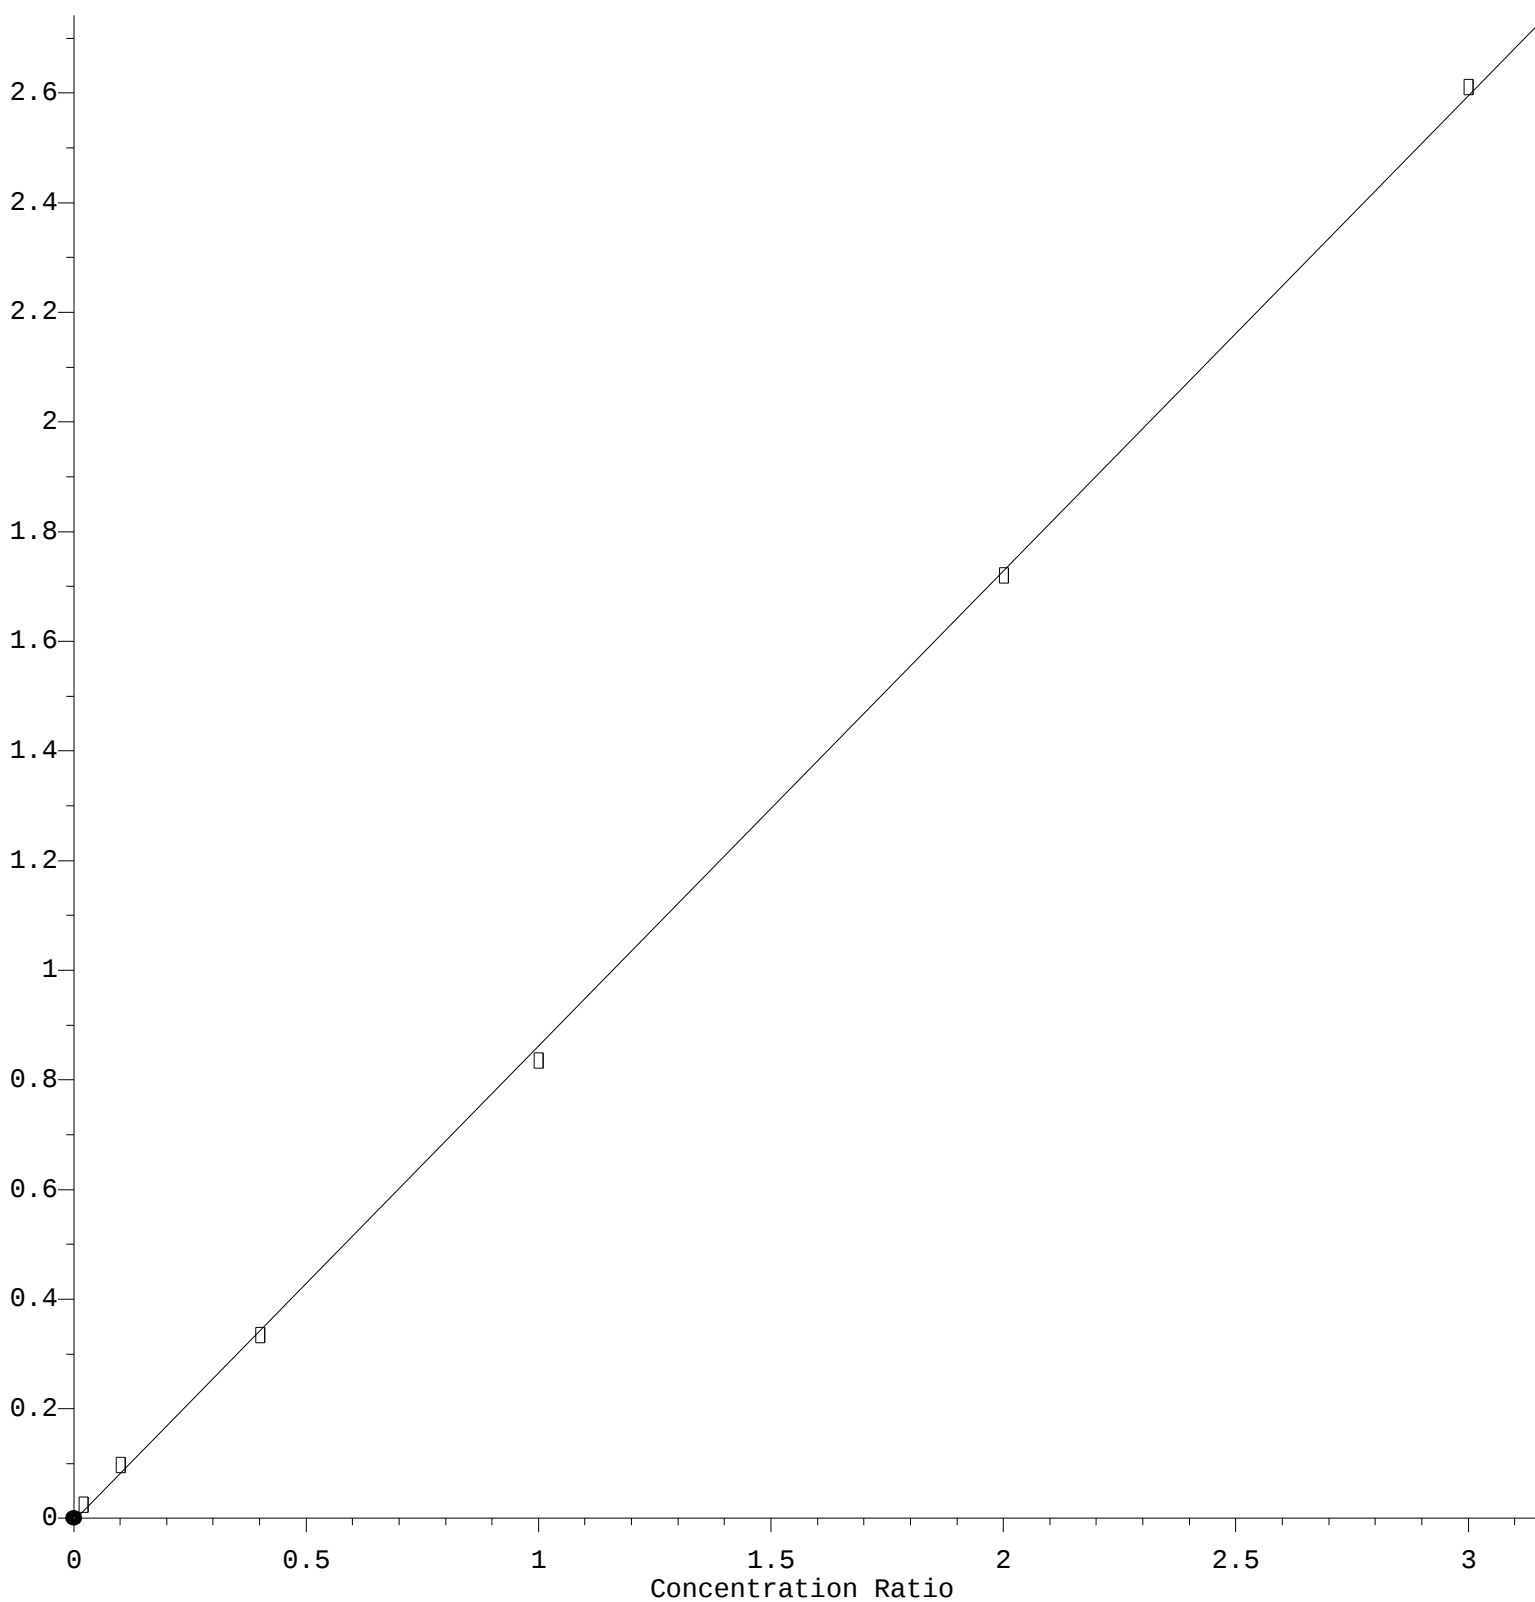

$$\text{Response} = 8.668\text{e-}001 * \text{Amt} - 5.128\text{e-}003$$


Coef of Det (r^2) = 0.999714 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Acrolein

Response Ratio

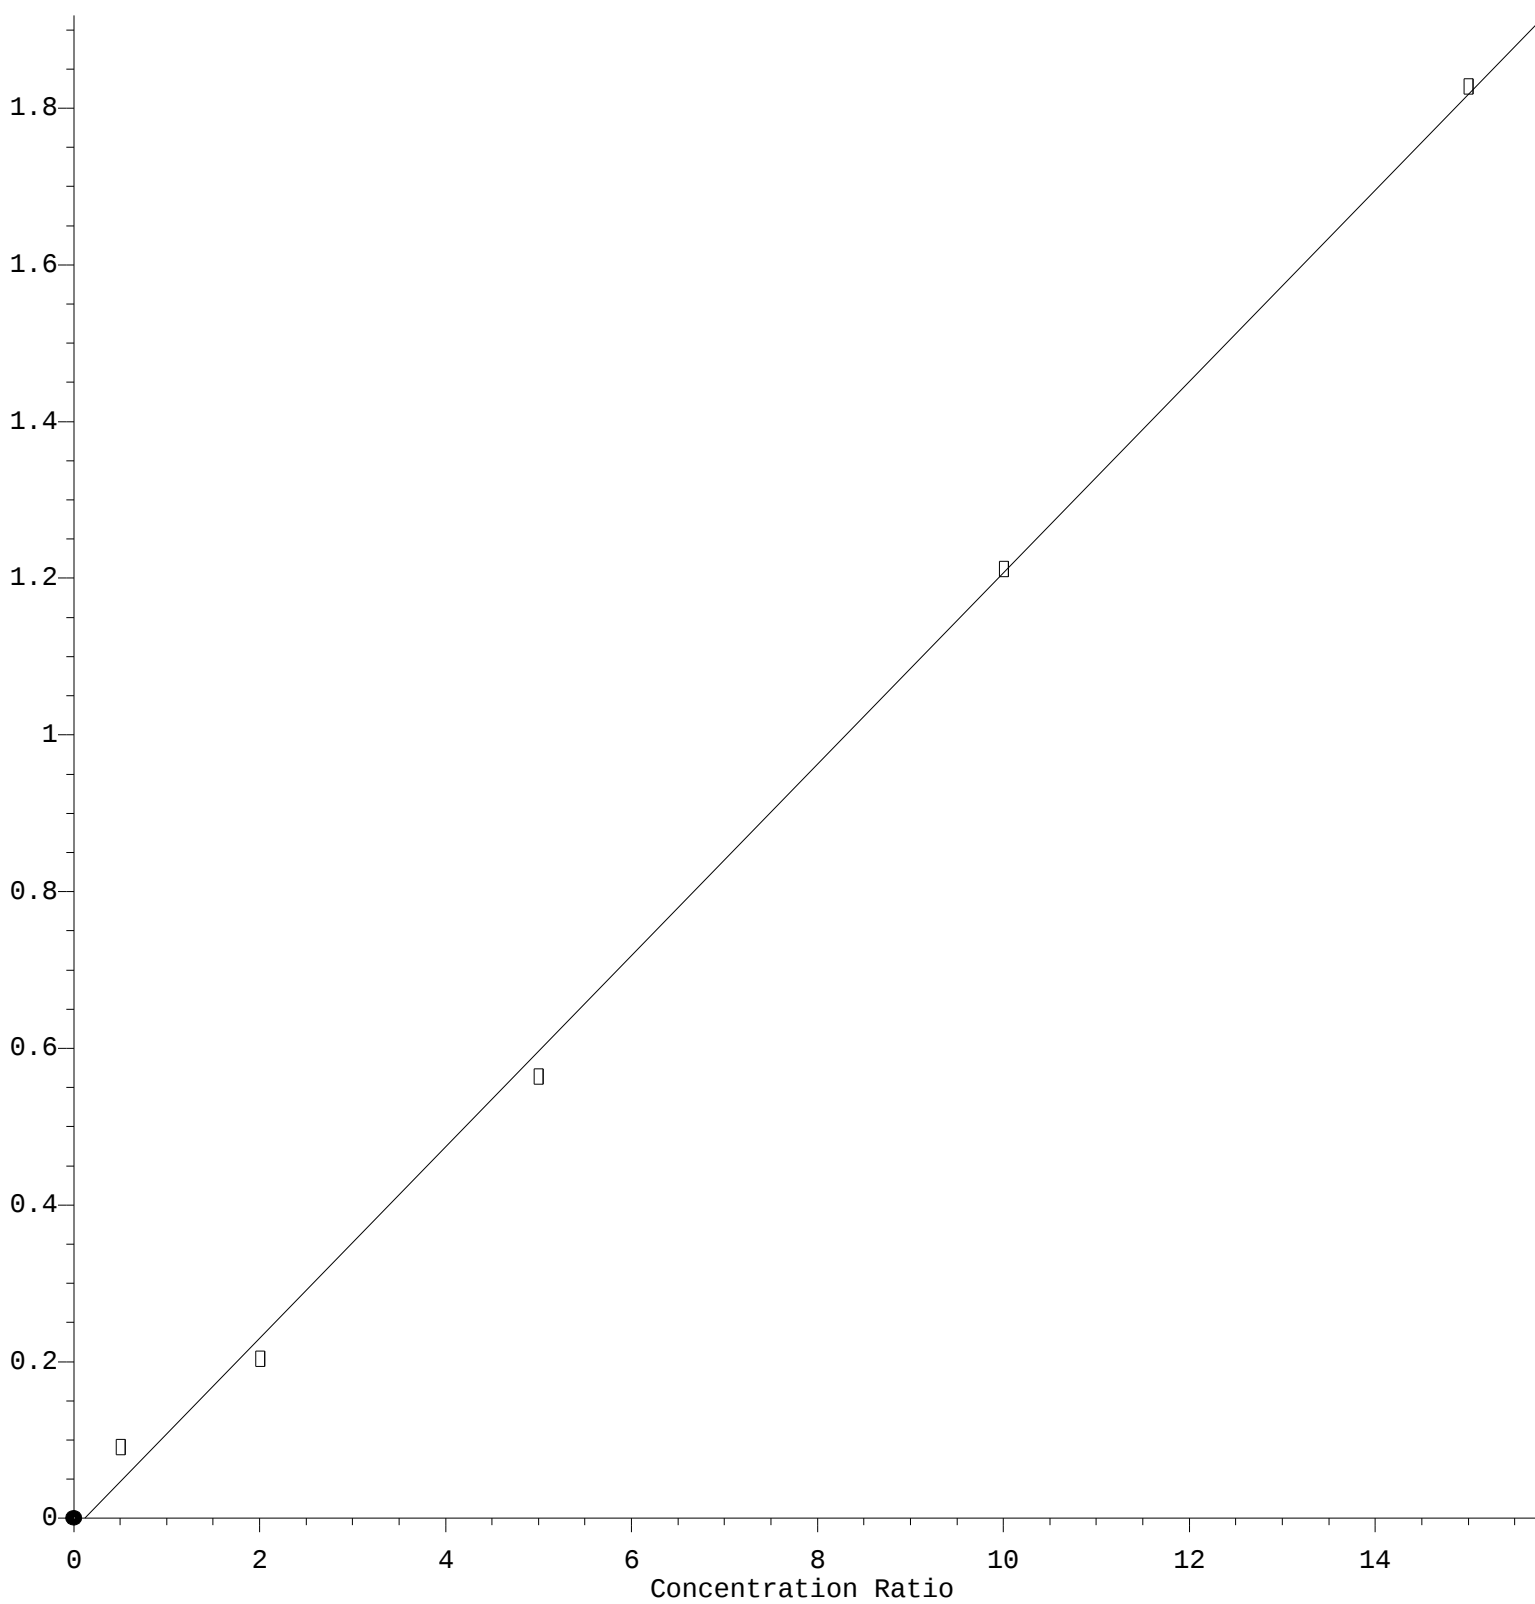

$$\text{Response} = 1.222\text{e-}001 * \text{Amt} - 1.475\text{e-}002$$


Coef of Det (r^2) = 0.998194 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Vinyl Acetate


Response Ratio

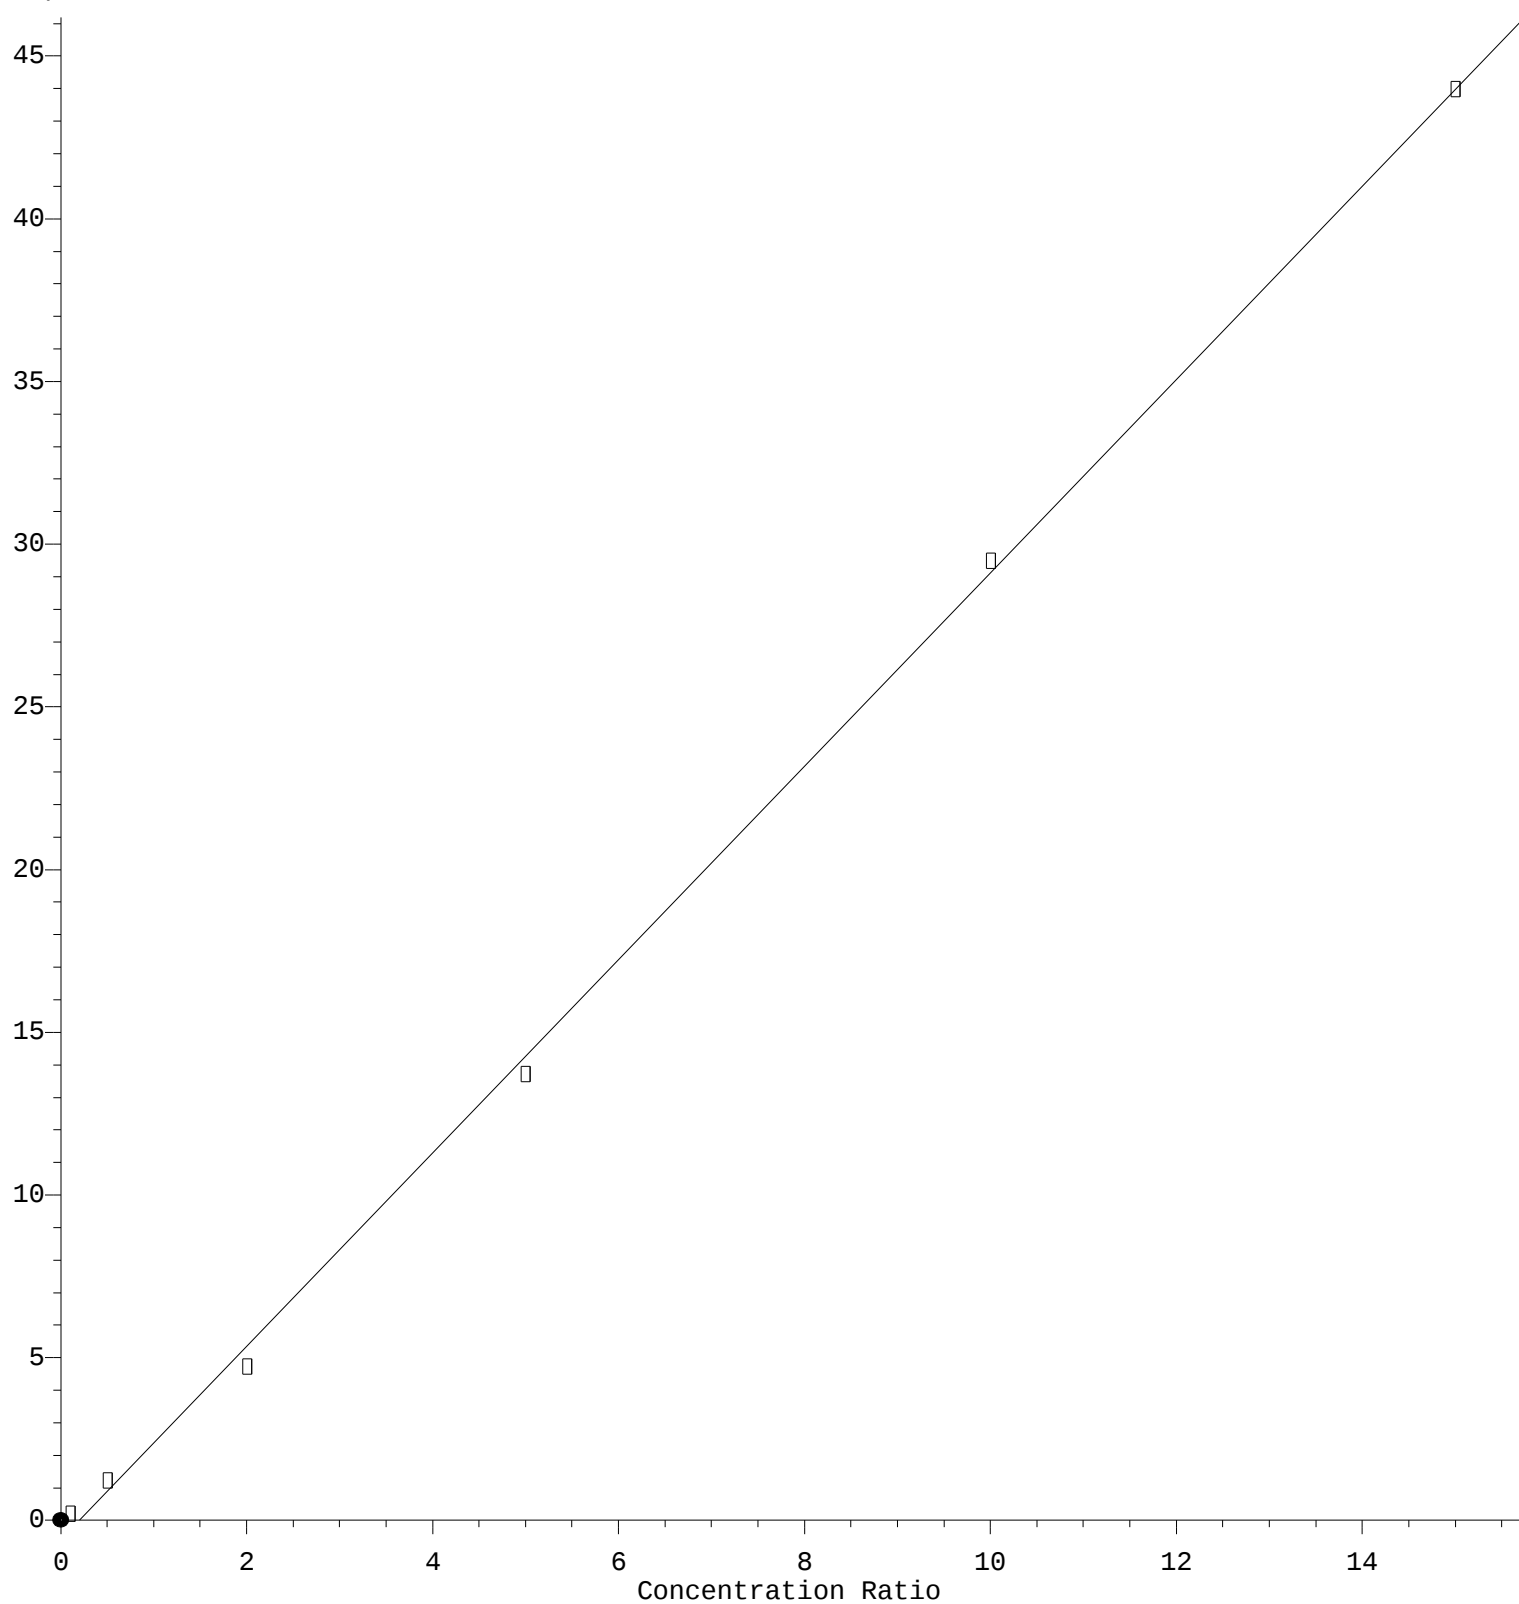

$\text{Response} = 2.971\text{e}+000 * \text{Amt} - 5.913\text{e}-001$
 Coef of Det (r^2) = 0.999249 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
 Calibration Table Last Updated: Thu May 06 07:26:23 2021

Methacrylonitrile

Response Ratio

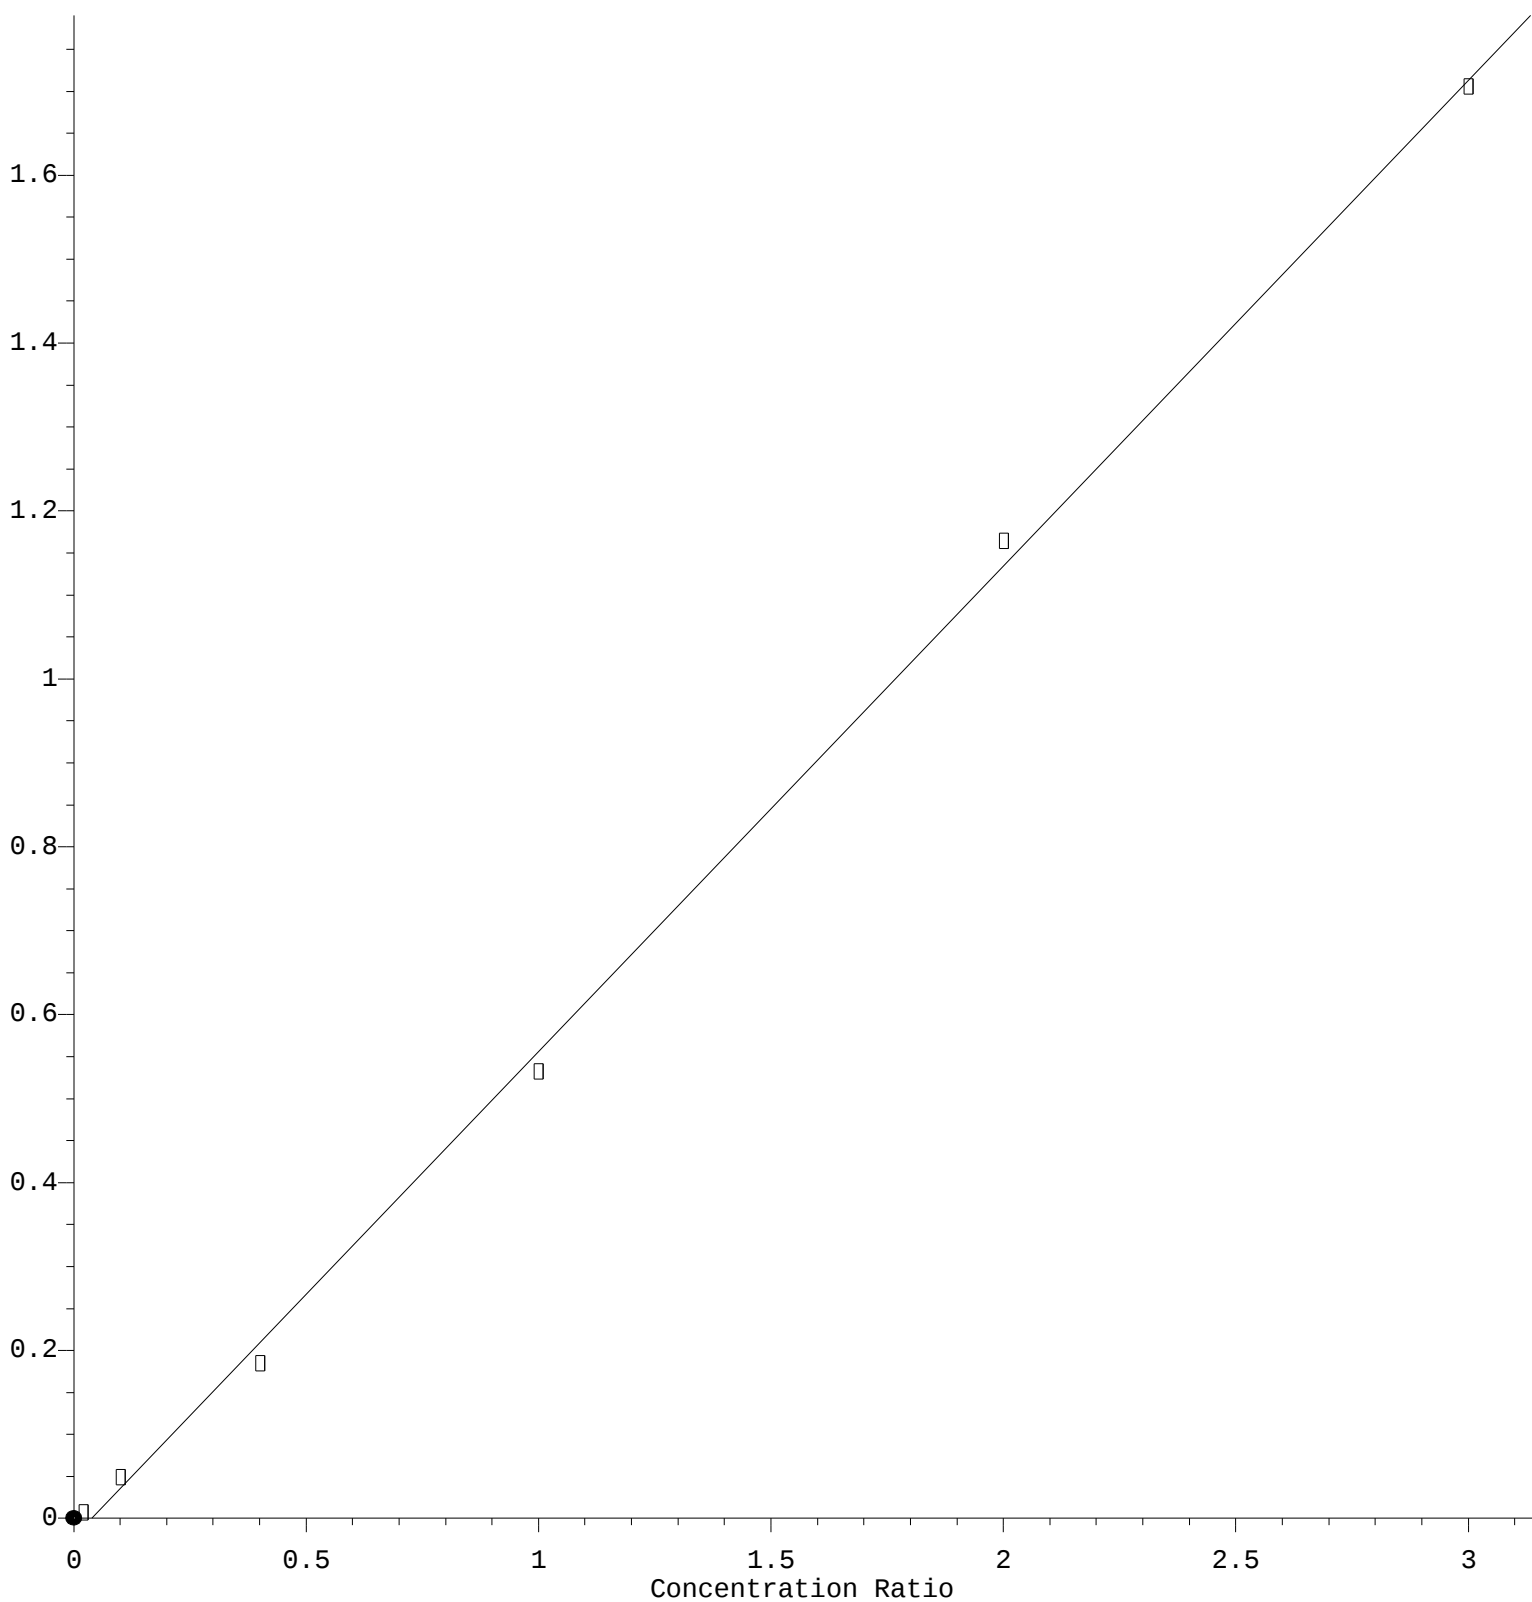


$$\text{Response} = 5.784\text{e-}001 * \text{Amt} - 2.178\text{e-}002$$

Coef of Det (r^2) = 0.998895 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021


1,4-Dioxane

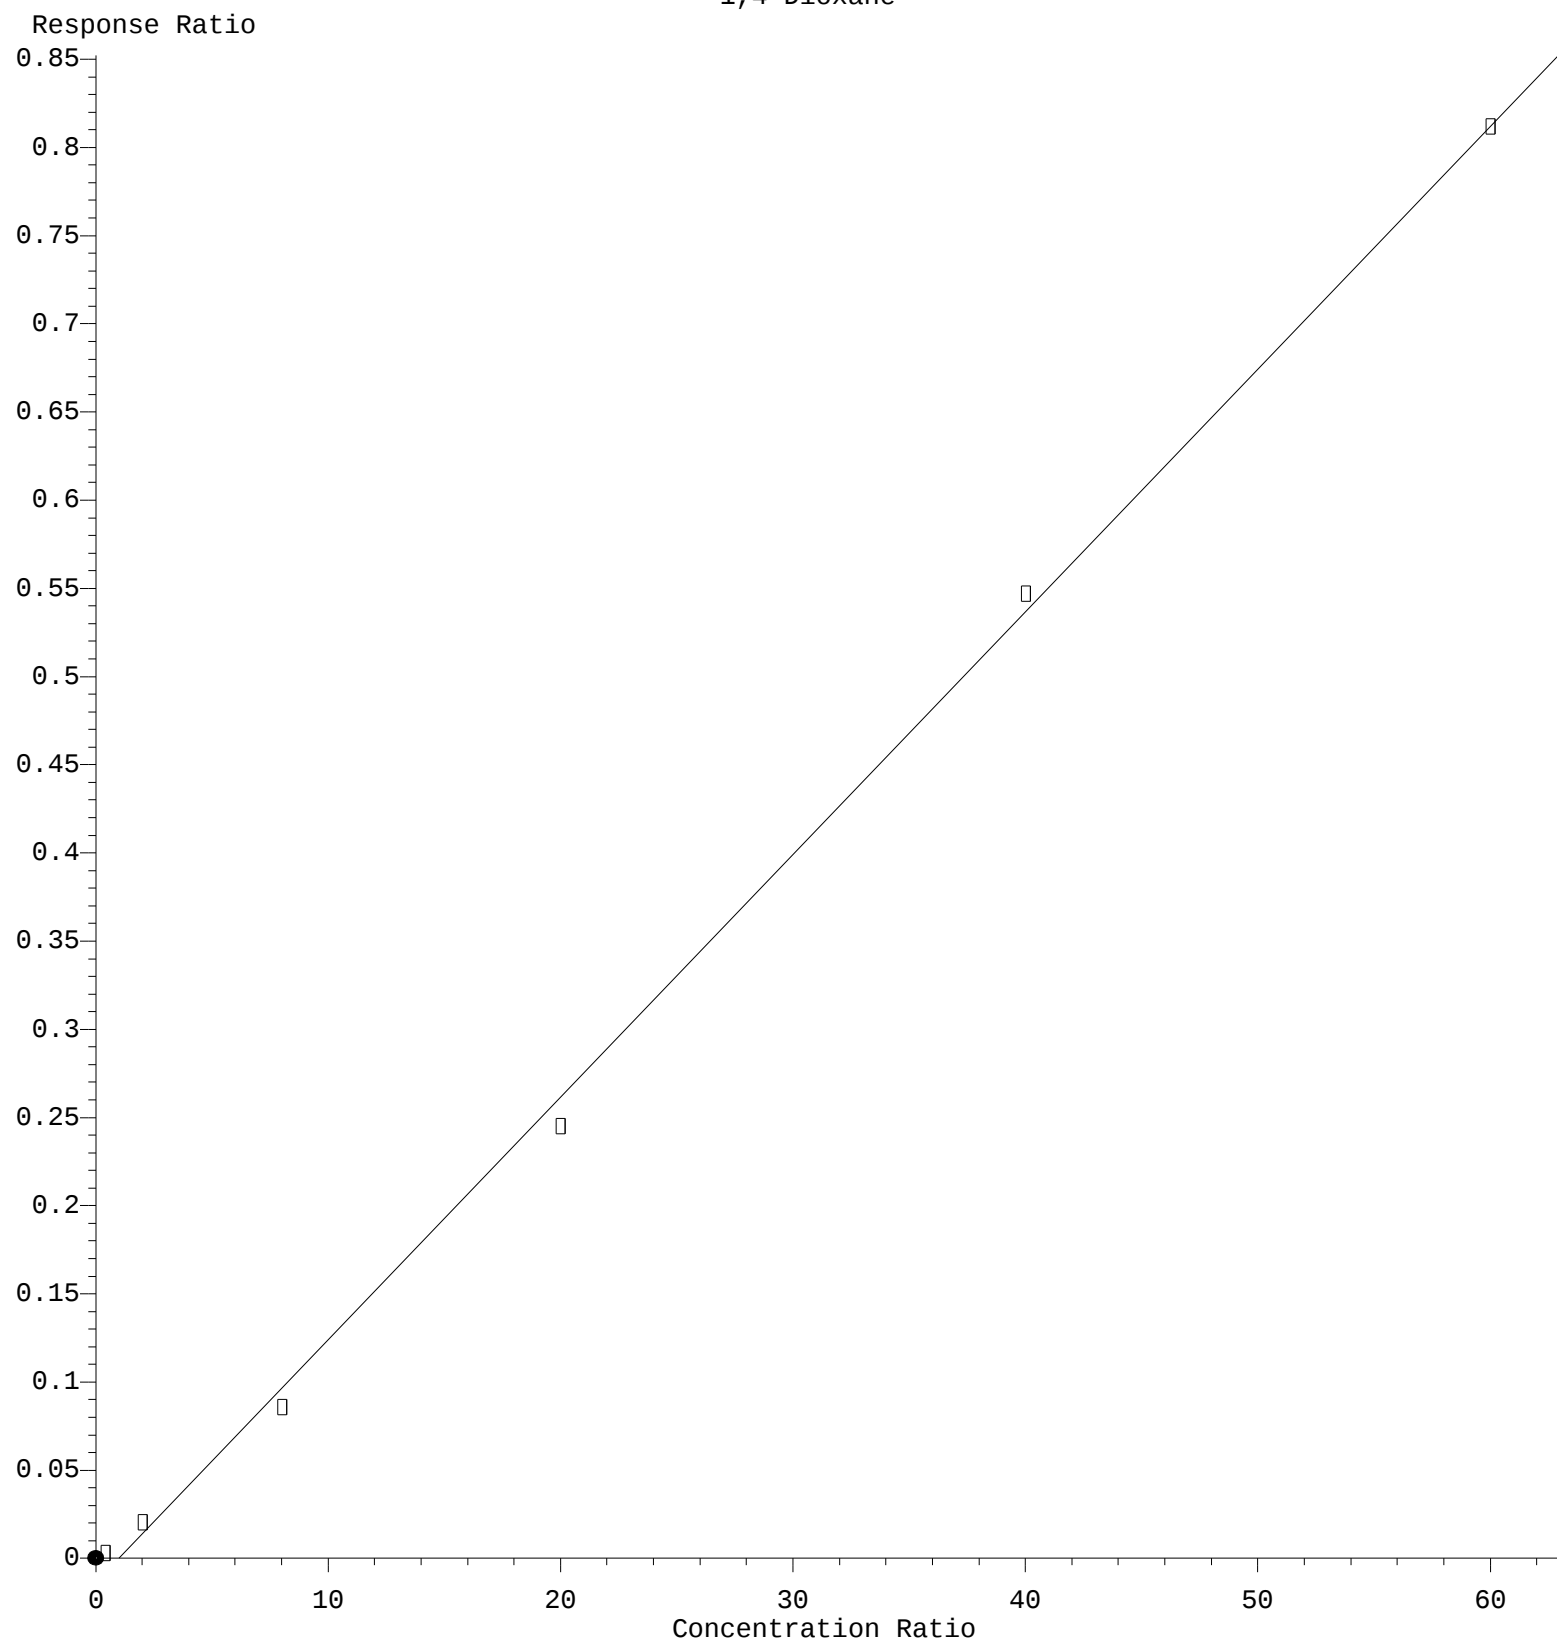

Response = $1.376 \times 10^{-2} \times \text{Amt} - 1.354 \times 10^{-2}$
 Coef of Det (r^2) = 0.998784 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
 Calibration Table Last Updated: Thu May 06 07:26:23 2021

4-Methyl-2-Pentanone

Response Ratio

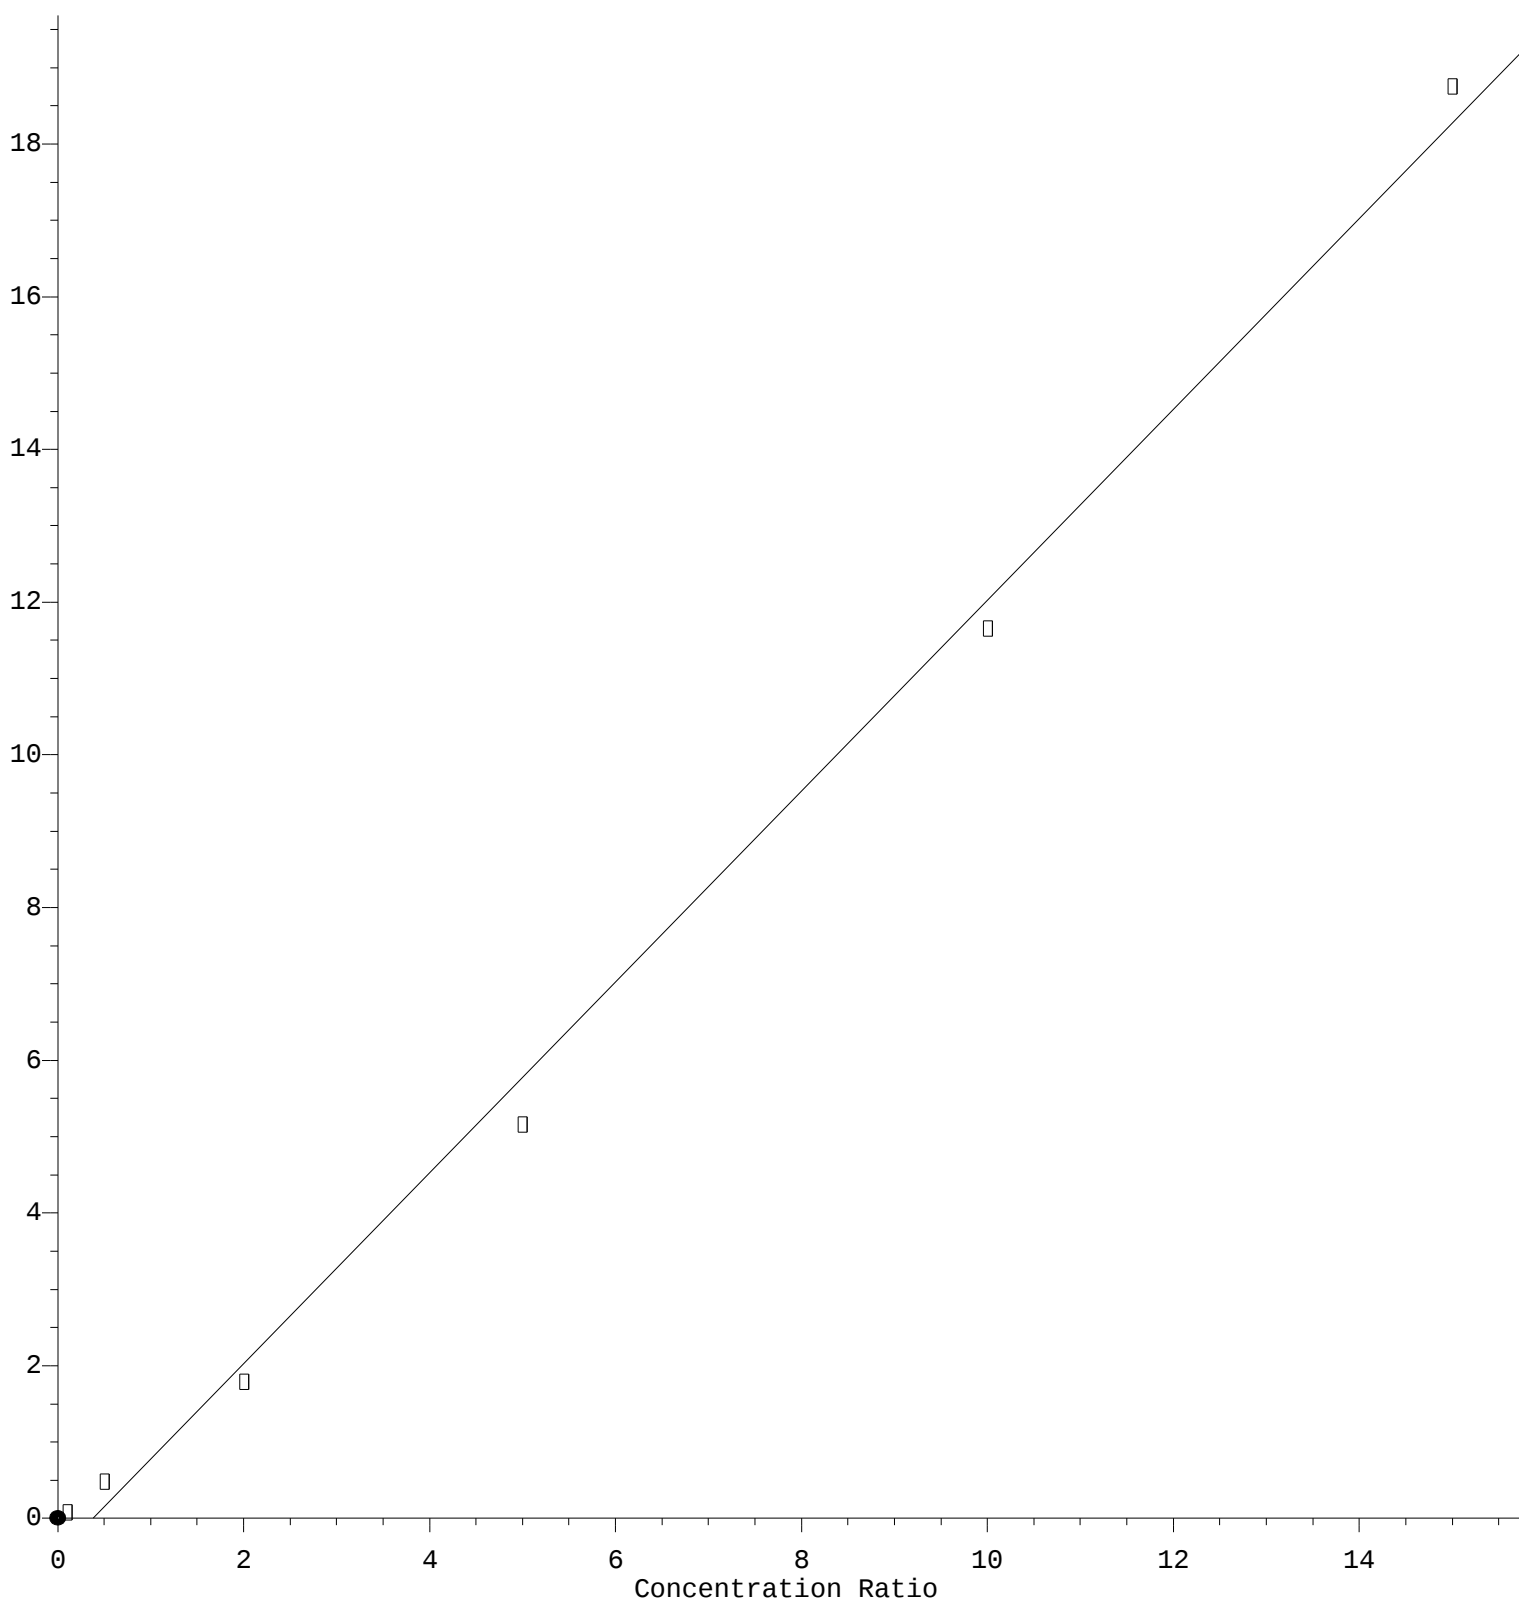

$$\text{Response} = 1.250\text{e}+000 * \text{Amt} - 4.798\text{e}-001$$


Coef of Det (r^2) = 0.996080 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

t-1,3-Dichloropropene

Response Ratio

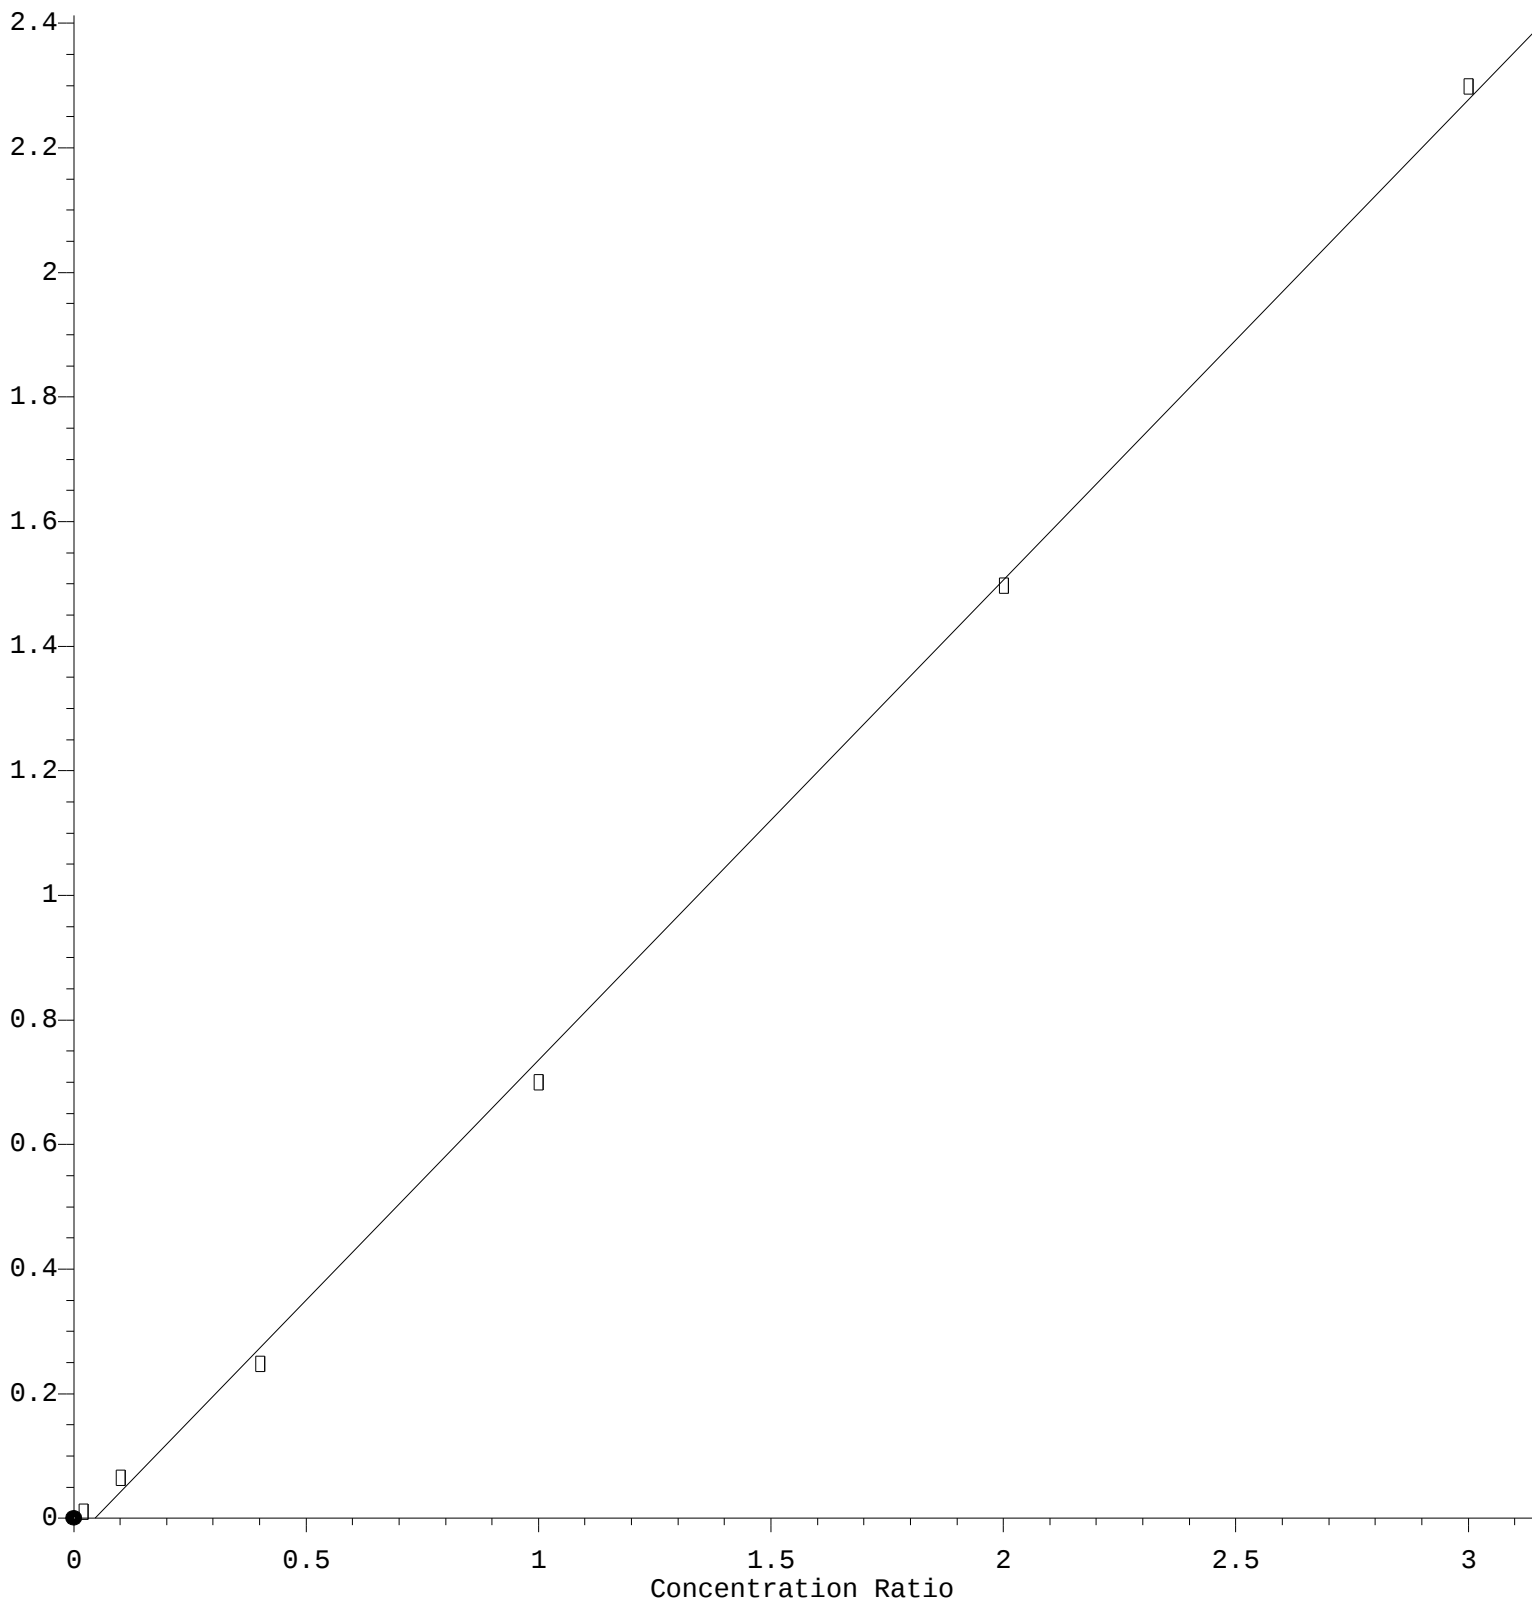

$$\text{Response} = 7.705\text{e-}001 * \text{Amt} - 3.457\text{e-}002$$


Coef of Det (r^2) = 0.999083 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Ethyl methacrylate

Response Ratio

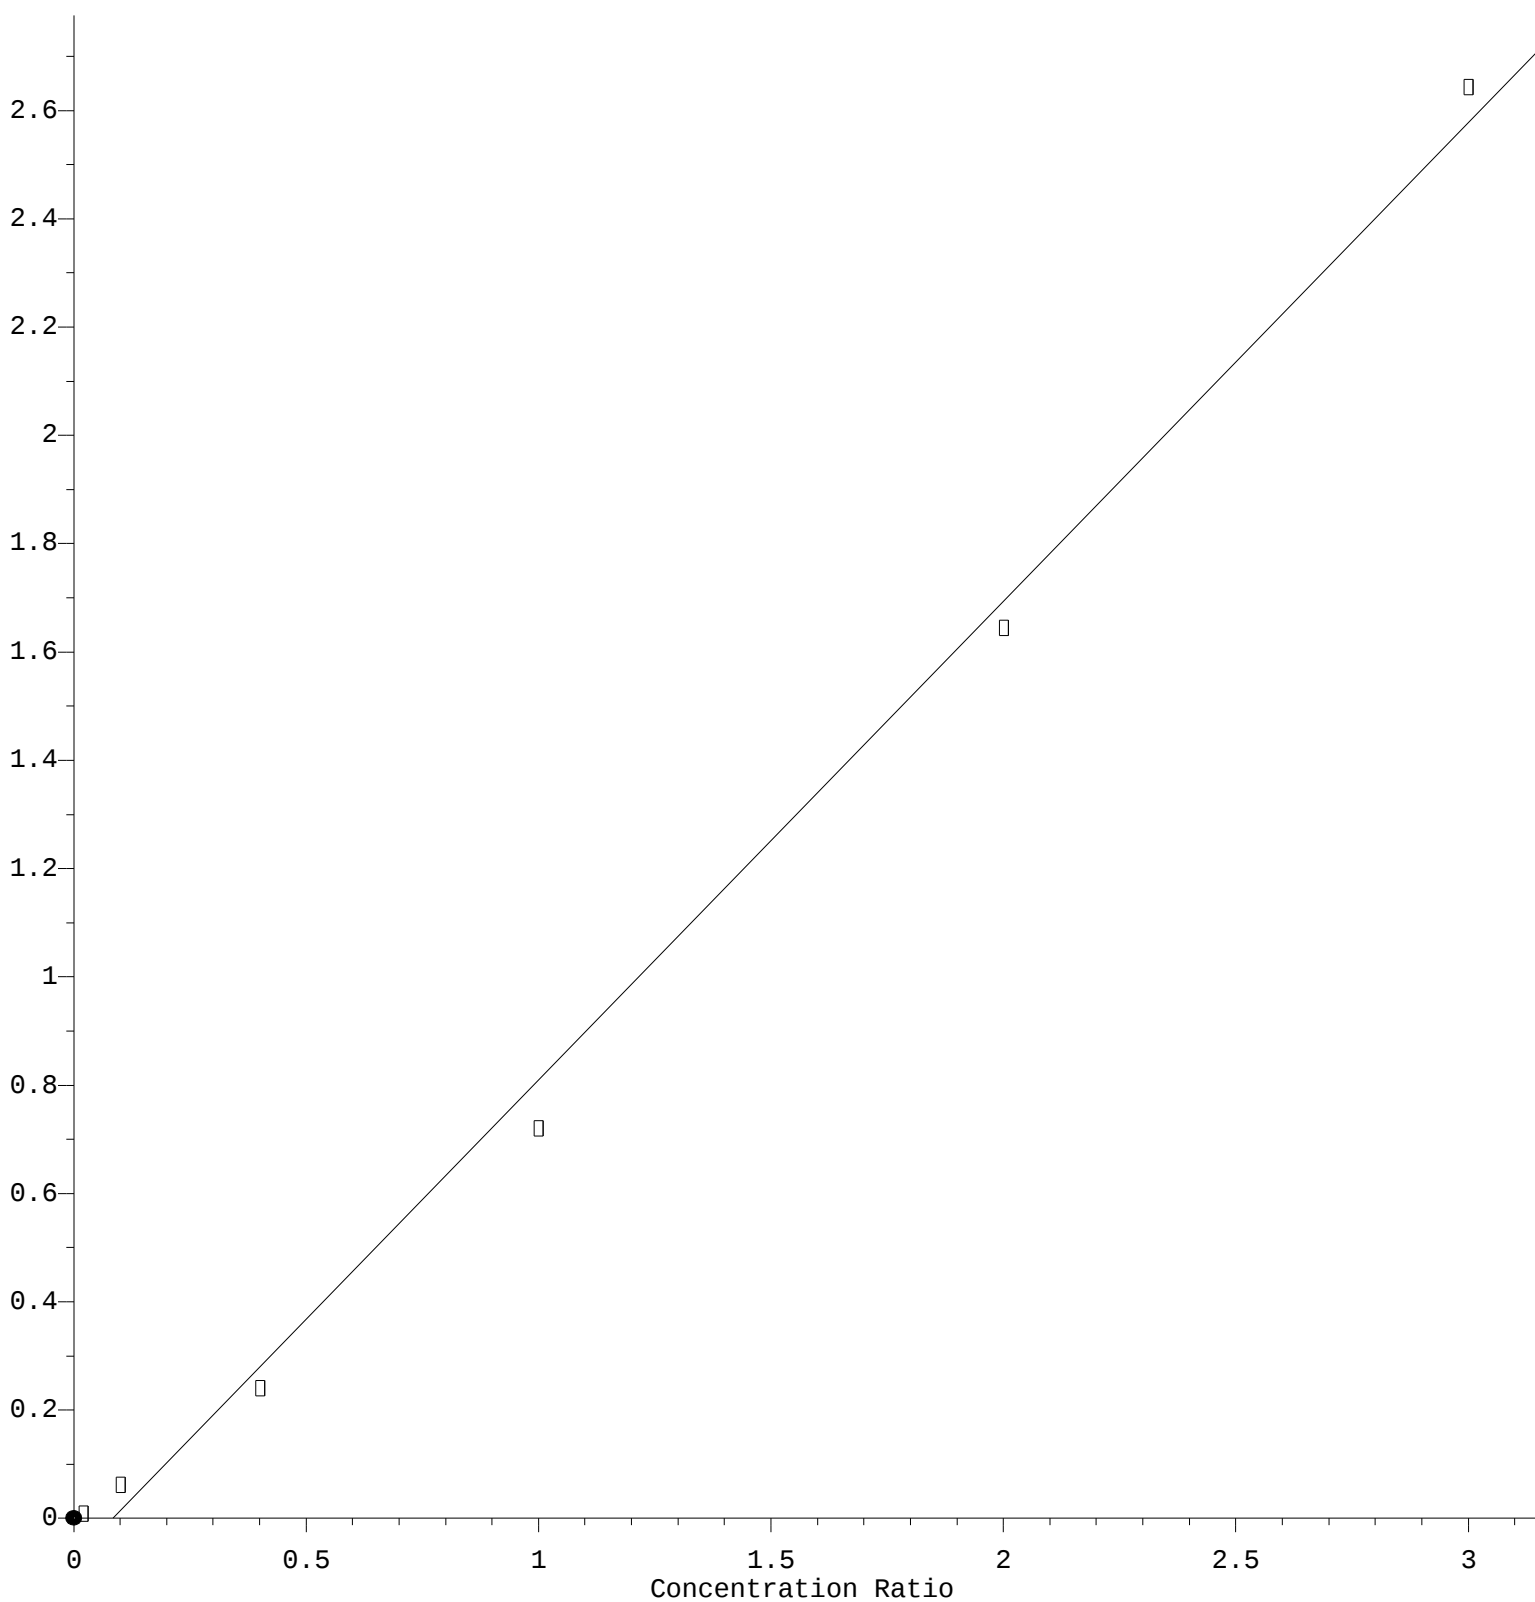

$$\text{Response} = 8.839\text{e-}001 * \text{Amt} - 7.463\text{e-}002$$


Coef of Det (r^2) = 0.995893 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

2-Chloroethyl Vinyl ether


Response Ratio

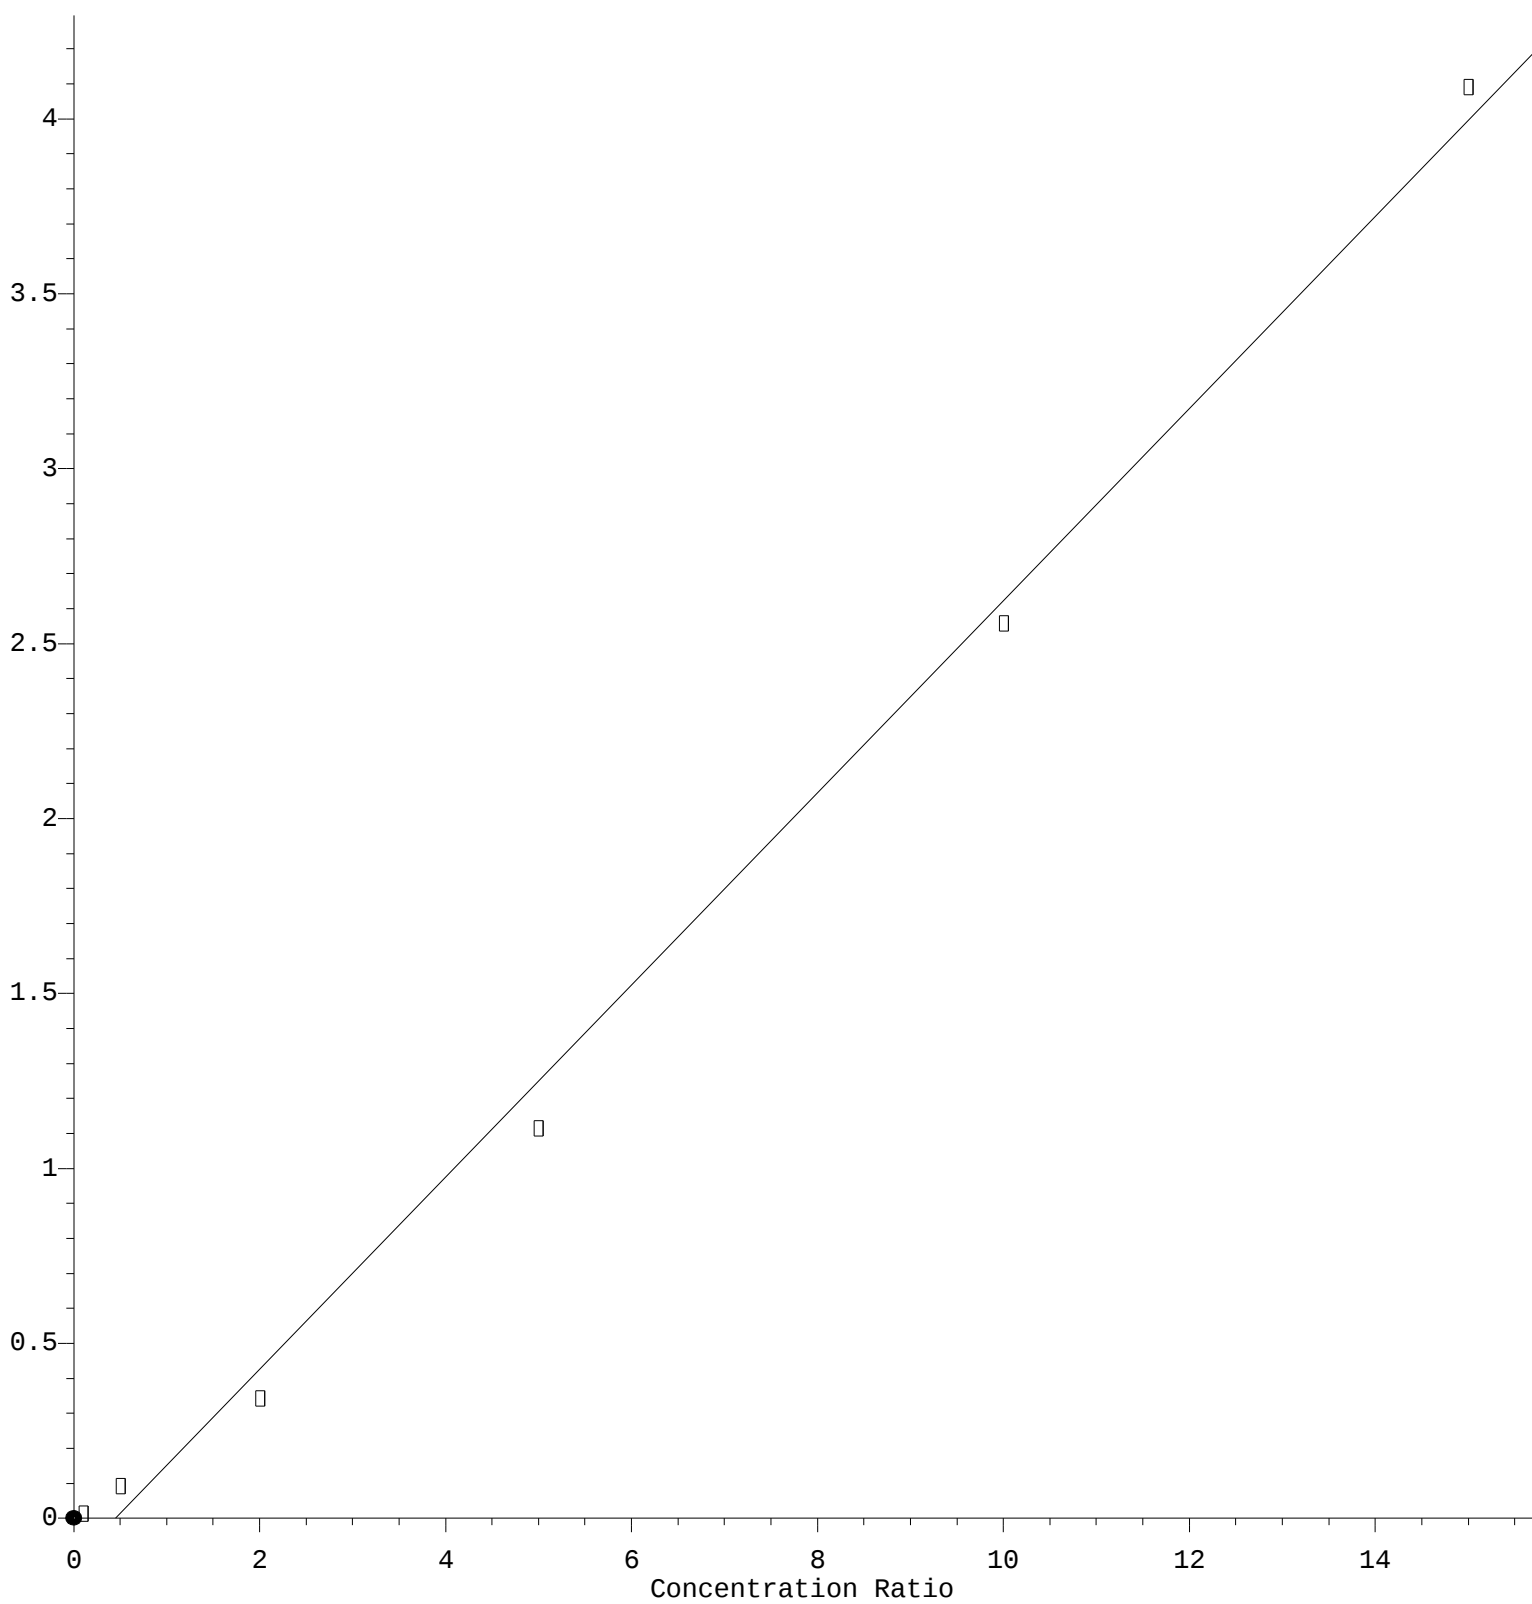

Response = $2.746 \times 10^{-1} \times \text{Amt} - 1.238 \times 10^{-1}$
Coef of Det (r^2) = 0.995796 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
Calibration Table Last Updated: Thu May 06 07:26:23 2021

2-Hexanone

Response Ratio

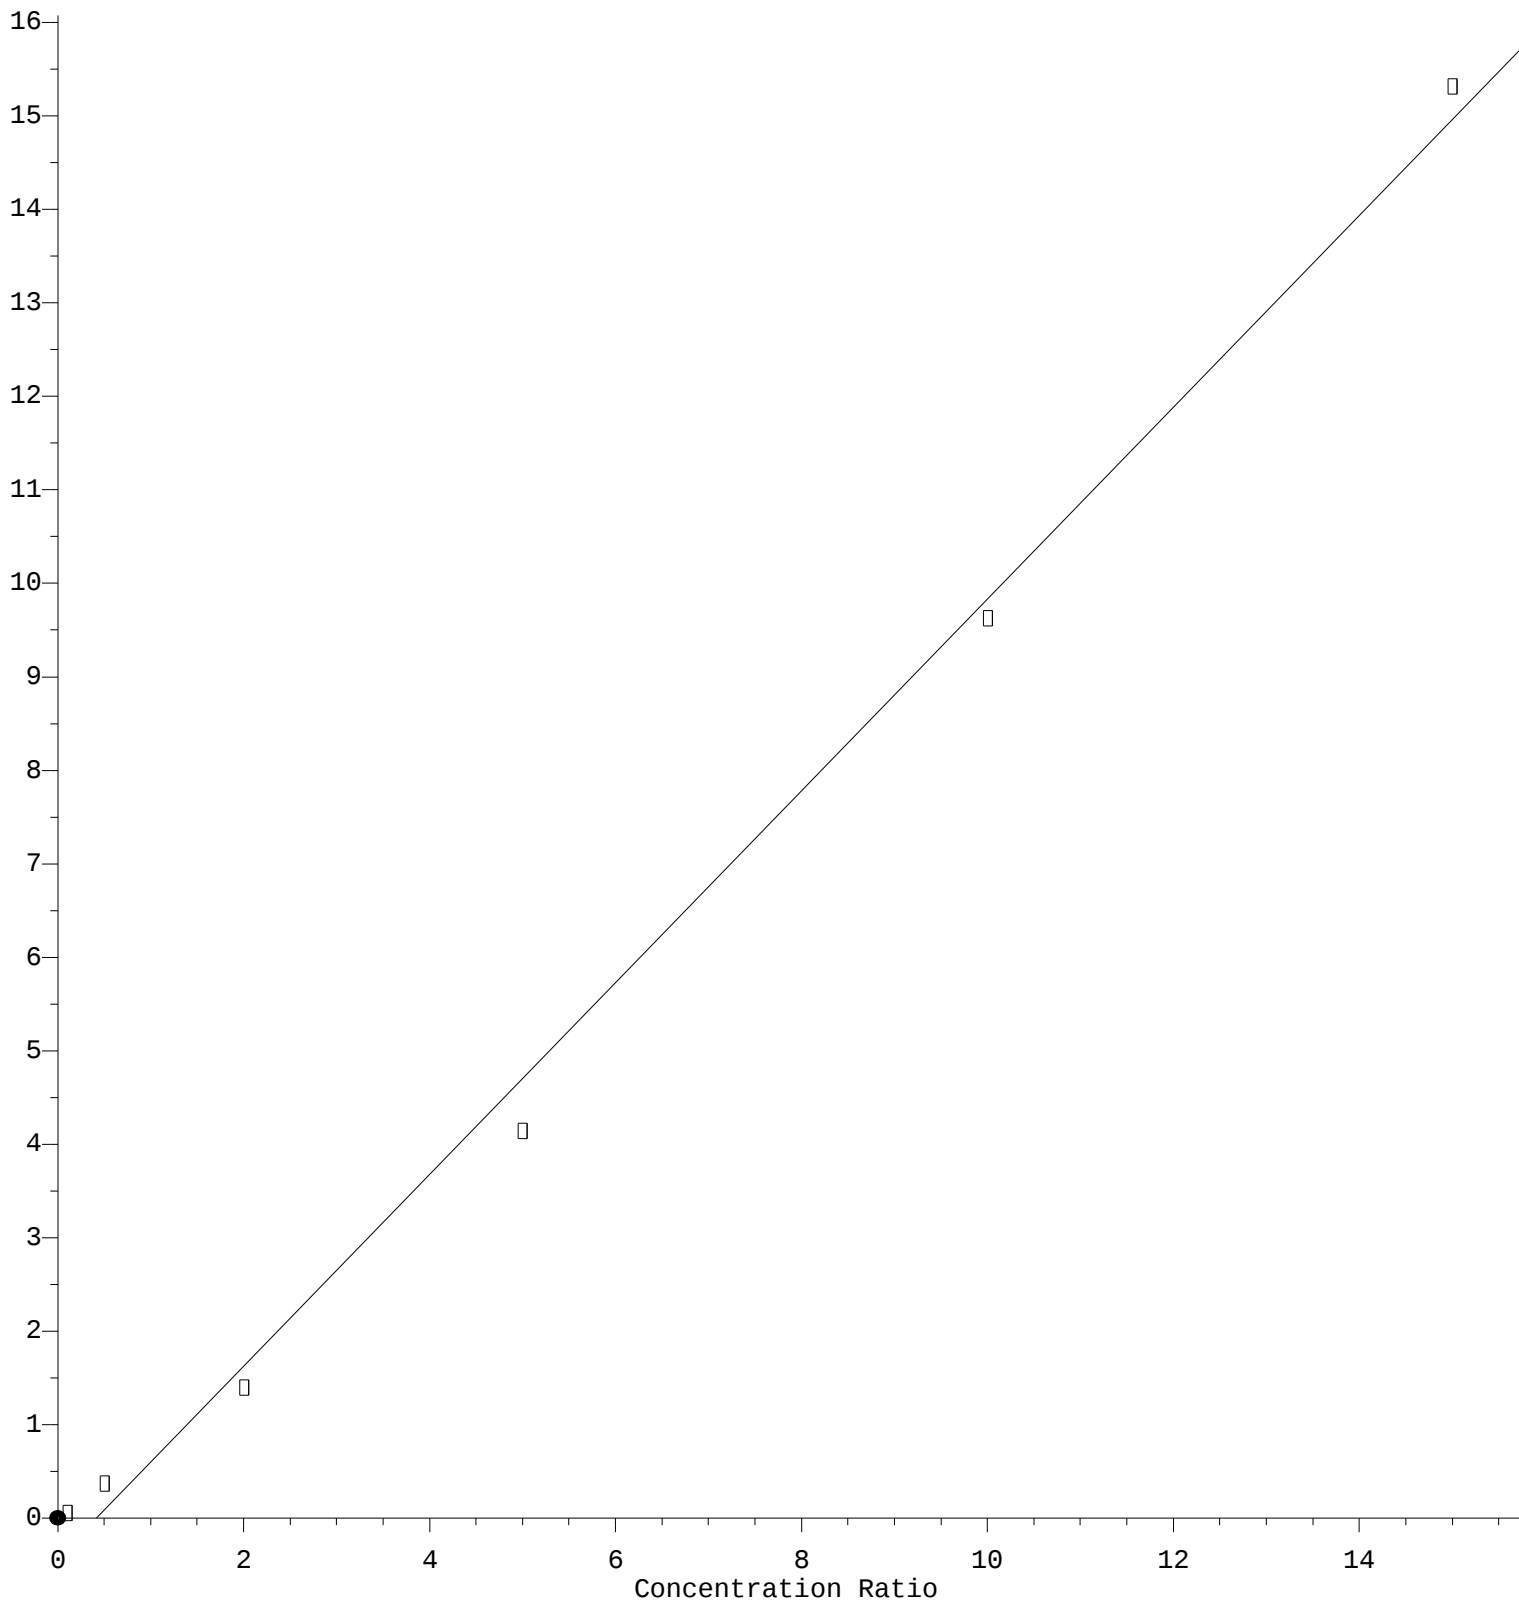

$$\text{Response} = 1.026e+000 * \text{Amt} - 4.250e-001$$


Coef of Det (r^2) = 0.995943 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Ethyl Benzene

Response Ratio

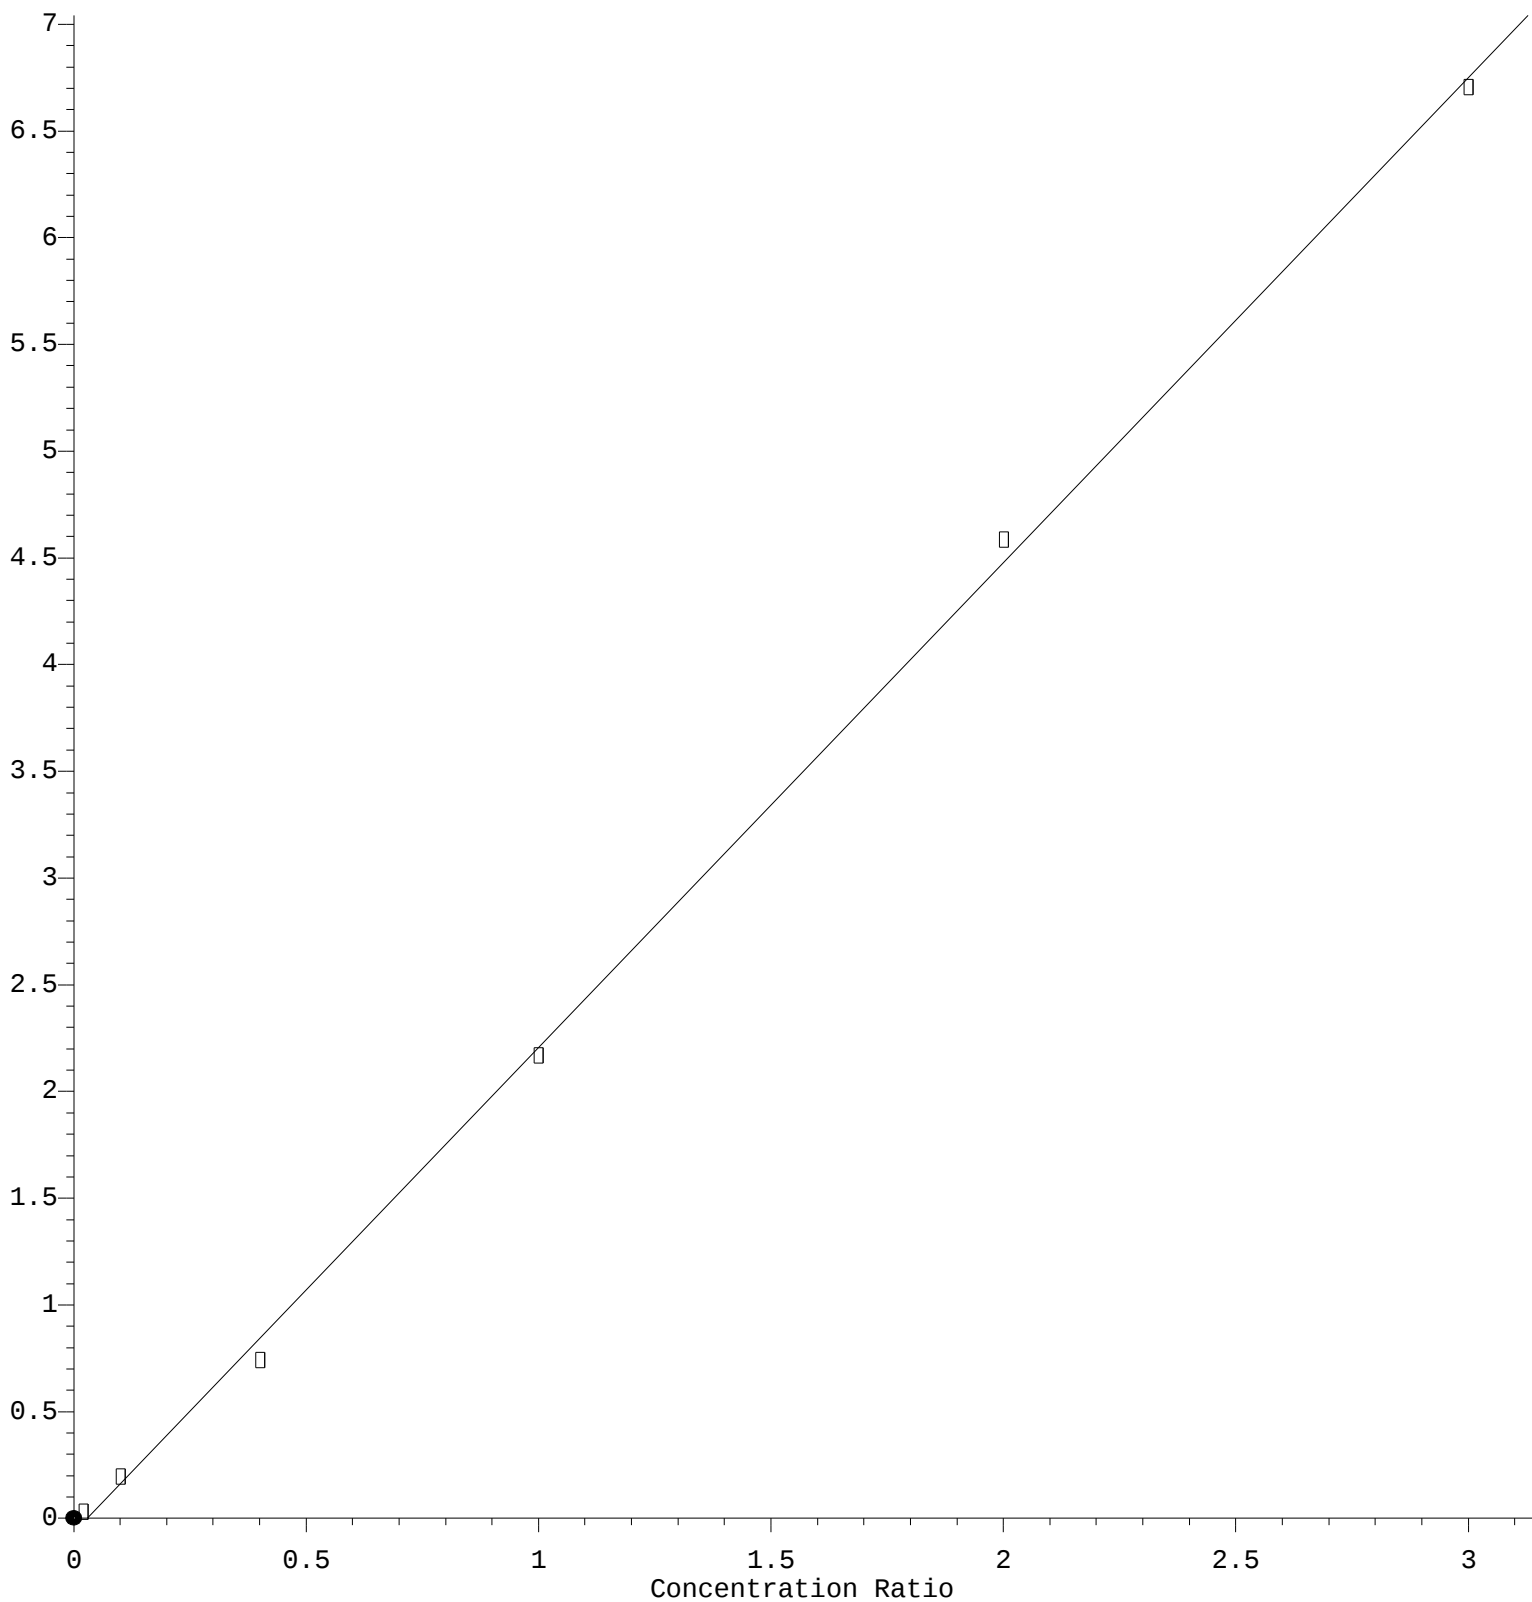

$$\text{Response} = 2.272\text{e}+000 * \text{Amt} - 6.595\text{e}-002$$


Coef of Det (r^2) = 0.999206 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

m/p-Xylenes


Response Ratio

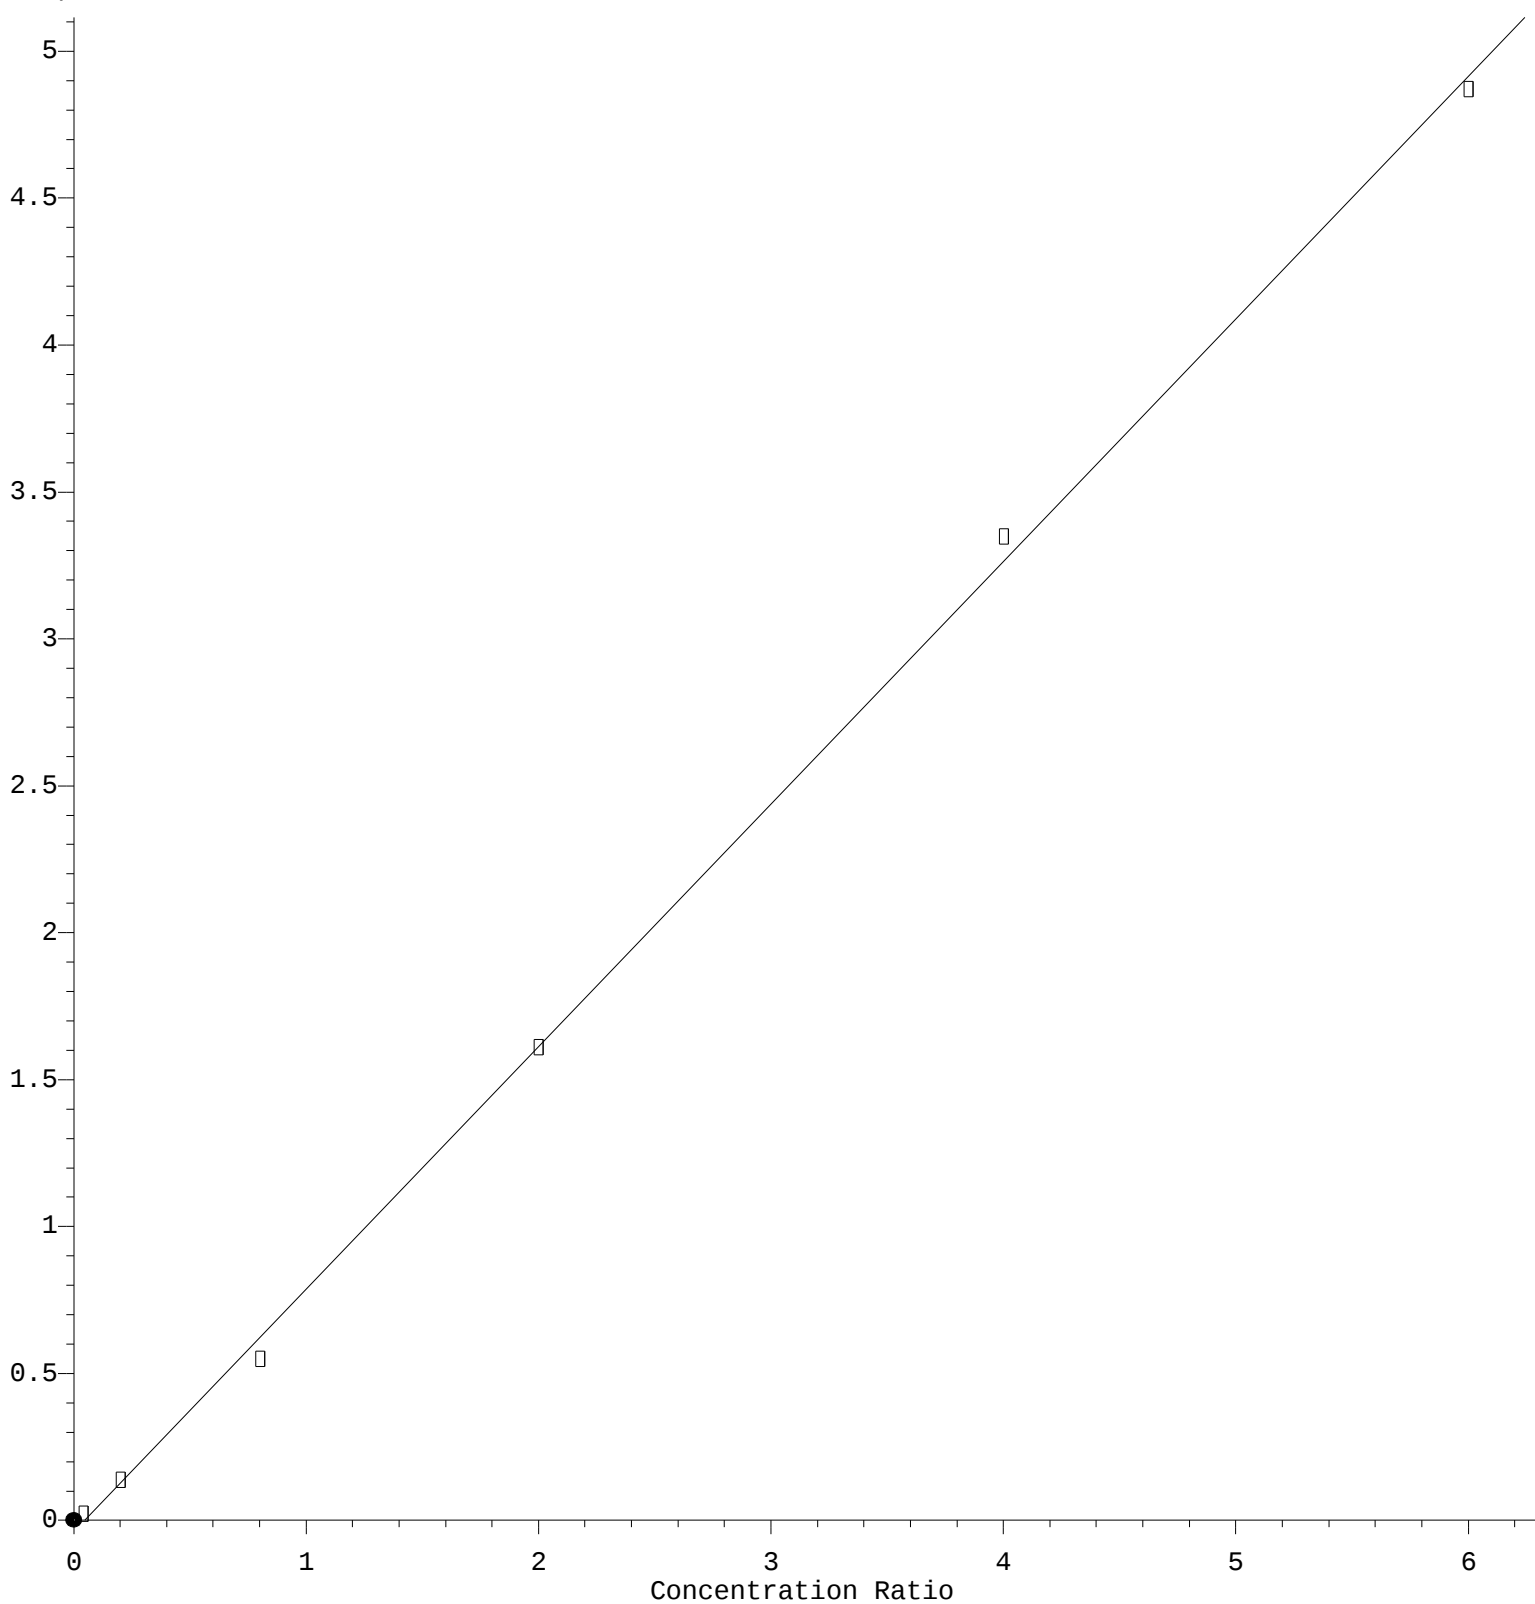

Response = $8.257 \times 10^{-1} \times \text{Amt} - 3.850 \times 10^{-2}$
 Coef of Det (r^2) = 0.999223 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
 Calibration Table Last Updated: Thu May 06 07:26:23 2021

o-Xylene

Response Ratio

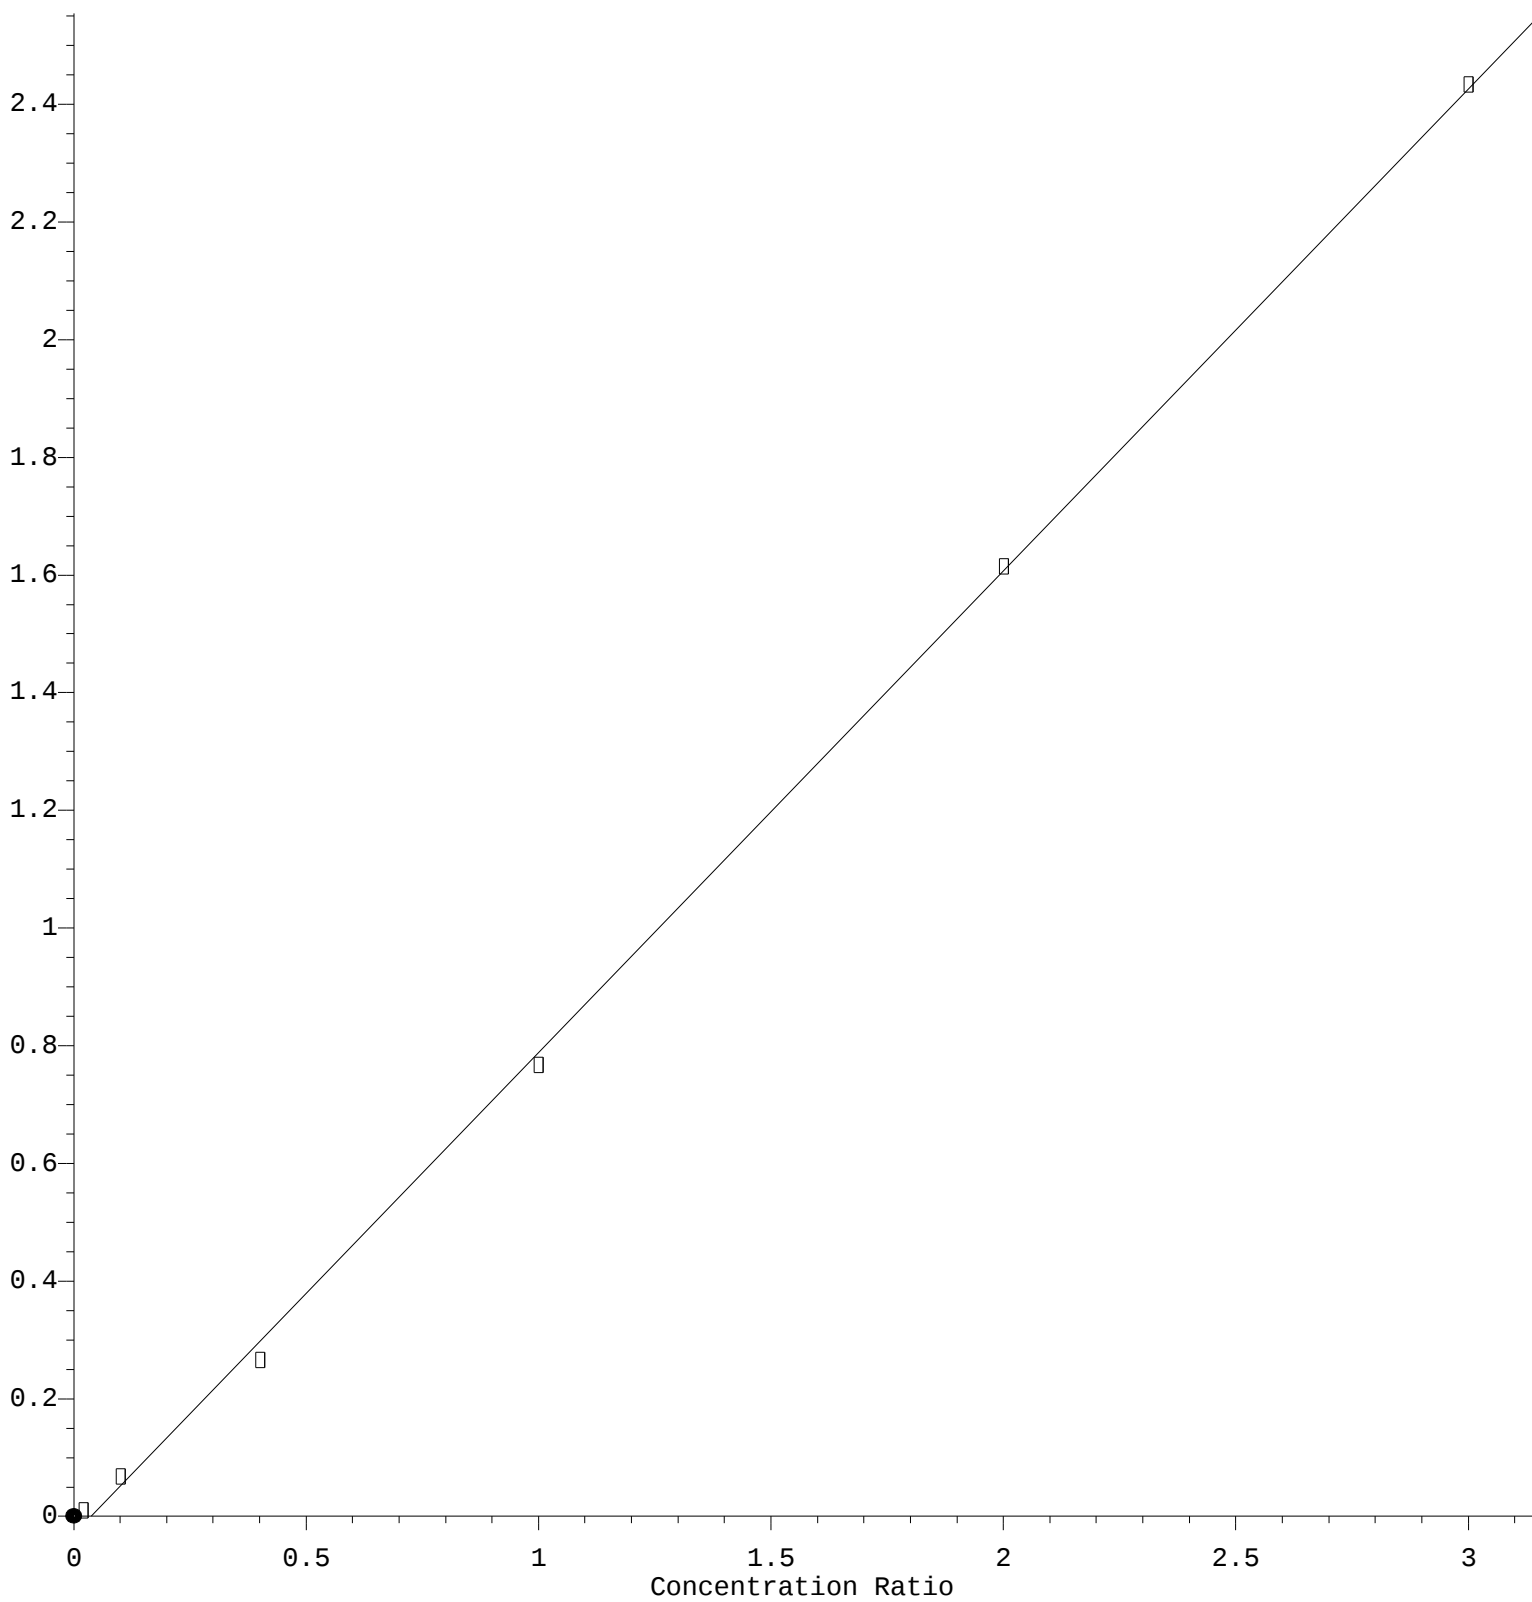

$$\text{Response} = 8.191\text{e-}001 * \text{Amt} - 3.062\text{e-}002$$


Coef of Det (r^2) = 0.999490 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Styrene

Response Ratio

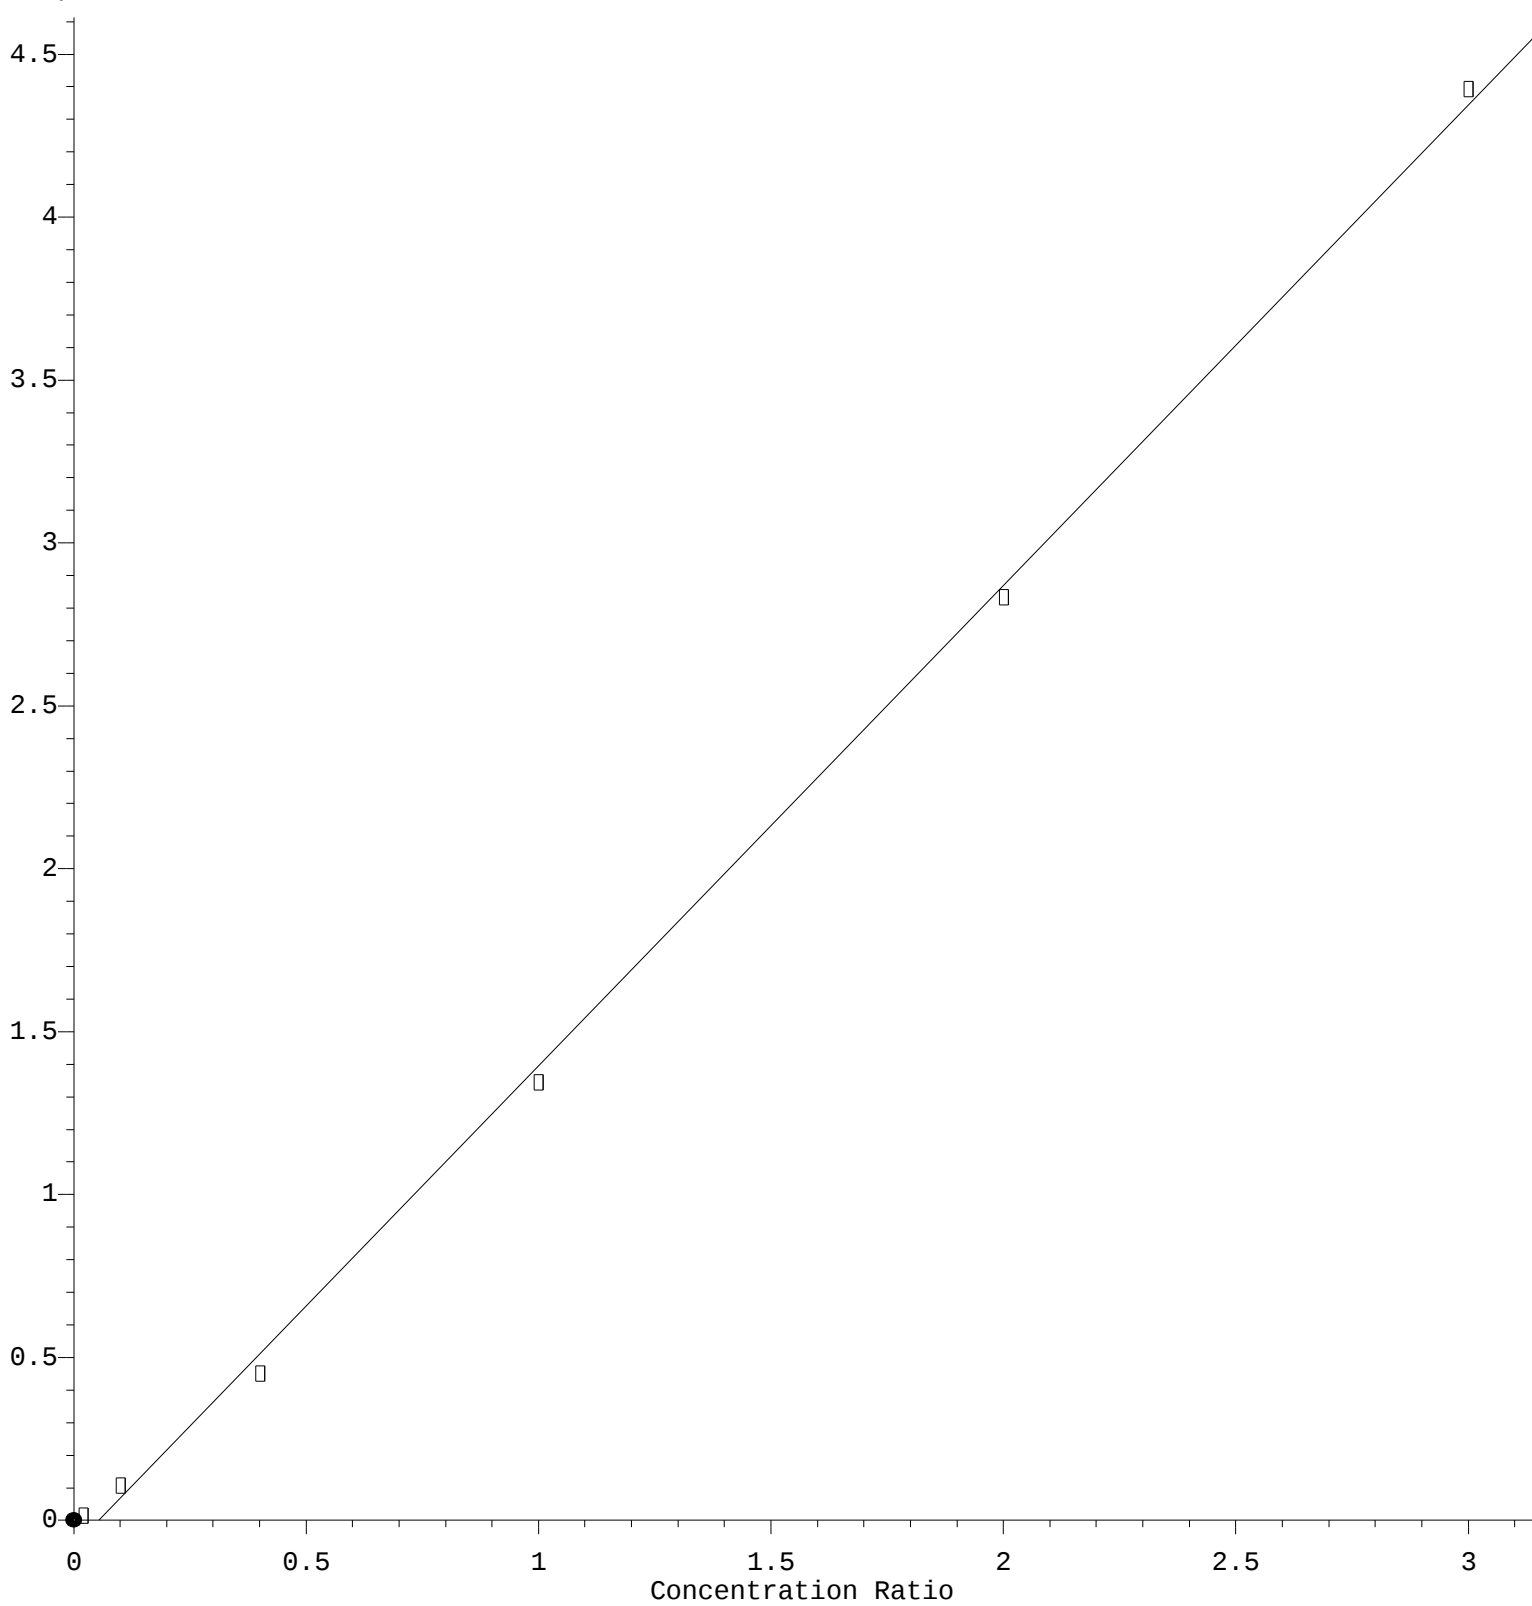

$$\text{Response} = 1.474\text{e}+000 * \text{Amt} - 7.935\text{e}-002$$


Coef of Det (r^2) = 0.998967 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Bromoform

Response Ratio

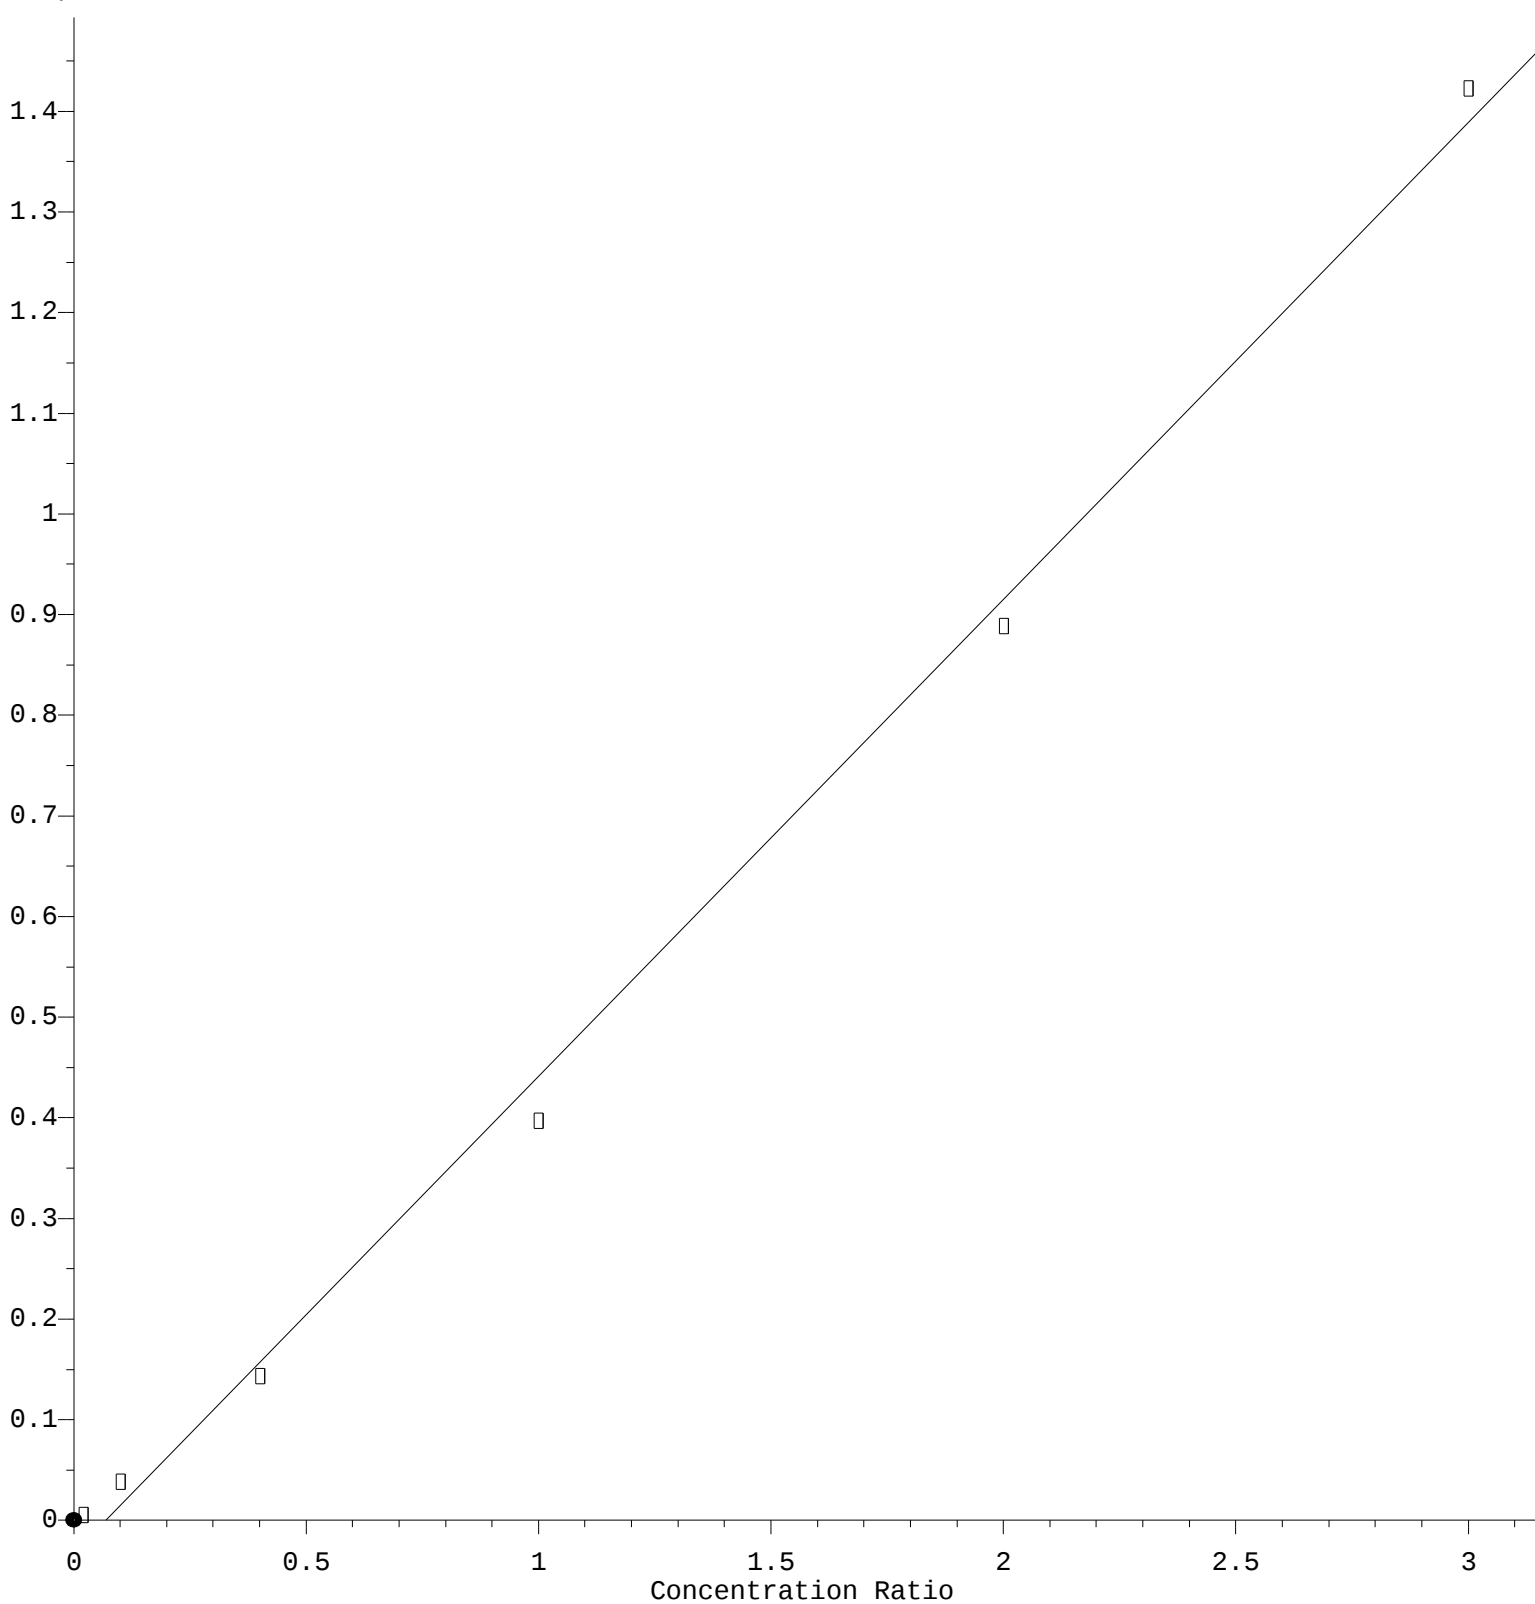

$$\text{Response} = 4.737\text{e-}001 * \text{Amt} - 3.252\text{e-}002$$


Coef of Det (r^2) = 0.996648 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

N-amy1 acetate

Response Ratio

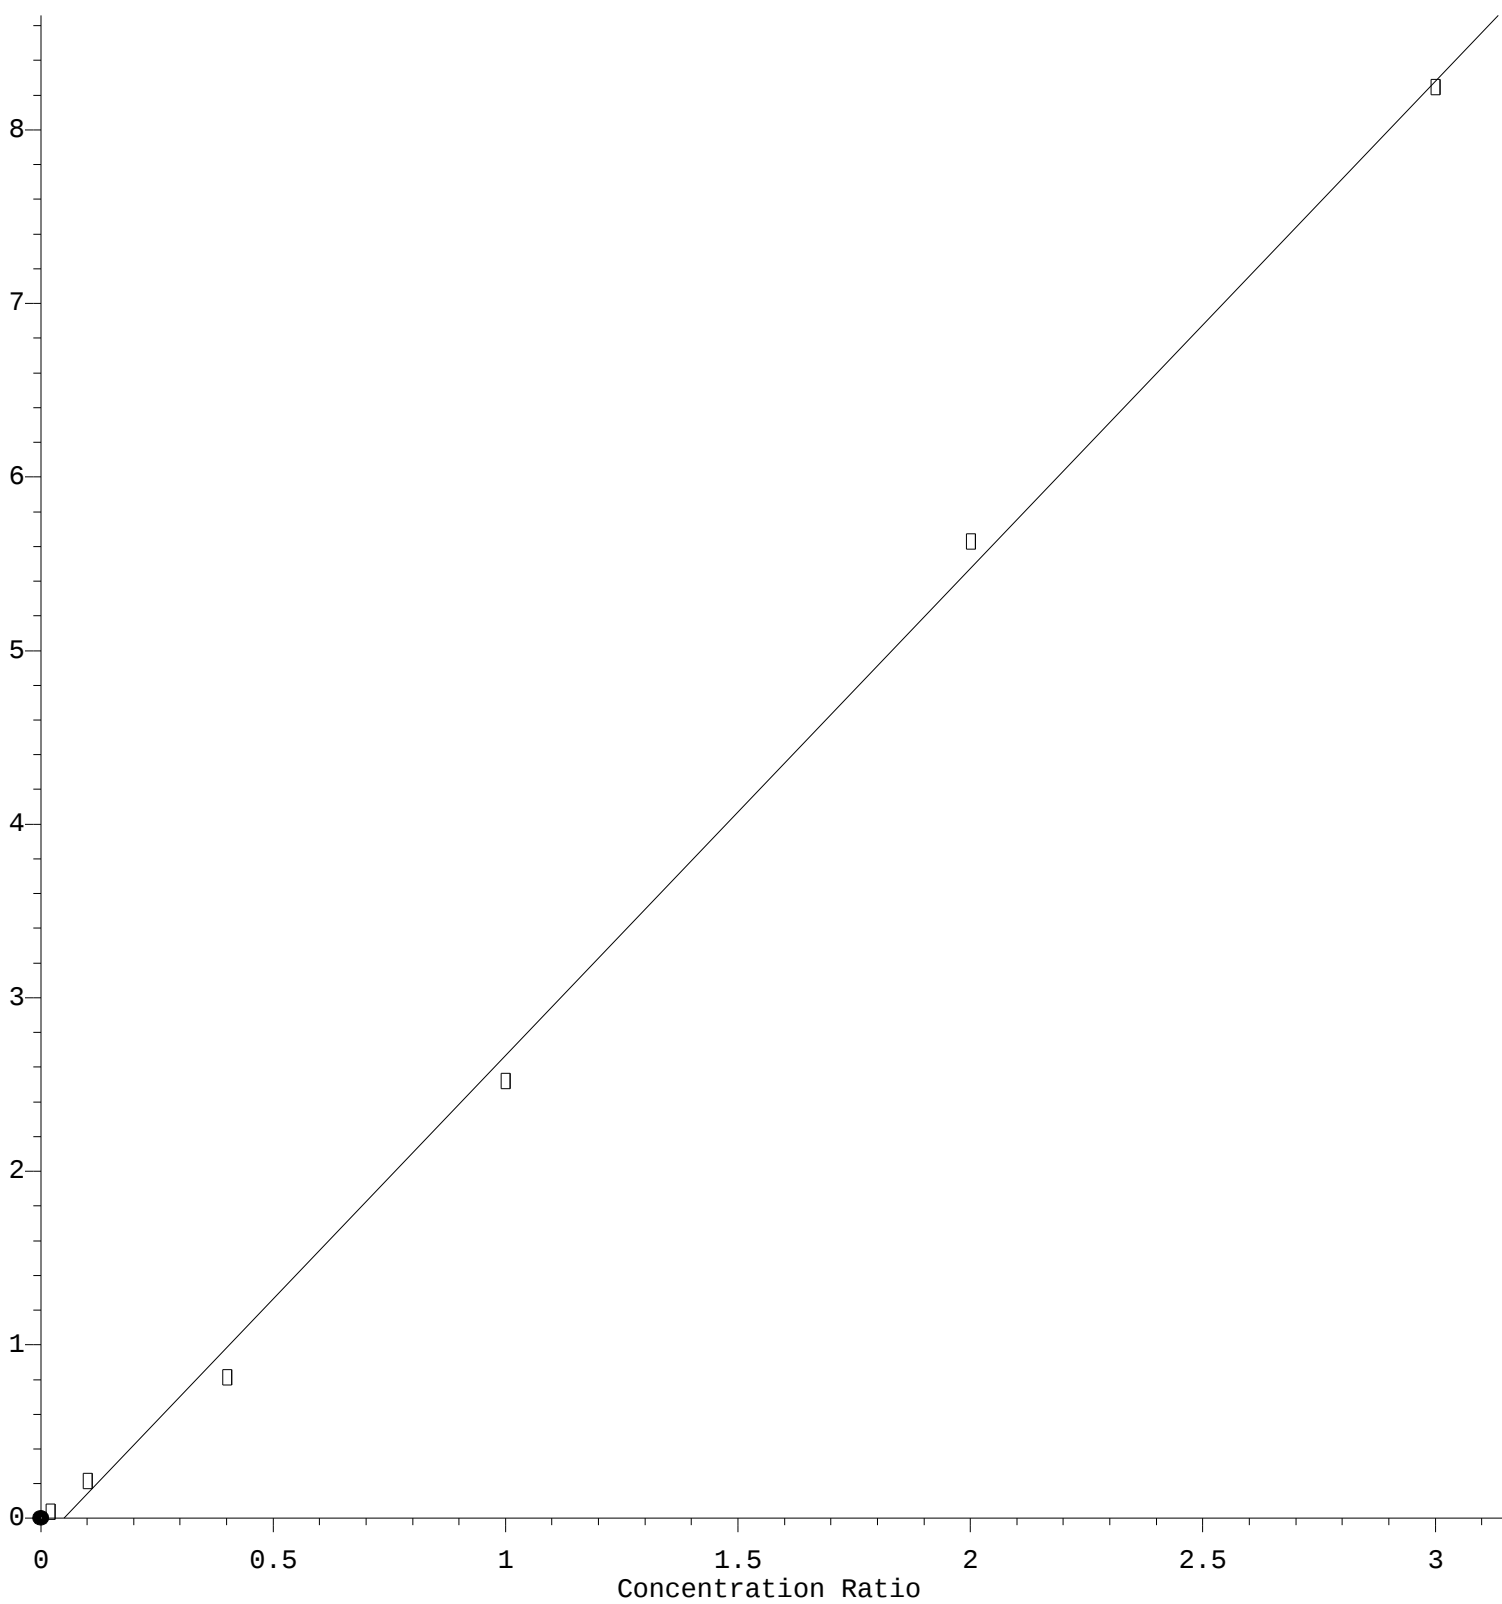

$$\text{Response} = 2.807\text{e}+000 * \text{Amt} - 1.414\text{e}-001$$


Coef of Det (r^2) = 0.998285 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

1,3,5-Trimethylbenzene

Response Ratio

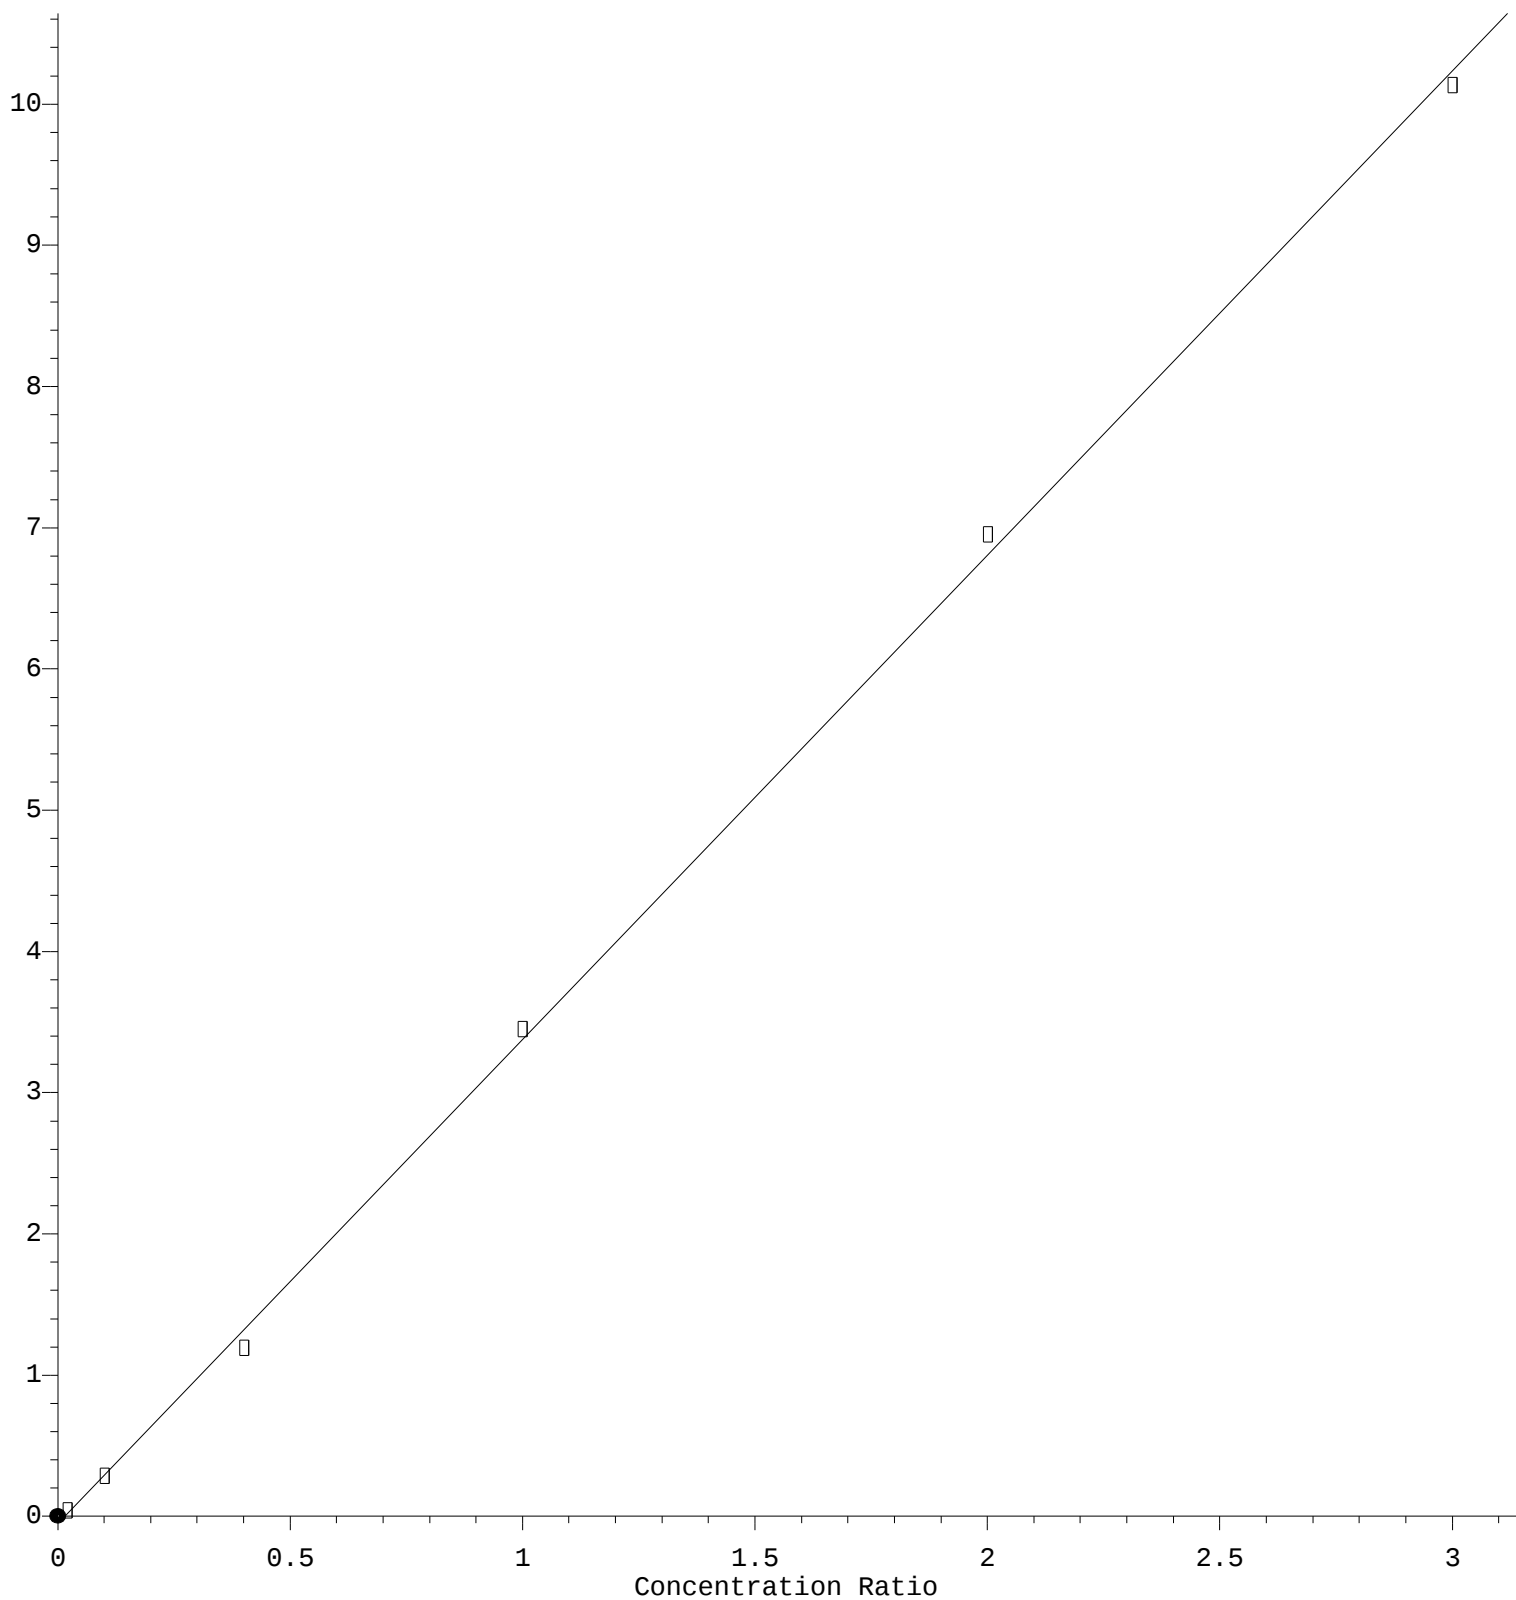

$$\text{Response} = 3.429\text{e}+000 * \text{Amt} - 5.021\text{e}-002$$


Coef of Det (r^2) = 0.999359 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

1,2,4-Trimethylbenzene

Response Ratio

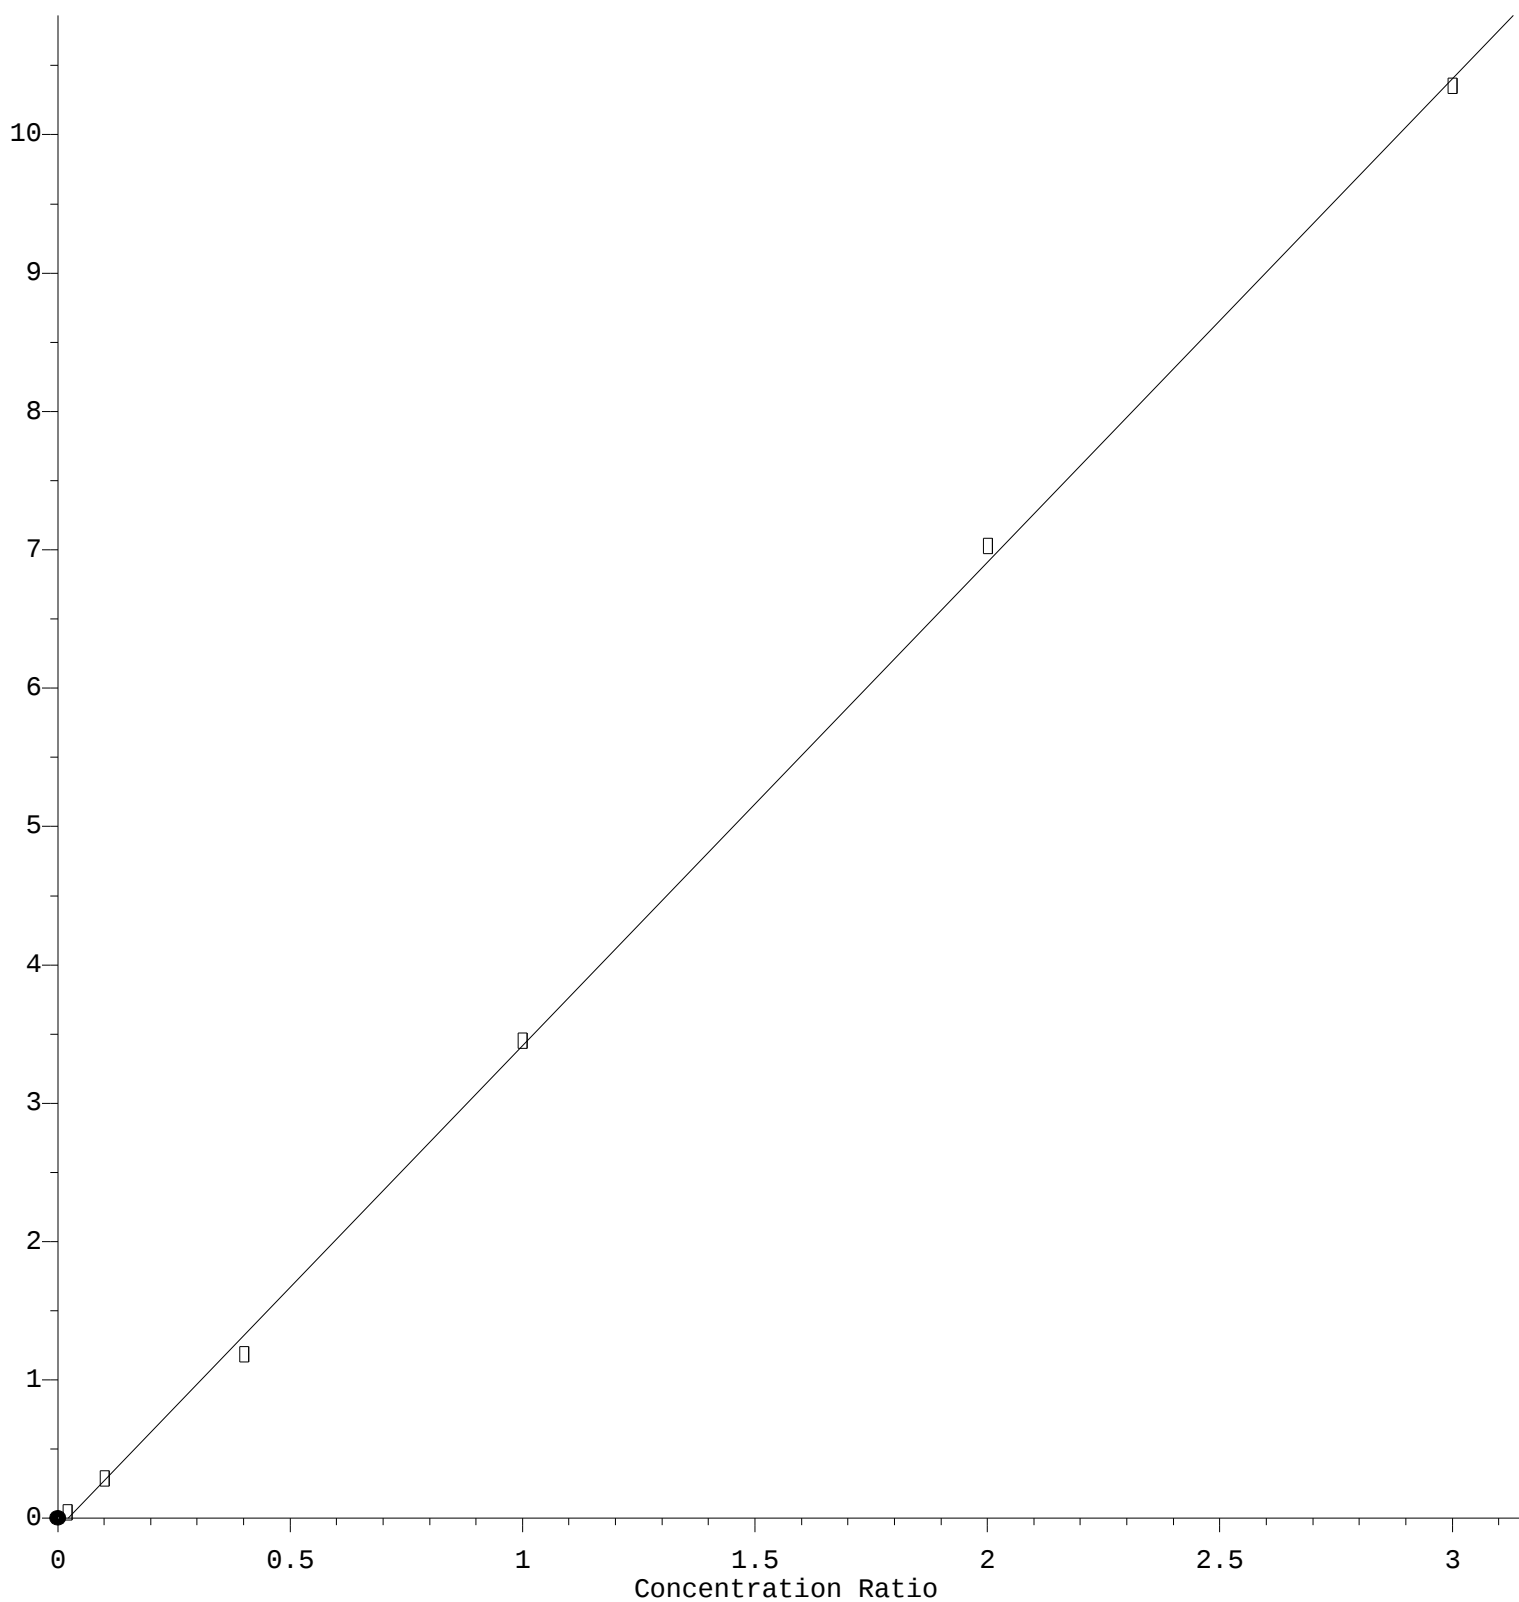

$$\text{Response} = 3.497\text{e}+000 * \text{Amt} - 7.775\text{e}-002$$


Coef of Det (r^2) = 0.999564 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

sec-Butylbenzene

Response Ratio

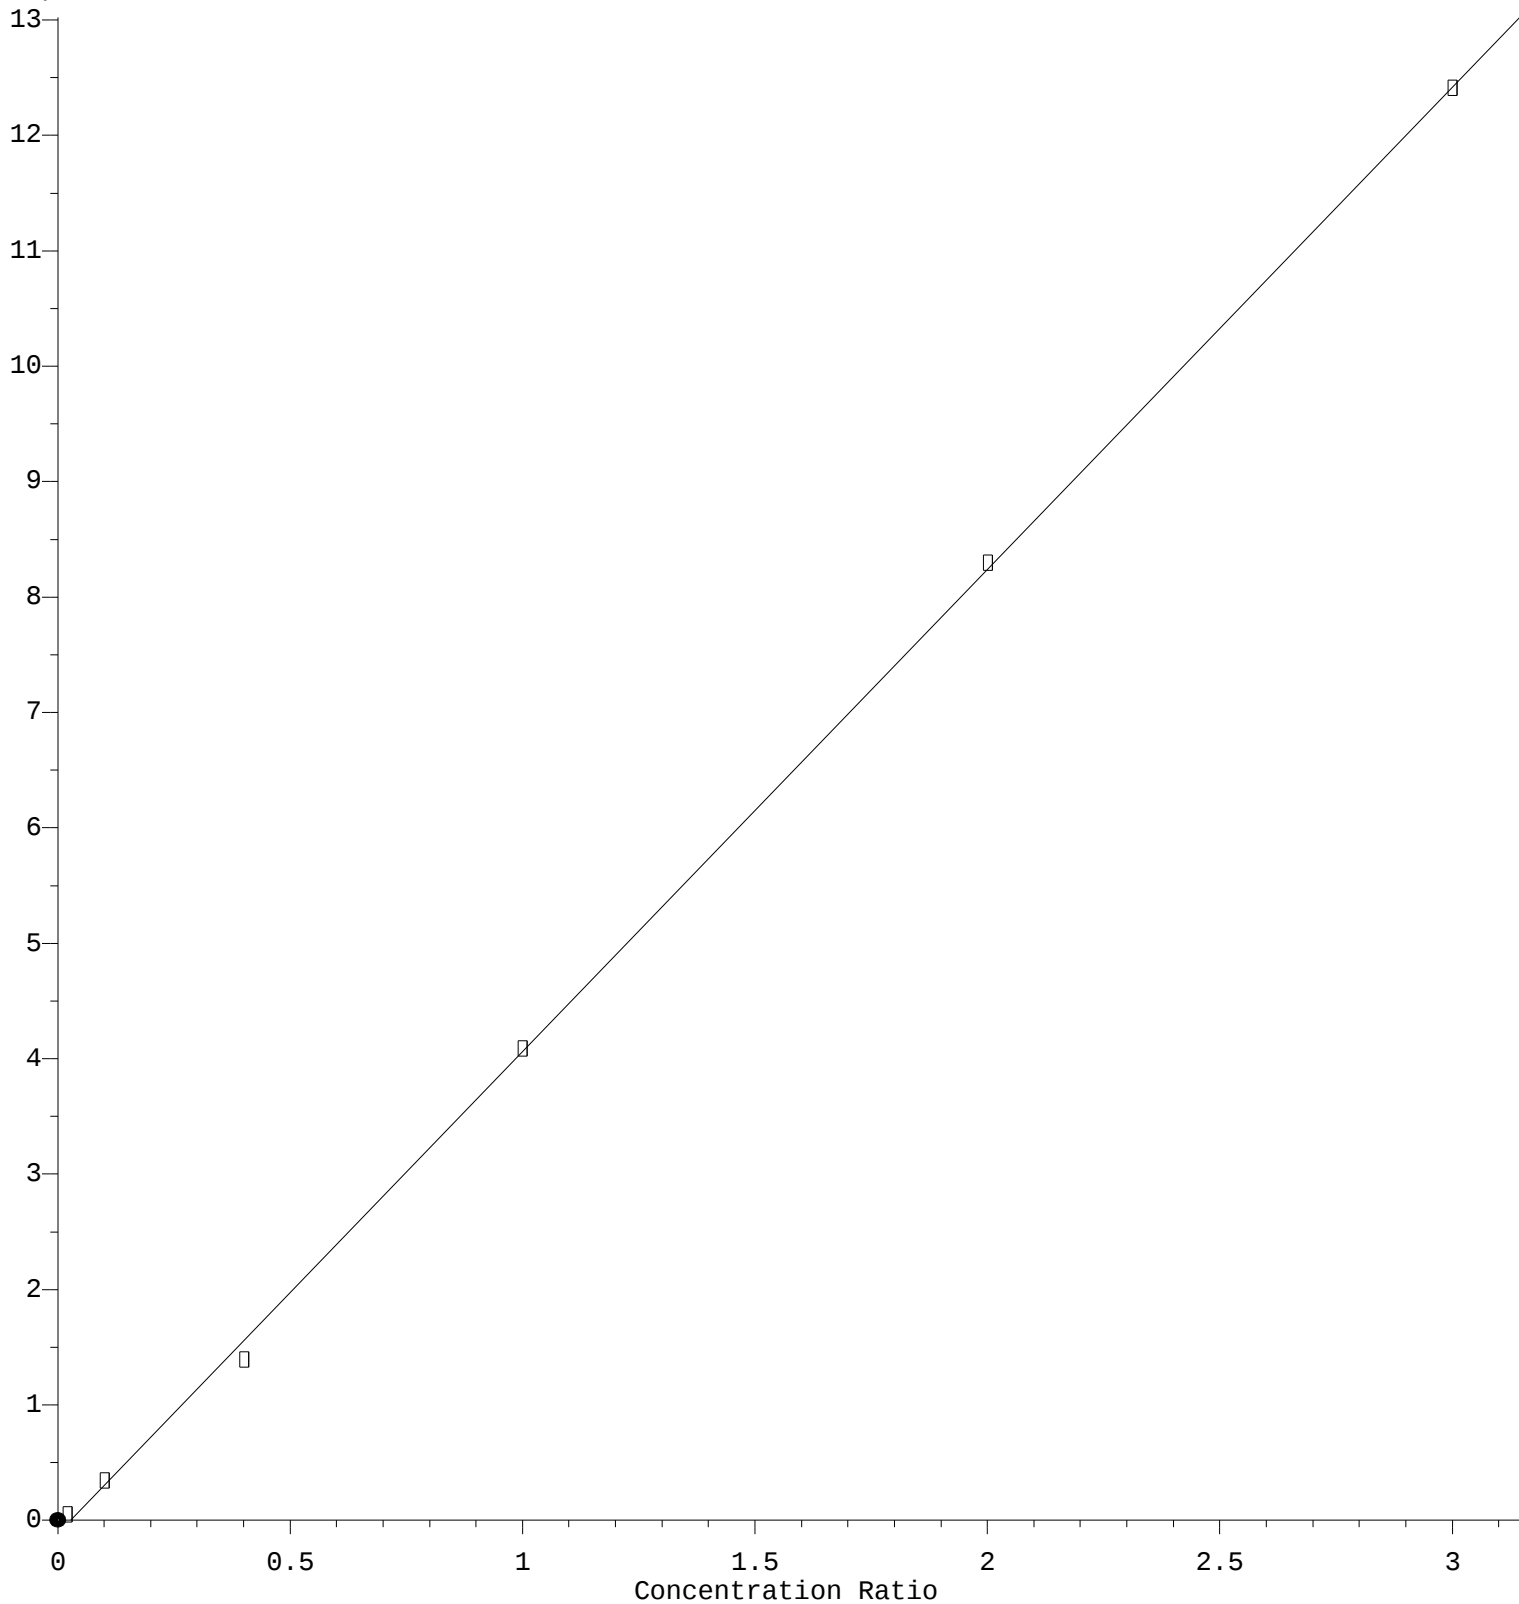

$$\text{Response} = 4.179 \times 10^0 \times \text{Amt} - 1.116 \times 10^{-1}$$


Coef of Det (r^2) = 0.999688 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

p-Isopropyltoluene

Response Ratio

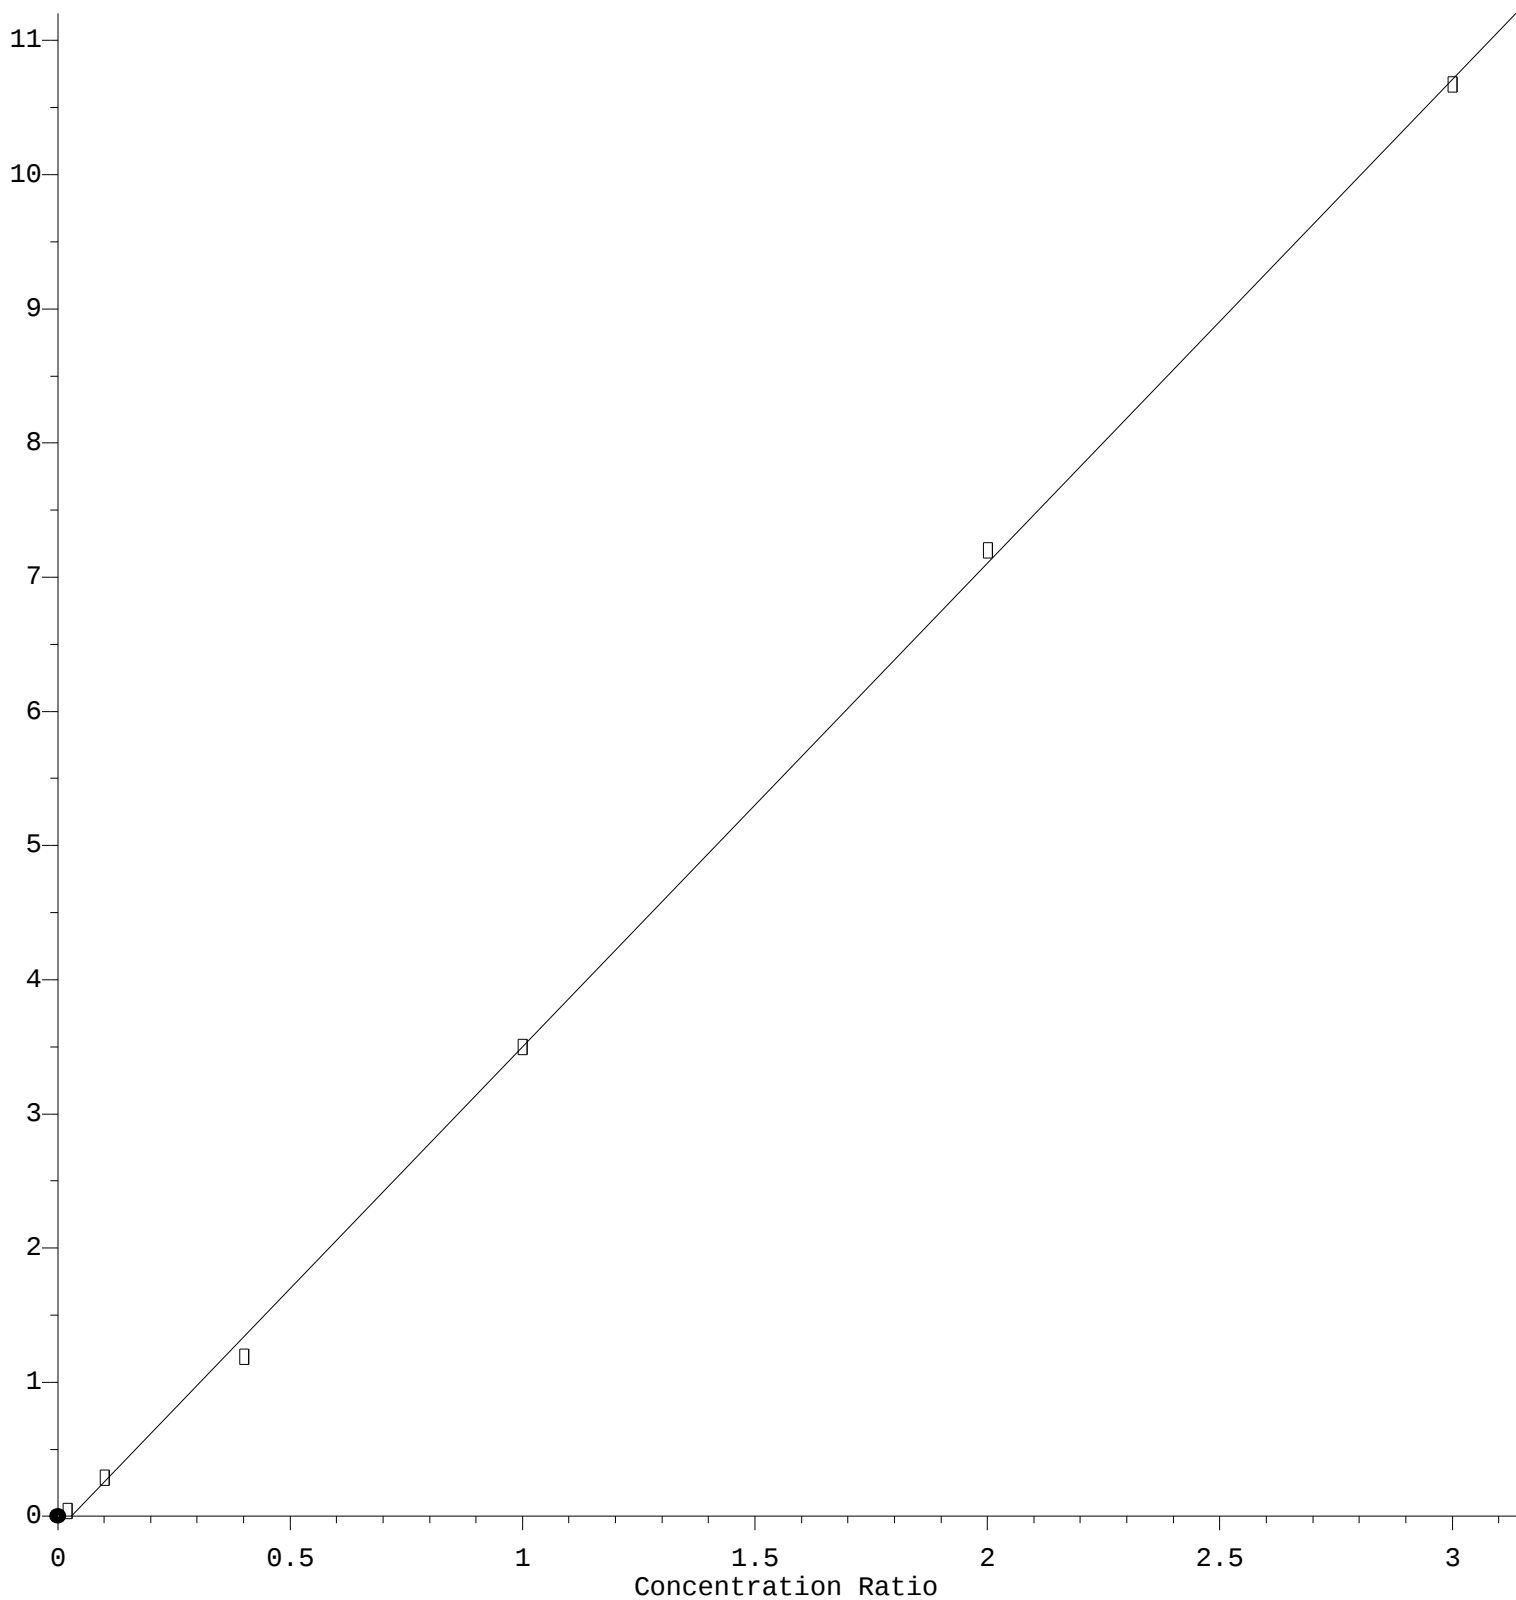

$$\text{Response} = 3.605\text{e}+000 * \text{Amt} - 1.061\text{e}-001$$


Coef of Det (r^2) = 0.999574 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

n-Butylbenzene

Response Ratio

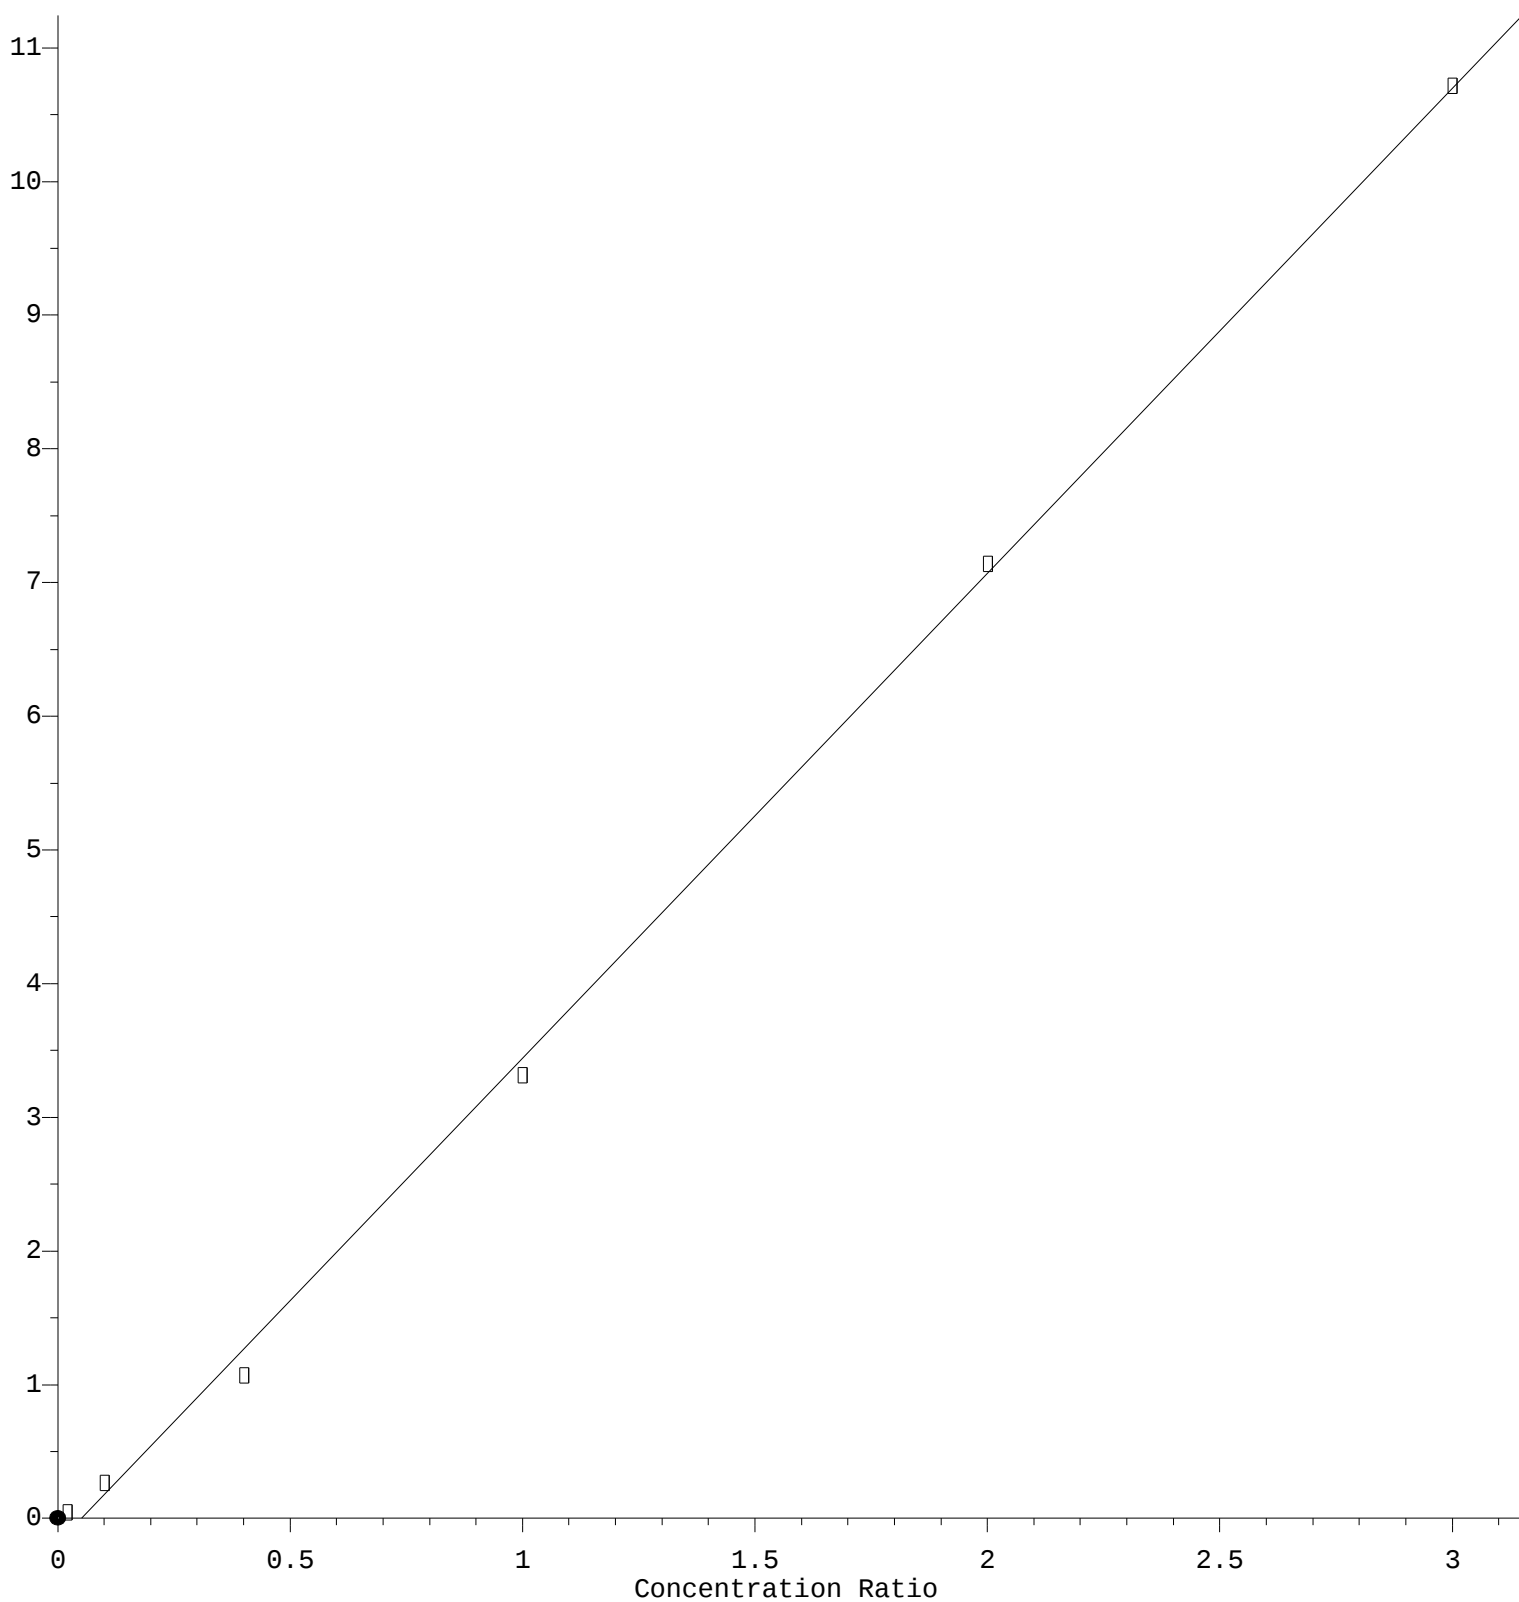

$$\text{Response} = 3.626e+000 * \text{Amt} - 1.834e-001$$


Coef of Det (r^2) = 0.999009 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021

Naphthalene

Response Ratio

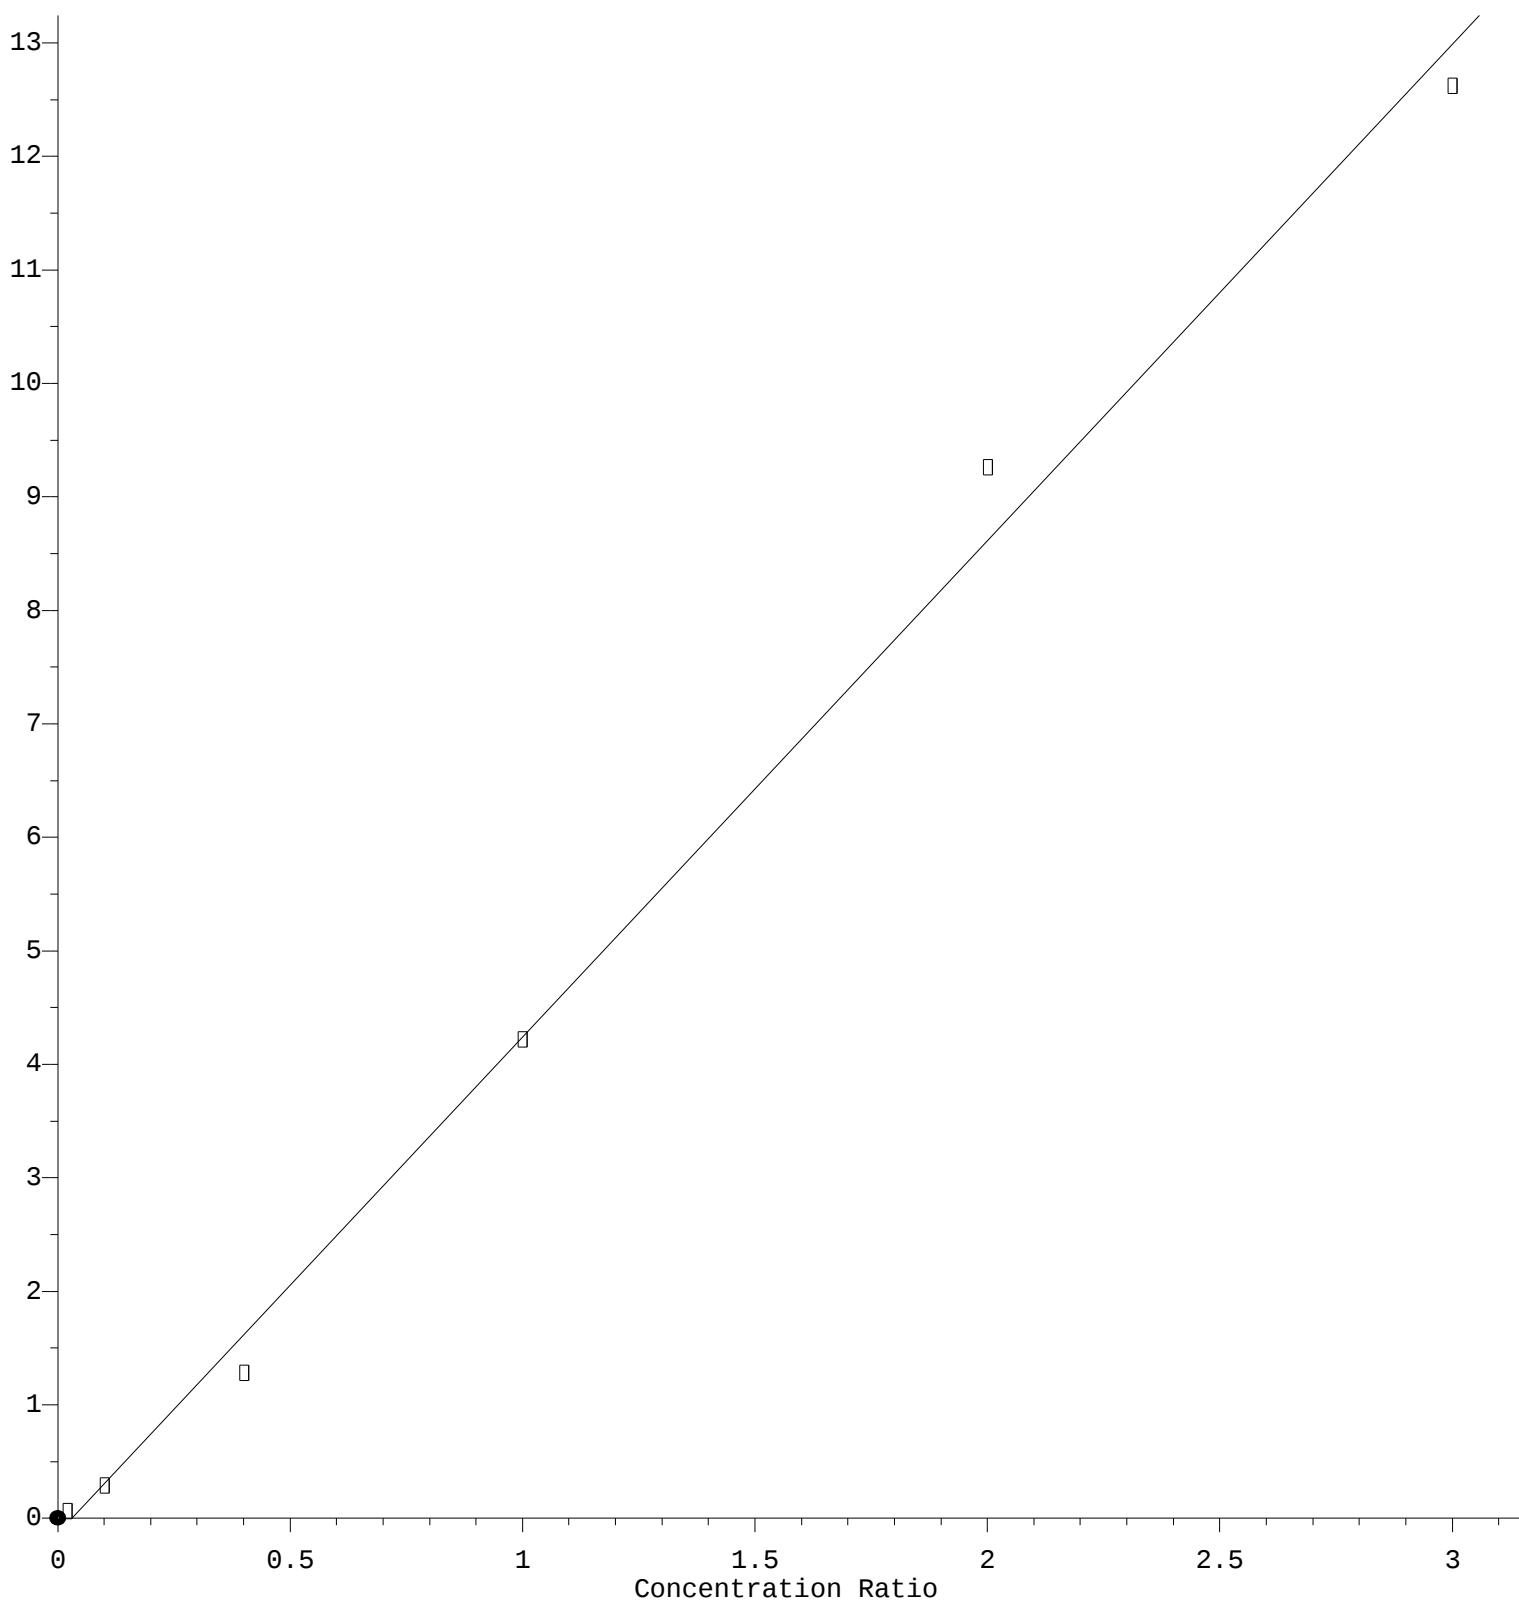

$$\text{Response} = 4.376e+000 * \text{Amt} - 1.333e-001$$

Coef of Det (r^2) = 0.995036 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M

Calibration Table Last Updated: Thu May 06 07:26:23 2021