


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050621\
Data File : VU043563.D
Acq On : 05 May 2021 21:18
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U050621W.M
Title : SW846 8260
Last Update : Thu May 06 07:26:23 2021

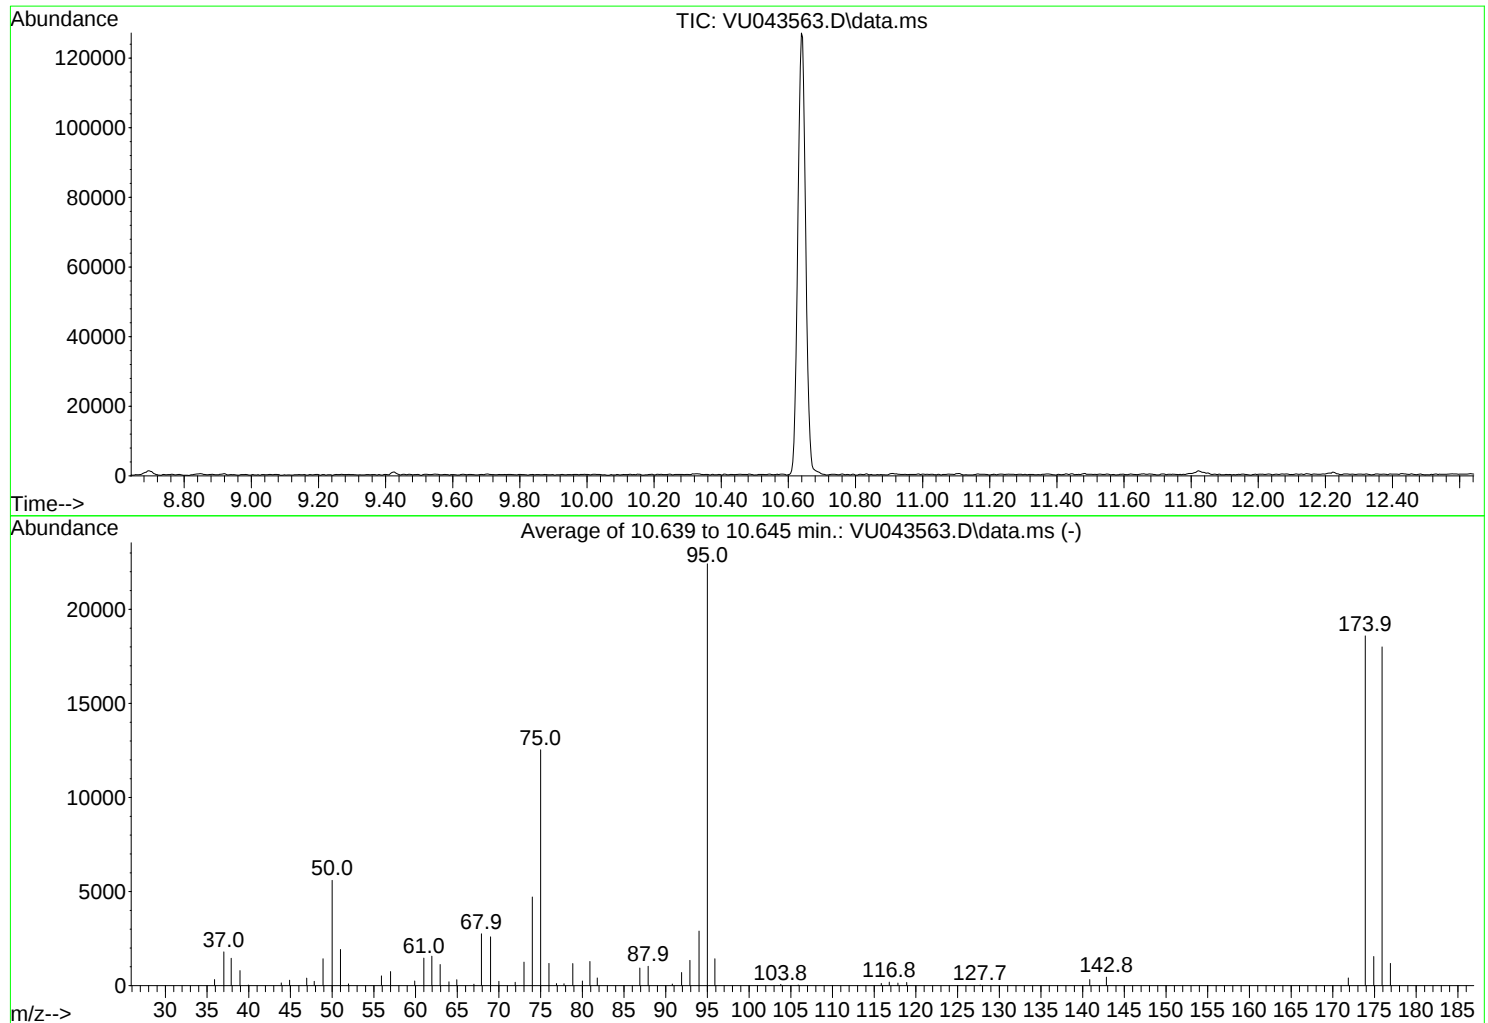

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2880

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	5598	PASS
75	95	30	60	55.9	12535	PASS
95	95	100	100	100.0	22419	PASS
96	95	5	9	6.4	1432	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	82.9	18587	PASS
175	174	5	9	8.3	1548	PASS
176	174	95	101	96.9	18003	PASS
177	176	5	9	6.6	1185	PASS