
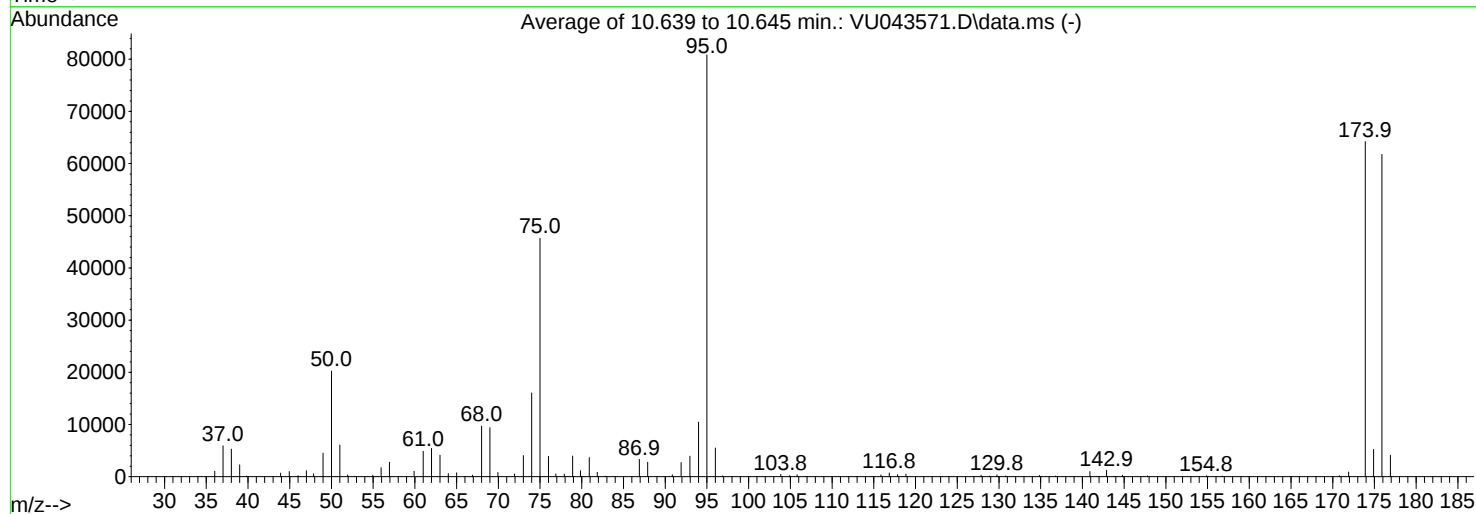


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_U\Data\VU050621\  
Data File : VU043571.D  
Acq On : 06 May 2021 09:45  
Operator : SY/MD  
Sample : BFB  
Misc : 5.0mL/MSVOA\_U/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_U  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_U\Method\82U050621W.M  
Title : SW846 8260  
Last Update : Thu May 06 07:26:23 2021

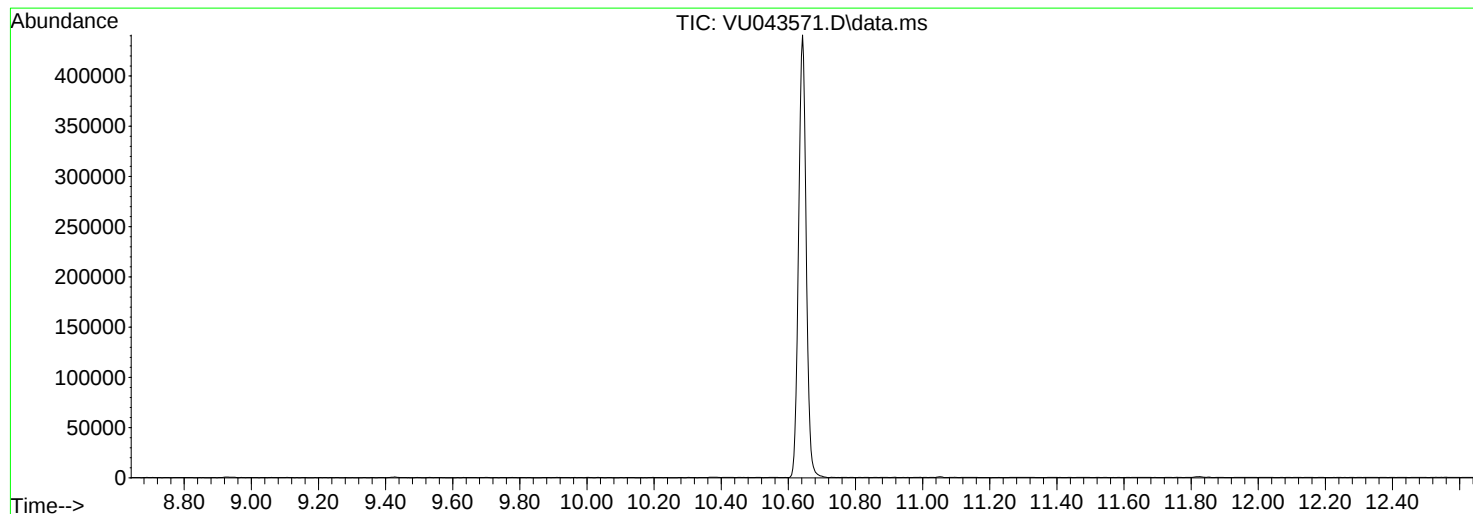

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 25.0         | 20227      | PASS                |
| 75             | 95              | 30              | 60              | 56.5         | 45685      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 80835      | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 5503       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 79.4         | 64205      | PASS                |
| 175            | 174             | 5               | 9               | 8.1          | 5224       | PASS                |
| 176            | 174             | 95              | 101             | 96.2         | 61771      | PASS                |
| 177            | 176             | 5               | 9               | 6.7          | 4122       | PASS                |