




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
Data File : VU058848.D
Acq On : 07 May 2024 17:58
Operator : MD/SY
Sample : P2392-06DL 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAQ7DL

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/08/2024
Supervised By :Semsettin Yesilyurt 05/08/2024

Quant Time: May 08 05:12:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 08 05:10:37 2024
Response via : Initial Calibration

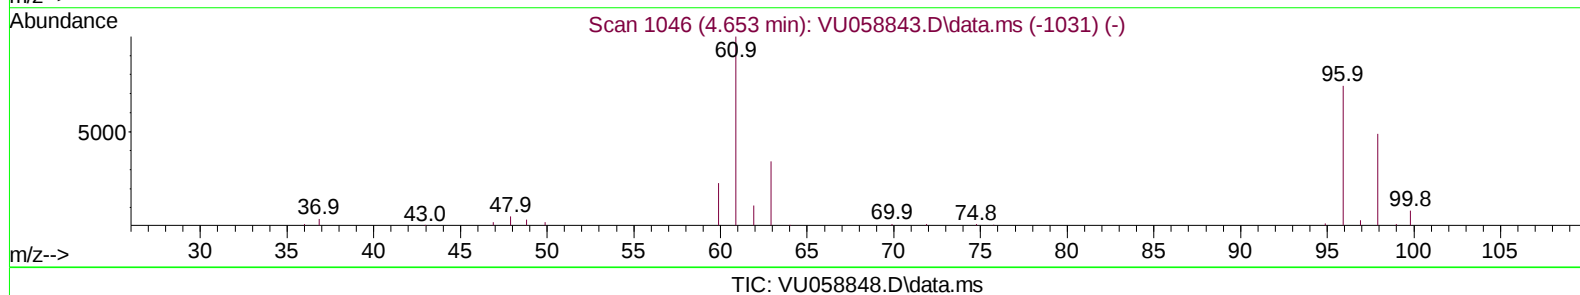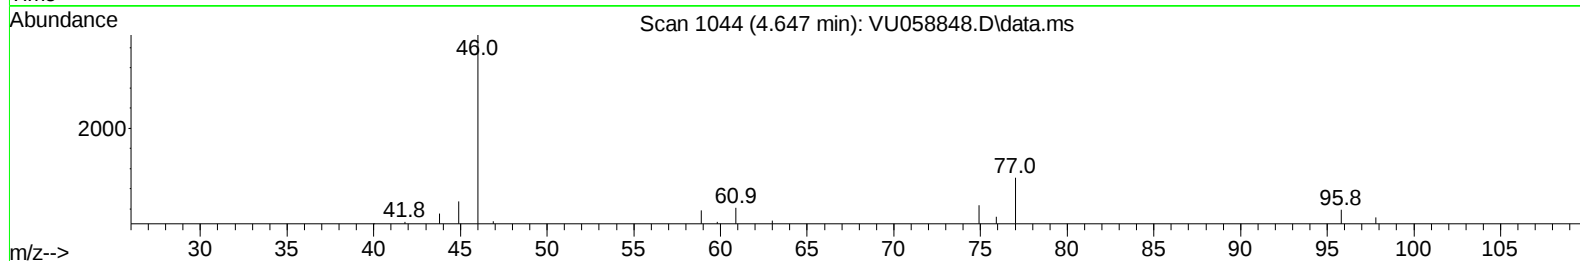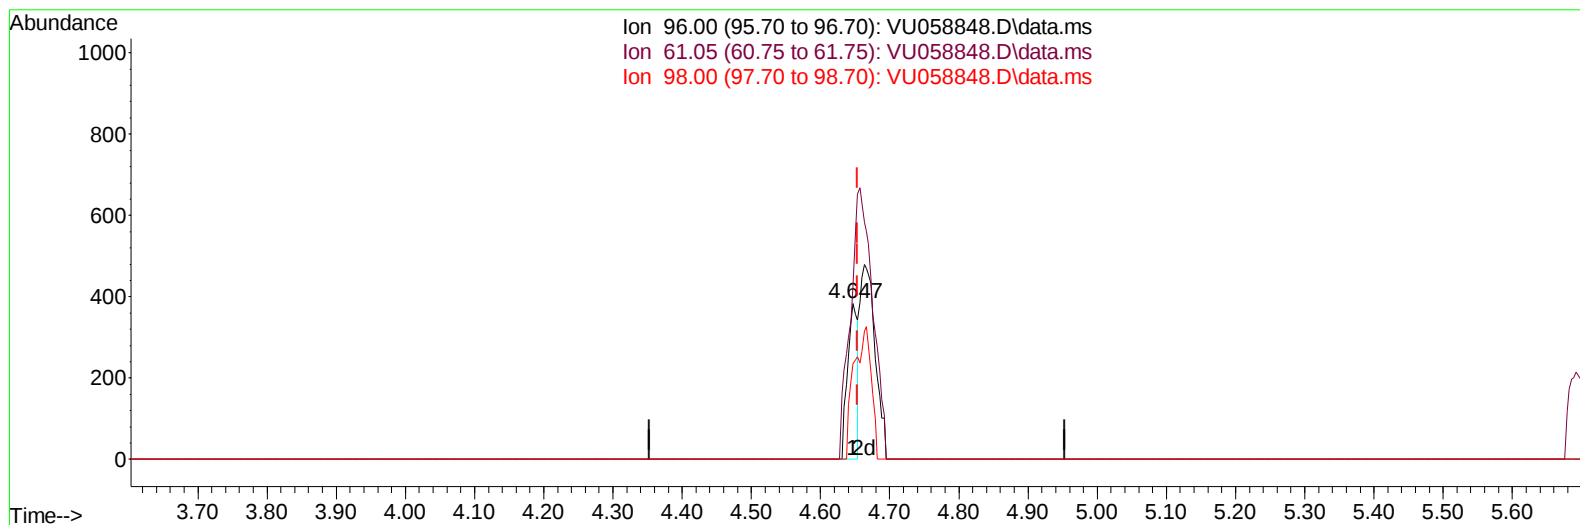

(22) cis-1,2-Dichloroethene (T)

4.647min (-0.006) 0.09 ug/L

response 384

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	143.40	110.94
98.00	64.40	61.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
Data File : VU058848.D
Acq On : 07 May 2024 17:58
Operator : MD/SY
Sample : P2392-06DL 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAQ7DL

Manual IntegrationsAPPROVED

Quant Time: May 08 05:12:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 08 05:10:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/08/2024
Supervised By :Semsettin Yesilyurt 05/08/2024

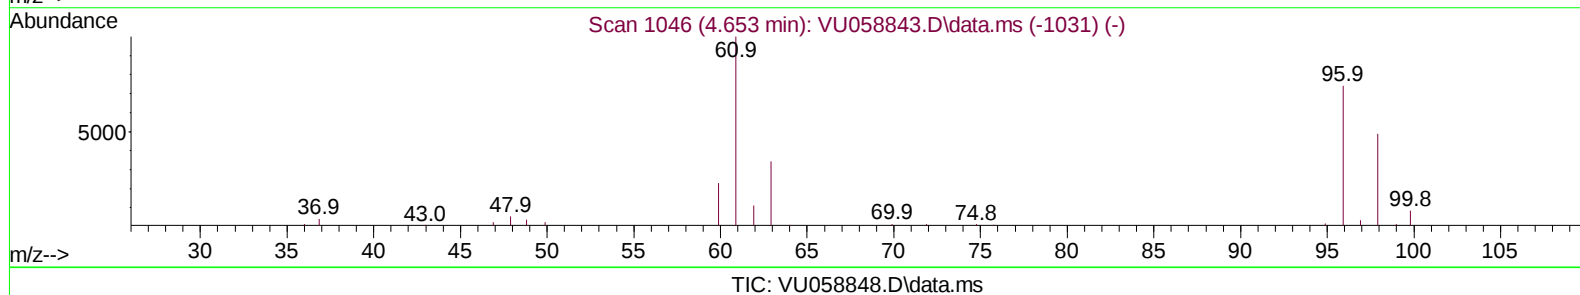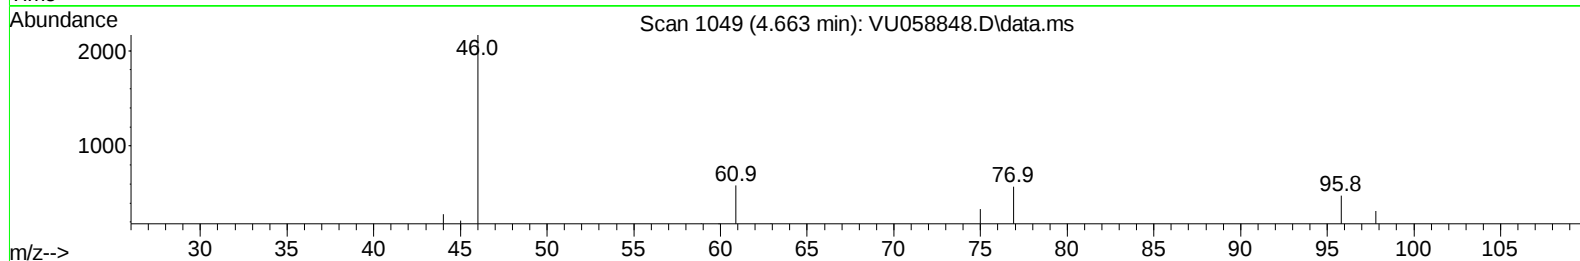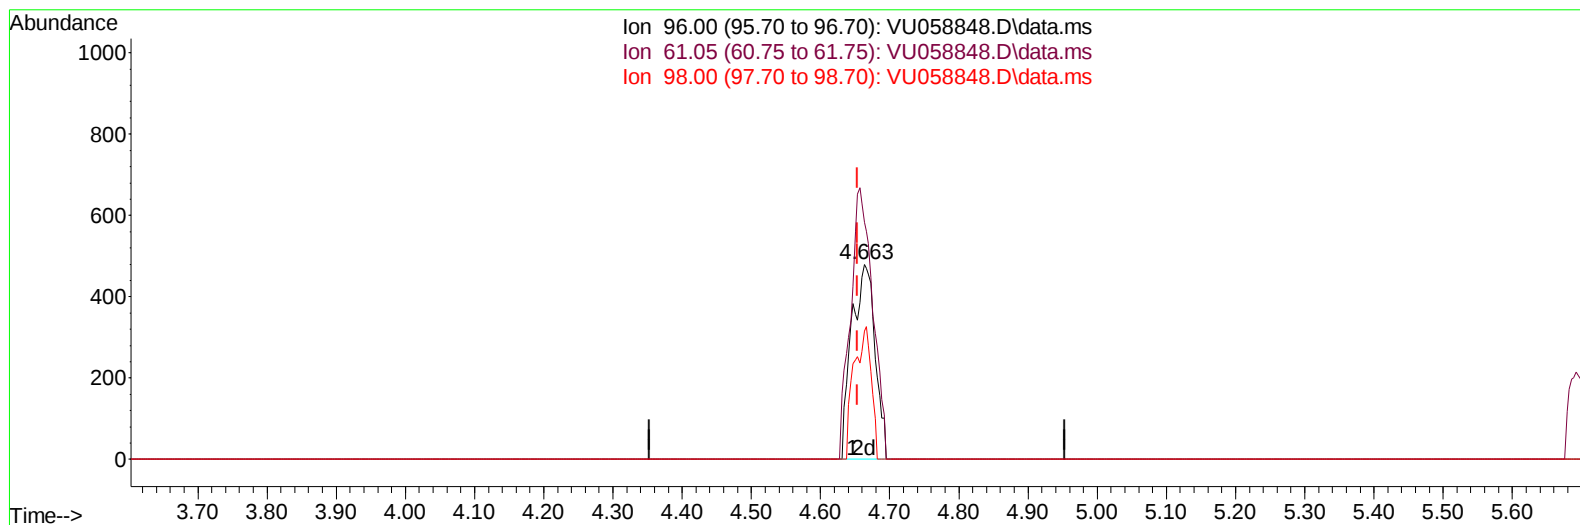

(22) cis-1,2-Dichloroethene (T)

4.663min (+ 0.010) 0.26 ug/L m

response 1124

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	143.40	121.67
98.00	64.40	65.63
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
 Data File : VU058848.D
 Acq On : 07 May 2024 17:58
 Operator : MD/SY
 Sample : P2392-06DL 2000X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAQ7DL

Manual IntegrationsAPPROVED

Quant Time: May 08 05:12:11 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 08 05:10:37 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/08/2024
 Supervised By :Semsettin Yesilyurt 05/08/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		53848	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		54705	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		24726	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.589	65		12661	2.989	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	59.800%	
7) Chloroethane-d5	1.904	69		11219	3.515	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	70.400%	
11) 1,1-Dichloroethene-d2	2.557	65		8378	3.929	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	78.600%	
20) 2-Butanone-d5	4.612	46		36564	49.134	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	98.260%	
24) Chloroform-d	5.052	84		45499	5.255	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	105.000%	
26) 1,2-Dichloroethane-d4	5.692	65		24176	5.760	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	115.200%	
32) Benzene-d6	5.718	84		74543	4.281	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	85.600%	
36) 1,2-Dichloropropane-d6	6.682	67		21470	4.134	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	82.600%	
41) Toluene-d8	7.891	98		64315	4.127	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	82.600%	
43) trans-1,3-Dichloroprop...	8.177	79		8728	4.616	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	92.400%	
46) 2-Hexanone-d5	8.627	63		26741	47.725	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	95.460%	
56) 1,1,2,2-Tetrachloroeth...	10.750	84		15845	5.009	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	100.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		23783	5.519	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	110.400%	
Target Compounds							
16) Methylene chloride	3.033	84		4157	0.985	ug/L	94
22) cis-1,2-Dichloroethene	4.663	96		1124m	0.260	ug/L	
47) Tetrachloroethene	8.547	164		41904	11.594	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
Data File : VU058848.D
Acq On : 07 May 2024 17:58
Operator : MD/SY
Sample : P2392-06DL 2000X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAQ7DL

Manual IntegrationsAPPROVED

Quant Time: May 08 05:12:11 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 08 05:10:37 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/08/2024
Supervised By :Semsettin Yesilyurt 05/08/2024

