

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
 Data File : VU058847.D
 Acq On : 07 May 2024 17:25
 Operator : MD/SY
 Sample : P2392-05DL 400X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAQ6DL

Quant Time: May 08 05:11:54 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 08 05:10:37 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	55950	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	54611	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	25471	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.589	65	13605	3.091	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	61.800%	
7) Chloroethane-d5	1.904	69	11753	3.544	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	70.800%	
11) 1,1-Dichloroethene-d2	2.557	65	8666	3.911	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	4.611	46	37408	48.380	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	96.760%	
24) Chloroform-d	5.049	84	46514	5.170	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.400%	
26) 1,2-Dichloroethane-d4	5.692	65	24925	5.716	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	114.400%	
32) Benzene-d6	5.718	84	76312	4.390	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.800%	
36) 1,2-Dichloropropane-d6	6.682	67	22671	4.373	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.400%	
41) Toluene-d8	7.891	98	66696	4.287	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	85.800%	
43) trans-1,3-Dichloroprop...	8.177	79	8800	4.662	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.200%	
46) 2-Hexanone-d5	8.627	63	27954	49.976	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	99.960%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84	15407	4.879	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	97.600%	
66) 1,2-Dichlorobenzene-d4	12.190	152	23604	5.317	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	106.400%	
Target Compounds						
16) Methylene chloride	3.033	84	2241	0.511	ug/L	86
22) cis-1,2-Dichloroethene	4.656	96	3991	0.890	ug/L	92
47) Tetrachloroethene	8.547	164	23756	6.584	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU050724\
Data File : VU058847.D
Acq On : 07 May 2024 17:25
Operator : MD/SY
Sample : P2392-05DL 400X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAQ6DL

Quant Time: May 08 05:11:54 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042224WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 08 05:10:37 2024
Response via : Initial Calibration




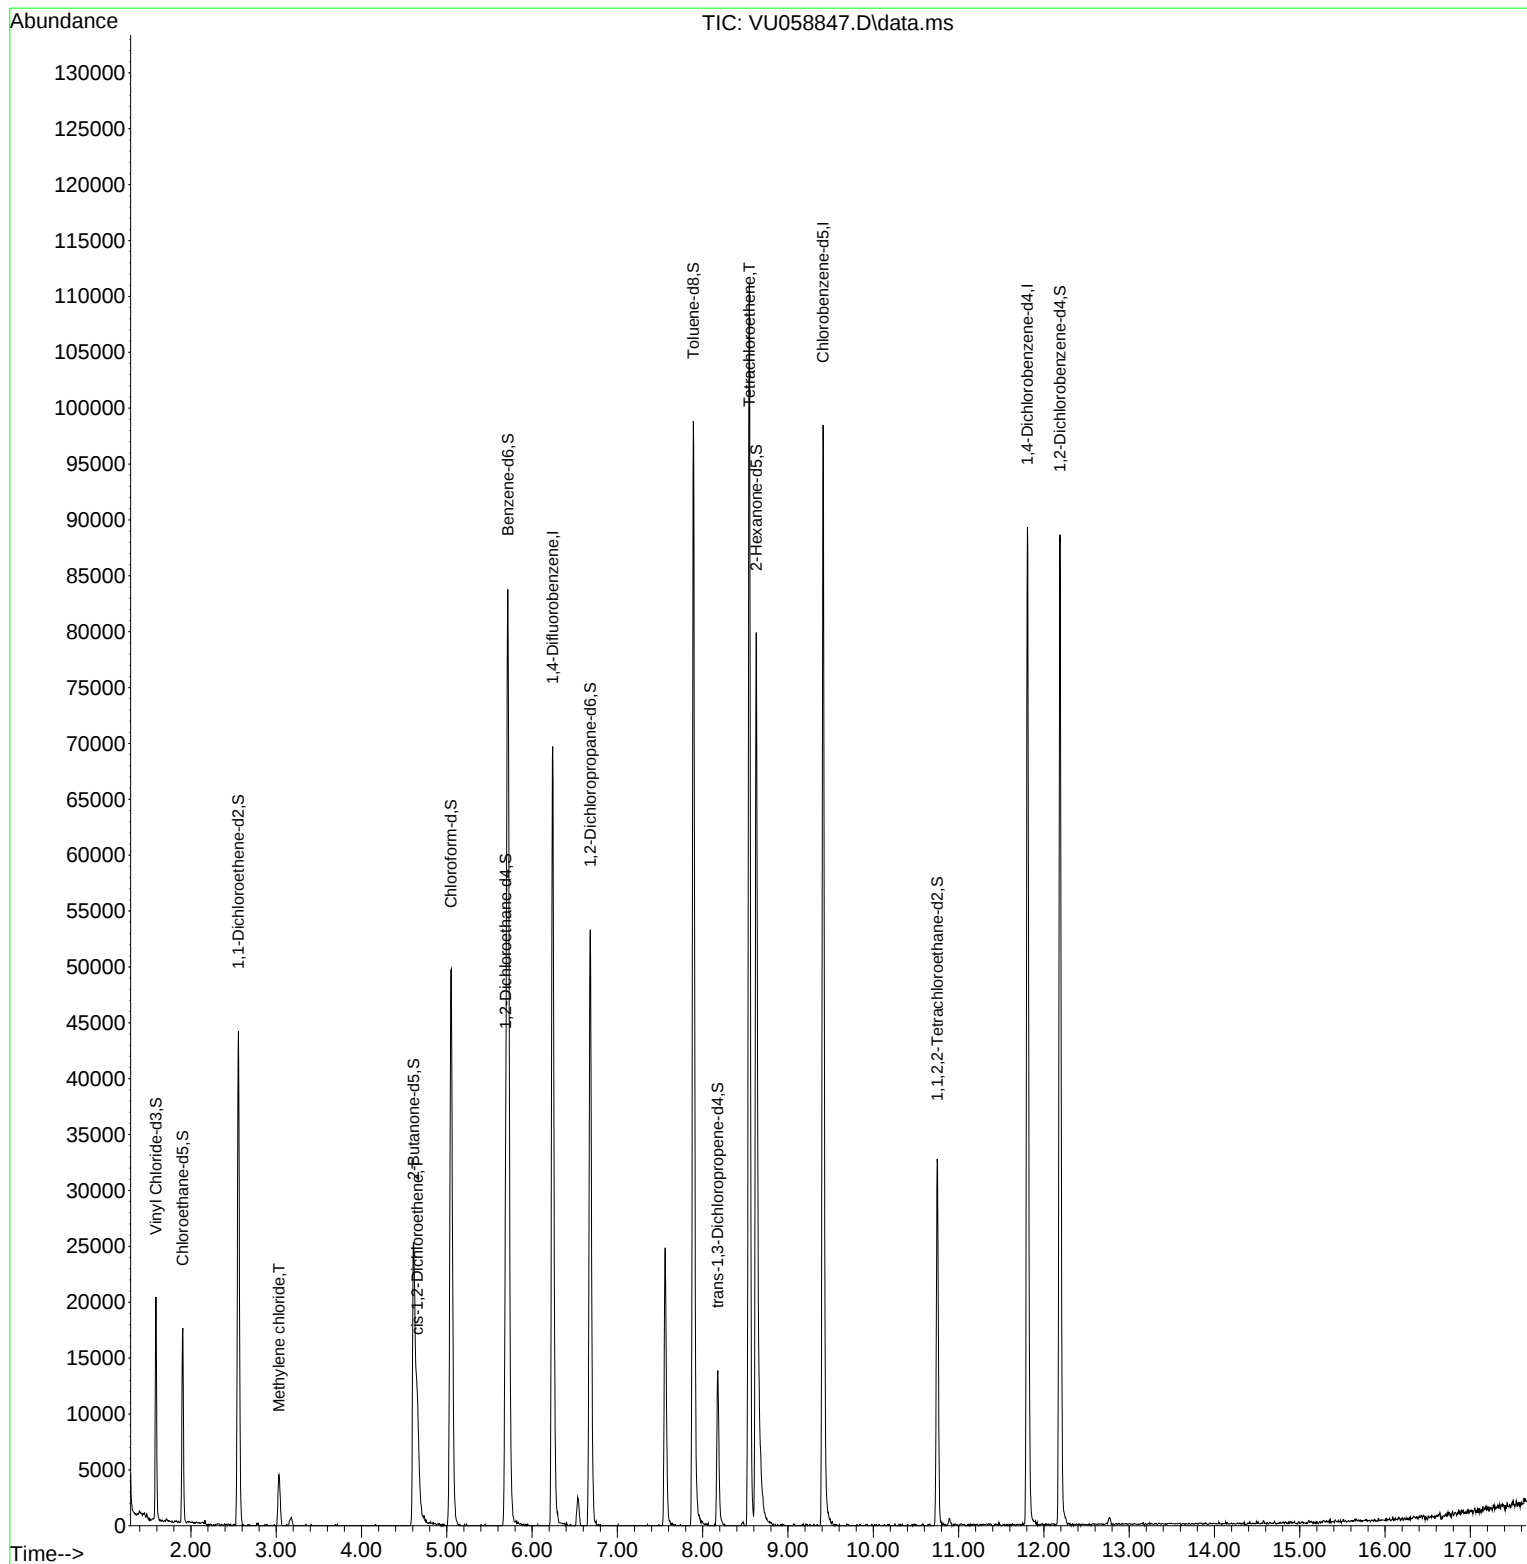


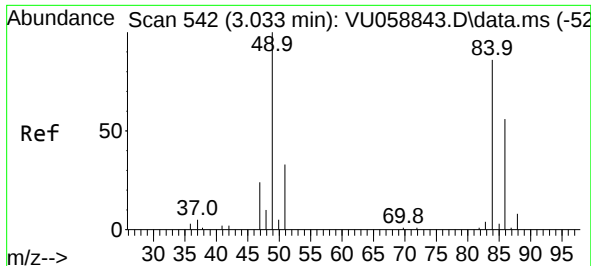

#16
Methylene chloride
Concen: 0.511 ug/L
RT: 3.033 min Scan# 54
Delta R.T. -0.000 min
Lab File: VU058847.D
Acq: 07 May 2024 17:25




Instrument :
MSVOA_U
ClientSampleId :
BHAQ6DL


Tgt Ion: 84 Resp: 2241
Ion Ratio Lower Upper
84 100
86 56.1 45.0 83.6
49 113.3 91.6 170.2

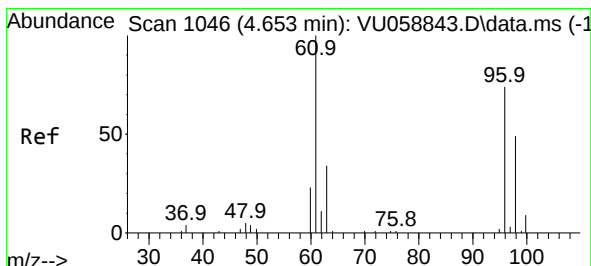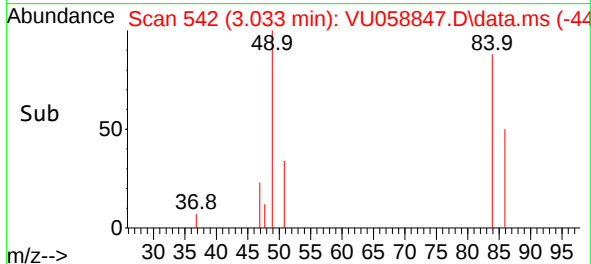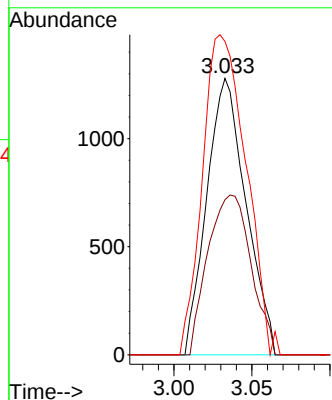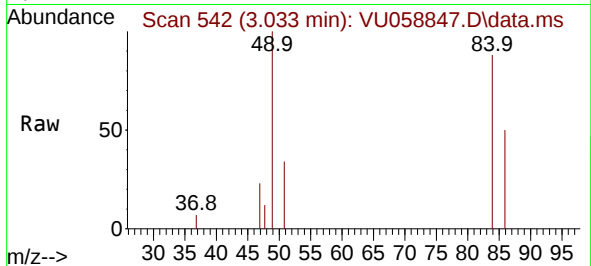

#22
cis-1,2-Dichloroethene
Concen: 0.890 ug/L
RT: 4.656 min Scan# 1047
Delta R.T. 0.003 min
Lab File: VU058847.D
Acq: 07 May 2024 17:25


Tgt Ion: 96 Resp: 3991
Ion Ratio Lower Upper
96 100
61 130.1 100.4 186.4
98 67.0 45.1 83.7

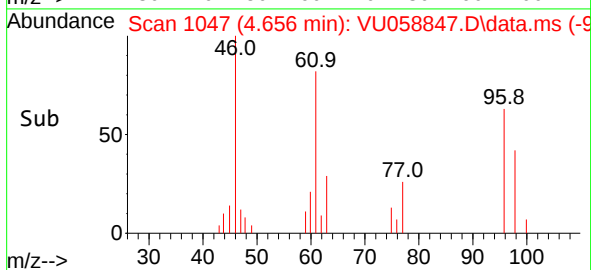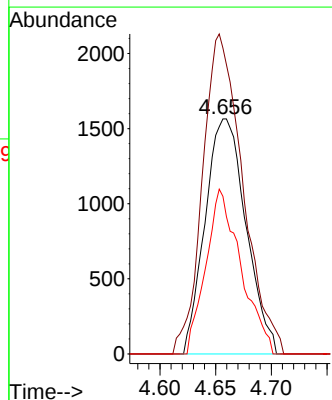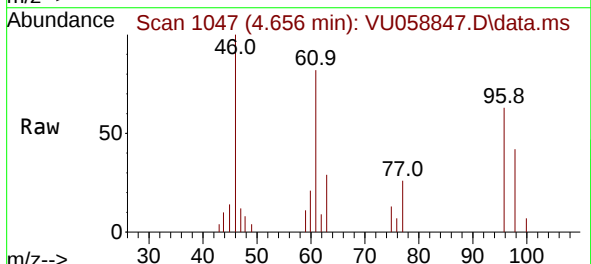

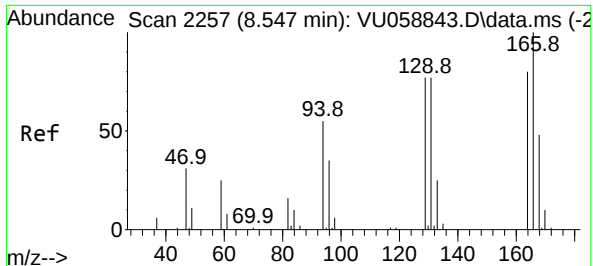

#47
Tetrachloroethene
Concen: 6.584 ug/L
RT: 8.547 min Scan# 21
Delta R.T. -0.000 min
Lab File: VU058847.D
Acq: 07 May 2024 17:25

Instrument :
MSVOA_U
ClientSampleId :
BHAQ6DL

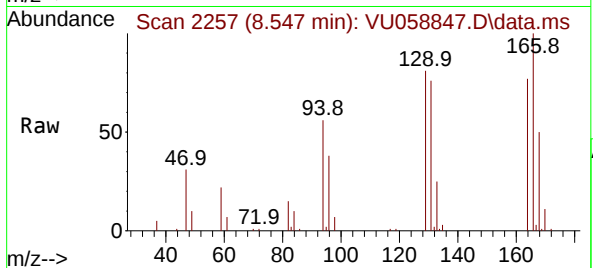

Tgt Ion:	164	Resp:	23756
Ion	Ratio	Lower	Upper
164	100		
129	104.5	71.5	132.9
131	97.8	65.0	120.6
166	129.1	89.5	166.1

