




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051424\
Data File : VU058884.D
Acq On : 14 May 2024 14:08
Operator : MD/SY
Sample : P2392-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS2

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/15/2024
Supervised By :Semsettin Yesilyurt 05/15/2024

Quant Time: May 15 01:07:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 15 00:49:30 2024
Response via : Initial Calibration

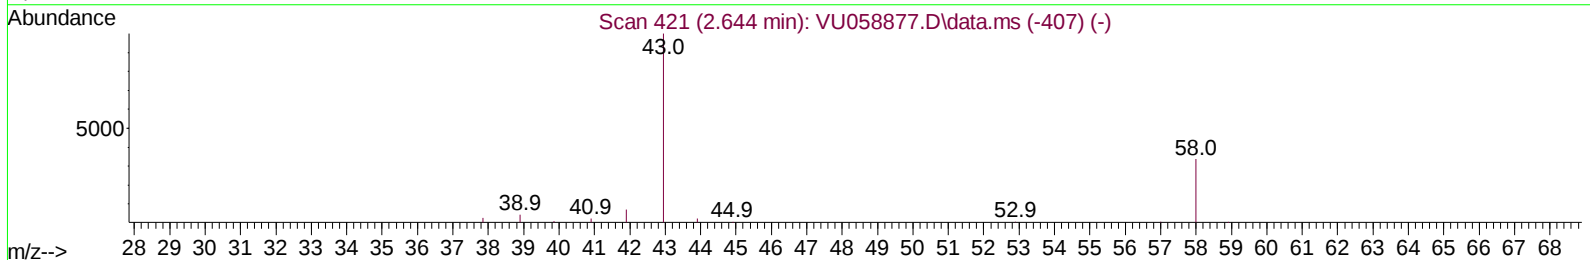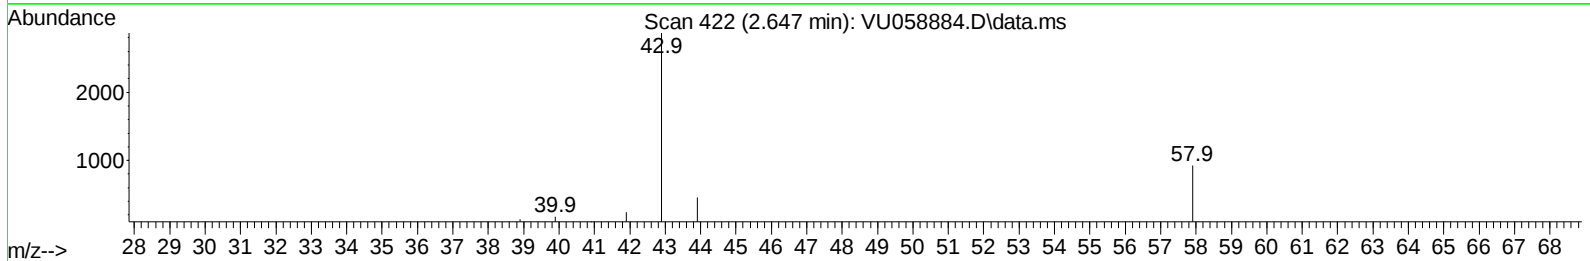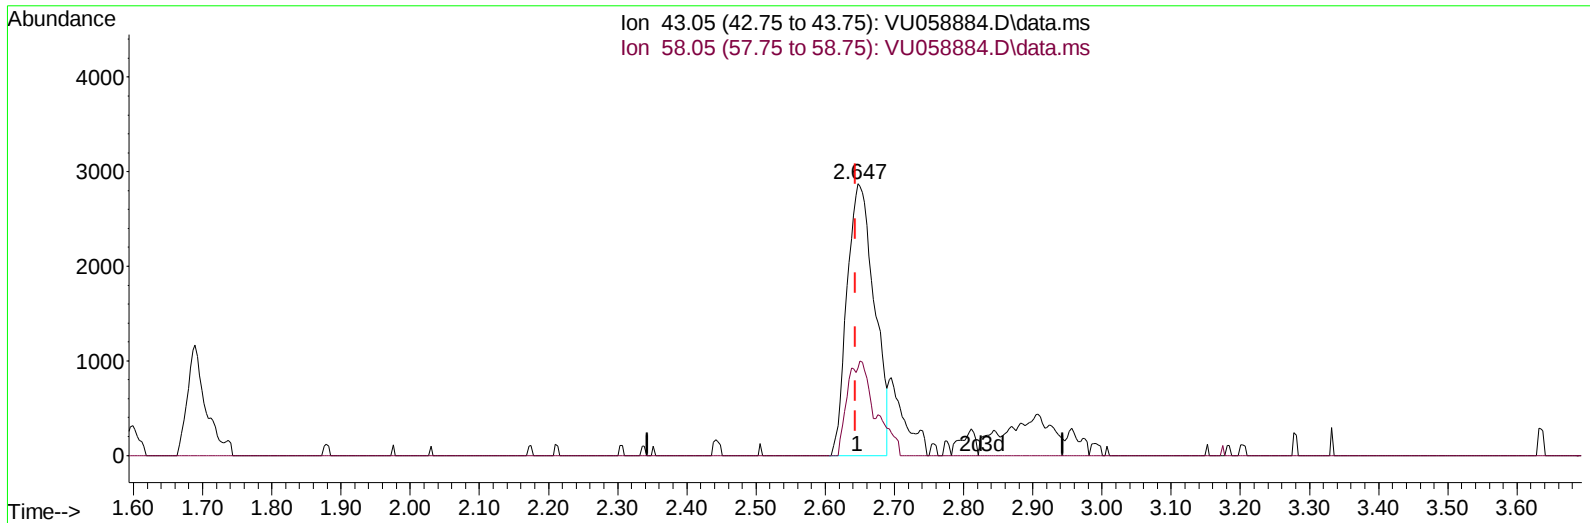

TIC: VU058884.D\data.ms

(13) Acetone (T)

2.647min (+ 0.004) 4.52 ug/L

response 7913

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	28.64
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051424\
Data File : VU058884.D
Acq On : 14 May 2024 14:08
Operator : MD/SY
Sample : P2392-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS2

Manual IntegrationsAPPROVED

Quant Time: May 15 01:07:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 15 00:49:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/15/2024
Supervised By :Semsettin Yesilyurt 05/15/2024

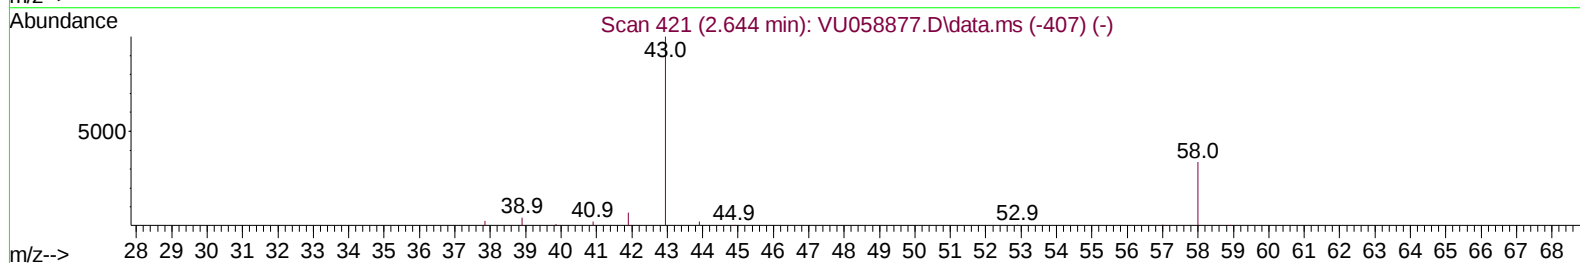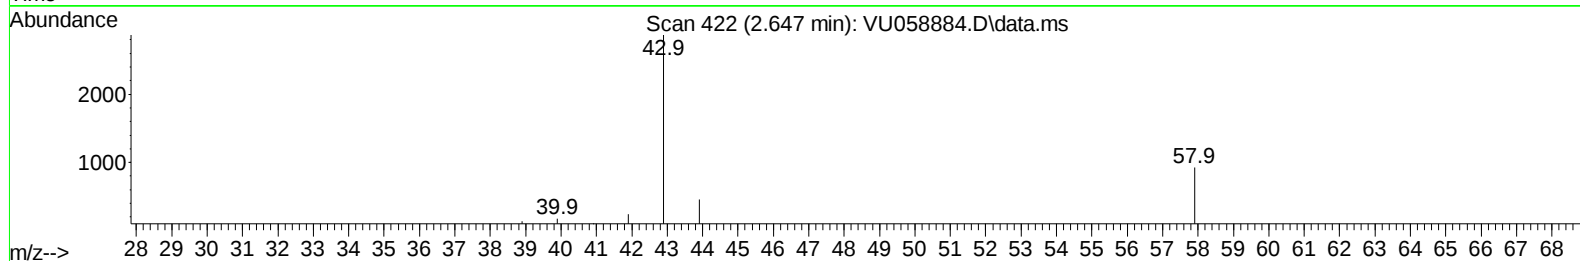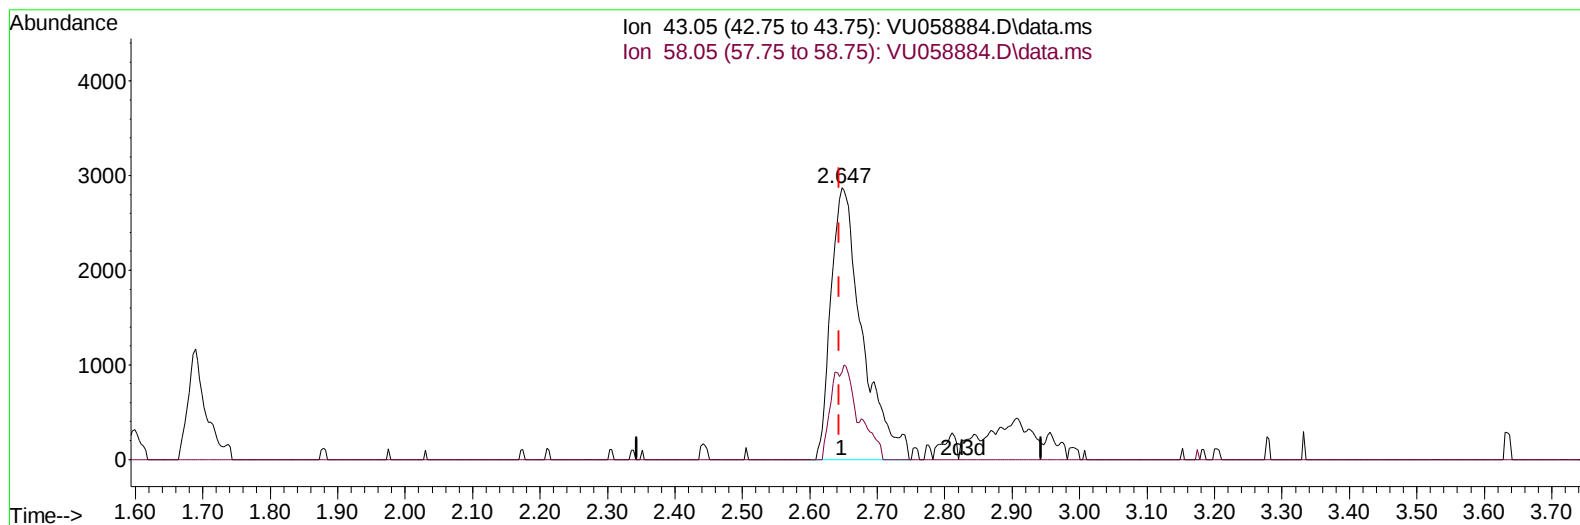

TIC: VU058884.D\data.ms

(13) Acetone (T)

2.647min (+ 0.004) 5.29 ug/L m

response 9266

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	24.45
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051424\
 Data File : VU058884.D
 Acq On : 14 May 2024 14:08
 Operator : MD/SY
 Sample : P2392-21
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHAS2

Manual IntegrationsAPPROVED

Quant Time: May 15 01:07:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed May 15 00:49:30 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/15/2024
 Supervised By :Semsettin Yesilyurt 05/15/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.242	114		160946	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		162594	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.808	152		74955	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.596	65		46750	4.795	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	96.000%	
7) Chloroethane-d5	1.911	69		43651	4.954	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	99.000%	
11) 1,1-Dichloroethene-d2	2.564	65		18547	4.668	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	93.400%	
20) 2-Butanone-d5	4.625	46		135642	53.514	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	107.020%	
24) Chloroform-d	5.056	84		97135	4.934	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	98.600%	
26) 1,2-Dichloroethane-d4	5.695	65		51587	5.098	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	102.000%	
32) Benzene-d6	5.721	84		188956	5.063	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	101.200%	
36) 1,2-Dichloropropane-d6	6.682	67		62503	5.026	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	100.600%	
41) Toluene-d8	7.891	98		156581	4.609	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...	8.178	79		21507	5.040	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	100.800%	
46) 2-Hexanone-d5	8.628	63		102319	49.960	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	99.920%	
56) 1,1,2,2-Tetrachloroeth...	10.747	84		52318	4.871	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	97.400%	
66) 1,2-Dichlorobenzene-d4	12.187	152		58851	5.221	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	104.400%	
Target Compounds							
13) Acetone	2.647	43		9266m	5.289	ug/L	
16) Methylene chloride	3.040	84		3174	0.233	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051424\
Data File : VU058884.D
Acq On : 14 May 2024 14:08
Operator : MD/SY
Sample : P2392-21
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHAS2

Manual IntegrationsAPPROVED

Quant Time: May 15 01:07:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed May 15 00:49:30 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/15/2024
Supervised By :Semsettin Yesilyurt 05/15/2024

