
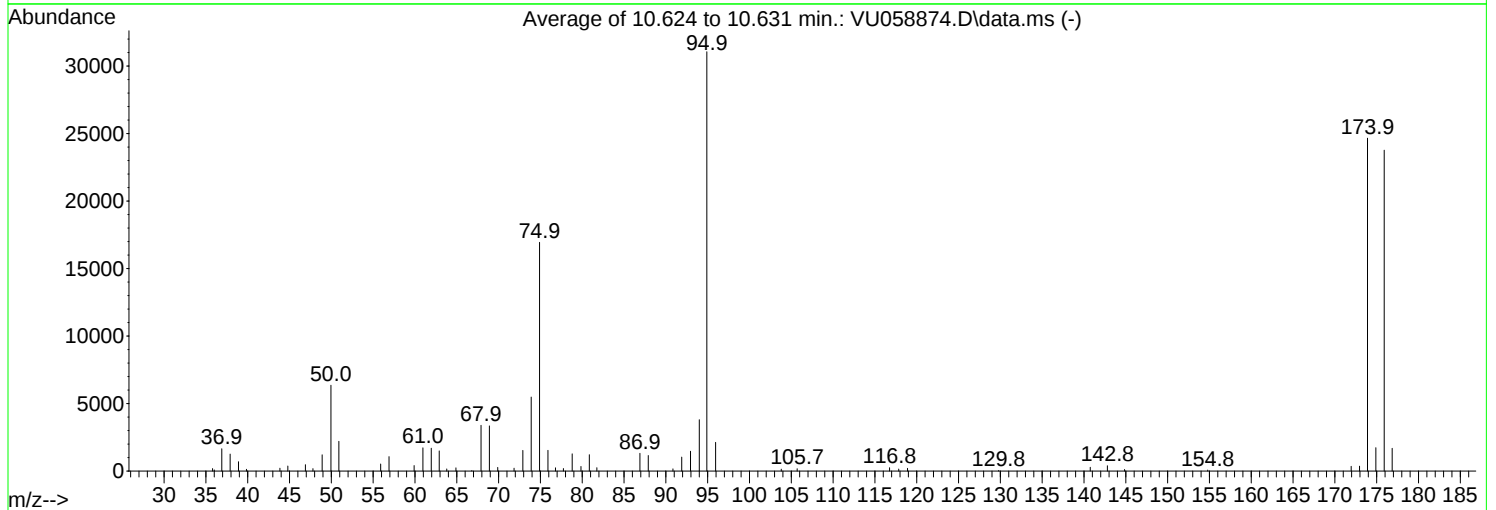


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051424\
Data File : VU058874.D
Acq On : 14 May 2024 09:07
Operator : MD/SY
Sample : BFB154
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB154

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed May 15 00:49:30 2024

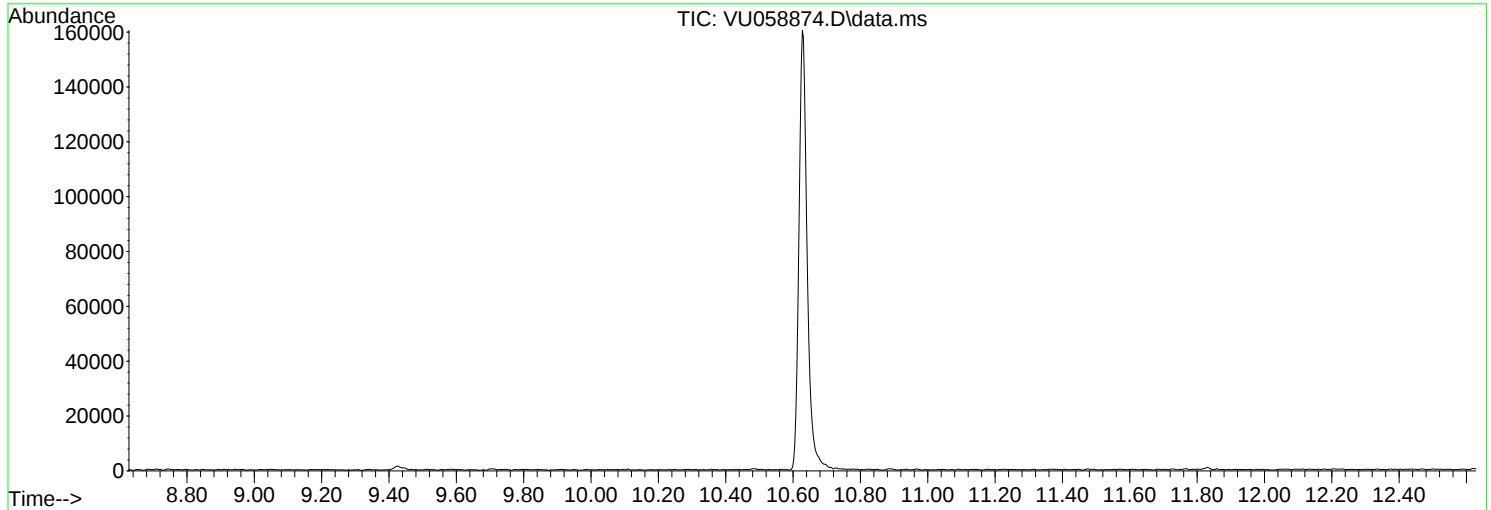

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2891

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.5	6357	PASS
75	95	30	80	54.5	16942	PASS
95	95	100	100	100.0	31061	PASS
96	95	5	9	6.8	2125	PASS
173	174	0.00	2	1.5	361	PASS
174	95	50	120	79.4	24656	PASS
175	174	5	9	7.0	1733	PASS
176	174	95	101	96.4	23768	PASS
177	176	5	9	7.1	1687	PASS

Scan 2891 (10.586 min): VU058874.D\data.ms
BFB154

m/z	Abundance
39.60	117.0
43.90	277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
35.80	282.0
36.90	1473.0
37.90	1243.0
38.90	650.0
39.80	140.0
43.90	468.0
44.80	339.0
46.90	424.0
47.80	204.0
48.90	1066.0
49.90	6156.0
50.90	2115.0
55.90	492.0
56.90	1024.0
59.90	324.0
61.00	1772.0
62.00	1687.0
62.90	1471.0
63.80	107.0
64.90	208.0
67.90	3336.0
68.90	3161.0
69.90	276.0
71.90	145.0
72.90	1476.0
73.90	5437.0
74.90	16099.0
75.90	1490.0
76.80	220.0
77.70	147.0
78.80	1194.0
79.90	333.0
80.80	1146.0
81.70	213.0
86.90	1228.0
87.90	1164.0
90.80	186.0
91.90	910.0
93.00	1310.0
94.00	3826.0
94.90	29128.0
95.90	2039.0
103.80	138.0
105.70	206.0
116.80	248.0
117.80	135.0
118.90	238.0
129.80	124.0
140.80	281.0
142.80	351.0
144.80	113.0
154.80	112.0
172.00	317.0
172.90	294.0
173.90	23200.0
174.90	1675.0
175.90	22368.0
176.80	1535.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
35.80	274.0
36.90	1724.0
37.90	1277.0
38.90	710.0
39.80	125.0
43.80	500.0
44.80	393.0
46.90	498.0
47.80	188.0
48.90	1239.0
50.00	6538.0
50.90	2268.0
55.90	534.0
56.90	1116.0
59.90	438.0
61.00	1793.0
62.00	1729.0
62.90	1566.0
63.80	178.0
64.90	251.0
67.90	3521.0
68.90	3462.0
69.90	272.0
71.90	231.0
72.90	1601.0
73.90	5677.0
74.90	17552.0
75.90	1607.0
76.80	248.0
77.70	198.0
78.80	1305.0
79.90	339.0
80.90	1245.0
81.80	259.0
86.90	1339.0
87.90	1170.0
90.80	168.0
91.90	1062.0
92.90	1483.0
94.00	3874.0
94.90	32152.0
95.90	2186.0
103.80	144.0
105.70	187.0
116.80	241.0
117.90	162.0
118.90	206.0
140.70	289.0
142.80	410.0
144.90	122.0
154.80	117.0
172.00	356.0
172.90	383.0
173.90	25488.0
174.90	1810.0
175.90	24600.0
176.90	1709.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154

m/z	Abundance
36.00	253.0
36.90	1759.0
37.90	1252.0
38.90	718.0
39.90	133.0
43.80	507.0
44.80	385.0
46.90	494.0
47.80	154.0
48.90	1306.0
50.00	6377.0
50.90	2230.0
55.90	541.0
56.90	1067.0
59.90	462.0
60.90	1600.0
61.90	1656.0
62.90	1448.0
63.80	189.0
64.90	255.0
66.80	110.0
67.90	3306.0
68.90	3410.0
69.90	263.0
71.80	260.0
72.90	1507.0
73.90	5338.0
74.90	17176.0
75.90	1511.0
76.80	258.0
77.80	223.0
78.80	1330.0
79.80	350.0
80.90	1250.0
81.80	277.0
86.90	1379.0
87.90	1121.0
90.90	135.0
91.90	1127.0
92.90	1615.0
94.00	3714.0
94.90	31904.0
96.00	2151.0
103.80	141.0
105.70	131.0
116.70	256.0
117.90	157.0
118.90	164.0
140.80	275.0
142.80	422.0
144.90	115.0
171.80	379.0
173.00	406.0
173.90	25280.0
174.90	1715.0
175.90	24336.0
176.90	1816.0

Instrument :
MSVOA_U
ClientSampleId :
BFB154