




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051724\
Data File : VU058907.D
Acq On : 17 May 2024 13:09
Operator : MD/SY
Sample : P2520-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB62

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 05/20/2024
Supervised By :Semsettin Yesilyurt 05/20/2024

Quant Time: May 18 00:12:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 18 00:11:42 2024
Response via : Initial Calibration

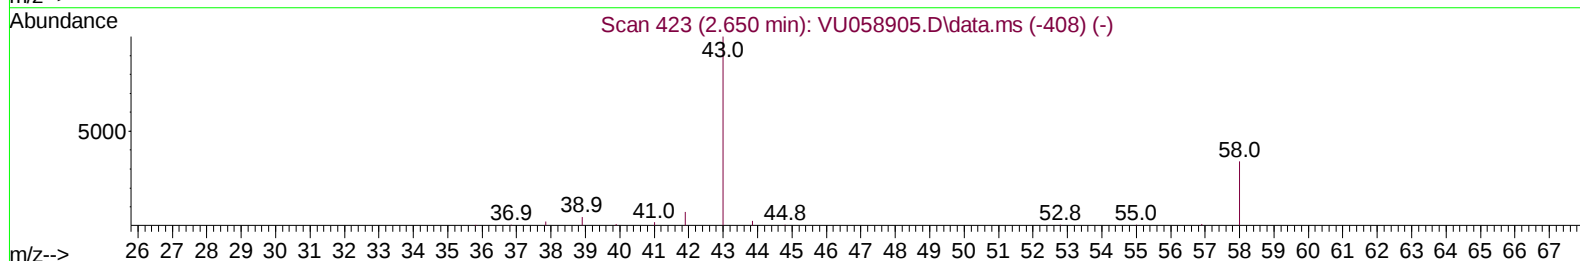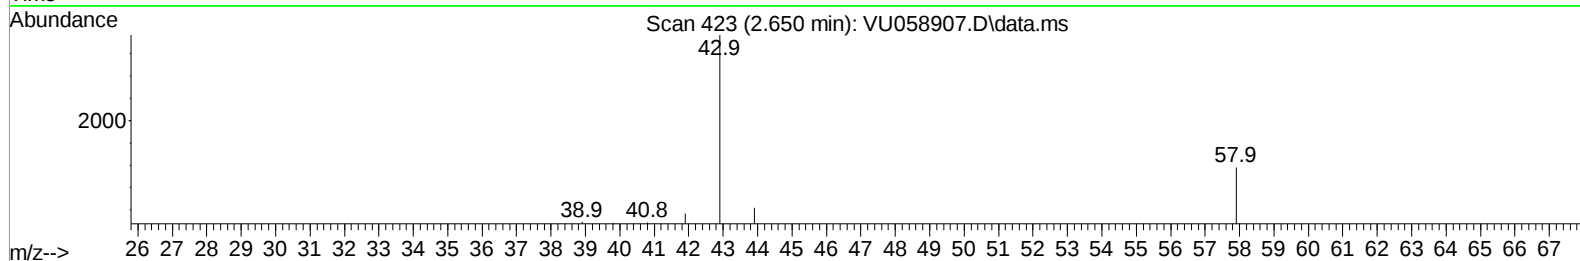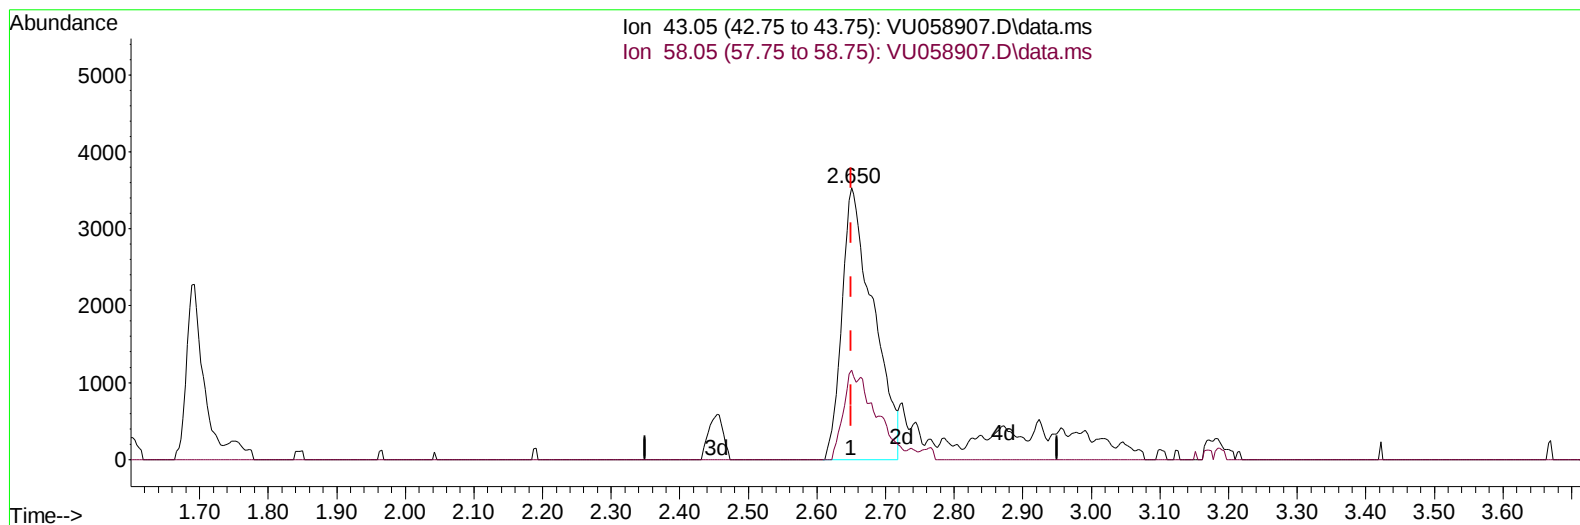

TIC: VU058907.D\data.ms

(13) Acetone (T)

2.650min (+ 0.000) 7.19 ug/L

response 11146

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	13.38
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051724\
Data File : VU058907.D
Acq On : 17 May 2024 13:09
Operator : MD/SY
Sample : P2520-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB62

Manual IntegrationsAPPROVED

Quant Time: May 18 00:12:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 18 00:11:42 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/20/2024
Supervised By :Semsettin Yesilyurt 05/20/2024

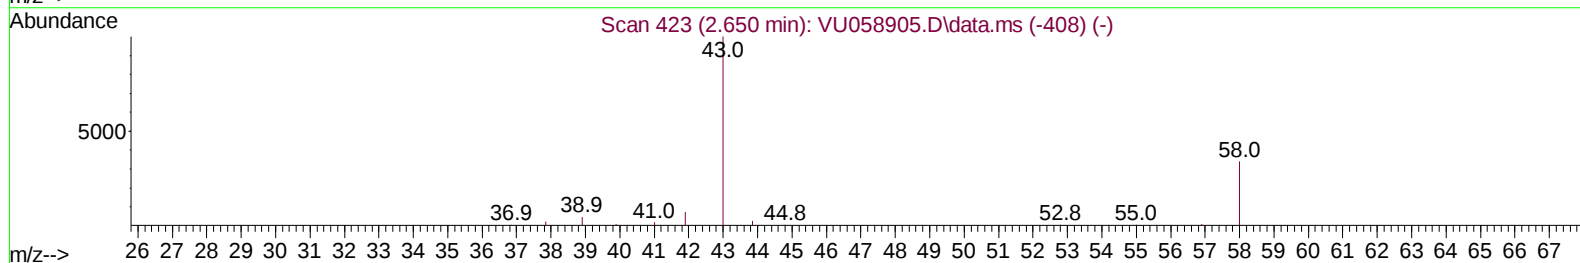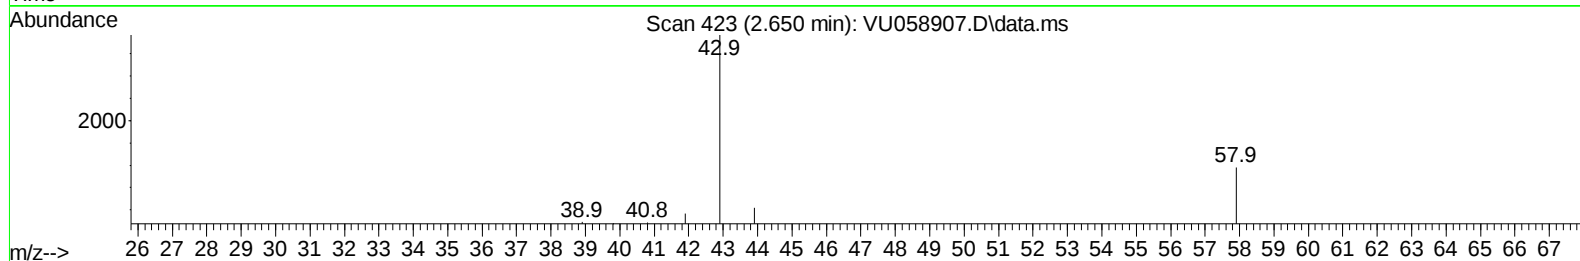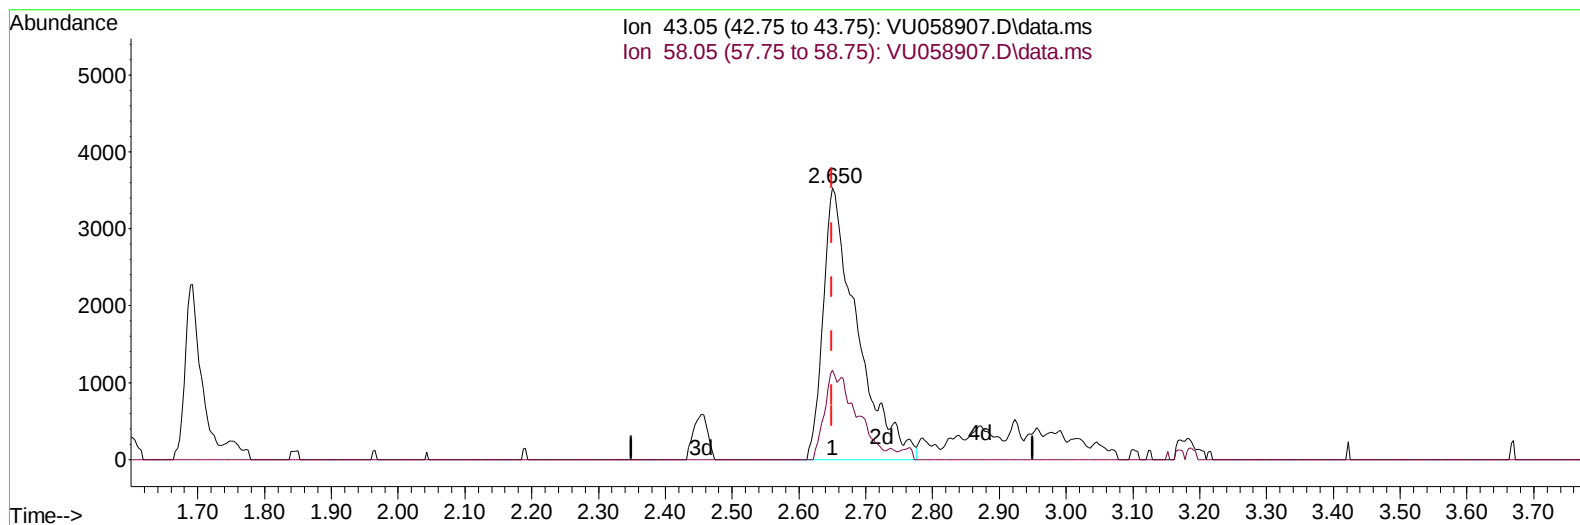

TIC: VU058907.D\data.ms

(13) Acetone (T)

2.650min (+ 0.000) 8.02 ug/L m

response 12435

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	34.00	11.99
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051724\
 Data File : VU058907.D
 Acq On : 17 May 2024 13:09
 Operator : MD/SY
 Sample : P2520-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHB62

Manual IntegrationsAPPROVED

Quant Time: May 18 00:12:16 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Sat May 18 00:11:42 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/20/2024
 Supervised By :Semsettin Yesilyurt 05/20/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.245	114		142498	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117		145329	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152		66275	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.599	65		37830	4.383	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.600%	
7) Chloroethane-d5	1.911	69		36706	4.705	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	2.563	65		15347	4.363	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	87.200%	
20) 2-Butanone-d5	4.634	46		128814	57.399	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	114.800%	
24) Chloroform-d	5.059	84		86682	4.973	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.400%	
26) 1,2-Dichloroethane-d4	5.698	65		45246	5.051	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.000%	
32) Benzene-d6	5.724	84		158690	4.757	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.200%	
36) 1,2-Dichloropropane-d6	6.685	67		56474	5.081	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	101.600%	
41) Toluene-d8	7.894	98		123505	4.068	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	81.400%	
43) trans-1,3-Dichloroprop...	8.177	79		16955	4.445	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	89.000%	
46) 2-Hexanone-d5	8.631	63		89116	48.683	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	97.360%	
56) 1,1,2,2-Tetrachloroeth...	10.753	84		47646	4.963	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	99.200%	
66) 1,2-Dichlorobenzene-d4	12.190	152		49665	4.983	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.600%	
Target Compounds							
13) Acetone	2.650	43		12435m	8.017	ug/L	
16) Methylene chloride	3.043	84		1783	0.148	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051724\
Data File : VU058907.D
Acq On : 17 May 2024 13:09
Operator : MD/SY
Sample : P2520-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHB62

Manual IntegrationsAPPROVED

Quant Time: May 18 00:12:16 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Sat May 18 00:11:42 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 05/20/2024
Supervised By :Semsettin Yesilyurt 05/20/2024

