


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU051724\
Data File : VU058904.D
Acq On : 17 May 2024 08:20
Operator : MD/SY
Sample : BFB156
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB156

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Sat May 18 00:11:42 2024

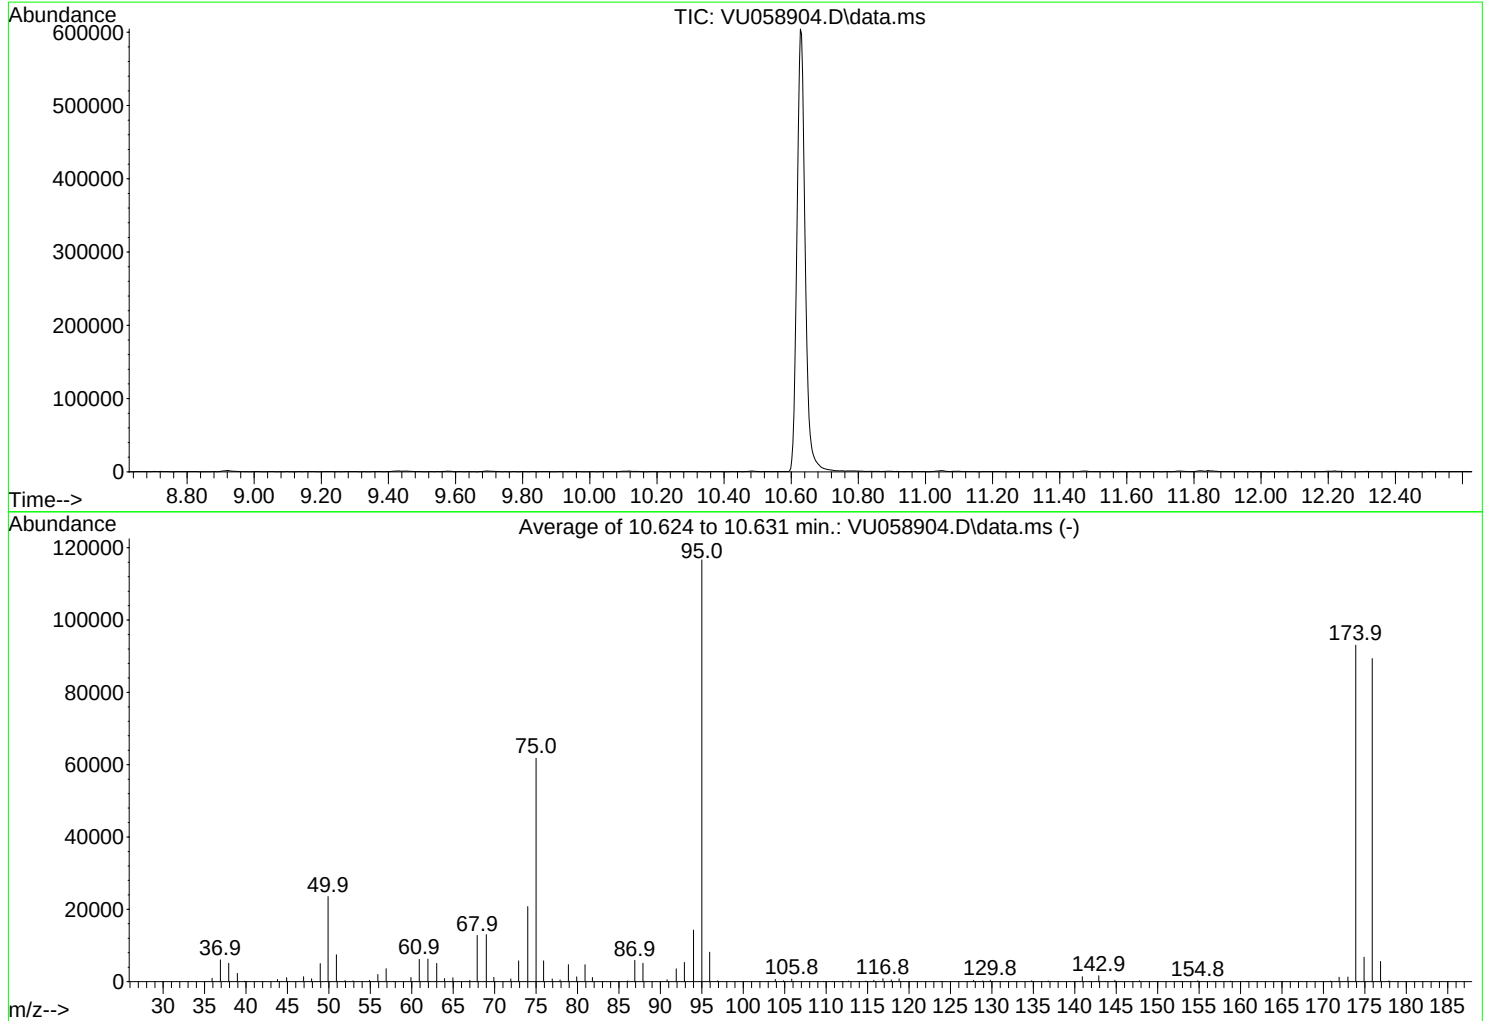

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.2	23547	PASS
75	95	30	80	53.0	61779	PASS
95	95	100	100	100.0	116659	PASS
96	95	5	9	7.0	8162	PASS
173	174	0.00	2	1.4	1288	PASS
174	95	50	120	79.8	93064	PASS
175	174	5	9	7.3	6777	PASS
176	174	95	101	96.0	89357	PASS
177	176	5	9	6.2	5556	PASS

m/z	Abundance
39.70	105.0
43.80	268.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	878.0
36.90	5841.0
37.90	4890.0
38.90	2255.0
39.90	298.0
43.90	996.0
44.90	1077.0
45.80	101.0
46.90	1328.0
47.90	791.0
49.00	4747.0
49.90	22792.0
50.90	7315.0
51.90	286.0
52.90	227.0
54.90	374.0
55.90	1830.0
56.90	3484.0
59.90	1042.0
60.90	5973.0
61.90	5939.0
63.00	4897.0
63.90	811.0
64.90	1068.0
67.00	336.0
67.90	12235.0
69.00	12438.0
69.90	1174.0
72.00	841.0
72.90	5475.0
74.00	19984.0
75.00	58936.0
75.90	5471.0
77.00	669.0
77.90	454.0
78.90	4742.0
79.90	1252.0
80.90	4439.0
81.80	1037.0
86.00	170.0
86.90	5605.0
87.90	4940.0
90.80	587.0
91.90	3568.0
92.90	5081.0
94.00	13712.0
95.00	110720.0
95.90	7714.0
96.90	238.0
103.90	562.0
104.90	235.0
105.80	709.0
111.90	130.0
112.70	210.0
114.80	132.0
115.80	432.0
116.90	930.0
117.80	450.0
118.80	829.0
123.80	110.0
127.80	425.0
128.90	186.0
129.80	414.0
134.80	209.0
136.90	143.0
140.90	1283.0
142.90	1552.0
144.90	384.0
147.80	256.0
154.90	263.0
158.80	116.0
160.80	111.0
170.90	144.0
171.90	1162.0
172.90	1240.0
173.90	86400.0
174.90	6361.0
175.90	83152.0
176.90	5147.0
177.90	183.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	929.0
36.90	6185.0
37.90	5199.0
38.90	2372.0
39.90	232.0
43.80	874.0
44.90	1162.0
47.00	1428.0
47.90	832.0
48.90	5168.0
49.90	24552.0
50.90	7652.0
52.00	322.0
52.90	252.0
54.90	321.0
55.90	2068.0
56.90	3661.0
57.80	141.0
59.90	1193.0
60.90	6371.0
61.90	6401.0
63.00	5198.0
64.00	862.0
65.00	1071.0
67.00	391.0
67.90	13240.0
69.00	13262.0
69.90	1238.0
71.90	751.0
72.90	5953.0
74.00	21336.0
75.00	63840.0
75.90	6075.0
76.90	809.0
77.90	496.0
78.90	4842.0
79.90	1349.0
80.90	4824.0
81.80	1219.0
82.90	106.0
86.10	248.0
86.90	6106.0
87.90	5274.0
90.80	579.0
91.90	3576.0
92.90	5504.0
94.00	14699.0
95.00	119904.0
96.00	8441.0
96.90	226.0
103.90	669.0
104.90	250.0
105.90	716.0
109.70	104.0
110.80	125.0
111.90	112.0
112.70	172.0
114.80	213.0
115.70	397.0
116.90	850.0
117.90	475.0
118.80	850.0
123.90	100.0
127.80	449.0
128.90	222.0
129.80	443.0
131.00	123.0
134.80	258.0
136.80	182.0
140.90	1442.0
141.80	153.0
142.90	1690.0
144.90	387.0
147.80	258.0
152.80	106.0
154.90	299.0
156.80	122.0
158.80	135.0
160.80	103.0
170.90	169.0
171.90	1253.0
172.90	1340.0
173.90	96408.0
174.90	6990.0
175.90	92168.0
176.90	5669.0
177.90	226.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156

m/z	Abundance
35.90	955.0
36.90	5974.0
37.90	5140.0
39.00	2294.0
39.80	207.0
43.90	723.0
44.90	1097.0
47.00	1405.0
47.90	814.0
48.90	5055.0
49.90	23296.0
50.90	7290.0
52.00	394.0
52.90	214.0
54.90	319.0
55.90	2114.0
56.90	3606.0
57.80	184.0
59.90	1172.0
60.90	6167.0
62.00	6383.0
63.00	4996.0
64.00	817.0
65.00	1099.0
67.00	360.0
67.90	12842.0
69.00	13401.0
69.90	1153.0
71.90	701.0
72.90	5821.0
74.00	20936.0
75.00	62560.0
75.90	5684.0
76.90	847.0
77.90	498.0
78.90	4538.0
79.90	1374.0
80.90	4826.0
81.80	1205.0
83.00	126.0
86.10	260.0
86.90	5926.0
87.90	5005.0
90.80	487.0
91.90	3473.0
92.90	5311.0
94.00	14341.0
95.00	119352.0
96.00	8330.0
96.90	199.0
103.80	625.0
104.80	267.0
105.90	641.0
109.70	105.0
110.80	131.0
112.80	127.0
114.80	225.0
115.70	345.0
116.80	745.0
117.90	486.0
118.80	778.0
127.80	381.0
128.90	223.0
129.80	412.0
131.00	159.0
134.80	301.0
136.70	208.0
140.90	1461.0
141.80	175.0
142.90	1622.0
143.70	121.0
144.80	389.0
145.70	146.0
147.80	242.0
152.80	130.0
154.80	260.0
156.80	172.0
158.80	154.0
170.90	231.0
171.90	1346.0
173.00	1284.0
173.90	96384.0
174.90	6980.0
175.90	92752.0
176.90	5852.0
177.90	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB156