


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU051920\
 Data File : VU038225.D
 Acq On : 19 May 2020 10:12
 Operator : JC/MD
 Sample : BFB26
 Misc : 25.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB26

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMUTR050720WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Wed May 20 01:25:15 2020

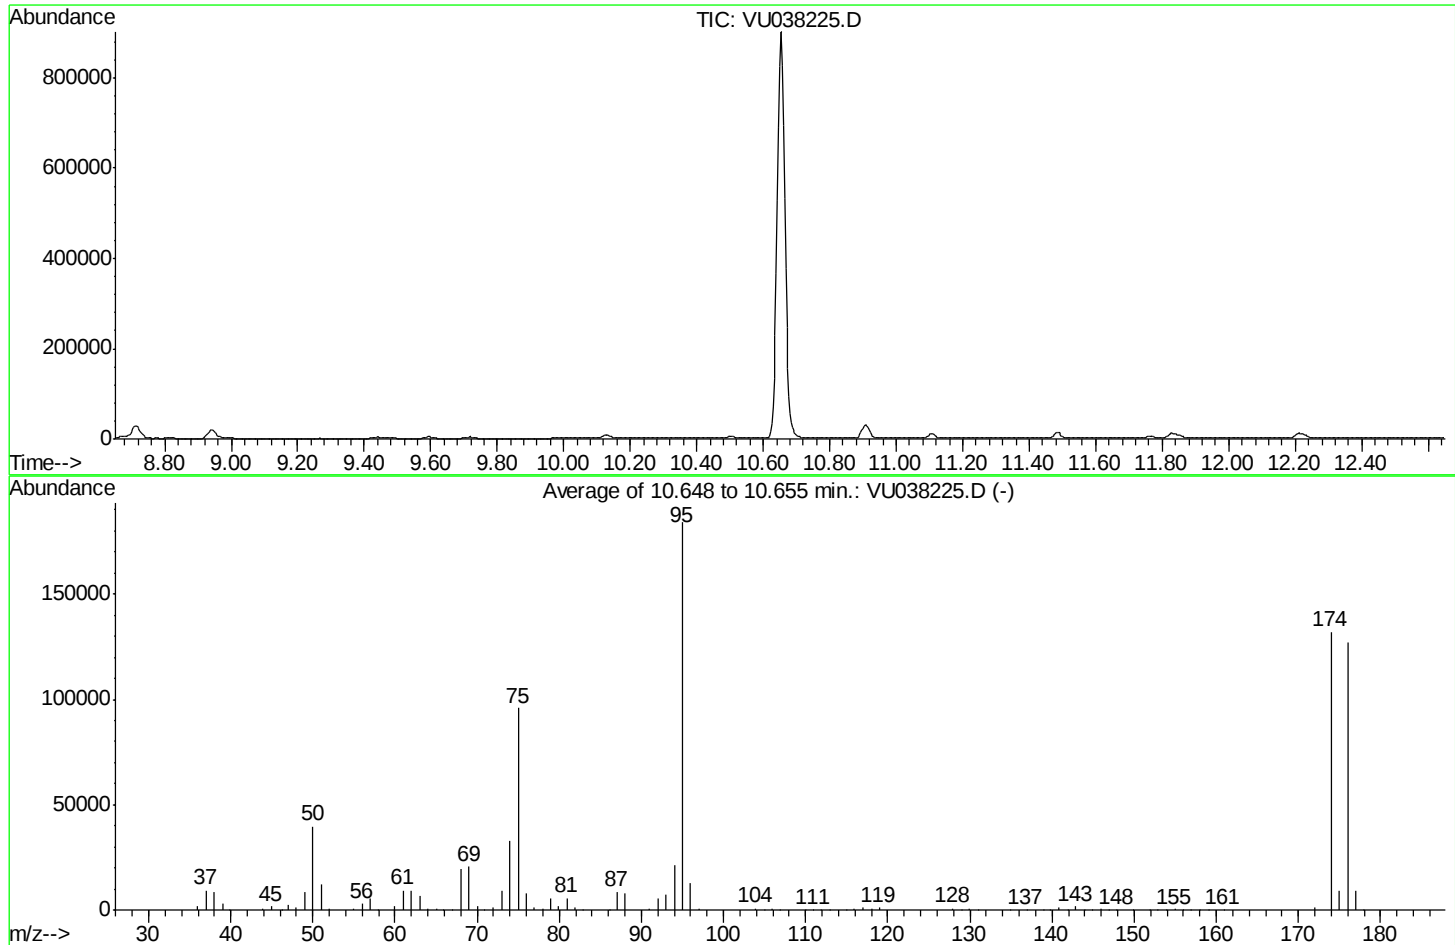

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2882

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	39634	PASS
75	95	30	80	52.2	96002	PASS
95	95	100	100	100.0	184085	PASS
96	95	5	9	6.8	12525	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	71.8	132192	PASS
175	174	5	9	7.1	9359	PASS
176	174	95	101	96.1	127085	PASS
177	176	5	9	7.0	8885	PASS

m/z	Abundance
36.00	2320.0
37.00	9037.0
38.00	8403.0
39.00	3081.0
40.00	405.0
44.00	1955.0
44.90	1491.0
46.20	257.0
47.00	2184.0
48.00	971.0
49.00	7826.0
50.00	37440.0
51.00	11232.0
52.00	459.0
55.00	426.0
56.00	2890.0
57.00	5102.0
57.90	219.0
60.00	1898.0
61.00	8888.0
62.00	8511.0
63.00	6517.0
64.00	799.0
65.00	756.0
65.90	104.0
66.90	459.0
68.00	18240.0
69.00	19456.0
70.00	1581.0
72.00	1021.0
73.00	8441.0
74.00	31712.0
75.00	90696.0
76.00	7926.0
76.90	985.0
78.00	849.0
78.90	4918.0
80.00	1725.0
80.90	5054.0
81.90	1010.0
82.80	124.0
86.00	306.0
87.00	7915.0
88.00	7822.0
90.90	558.0
92.00	5116.0
93.00	6750.0
94.00	20672.0
95.00	176256.0
96.00	11853.0
97.00	382.0
103.90	758.0
104.90	225.0
105.90	609.0
106.80	168.0
109.90	160.0
110.90	203.0
111.90	100.0
112.90	157.0
114.90	215.0
115.90	611.0
116.90	839.0
118.00	596.0
119.00	878.0
127.90	518.0
128.90	230.0
129.90	486.0
131.00	246.0
134.90	140.0
136.90	264.0
139.80	113.0
140.90	1357.0
141.90	208.0
142.90	1685.0
144.00	101.0
144.90	251.0
146.00	223.0
146.90	133.0
147.80	265.0
149.90	168.0
151.90	103.0
153.90	160.0
154.90	297.0
156.80	182.0
159.00	125.0
160.90	225.0
172.00	1013.0
174.00	122208.0
175.00	8773.0
176.00	115864.0
177.00	8521.0
177.90	196.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	2366.0
37.00	9580.0
38.00	8795.0
39.00	3380.0
40.00	373.0
43.90	1919.0
44.90	1650.0
46.20	294.0
47.00	2349.0
47.90	1086.0
49.00	8828.0
50.00	41192.0
51.00	12266.0
52.00	521.0
55.00	389.0
56.00	2955.0
57.00	5699.0
57.90	279.0
60.00	1907.0
61.00	9543.0
62.00	9136.0
63.00	7078.0
64.00	728.0
65.00	788.0
66.90	467.0
68.00	20168.0
69.00	21176.0
70.00	1724.0
72.00	1081.0
73.00	9168.0
74.00	34128.0
75.00	98832.0
76.00	8390.0
76.90	1200.0
78.00	806.0
78.90	5325.0
79.90	1997.0
80.90	5664.0
81.90	1347.0
82.80	139.0
86.10	326.0
87.00	8850.0
88.00	8118.0
90.90	617.0
92.00	5711.0
93.00	7109.0
94.00	22000.0
95.00	189248.0
96.00	13044.0
97.00	364.0
103.90	891.0
104.90	215.0
105.90	685.0
106.90	212.0
109.90	111.0
111.00	209.0
111.90	111.0
112.90	186.0
114.90	256.0
115.90	583.0
116.90	988.0
118.00	660.0
119.00	1024.0
128.00	672.0
128.90	273.0
129.90	623.0
130.90	286.0
134.90	131.0
136.90	266.0
139.00	100.0
139.80	114.0
140.90	1544.0
142.00	172.0
142.90	1808.0
144.00	102.0
144.90	271.0
146.00	346.0
146.90	124.0
147.90	250.0
149.90	184.0
152.90	106.0
153.90	205.0
155.00	385.0
155.90	127.0
156.80	221.0
157.90	102.0
160.90	261.0
172.00	1195.0
174.00	135744.0
175.00	9641.0
176.00	130736.0
177.00	9122.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

177.90

277.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

m/z	Abundance
36.00	2122.0
37.00	9472.0
38.00	8603.0
39.00	3280.0
39.90	325.0
43.90	1766.0
45.00	1689.0
46.20	288.0
47.00	2172.0
47.90	1112.0
49.00	8794.0
50.00	40272.0
51.00	12223.0
52.00	522.0
55.00	376.0
56.00	2826.0
57.00	5768.0
58.00	286.0
60.00	1828.0
61.00	9384.0
62.00	9146.0
63.00	7104.0
64.00	676.0
65.00	874.0
68.00	20640.0
69.00	21160.0
70.00	1791.0
70.90	102.0
72.00	1031.0
73.00	9071.0
74.00	33432.0
75.00	98480.0
76.00	8248.0
76.90	1291.0
77.90	736.0
78.90	5374.0
79.90	2007.0
80.90	5831.0
81.90	1540.0
82.90	126.0
86.20	335.0
87.00	8847.0
87.90	7758.0
90.90	626.0
92.00	5772.0
93.00	7246.0
94.00	21736.0
95.00	186752.0
96.00	12678.0
97.00	380.0
103.90	873.0
104.90	215.0
105.90	653.0
107.00	216.0
111.00	212.0
112.90	164.0
115.00	251.0
115.90	529.0
116.90	1088.0
118.00	674.0
119.00	1035.0
128.00	712.0
128.90	233.0
129.90	647.0
130.90	317.0
135.00	150.0
136.90	247.0
138.90	113.0
140.90	1596.0
142.00	130.0
142.90	1641.0
144.90	241.0
146.00	419.0
146.80	102.0
148.00	279.0
149.90	135.0
152.90	142.0
153.90	205.0
155.00	419.0
155.90	121.0
156.80	279.0
160.90	283.0
172.00	1194.0
174.00	138624.0
175.00	9664.0
176.00	134656.0
177.00	9012.0
177.90	301.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26

Scan 2882 (10.607 min): VU038225.D
BFB26

m/z	Abundance
35.80	641.0
37.90	220.0
39.80	245.0
41.20	140.0
43.90	1082.0

Instrument :
MSVOA_U
ClientSampleId :
BFB26