

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052124\
 Data File : VU058929.D
 Acq On : 21 May 2024 14:07
 Operator : MD/SY
 Sample : VU0521WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 22 07:08:48 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052124.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Wed May 22 07:04:21 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.258	114	6375	0.500	ug/L	0.00
5) Chlorobenzene-d5	9.418	117	10038	0.500	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.808	152	3430	0.500	ug/L	0.00
System Monitoring Compounds						
2) Vinyl Chloride-d3	1.597	65	2746	0.510	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.000%
4) 1,2-Dichloroethane-d4	5.709	65	3138	0.498	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	100.000%
7) 1,2-Dichloropropane-d6	6.687	67	3861	0.527	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.000%
8) Toluene-d8	7.887	98	7064	0.493	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.000%
10) 1,1,2,2-Tetrachloroeth...	10.745	84	3604	0.519	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	104.000%
Target Compounds						
12) 1,2,3-Trichloropropane	10.814	75	89	0.019	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052124\
Data File : VU058929.D
Acq On : 21 May 2024 14:07
Operator : MD/SY
Sample : VU0521WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 22 07:08:48 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052124.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Wed May 22 07:04:21 2024
Response via : Initial Calibration

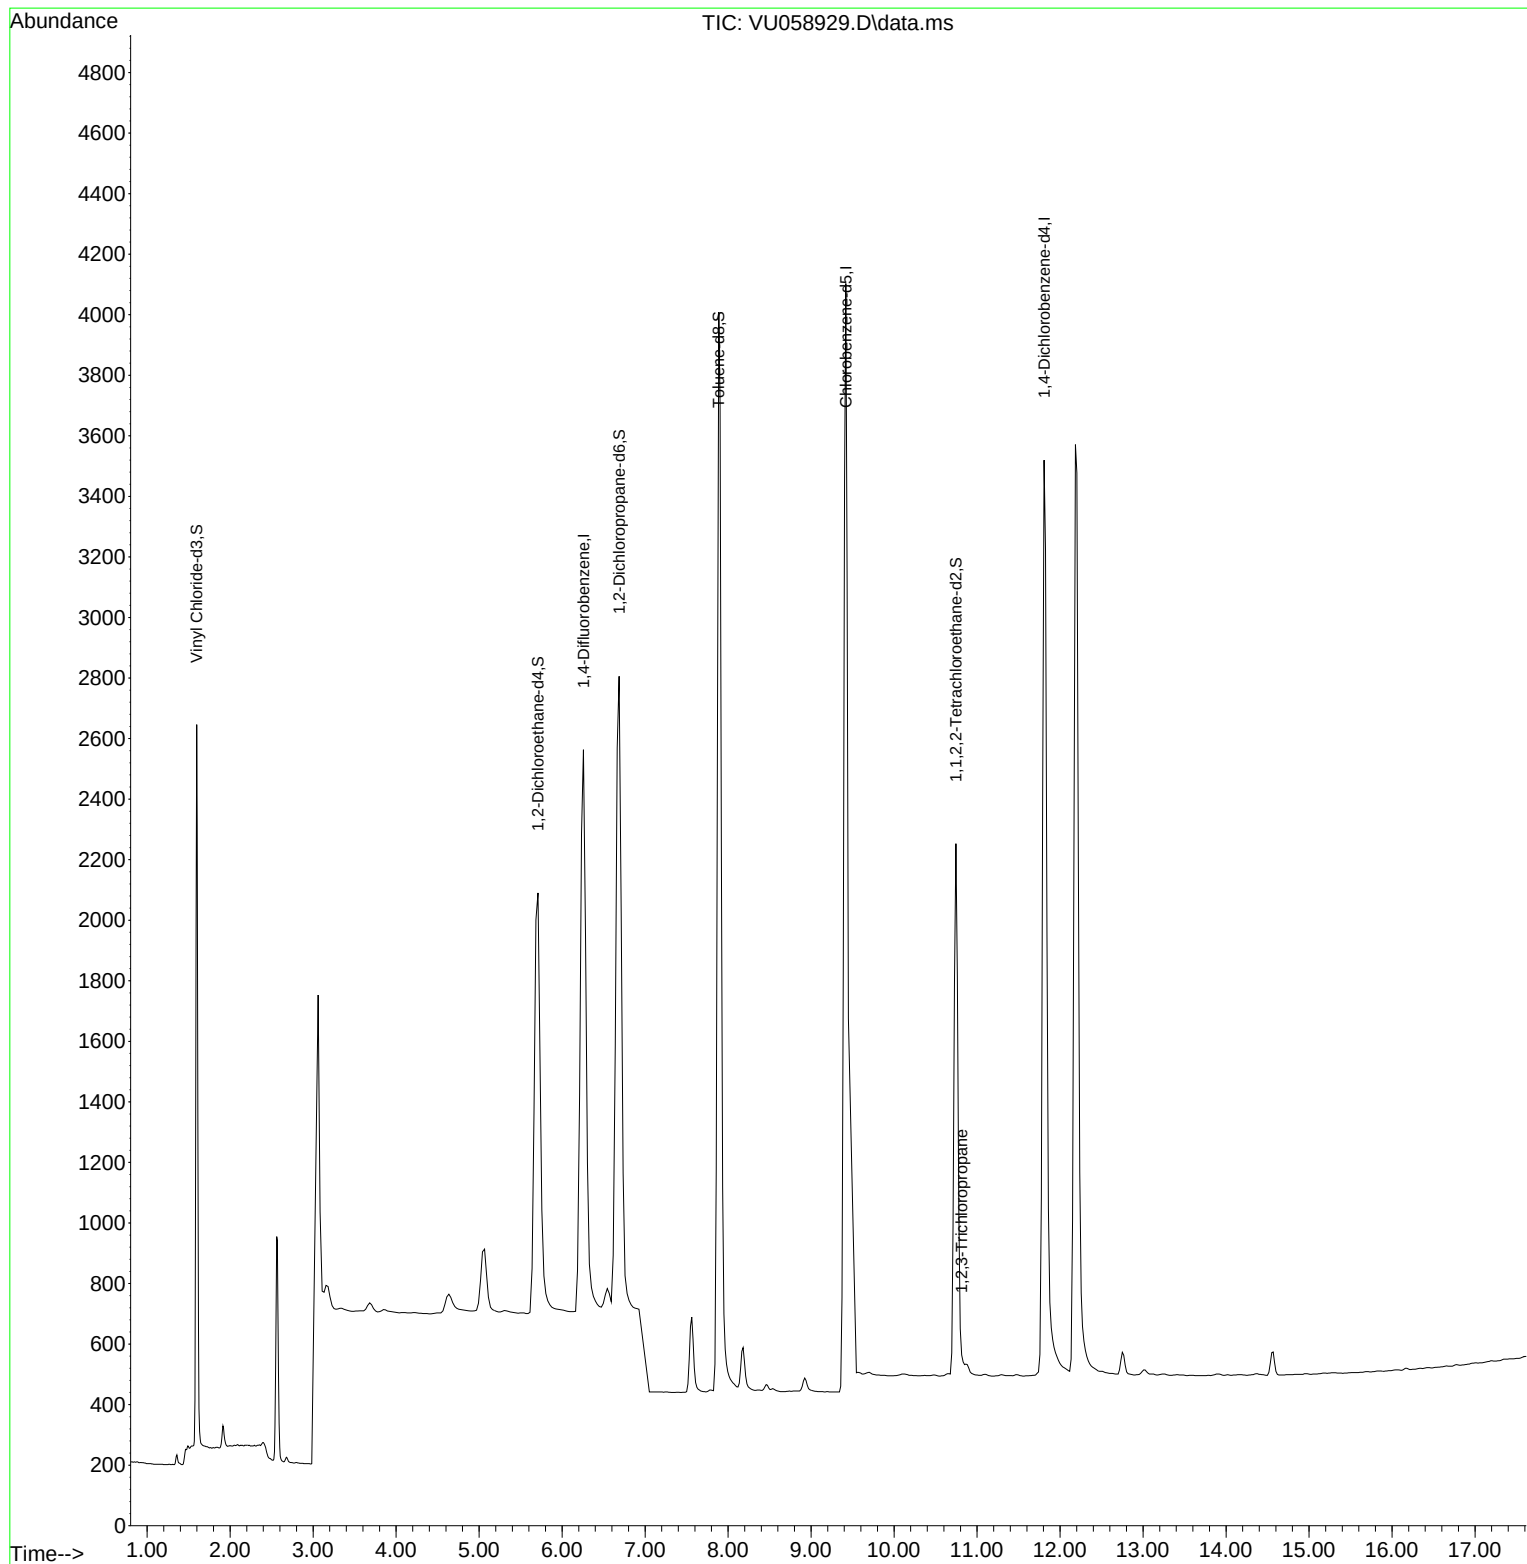

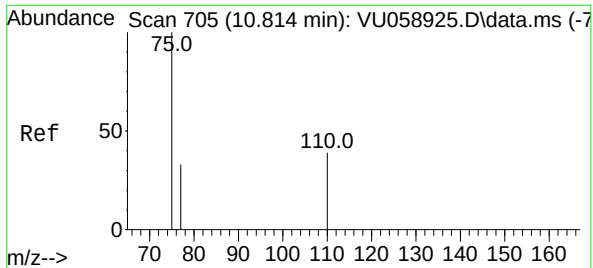

#12
 1,2,3-Trichloropropane
 Concen: 0.019 ug/L
 RT: 10.814 min Scan# 70
 Delta R.T. -0.000 min
 Lab File: VU058929.D
 Acq: 21 May 2024 14:07

Instrument :
 MSVOA_U
 ClientSampleId :

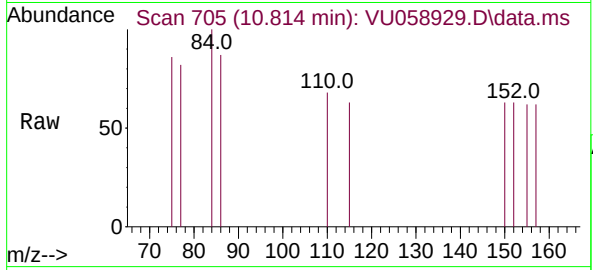

Tgt Ion: 75	Resp:	89
Ion	Ratio	Lower Upper
75	100	
110	34.8	30.1 45.1
77	37.1	26.3 39.5

