


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052124\
Data File : VU058920.D
Acq On : 21 May 2024 08:04
Operator : MD/SY
Sample : BFB007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB007

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052124.M
Title : TRACE VOA SOM01.0
Last Update : Wed May 22 07:04:21 2024

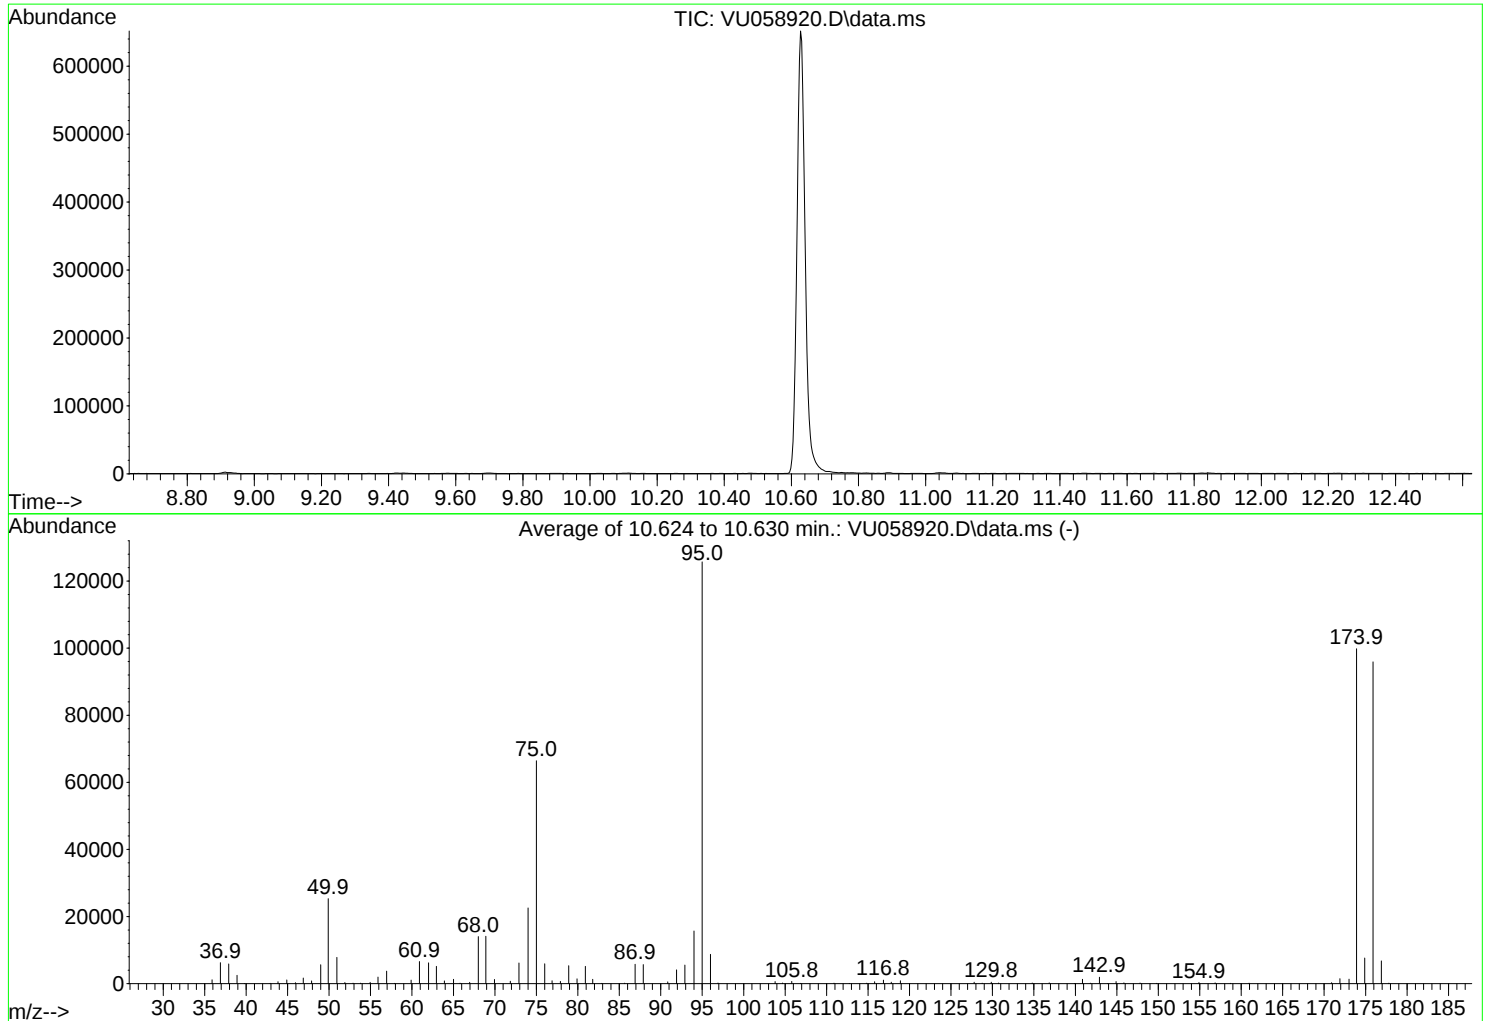

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	25349	PASS
75	95	30	80	52.9	66456	PASS
95	95	100	100	100.0	125731	PASS
96	95	5	9	6.9	8719	PASS
173	174	0.00	2	1.3	1341	PASS
174	95	50	120	79.4	99832	PASS
175	174	5	9	7.7	7660	PASS
176	174	95	101	96.1	95923	PASS
177	176	5	9	7.1	6766	PASS

m/z	Abundance
39.80	330.0
43.80	405.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	1108.0
36.90	6146.0
37.90	5939.0
38.90	2323.0
39.80	433.0
43.90	1068.0
44.90	1048.0
45.90	322.0
46.90	1529.0
47.90	858.0
49.00	5482.0
49.90	24080.0
50.90	7745.0
51.90	421.0
52.90	135.0
53.80	127.0
55.00	412.0
55.90	1827.0
56.90	3745.0
59.90	1097.0
60.90	6326.0
62.00	6221.0
62.90	5069.0
63.90	883.0
65.00	1185.0
65.80	180.0
67.00	430.0
68.00	13459.0
68.90	13851.0
70.00	1174.0
71.90	724.0
72.90	6356.0
74.00	21512.0
75.00	64208.0
76.00	5673.0
76.90	891.0
77.90	630.0
78.90	5305.0
79.90	1319.0
80.90	5013.0
81.80	1227.0
85.70	158.0
86.90	5606.0
87.90	5460.0
90.90	504.0
91.90	3963.0
92.90	5314.0
94.00	15333.0
95.00	121840.0
96.00	8312.0
96.90	153.0
103.80	685.0
104.70	216.0
105.80	610.0
106.80	115.0
110.90	148.0
112.70	109.0
114.80	143.0
115.80	525.0
116.90	1000.0
117.80	388.0
118.90	786.0
127.80	427.0
128.70	123.0
129.90	418.0
130.80	222.0
134.80	169.0
136.90	228.0
140.90	1100.0
141.80	129.0
142.90	1742.0
144.90	583.0
145.80	219.0
147.80	263.0
149.80	115.0
154.90	301.0
156.90	239.0
158.70	129.0
161.00	186.0
170.90	228.0
171.90	1361.0
173.00	1225.0
173.90	94952.0
174.90	7278.0
175.90	90440.0
176.90	6601.0
177.80	151.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	1159.0
36.90	6427.0
37.90	6079.0
38.90	2569.0
39.80	377.0
42.90	114.0
43.90	941.0
44.90	1156.0
46.00	313.0
46.90	1769.0
47.90	862.0
49.00	5837.0
49.90	26072.0
50.90	8029.0
51.90	348.0
52.90	145.0
53.80	161.0
54.90	372.0
55.90	2008.0
57.00	3788.0
57.90	137.0
59.90	1075.0
60.90	6800.0
62.00	6347.0
62.90	5257.0
63.90	850.0
65.00	1329.0
65.80	142.0
67.00	397.0
68.00	14575.0
68.90	14539.0
69.90	1297.0
71.90	719.0
72.90	6397.0
74.00	23392.0
75.00	68624.0
76.00	6188.0
76.90	877.0
77.90	704.0
78.90	5495.0
79.90	1487.0
80.90	5359.0
81.80	1372.0
82.90	127.0
85.70	162.0
86.90	5980.0
87.90	5850.0
90.90	551.0
91.90	4255.0
92.90	5691.0
94.00	16139.0
95.00	129336.0
96.00	9048.0
96.90	184.0
103.80	612.0
104.70	233.0
105.80	671.0
106.80	133.0
110.90	164.0
112.80	123.0
114.90	145.0
115.80	576.0
116.80	1095.0
117.80	486.0
118.90	887.0
127.80	444.0
128.80	166.0
129.80	439.0
130.80	214.0
134.80	206.0
136.90	220.0
139.90	120.0
140.90	1357.0
141.80	140.0
142.90	2016.0
143.90	105.0
144.90	626.0
145.80	241.0
147.80	208.0
149.80	123.0
154.90	333.0
156.80	251.0
158.70	130.0
161.00	173.0
170.90	285.0
171.90	1531.0
173.00	1361.0
173.90	102880.0
174.90	7920.0
175.90	98728.0
176.90	7079.0
177.80	158.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007

m/z	Abundance
35.90	1128.0
36.90	6144.0
37.90	5593.0
38.90	2568.0
39.80	330.0
42.90	146.0
43.90	899.0
44.90	1085.0
46.00	292.0
46.90	1757.0
47.90	785.0
49.00	5615.0
49.90	25896.0
51.00	7657.0
51.90	275.0
52.90	187.0
53.80	143.0
54.90	366.0
55.90	1993.0
57.00	3660.0
57.90	169.0
59.90	1062.0
60.90	6554.0
62.00	6069.0
63.00	5197.0
63.90	772.0
65.00	1321.0
65.90	105.0
66.90	306.0
68.00	14014.0
68.90	14037.0
69.90	1284.0
71.80	692.0
72.90	5776.0
74.00	22736.0
75.00	66536.0
76.00	5856.0
76.90	875.0
77.90	674.0
78.90	5184.0
79.90	1511.0
80.90	5170.0
81.80	1346.0
82.90	166.0
85.60	161.0
86.90	5750.0
87.90	5793.0
90.80	558.0
91.90	4081.0
92.90	5649.0
94.00	15550.0
95.00	126016.0
96.00	8796.0
96.90	218.0
103.80	551.0
104.70	201.0
105.80	688.0
106.90	113.0
110.90	149.0
114.90	124.0
115.80	586.0
116.90	1076.0
117.80	454.0
118.90	870.0
127.80	390.0
128.80	202.0
129.80	444.0
130.70	163.0
134.80	224.0
136.80	223.0
139.90	102.0
140.80	1478.0
141.80	126.0
142.90	2011.0
143.90	115.0
144.90	631.0
145.90	215.0
147.80	177.0
149.80	128.0
154.90	342.0
156.80	247.0
158.70	114.0
160.80	142.0
170.90	298.0
171.90	1535.0
173.00	1437.0
173.90	101664.0
174.90	7781.0
175.90	98600.0
176.90	6619.0
177.80	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB007