


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052224\
Data File : VU058932.D
Acq On : 22 May 2024 08:28
Operator : MD/SY
Sample : BFB008
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB008

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM052124.M
Title : TRACE VOA SOM01.0
Last Update : Wed May 22 07:04:21 2024

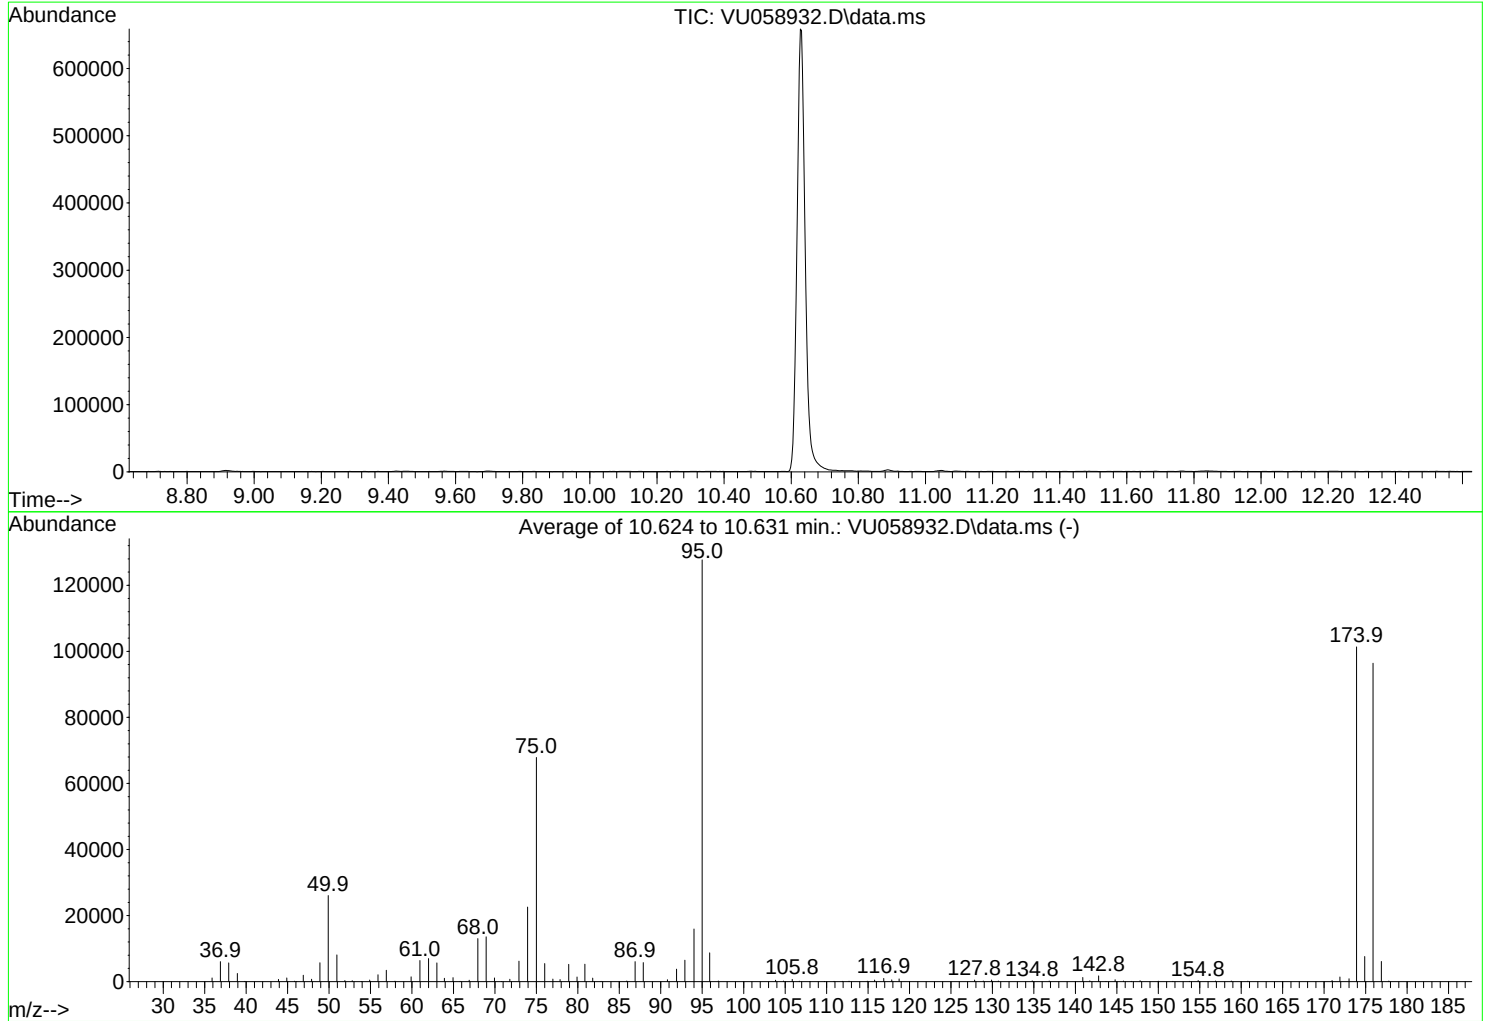

AutoFind: Scans 2903, 2904, 2905; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	26064	PASS
75	95	30	80	53.1	67856	PASS
95	95	100	100	100.0	127696	PASS
96	95	5	9	6.8	8744	PASS
173	174	0.00	2	0.8	861	PASS
174	95	50	120	79.4	101328	PASS
175	174	5	9	7.5	7605	PASS
176	174	95	101	95.2	96419	PASS
177	176	5	9	6.4	6124	PASS

m/z	Abundance
39.80	253.0
43.90	356.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1189.0
36.90	5931.0
37.90	5577.0
39.00	2325.0
39.90	403.0
43.90	1038.0
44.90	1121.0
45.80	172.0
46.10	168.0
46.90	1780.0
47.90	708.0
48.90	4981.0
49.90	24656.0
50.90	7761.0
51.90	278.0
52.80	341.0
54.90	512.0
55.90	1939.0
56.90	3117.0
57.90	133.0
59.90	1382.0
61.00	5878.0
62.00	6817.0
63.00	5109.0
63.90	1036.0
65.00	1136.0
66.90	352.0
67.90	12498.0
69.00	12747.0
70.00	1069.0
70.80	117.0
71.80	667.0
72.90	5877.0
74.00	21160.0
75.00	64520.0
76.00	5419.0
77.00	694.0
77.90	667.0
78.90	5078.0
79.90	1373.0
80.90	5009.0
81.80	1119.0
82.80	199.0
86.00	144.0
86.90	5730.0
87.90	5423.0
90.80	628.0
91.90	3513.0
92.90	5998.0
94.00	14987.0
95.00	121312.0
95.90	8317.0
96.90	181.0
103.90	340.0
104.80	223.0
105.80	554.0
106.70	148.0
111.80	118.0
112.70	121.0
114.90	179.0
115.80	479.0
116.90	936.0
117.90	548.0
118.70	859.0
127.90	497.0
128.90	176.0
129.90	484.0
130.70	162.0
134.80	218.0
136.80	160.0
140.90	1165.0
141.80	243.0
142.80	1674.0
143.70	108.0
144.80	554.0
145.80	185.0
146.80	108.0
147.80	203.0
150.00	158.0
151.80	113.0
153.80	144.0
154.80	348.0
156.90	193.0
158.80	166.0
160.90	142.0
171.00	321.0
171.90	1264.0
173.00	1229.0
173.90	93216.0
174.90	7279.0
175.90	88392.0
176.90	5699.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

177.80

148.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1180.0
36.90	6191.0
37.90	5844.0
39.00	2586.0
39.90	383.0
43.90	1069.0
44.90	1138.0
45.80	185.0
46.90	1997.0
47.90	744.0
48.90	5903.0
49.90	27080.0
51.00	8345.0
51.90	330.0
52.80	288.0
54.90	533.0
55.90	2162.0
56.90	3534.0
57.90	125.0
59.90	1476.0
60.90	6568.0
62.00	7152.0
63.00	5871.0
63.90	1034.0
64.90	1237.0
65.80	154.0
66.90	457.0
67.90	13388.0
69.00	13909.0
69.90	1172.0
71.80	763.0
72.90	6421.0
74.00	23184.0
75.00	69944.0
76.00	5624.0
77.00	813.0
77.90	643.0
78.90	5427.0
79.90	1484.0
80.90	5491.0
81.80	1140.0
82.80	149.0
85.90	193.0
86.90	6276.0
87.90	5997.0
90.80	620.0
91.90	3865.0
92.90	6831.0
94.00	16382.0
95.00	131584.0
95.90	8978.0
97.00	226.0
103.80	444.0
104.80	195.0
105.90	718.0
106.70	146.0
108.00	104.0
109.70	102.0
110.90	109.0
111.90	128.0
112.70	154.0
114.90	165.0
115.80	508.0
116.90	1005.0
117.90	559.0
118.80	842.0
127.80	534.0
128.90	213.0
129.90	479.0
130.70	195.0
134.80	266.0
136.90	196.0
140.90	1312.0
141.80	226.0
142.80	1795.0
144.80	568.0
145.80	222.0
146.70	118.0
147.80	301.0
150.00	148.0
151.70	133.0
153.70	118.0
154.80	349.0
156.90	222.0
158.80	193.0
160.80	152.0
170.90	338.0
171.90	1441.0
173.00	1354.0
173.90	104416.0
174.90	7943.0
175.90	99680.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

176.906326.0

177.80207.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008

m/z	Abundance
35.90	1044.0
36.90	6064.0
37.90	5660.0
38.90	2558.0
39.90	345.0
43.90	1069.0
44.90	1061.0
45.90	151.0
46.90	2026.0
47.90	747.0
48.90	6217.0
49.90	26456.0
51.00	8149.0
51.90	394.0
52.90	187.0
53.90	106.0
54.90	442.0
55.90	2148.0
56.90	3723.0
58.00	133.0
59.90	1486.0
60.90	6734.0
62.00	7020.0
63.00	6005.0
63.90	937.0
64.90	1221.0
65.80	175.0
66.90	445.0
68.00	13178.0
68.90	14097.0
69.90	1188.0
71.80	764.0
72.90	6349.0
73.90	23368.0
75.00	69104.0
76.00	5457.0
77.00	846.0
77.80	625.0
78.90	5279.0
79.90	1419.0
80.80	5419.0
81.80	1010.0
85.80	257.0
86.90	6213.0
87.90	5851.0
90.80	534.0
91.90	3916.0
92.90	6696.0
94.00	16488.0
95.00	130192.0
95.90	8936.0
97.00	239.0
103.80	518.0
104.80	170.0
105.90	790.0
106.70	132.0
108.00	117.0
109.80	116.0
110.90	158.0
112.00	107.0
112.70	158.0
114.90	142.0
115.80	499.0
116.90	1051.0
117.80	480.0
118.80	792.0
127.80	493.0
128.90	232.0
129.90	475.0
130.70	201.0
134.80	284.0
136.90	194.0
140.90	1298.0
141.70	212.0
142.80	1761.0
144.80	587.0
145.80	189.0
146.70	128.0
147.80	324.0
150.00	128.0
151.70	118.0
154.80	330.0
156.90	252.0
158.80	220.0
160.70	130.0
170.90	317.0
171.90	1499.0
173.90	106352.0
174.90	7593.0
175.90	101184.0
176.90	6348.0
177.80	230.0

Instrument :
MSVOA_U
ClientSampleId :
BFB008