


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052324\
Data File : VU058937.D
Acq On : 22 May 2024 11:19
Operator : MD/SY
Sample : BFB157
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB157

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR051424WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu May 23 06:11:29 2024

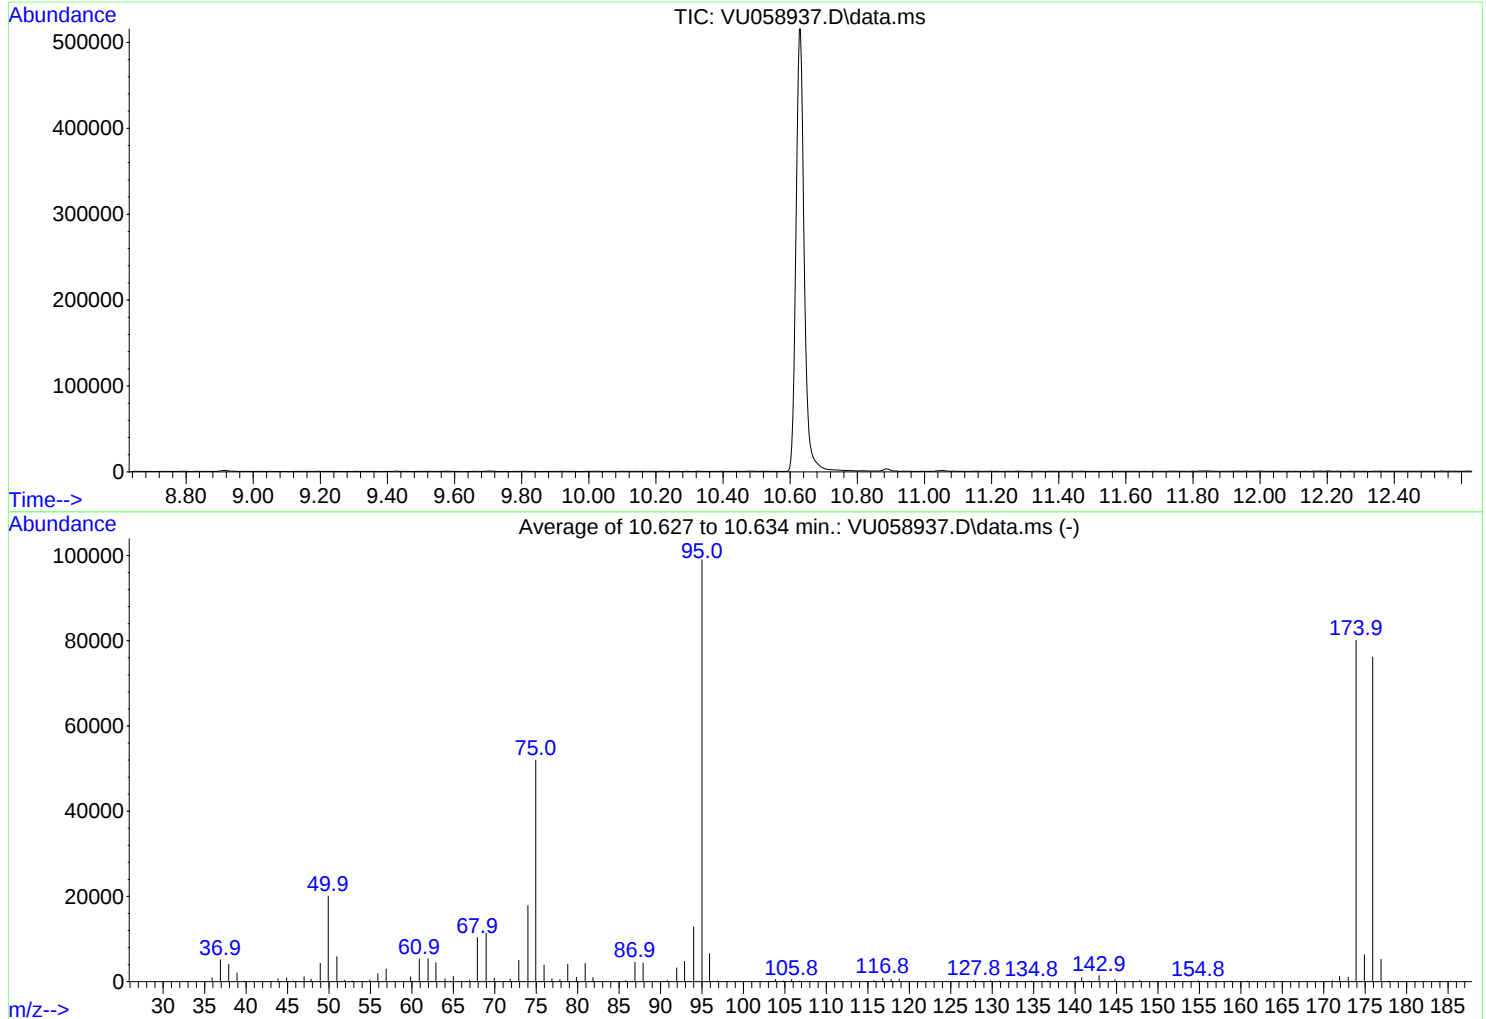

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2890

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.3	20072	PASS
75	95	30	80	52.5	51968	PASS
95	95	100	100	100.0	98989	PASS
96	95	5	9	6.6	6565	PASS
173	174	0.00	2	1.3	1070	PASS
174	95	50	120	80.9	80096	PASS
175	174	5	9	7.9	6306	PASS
176	174	95	101	95.1	76152	PASS
177	176	5	9	6.9	5242	PASS

m/z	Abundance
39.80	272.0
43.80	386.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	993.0
36.90	5475.0
37.90	4127.0
38.90	2109.0
39.80	358.0
43.90	1131.0
44.90	956.0
45.70	202.0
47.00	1090.0
47.80	696.0
49.00	4662.0
49.90	21288.0
51.00	6254.0
51.90	341.0
52.80	153.0
54.90	325.0
55.90	1743.0
56.90	3074.0
57.90	139.0
59.90	1238.0
60.90	5543.0
61.90	5519.0
62.90	4758.0
64.00	693.0
65.00	1275.0
66.00	131.0
67.00	290.0
67.90	10613.0
69.00	11907.0
70.00	979.0
71.90	619.0
72.90	5267.0
74.00	19016.0
75.00	54128.0
76.00	4039.0
76.90	781.0
77.80	537.0
78.80	4126.0
79.80	1005.0
80.90	4565.0
81.90	988.0
82.80	118.0
85.80	290.0
86.90	4690.0
87.90	4434.0
90.80	350.0
92.00	3441.0
92.90	4781.0
94.00	13108.0
95.00	101584.0
95.90	6994.0
96.90	209.0
103.90	493.0
104.80	179.0
105.80	584.0
106.80	124.0
114.80	130.0
115.70	291.0
116.80	837.0
117.80	570.0
118.80	608.0
127.80	342.0
128.70	132.0
129.80	295.0
130.90	128.0
134.80	170.0
136.80	191.0
140.80	1047.0
141.80	185.0
142.90	1453.0
143.80	103.0
144.80	555.0
145.90	151.0
147.80	289.0
154.80	228.0
156.80	109.0
158.80	124.0
160.80	143.0
171.10	220.0
171.90	1260.0
172.90	1140.0
173.90	80080.0
174.90	6730.0
175.90	77832.0
176.90	5493.0
177.90	212.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	898.0
36.90	5324.0
37.90	4185.0
38.90	2111.0
39.80	393.0
43.90	1159.0
44.90	947.0
45.80	168.0
47.00	1268.0
47.90	592.0
48.90	4393.0
49.90	20720.0
50.90	5920.0
51.90	361.0
52.80	215.0
54.90	391.0
55.90	1949.0
56.90	3031.0
57.90	122.0
59.90	1150.0
60.90	5373.0
61.90	5524.0
62.90	4609.0
64.00	729.0
65.00	1292.0
66.00	140.0
66.90	311.0
67.90	10625.0
69.00	11799.0
70.00	861.0
71.80	609.0
72.90	5140.0
74.00	18320.0
75.00	53248.0
75.90	3927.0
76.90	691.0
77.80	492.0
78.80	4139.0
79.90	1047.0
80.90	4423.0
81.90	990.0
85.80	274.0
86.90	4635.0
87.90	4484.0
90.80	337.0
92.00	3319.0
92.90	4842.0
94.00	13442.0
95.00	102312.0
95.90	6748.0
96.90	187.0
103.80	485.0
104.80	178.0
105.80	513.0
106.80	154.0
110.70	125.0
112.90	137.0
114.80	124.0
115.80	308.0
116.80	871.0
117.80	567.0
118.80	588.0
127.80	354.0
128.80	130.0
129.80	280.0
130.90	158.0
134.70	160.0
136.70	151.0
140.80	1014.0
141.80	146.0
142.90	1457.0
144.80	466.0
146.00	175.0
147.80	289.0
154.90	224.0
158.80	140.0
160.80	162.0
171.10	240.0
171.90	1255.0
172.90	1091.0
173.90	82728.0
174.90	6472.0
175.90	78608.0
176.90	5453.0
177.90	155.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157

m/z	Abundance
35.90	781.0
36.90	4622.0
37.90	3810.0
38.90	1892.0
39.80	398.0
43.90	1011.0
44.90	786.0
45.80	123.0
47.00	1181.0
47.80	479.0
48.90	3802.0
49.90	18208.0
50.90	5429.0
51.90	329.0
52.80	230.0
54.90	379.0
55.90	1955.0
56.90	2807.0
59.80	989.0
60.90	4949.0
62.00	5048.0
62.90	3949.0
64.00	647.0
65.00	1178.0
65.90	138.0
66.90	310.0
67.90	9866.0
68.90	10378.0
69.90	632.0
71.90	560.0
72.90	4595.0
74.00	16147.0
74.90	48528.0
75.90	3664.0
76.90	564.0
77.90	455.0
78.80	3913.0
79.90	948.0
80.90	3873.0
81.80	922.0
85.80	204.0
86.90	4338.0
87.90	4112.0
90.80	326.0
91.90	2902.0
92.90	4593.0
94.00	11972.0
95.00	93072.0
95.90	5954.0
96.90	152.0
103.80	437.0
104.80	172.0
105.80	428.0
106.80	135.0
110.70	159.0
112.90	147.0
115.00	115.0
115.80	326.0
116.80	829.0
117.80	481.0
118.80	511.0
127.80	279.0
128.80	130.0
129.80	269.0
130.90	147.0
134.80	163.0
136.70	133.0
140.80	905.0
141.70	113.0
142.90	1364.0
144.80	380.0
146.00	184.0
147.80	283.0
154.80	190.0
156.80	103.0
158.80	144.0
160.80	149.0
170.90	225.0
171.90	1159.0
173.00	978.0
173.90	77480.0
174.90	5715.0
175.90	72016.0
176.90	4781.0
177.80	135.0

Instrument :
MSVOA_U
ClientSampleId :
BFB157