

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058990.D
 Acq On : 25 May 2024 11:40
 Operator : MD/SY
 Sample : VU0525MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 27 04:11:27 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 04:10:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.238	114	130063	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	124949	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	54019	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	62815	45.664	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.320%
7) Chloroethane-d5	1.875	69	59136	51.727	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	103.460%
11) 1,1-Dichloroethene-d2	2.550	63	82547	39.277	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	78.560%
21) 2-Butanone-d5	4.611	46	103954	110.016	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	110.020%
24) Chloroform-d	5.052	84	117342	49.731	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.460%
26) 1,2-Dichloroethane-d4	5.689	65	79947	55.403	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	110.800%
32) Benzene-d6	5.717	84	237460	55.745	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	111.480%
36) 1,2-Dichloropropane-d6	6.679	67	82399	58.564	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	117.120%
41) Toluene-d8	7.891	98	193465	50.669	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.340%
43) trans-1,3-Dichloroprop...	8.174	79	32063	50.751	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	101.500%
47) 2-Hexanone-d5	8.627	63	64313	110.521	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	110.520%
56) 1,1,2,2-Tetrachloroeth...	10.749	84	122582	57.912	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	115.820%
66) 1,2-Dichlorobenzene-d4	12.187	152	64179	57.580	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	115.160%
Target Compounds						
37) 1,2-Dichloropropane	6.682	63	8712	7.136	ug/L	Qvalue # 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058990.D
Acq On : 25 May 2024 11:40
Operator : MD/SY
Sample : VU0525MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 27 04:11:27 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 04:10:55 2024
Response via : Initial Calibration

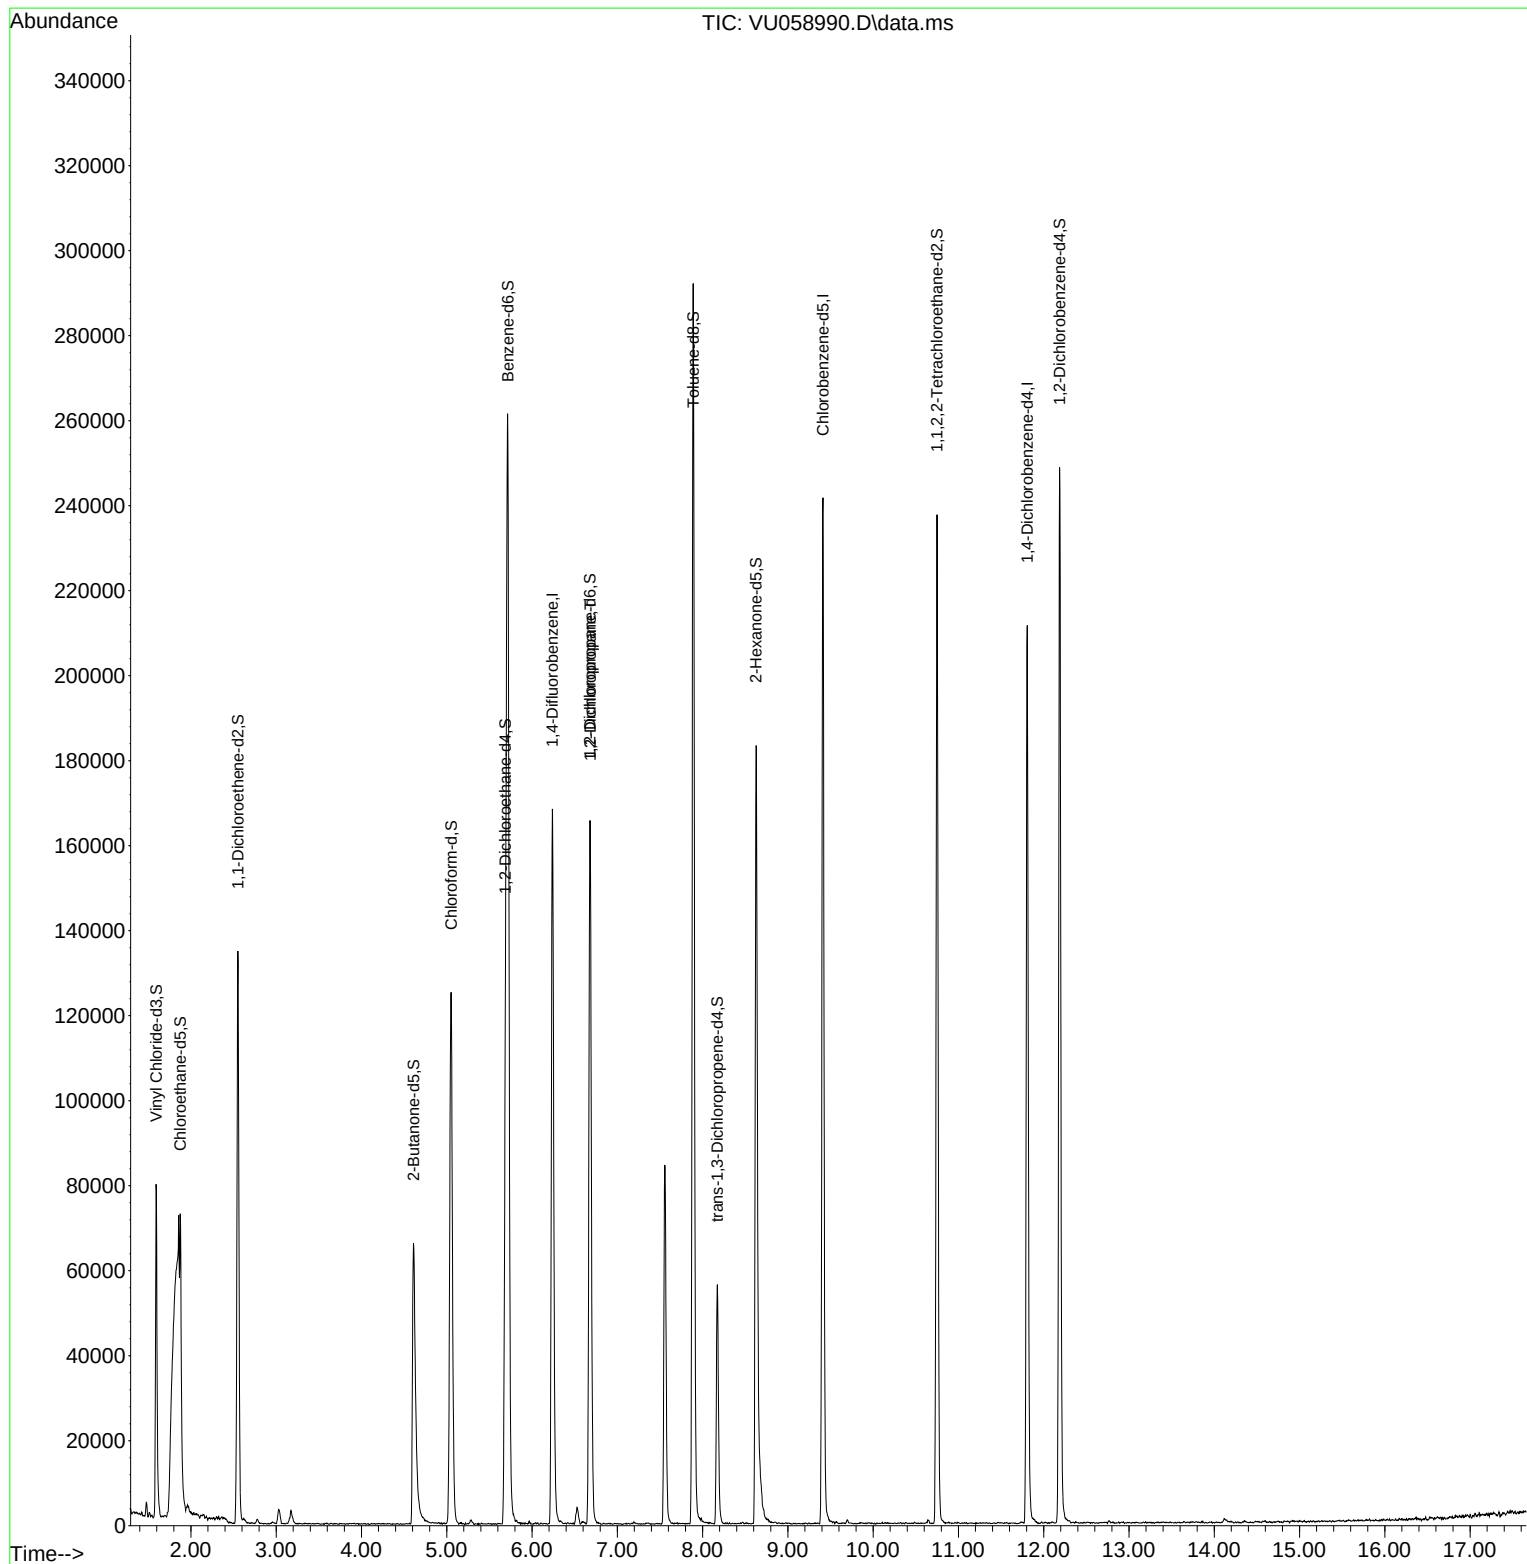

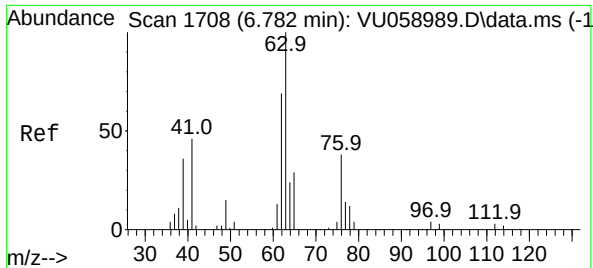

#37
 1,2-Dichloropropane
 Concen: 7.136 ug/L
 RT: 6.682 min Scan# 1
 Delta R.T. -0.100 min
 Lab File: VU058990.D
 Acq: 25 May 2024 11:40

Instrument :
 MSVOA_U
 ClientSampleId :

Tgt Ion: 63 Resp: 8712
 Ion Ratio Lower Upper
 63 100
 112 0.0 2.5 3.7#

