

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058991.D
 Acq On : 25 May 2024 12:05
 Operator : MD/SY
 Sample : VU0525WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 27 04:11:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 04:10:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.242	114	129706	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	127391	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.807	152	53870	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	60966	44.442	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 88.880%			
7) Chloroethane-d5	1.872	69	65765	57.684	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 115.360%			
11) 1,1-Dichloroethene-d2	2.551	63	81542	38.906	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 77.820%			
21) 2-Butanone-d5	4.612	46	114176	121.166	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 121.170%			
24) Chloroform-d	5.049	84	118465	50.346	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 100.700%			
26) 1,2-Dichloroethane-d4	5.692	65	78466	54.526	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 109.060%			
32) Benzene-d6	5.714	84	234146	53.913	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 107.820%			
36) 1,2-Dichloropropane-d6	6.682	67	80008	55.775	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 111.540%			
41) Toluene-d8	7.891	98	190898	49.038	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 98.080%			
43) trans-1,3-Dichloroprop...	8.174	79	32203	49.995	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 100.000%			
47) 2-Hexanone-d5	8.631	63	68461	115.394	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 115.390%			
56) 1,1,2,2-Tetrachloroeth...	10.750	84	124889	57.871	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 115.740%			
66) 1,2-Dichlorobenzene-d4	12.187	152	63598	57.216	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 114.440%			
Target Compounds						Qvalue
60) 1,2,3-Trichloropropane	11.807	75	7686	5.607	ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058991.D
Acq On : 25 May 2024 12:05
Operator : MD/SY
Sample : VU0525WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :


Quant Time: May 27 04:11:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 04:10:55 2024
Response via : Initial Calibration

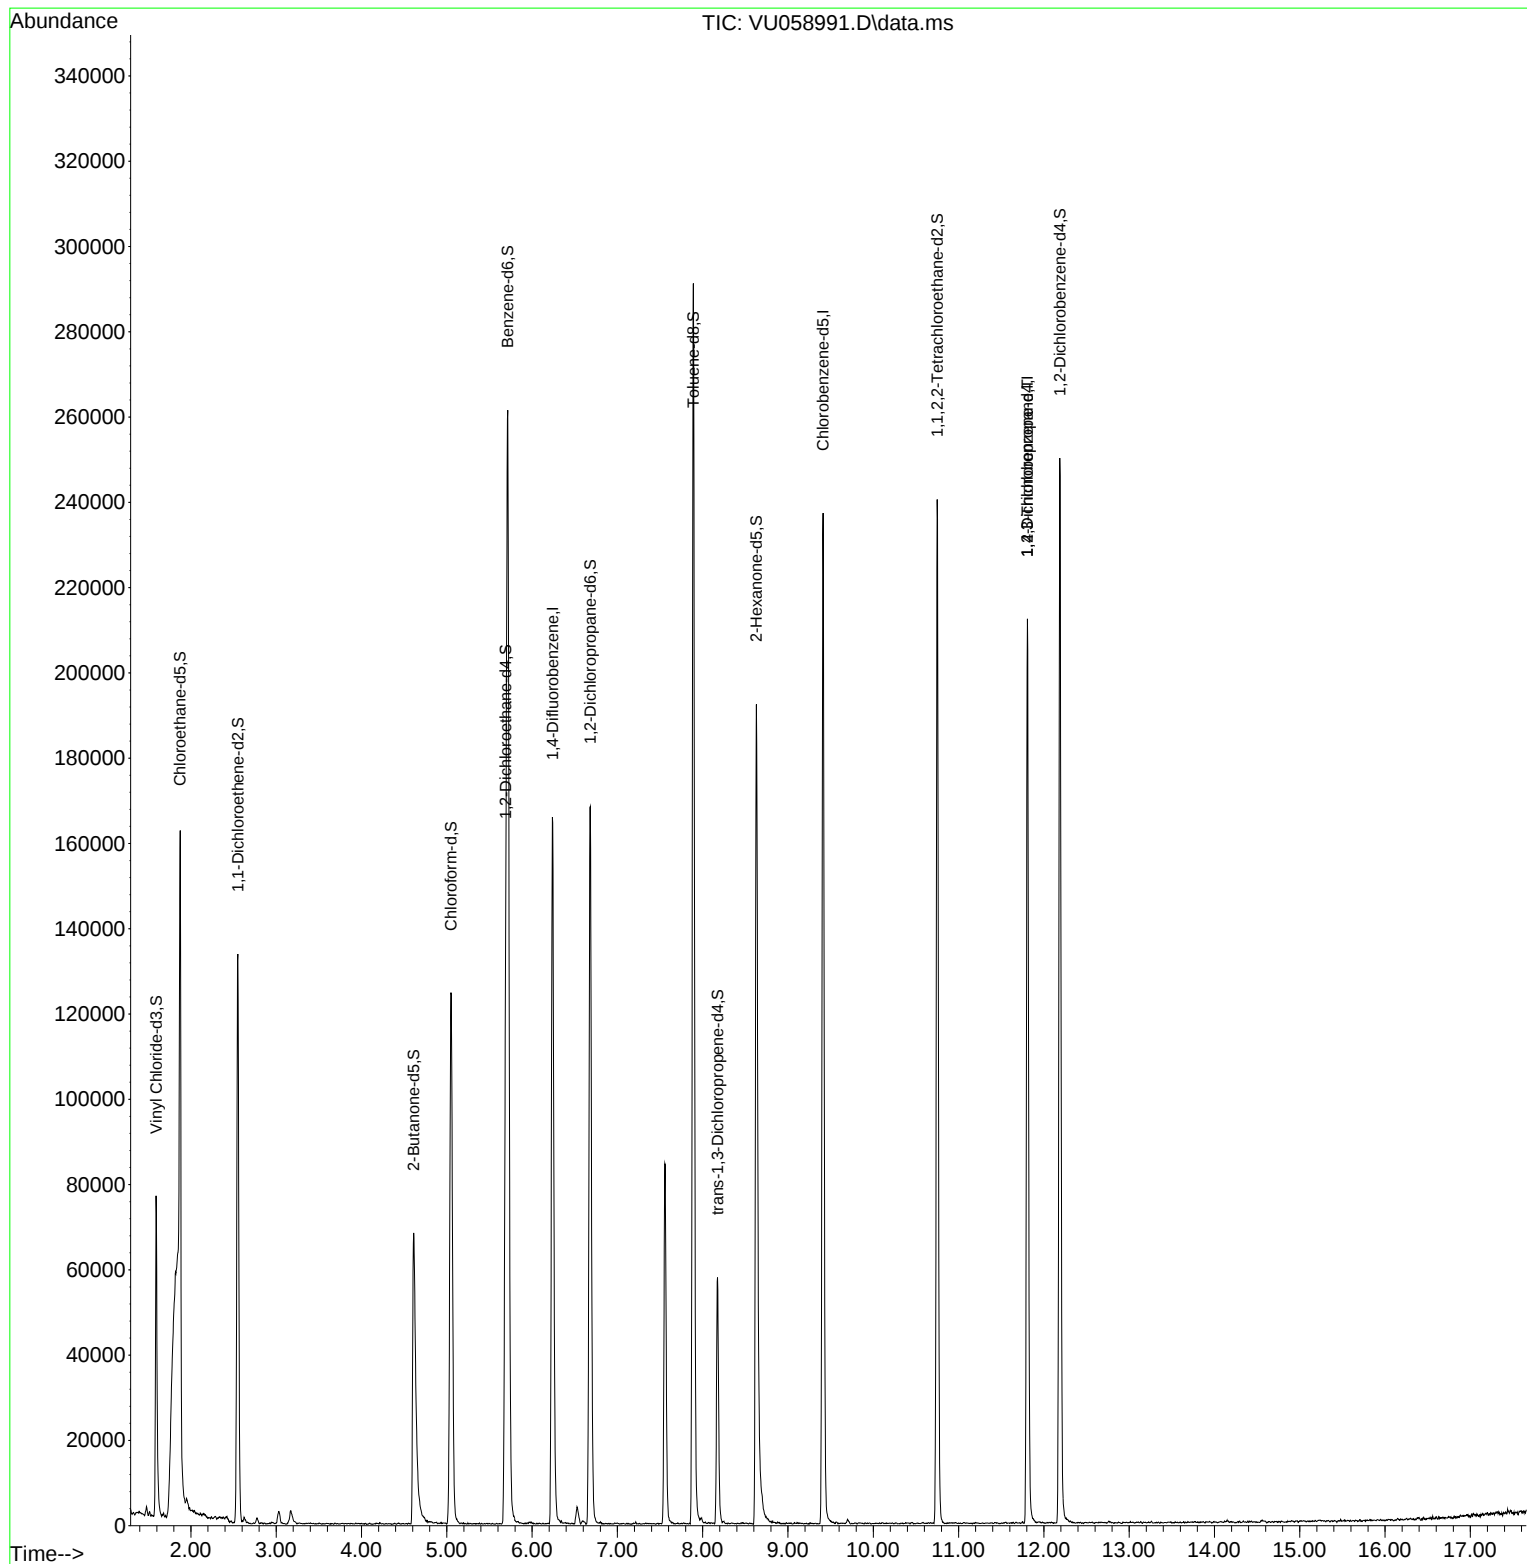

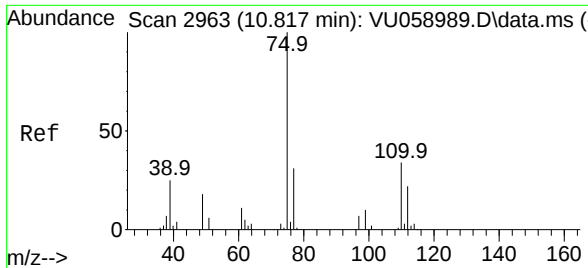

#60
1,2,3-Trichloropropane
Concen: 5.607 ug/L
RT: 11.807 min Scan# 31
Delta R.T. 0.990 min
Lab File: VU058991.D
Acq: 25 May 2024 12:05

Instrument :
MSVOA_U
ClientSampleId :

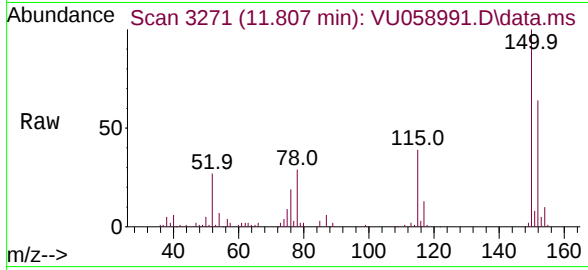

Tgt Ion:	75	Resp:	7686
Ion	Ratio	Lower	Upper
75	100		
77	32.0	25.8	38.6
110	0.0	28.3	42.5#

