

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU059011.D
 Acq On : 25 May 2024 20:15
 Operator : MD/SY
 Sample : P2568-19ME
 Misc : 5.78mL/MSVOA_U/WATER/MSVOA_U/MEOH
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :

Quant Time: May 27 04:16:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon May 27 04:10:55 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.239	114	172585	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.412	117	169831	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.811	152	64732	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.592	65	64590	35.385	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	70.780%		
7) Chloroethane-d5	1.872	69	56826	37.460	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	74.920%		
11) 1,1-Dichloroethene-d2	2.528	63	88627	31.780	ug/L	-0.02
Spiked Amount 50.000	Range 60 - 125		Recovery =	63.560%		
21) 2-Butanone-d5	4.624	46	129600	103.364	ug/L	0.02
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.360%		
24) Chloroform-d	5.052	84	128637	41.086	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	82.180%		
26) 1,2-Dichloroethane-d4	5.689	65	91349	47.707	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.420%		
32) Benzene-d6	5.711	84	263290	45.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.940%		
36) 1,2-Dichloropropane-d6	6.682	67	92984	48.622	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.240%		
41) Toluene-d8	7.891	98	214725	41.375	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	82.740%		
43) trans-1,3-Dichloroprop...	8.174	79	36559	42.574	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.140%		
47) 2-Hexanone-d5	8.644	63	77609	98.124	ug/L	0.02
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.120%		
56) 1,1,2,2-Tetrachloroeth...	10.756	84	133049	46.246	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.500%		
66) 1,2-Dichlorobenzene-d4	12.190	152	64653	48.405	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	96.820%		
Target Compounds			Qvalue			
37) 1,2-Dichloropropane	6.682	63	9940	5.990	ug/L #	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU059011.D
Acq On : 25 May 2024 20:15
Operator : MD/SY
Sample : P2568-19ME
Misc : 5.78mL/MSVOA_U/WATER/MSVOA_U/MEOH
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :

Quant Time: May 27 04:16:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis
QLast Update : Mon May 27 04:10:55 2024
Response via : Initial Calibration

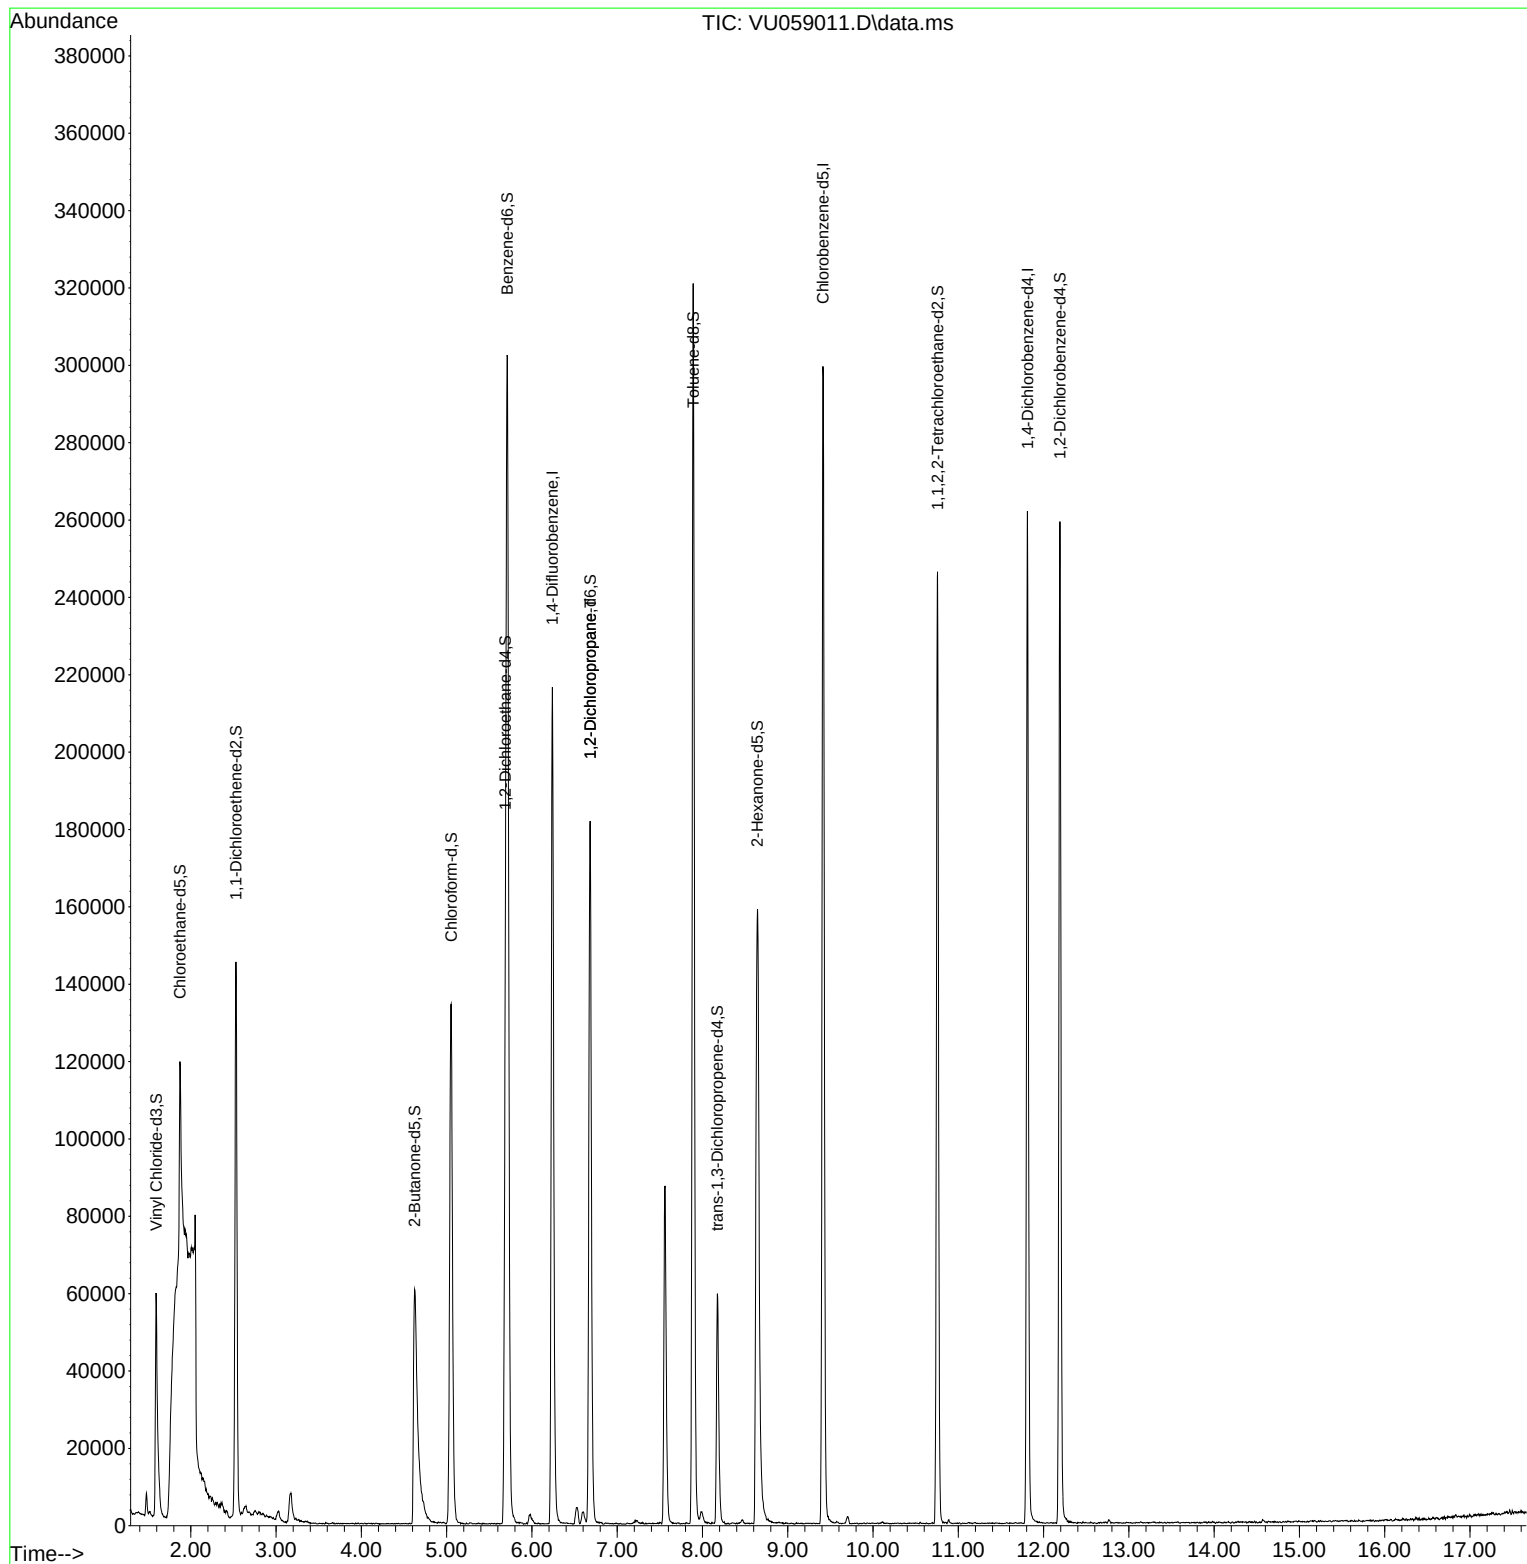

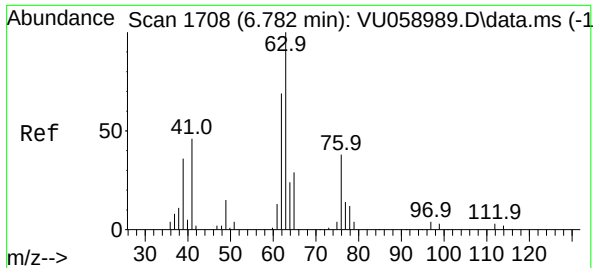

#37
1,2-Dichloropropane
Concen: 5.990 ug/L
RT: 6.682 min Scan# 1
Delta R.T. -0.100 min
Lab File: VU059011.D
Acq: 25 May 2024 20:15

Instrument :
MSVOA_U
ClientSampleId :

Tgt Ion: 63 Resp: 9940
Ion Ratio Lower Upper
63 100
112 0.0 2.5 3.7#

