

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058996.D
 Acq On : 25 May 2024 14:07
 Operator : MD/SY
 Sample : P2566-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU058996.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	110	rBV	61811	78091	12.61%	1.607%
2	2.551	380	392	407	rBV	93564	152070	24.55%	3.130%
3	2.891	495	498	501	rBV2	205	134	0.02%	0.003%
4	2.988	525	528	530	rBV2	134	83	0.01%	0.002%
5	3.033	532	542	551	rVV3	3784	6670	1.08%	0.137%
6	3.171	571	585	613	rBV	21454	55735	9.00%	1.147%
7	3.325	627	633	637	rBV	154	172	0.03%	0.004%
8	3.358	638	643	644	rBV	241	212	0.03%	0.004%
9	3.486	680	683	685	rBV	168	124	0.02%	0.003%
10	3.518	690	693	696	rVB2	301	190	0.03%	0.004%
11	3.534	696	698	700	rBV	112	59	0.01%	0.001%
12	3.743	761	763	770	rBV2	117	114	0.02%	0.002%
13	3.952	825	828	832	rBV	140	101	0.02%	0.002%
14	4.136	883	885	887	rBV	157	104	0.02%	0.002%
15	4.203	903	906	910	rBV2	126	126	0.02%	0.003%
16	4.226	910	913	915	rVB	183	106	0.02%	0.002%
17	4.239	915	917	920	rBV	131	71	0.01%	0.001%
18	4.280	927	930	936	rBV	250	259	0.04%	0.005%
19	4.309	936	939	940	rBV	133	71	0.01%	0.001%
20	4.454	982	984	986	rBV	159	92	0.01%	0.002%
21	4.615	1019	1034	1076	rBV	68729	188861	30.49%	3.887%
22	4.907	1123	1125	1127	rBV2	197	118	0.02%	0.002%
23	4.978	1144	1147	1150	rVB2	174	123	0.02%	0.003%
24	5.049	1150	1169	1195	rBV	107922	240089	38.76%	4.941%
25	5.139	1195	1197	1204	rVB3	497	416	0.07%	0.009%
26	5.193	1211	1214	1217	rBV2	336	301	0.05%	0.006%
27	5.238	1225	1228	1232	rVB2	314	217	0.04%	0.004%
28	5.261	1232	1235	1240	rBV2	195	207	0.03%	0.004%
29	5.348	1258	1262	1263	rBV	110	80	0.01%	0.002%
30	5.383	1269	1273	1275	rBV	204	164	0.03%	0.003%
31	5.493	1305	1307	1308	rBV	105	49	0.01%	0.001%
32	5.714	1356	1376	1405	rBV2	211014	591018	95.42%	12.163%
33	5.923	1437	1441	1443	rBV	240	132	0.02%	0.003%
34	5.988	1459	1461	1466	rVB	258	136	0.02%	0.003%
35	6.113	1497	1500	1503	rBV2	281	195	0.03%	0.004%
36	6.158	1511	1514	1521	rBV2	218	258	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058996.D
 Acq On : 25 May 2024 14:07
 Operator : MD/SY
 Sample : P2566-17
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.238	1526	1539	1566	rBV	279390	531016	85.73%	10.928%
38	6.393	1584	1587	1589	rBV3	457	240	0.04%	0.005%
39	6.441	1597	1602	1607	rBB3	347	281	0.05%	0.006%
40	6.470	1607	1611	1613	rBV3	320	240	0.04%	0.005%
41	6.531	1618	1630	1642	rBV7	3584	7010	1.13%	0.144%
42	6.592	1643	1649	1650	rBV3	677	542	0.09%	0.011%
43	6.682	1663	1677	1701	rBV	142014	279964	45.20%	5.762%
44	6.820	1718	1720	1721	rBV	203	62	0.01%	0.001%
45	6.856	1728	1731	1734	rBV	273	185	0.03%	0.004%
46	6.875	1734	1737	1740	rVB2	255	183	0.03%	0.004%
47	7.023	1782	1783	1788	rVB	232	114	0.02%	0.002%
48	7.049	1788	1791	1793	rBV	132	80	0.01%	0.002%
49	7.164	1824	1827	1830	rBV	151	116	0.02%	0.002%
50	7.248	1849	1853	1856	rBV	173	130	0.02%	0.003%
51	7.271	1856	1860	1863	rBV2	200	196	0.03%	0.004%
52	7.351	1881	1885	1888	rBV2	255	223	0.04%	0.005%
53	7.412	1901	1904	1907	rVB2	272	156	0.03%	0.003%
54	7.521	1931	1938	1939	rBV	270	258	0.04%	0.005%
55	7.560	1939	1950	1978	rVB2	63488	113744	18.36%	2.341%
56	7.705	1992	1995	1998	rVB3	363	247	0.04%	0.005%
57	7.785	2014	2020	2033	rBV6	817	1722	0.28%	0.035%
58	7.891	2041	2053	2072	rBV	204234	354973	57.31%	7.305%
59	8.084	2109	2113	2117	rBV2	250	156	0.03%	0.003%
60	8.107	2117	2120	2125	rVB2	338	231	0.04%	0.005%
61	8.132	2125	2128	2131	rBV2	176	113	0.02%	0.002%
62	8.174	2131	2141	2161	rBV2	45515	78220	12.63%	1.610%
63	8.290	2174	2177	2180	rBV2	160	113	0.02%	0.002%
64	8.631	2272	2283	2316	rBV	192261	387118	62.50%	7.967%
65	8.853	2351	2352	2360	rVB2	357	322	0.05%	0.007%
66	9.033	2405	2408	2412	rBV	351	216	0.03%	0.004%
67	9.267	2477	2481	2485	rBV	211	216	0.03%	0.004%
68	9.412	2513	2526	2549	rBV	375511	619401	100.00%	12.747%
69	9.627	2592	2593	2596	rVB2	170	54	0.01%	0.001%
70	9.647	2596	2599	2600	rBV	198	119	0.02%	0.002%
71	9.878	2668	2671	2672	rBV	124	82	0.01%	0.002%
72	10.261	2786	2790	2797	rBV2	354	450	0.07%	0.009%
73	10.489	2859	2861	2865	rBV3	200	132	0.02%	0.003%
74	10.656	2910	2913	2918	rBV	213	188	0.03%	0.004%
75	10.750	2930	2942	2966	rBV	216783	361146	58.31%	7.432%
76	10.920	2993	2995	3000	rBV2	200	117	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058996.D
Acq On : 25 May 2024 14:07
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis

77	11.569	3194	3197	3200	rBV	277	170	0.03%	0.003%
78	11.749	3251	3253	3254	rBV	245	89	0.01%	0.002%
79	11.807	3260	3271	3297	rBV	314499	503589	81.30%	10.364%
80	12.190	3377	3390	3409	rBV	176252	297793	48.08%	6.128%
81	12.756	3562	3566	3567	rBV2	665	504	0.08%	0.010%




Sum of corrected areas: 4859169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058996.D
Acq On : 25 May 2024 14:07
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

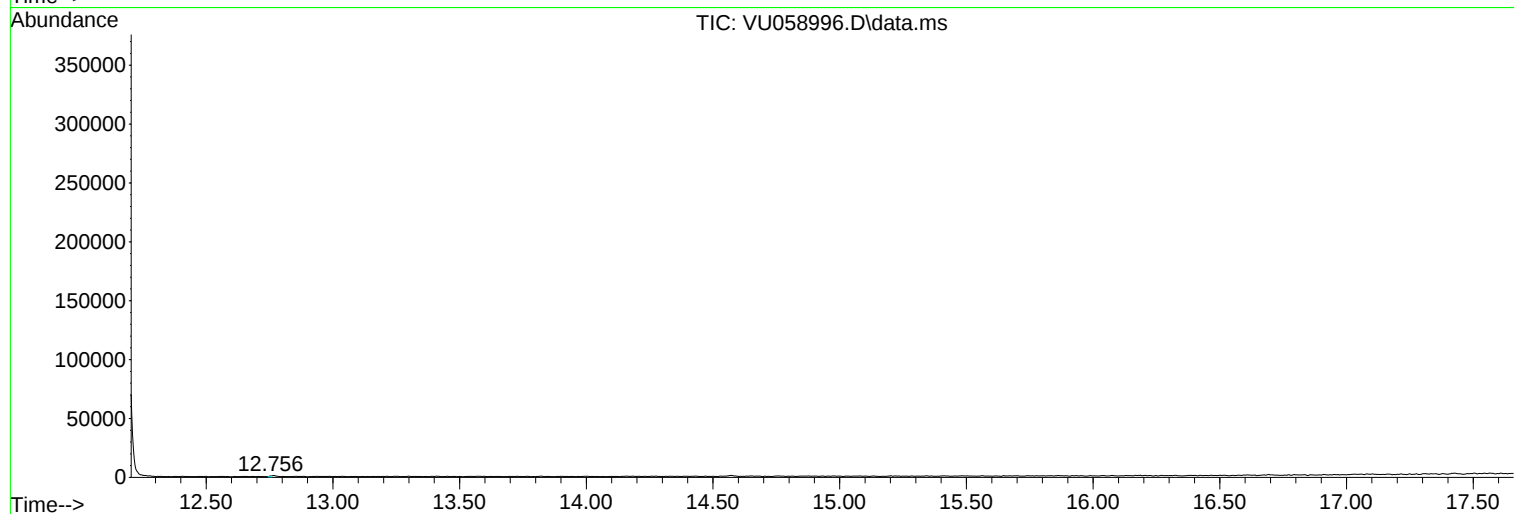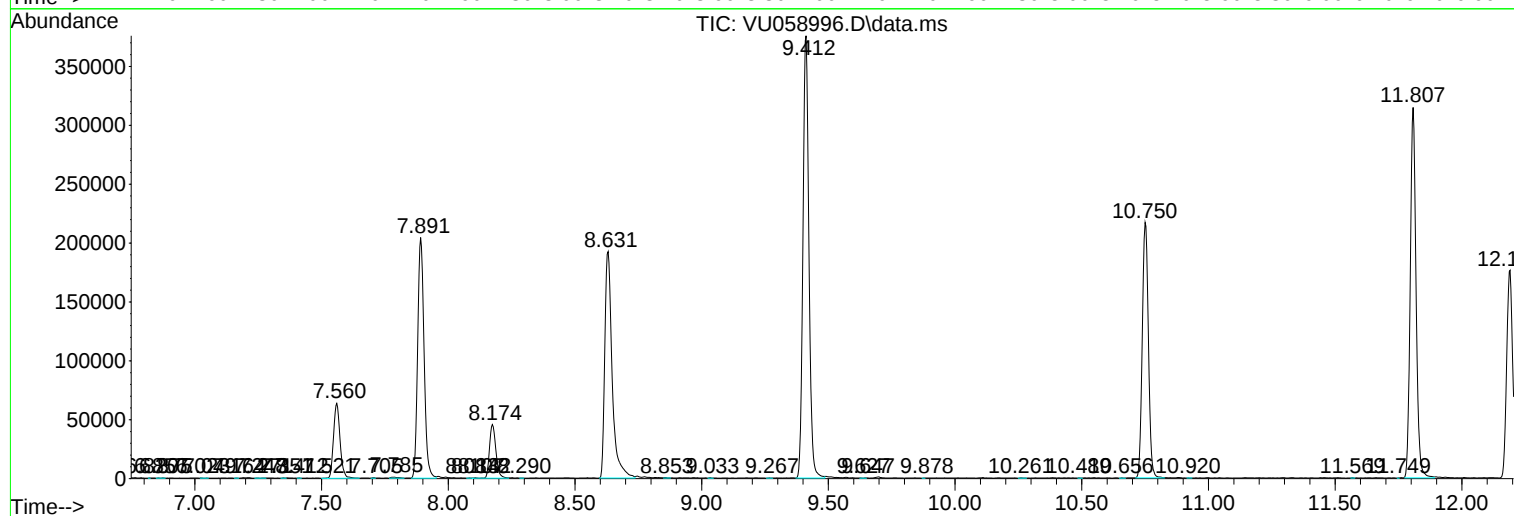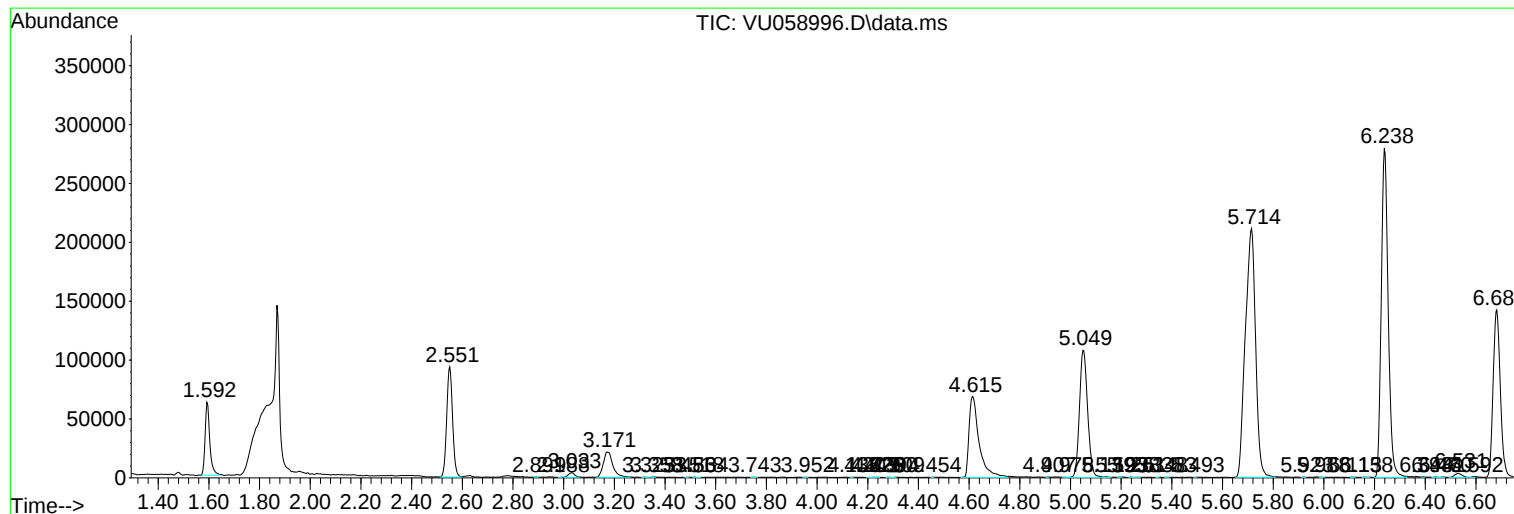

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058996.D
Acq On : 25 May 2024 14:07
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058996.D
Acq On : 25 May 2024 14:07
Operator : MD/SY
Sample : P2566-17
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------