

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058997.D
 Acq On : 25 May 2024 14:32
 Operator : MD/SY
 Sample : P2566-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

Signal : TIC: VU058997.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	115	rVB	58876	80243	12.82%	1.930%
2	2.544	379	390	408	rVB	98748	160862	25.70%	3.870%
3	2.631	410	417	426	rVB4	1889	2745	0.44%	0.066%
4	3.033	532	542	551	rBV5	3618	6662	1.06%	0.160%
5	3.174	572	586	600	rBV	15328	37370	5.97%	0.899%
6	3.814	783	785	789	rVB	223	124	0.02%	0.003%
7	3.917	815	817	820	rVB2	283	148	0.02%	0.004%
8	3.940	820	824	826	rBV2	363	216	0.03%	0.005%
9	3.981	833	837	840	rBV	180	157	0.03%	0.004%
10	4.081	865	868	869	rBV	85	49	0.01%	0.001%
11	4.136	883	885	888	rBV	91	57	0.01%	0.001%
12	4.165	891	894	900	rBV	189	148	0.02%	0.004%
13	4.194	900	903	908	rBV	341	268	0.04%	0.006%
14	4.290	926	933	936	rBV2	397	424	0.07%	0.010%
15	4.399	964	967	969	rBV	153	98	0.02%	0.002%
16	4.480	988	992	998	rBV2	199	196	0.03%	0.005%
17	4.509	998	1001	1003	rVV2	102	52	0.01%	0.001%
18	4.615	1024	1034	1077	rBV2	62987	183736	29.35%	4.420%
19	5.052	1154	1170	1194	rBV	110514	250635	40.04%	6.029%
20	5.219	1219	1222	1224	rBV	126	79	0.01%	0.002%
21	5.300	1246	1247	1248	rBV	156	50	0.01%	0.001%
22	5.361	1262	1266	1268	rBV	263	204	0.03%	0.005%
23	5.473	1297	1301	1306	rBV2	194	221	0.04%	0.005%
24	5.573	1329	1332	1334	rBV	187	118	0.02%	0.003%
25	5.711	1356	1375	1406	rBV2	223818	625961	100.00%	15.058%
26	5.898	1431	1433	1436	rVB	359	179	0.03%	0.004%
27	5.923	1436	1441	1444	rBV2	222	188	0.03%	0.005%
28	5.939	1444	1446	1449	rVB2	214	98	0.02%	0.002%
29	5.975	1449	1457	1460	rBV4	685	783	0.13%	0.019%
30	6.004	1464	1466	1470	rVB	160	94	0.02%	0.002%
31	6.026	1471	1473	1474	rBV	119	59	0.01%	0.001%
32	6.129	1502	1505	1510	rBV	354	294	0.05%	0.007%
33	6.181	1517	1521	1527	rVB	261	261	0.04%	0.006%
34	6.239	1527	1539	1566	rBV	143228	280358	44.79%	6.744%
35	6.441	1598	1602	1608	rVB2	227	266	0.04%	0.006%
36	6.473	1608	1612	1615	rBV	173	143	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
 Data File : VU058997.D
 Acq On : 25 May 2024 14:32
 Operator : MD/SY
 Sample : P2566-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHHT5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
 Title : VOC Analysis

37	6.528	1620	1629	1641	rVB8	3557	7083	1.13%	0.170%
38	6.589	1641	1648	1650	rBV2	880	917	0.15%	0.022%
39	6.682	1663	1677	1699	rBV2	150978	297103	47.46%	7.147%
40	6.820	1717	1720	1722	rBV	192	80	0.01%	0.002%
41	6.927	1750	1753	1758	rBV2	173	163	0.03%	0.004%
42	6.952	1759	1761	1764	rVB	192	104	0.02%	0.003%
43	7.094	1802	1805	1807	rBV2	193	126	0.02%	0.003%
44	7.145	1818	1821	1824	rBV2	119	71	0.01%	0.002%
45	7.165	1824	1827	1830	rBV2	193	101	0.02%	0.002%
46	7.203	1833	1839	1841	rBV3	507	497	0.08%	0.012%
47	7.338	1879	1881	1882	rBV3	201	73	0.01%	0.002%
48	7.377	1890	1893	1896	rVB	209	134	0.02%	0.003%
49	7.438	1908	1912	1914	rBV2	161	129	0.02%	0.003%
50	7.505	1930	1933	1935	rBV	167	117	0.02%	0.003%
51	7.560	1938	1950	1965	rBV	66375	118954	19.00%	2.861%
52	7.788	2014	2021	2026	rBV3	668	903	0.14%	0.022%
53	7.846	2035	2039	2041	rBV2	354	258	0.04%	0.006%
54	7.891	2041	2053	2077	rVV	219393	381632	60.97%	9.180%
55	8.065	2105	2107	2115	rVB3	451	326	0.05%	0.008%
56	8.097	2115	2117	2119	rBV2	231	139	0.02%	0.003%
57	8.174	2131	2141	2156	rBV2	45649	80236	12.82%	1.930%
58	8.267	2168	2170	2172	rBV	121	61	0.01%	0.001%
59	8.409	2211	2214	2216	rBV	130	84	0.01%	0.002%
60	8.454	2225	2228	2231	rBV	179	138	0.02%	0.003%
61	8.634	2272	2284	2320	rBV2	174056	376741	60.19%	9.063%
62	8.968	2387	2388	2391	rBV	173	90	0.01%	0.002%
63	9.010	2398	2401	2403	rBV	146	89	0.01%	0.002%
64	9.094	2424	2427	2428	rBV	129	80	0.01%	0.002%
65	9.216	2461	2465	2469	rVB2	245	225	0.04%	0.005%
66	9.251	2469	2476	2481	rBV2	318	466	0.07%	0.011%
67	9.325	2496	2499	2500	rBV	93	52	0.01%	0.001%
68	9.412	2515	2526	2548	rBV	191703	327404	52.30%	7.876%
69	9.743	2626	2629	2633	rBV2	186	142	0.02%	0.003%
70	10.100	2735	2740	2743	rBV2	479	424	0.07%	0.010%
71	10.335	2810	2813	2814	rBV	202	133	0.02%	0.003%
72	10.753	2931	2943	2964	rVB	224330	367686	58.74%	8.845%
73	11.309	3113	3116	3118	rBV2	260	178	0.03%	0.004%
74	11.811	3260	3272	3296	rBV	156676	258126	41.24%	6.209%
75	12.190	3378	3390	3414	rBV	178198	301835	48.22%	7.261%
76	12.405	3454	3457	3458	rBV	196	112	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058997.D
Acq On : 25 May 2024 14:32
Operator : MD/SY
Sample : P2566-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Title : VOC Analysis

77	12.798	3576	3579	3583	rBV	266	196	0.03%	0.005%
78	13.045	3654	3656	3658	rBV	340	110	0.02%	0.003%




Sum of corrected areas: 4157064

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058997.D
Acq On : 25 May 2024 14:32
Operator : MD/SY
Sample : P2566-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

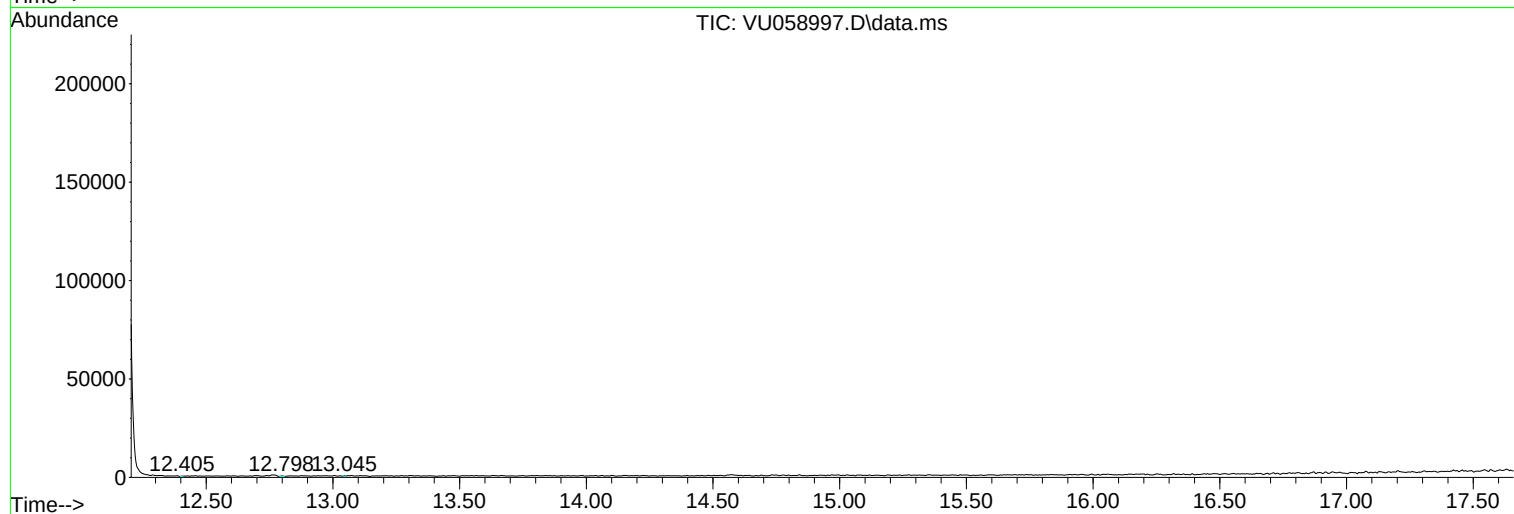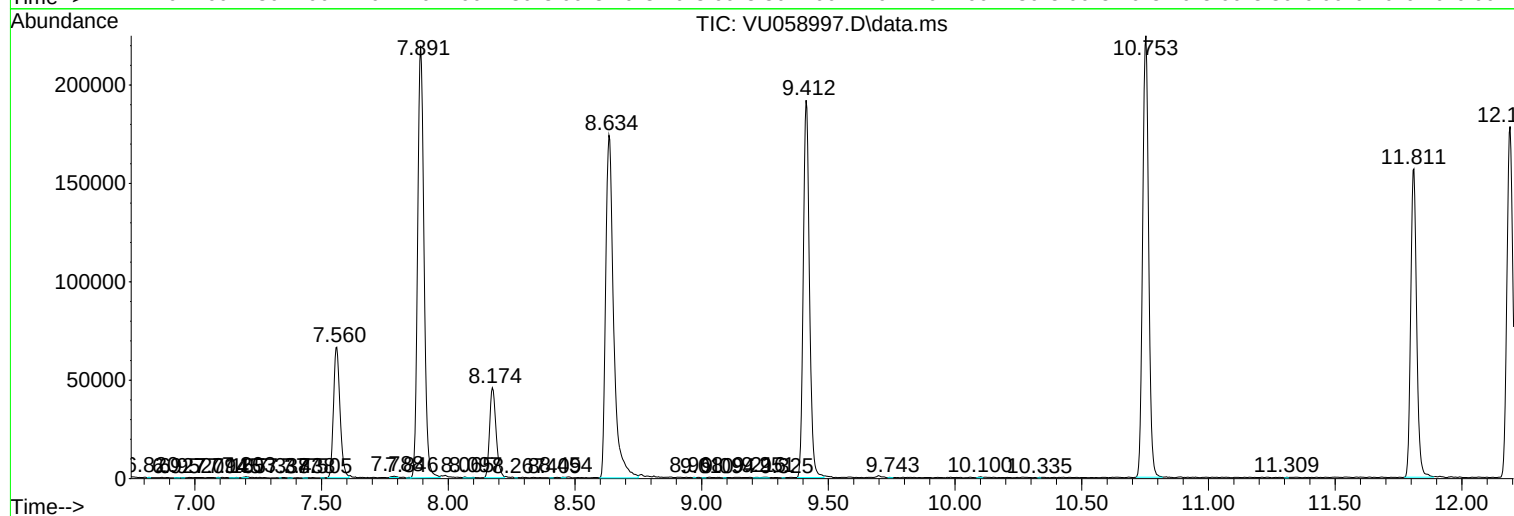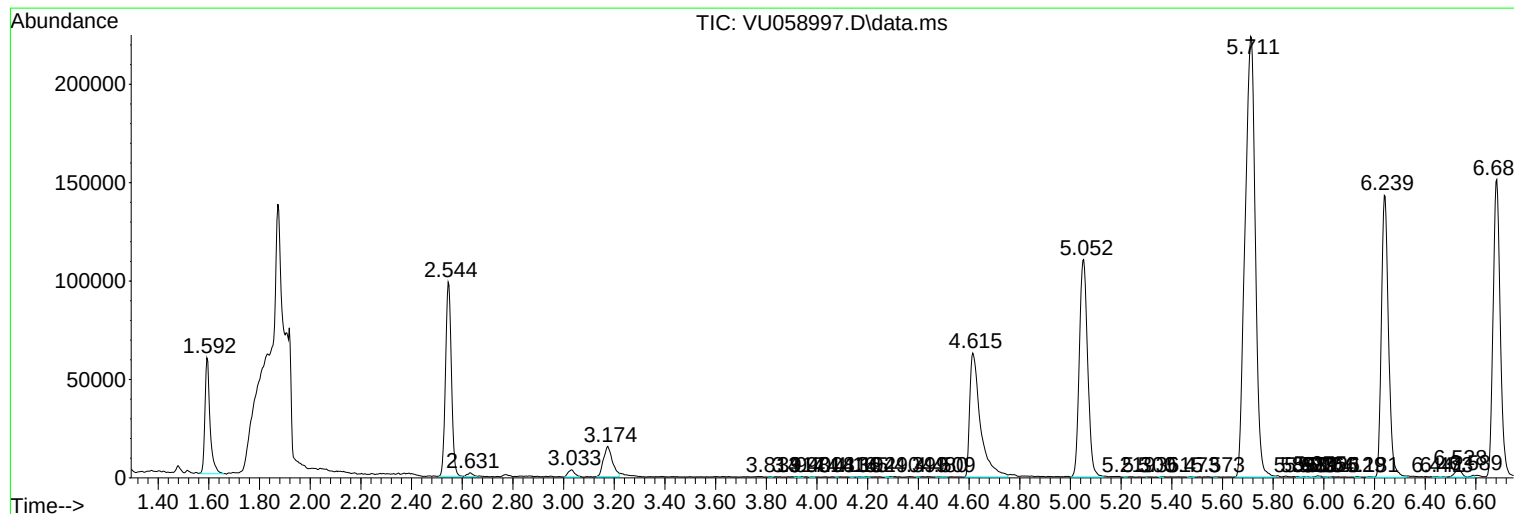

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058997.D
Acq On : 25 May 2024 14:32
Operator : MD/SY
Sample : P2566-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU052524\
Data File : VU058997.D
Acq On : 25 May 2024 14:32
Operator : MD/SY
Sample : P2566-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHHT5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM052324WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------